

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
 Data File : VX025344.D
 Acq On : 26 Nov 2021 10:13
 Operator : JC/MD
 Sample : VX1126WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK642

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	55	rVB	87406	84841	14.81%	1.887%
2	1.666	91	95	103	rVB	66495	83505	14.58%	1.858%
3	2.306	194	200	210	rBV	120577	197827	34.53%	4.401%
4	2.513	230	234	242	rBV4	567	1314	0.23%	0.029%
5	2.702	263	265	270	rVB2	398	471	0.08%	0.010%
6	2.788	272	279	287	rVB4	966	1982	0.35%	0.044%
7	2.843	287	288	290	rBV2	140	118	0.02%	0.003%
8	2.965	305	308	311	rVV	139	153	0.03%	0.003%
9	3.099	324	330	333	rBV4	571	1134	0.20%	0.025%
10	3.349	369	371	373	rBV2	114	141	0.02%	0.003%
11	3.465	388	390	392	rBV2	154	118	0.02%	0.003%
12	3.611	410	414	417	rVV3	374	512	0.09%	0.011%
13	3.678	424	425	429	rVB	196	134	0.02%	0.003%
14	4.190	506	509	510	rBV	171	144	0.03%	0.003%
15	4.452	541	552	565	rBV	49328	137118	23.93%	3.050%
16	4.720	593	596	598	rVB	137	138	0.02%	0.003%
17	4.763	601	603	606	rVB2	147	144	0.03%	0.003%
18	4.934	630	631	635	rVB2	172	200	0.03%	0.004%
19	5.056	638	651	669	rBV	74219	231181	40.35%	5.143%
20	5.226	676	679	680	rVB	240	173	0.03%	0.004%
21	5.330	693	696	698	rBV2	149	189	0.03%	0.004%
22	5.391	701	706	713	rVB4	689	1482	0.26%	0.033%
23	5.470	715	719	722	rBV3	335	471	0.08%	0.010%
24	5.678	750	753	754	rVV2	250	296	0.05%	0.007%
25	5.970	788	801	824	rVV2	190125	572882	100.00%	12.744%
26	6.251	845	847	849	rBV2	180	161	0.03%	0.004%
27	6.501	886	888	890	rVB	176	124	0.02%	0.003%
28	6.531	890	893	894	rBV2	195	188	0.03%	0.004%
29	6.763	921	931	942	rBV	142677	343229	59.91%	7.636%
30	6.994	967	969	972	rBV2	178	234	0.04%	0.005%
31	7.110	980	988	996	rVB3	3646	8169	1.43%	0.182%
32	7.311	1011	1021	1031	rBV	116508	258014	45.04%	5.740%
33	7.689	1082	1083	1087	rBV2	100	120	0.02%	0.003%
34	7.817	1100	1104	1109	rVB4	451	841	0.15%	0.019%
35	7.860	1109	1111	1116	rVB2	154	226	0.04%	0.005%
36	7.927	1116	1122	1131	rBV2	996	2132	0.37%	0.047%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
 Data File : VX025344.D
 Acq On : 26 Nov 2021 10:13
 Operator : JC/MD
 Sample : VX1126WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK642

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	8.183	1162	1164	1166	rVB	181	127	0.02%	0.003%
38	8.323	1181	1187	1199	rBV	87996	141774	24.75%	3.154%
39	8.470	1208	1211	1214	rVB3	624	756	0.13%	0.017%
40	8.573	1223	1228	1234	rBV3	904	1514	0.26%	0.034%
41	8.646	1234	1240	1248	rVV	298416	470646	82.15%	10.470%
42	8.720	1248	1252	1259	rVV	5129	8262	1.44%	0.184%
43	8.793	1262	1264	1266	rBV2	108	141	0.02%	0.003%
44	8.951	1284	1290	1301	rVV	61765	91985	16.06%	2.046%
45	9.024	1301	1302	1305	rVB2	300	207	0.04%	0.005%
46	9.153	1319	1323	1327	rVB3	411	580	0.10%	0.013%
47	9.274	1340	1343	1347	rVB2	1058	1270	0.22%	0.028%
48	9.323	1347	1351	1352	rBV2	139	139	0.02%	0.003%
49	9.384	1355	1361	1380	rBV	217945	306965	53.58%	6.829%
50	9.616	1394	1399	1402	rVB2	390	535	0.09%	0.012%
51	9.701	1409	1413	1417	rVB2	919	1204	0.21%	0.027%
52	10.055	1465	1471	1487	rVB	300353	408143	71.24%	9.080%
53	10.195	1490	1494	1499	rVB	1551	2037	0.36%	0.045%
54	10.238	1499	1501	1504	rBV2	118	155	0.03%	0.003%
55	10.299	1507	1511	1518	rVB	1863	2561	0.45%	0.057%
56	10.402	1526	1528	1533	rVB2	98	121	0.02%	0.003%
57	10.652	1564	1569	1575	rVB4	1922	3573	0.62%	0.079%
58	10.805	1590	1594	1597	rBV2	302	358	0.06%	0.008%
59	10.963	1617	1620	1624	rVB	1728	1976	0.34%	0.044%
60	11.024	1627	1630	1632	rBV2	96	128	0.02%	0.003%
61	11.085	1637	1640	1642	rBV3	248	251	0.04%	0.006%
62	11.122	1642	1646	1650	rVB	1096	1472	0.26%	0.033%
63	11.195	1652	1658	1665	rBV	227132	292387	51.04%	6.505%
64	11.274	1669	1671	1674	rBV2	334	510	0.09%	0.011%
65	11.384	1687	1689	1691	rVB2	242	184	0.03%	0.004%
66	11.451	1697	1700	1711	rVV	1828	2409	0.42%	0.054%
67	11.548	1714	1716	1719	rBV	172	156	0.03%	0.003%
68	11.750	1745	1749	1754	rBV2	2911	3409	0.60%	0.076%
69	11.811	1757	1759	1762	rBV	168	201	0.04%	0.004%
70	11.896	1769	1773	1776	rBV2	136	218	0.04%	0.005%
71	11.933	1776	1779	1782	rVB2	607	576	0.10%	0.013%
72	11.975	1782	1786	1789	rBV	1485	1811	0.32%	0.040%
73	12.024	1789	1794	1801	rBV	314177	386900	67.54%	8.607%
74	12.128	1807	1811	1812	rBV3	440	551	0.10%	0.012%
75	12.152	1812	1815	1819	rVB2	670	810	0.14%	0.018%
76	12.256	1830	1832	1837	rBV2	140	197	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
 Data File : VX025344.D
 Acq On : 26 Nov 2021 10:13
 Operator : JC/MD
 Sample : VX1126WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK642

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1850	rBV	332664	417576	72.89%	9.289%
78	12.426	1858	1860	1863	rBV2	344	242	0.04%	0.005%
79	12.487	1866	1870	1874	rBV	153	268	0.05%	0.006%
80	12.768	1912	1916	1918	rVV	356	393	0.07%	0.009%
81	12.945	1943	1945	1948	rVB2	180	171	0.03%	0.004%
82	13.115	1970	1973	1976	rBV	1123	1295	0.23%	0.029%
83	13.396	2017	2019	2021	rVB2	135	129	0.02%	0.003%
84	13.457	2027	2029	2033	rBV2	85	119	0.02%	0.003%
85	13.597	2048	2052	2056	rVB2	975	1185	0.21%	0.026%
86	13.786	2078	2083	2086	rVB2	854	1309	0.23%	0.029%
87	13.847	2091	2093	2097	rVB2	118	169	0.03%	0.004%
88	13.963	2109	2112	2116	rVB3	1024	1257	0.22%	0.028%
89	14.066	2126	2129	2132	rBV2	119	173	0.03%	0.004%
90	14.139	2135	2141	2144	rBV2	775	1162	0.20%	0.026%
91	14.213	2151	2153	2157	rBV2	177	211	0.04%	0.005%
92	14.255	2157	2160	2161	rBV	179	178	0.03%	0.004%
93	14.322	2169	2171	2173	rBV	180	147	0.03%	0.003%
94	14.395	2179	2183	2184	rBV	160	165	0.03%	0.004%
95	14.584	2211	2214	2215	rBV	200	189	0.03%	0.004%
96	14.688	2228	2231	2235	rBV2	207	289	0.05%	0.006%
97	15.121	2300	2302	2303	rBV2	213	178	0.03%	0.004%
98	15.645	2386	2388	2392	rBV2	265	282	0.05%	0.006%
99	16.401	2508	2512	2515	rBV2	260	440	0.08%	0.010%
100	16.505	2527	2529	2533	rBV2	225	310	0.05%	0.007%


Sum of corrected areas: 4495142

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
Data File : VX025344.D
Acq On : 26 Nov 2021 10:13
Operator : JC/MD
Sample : VX1126WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK642

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

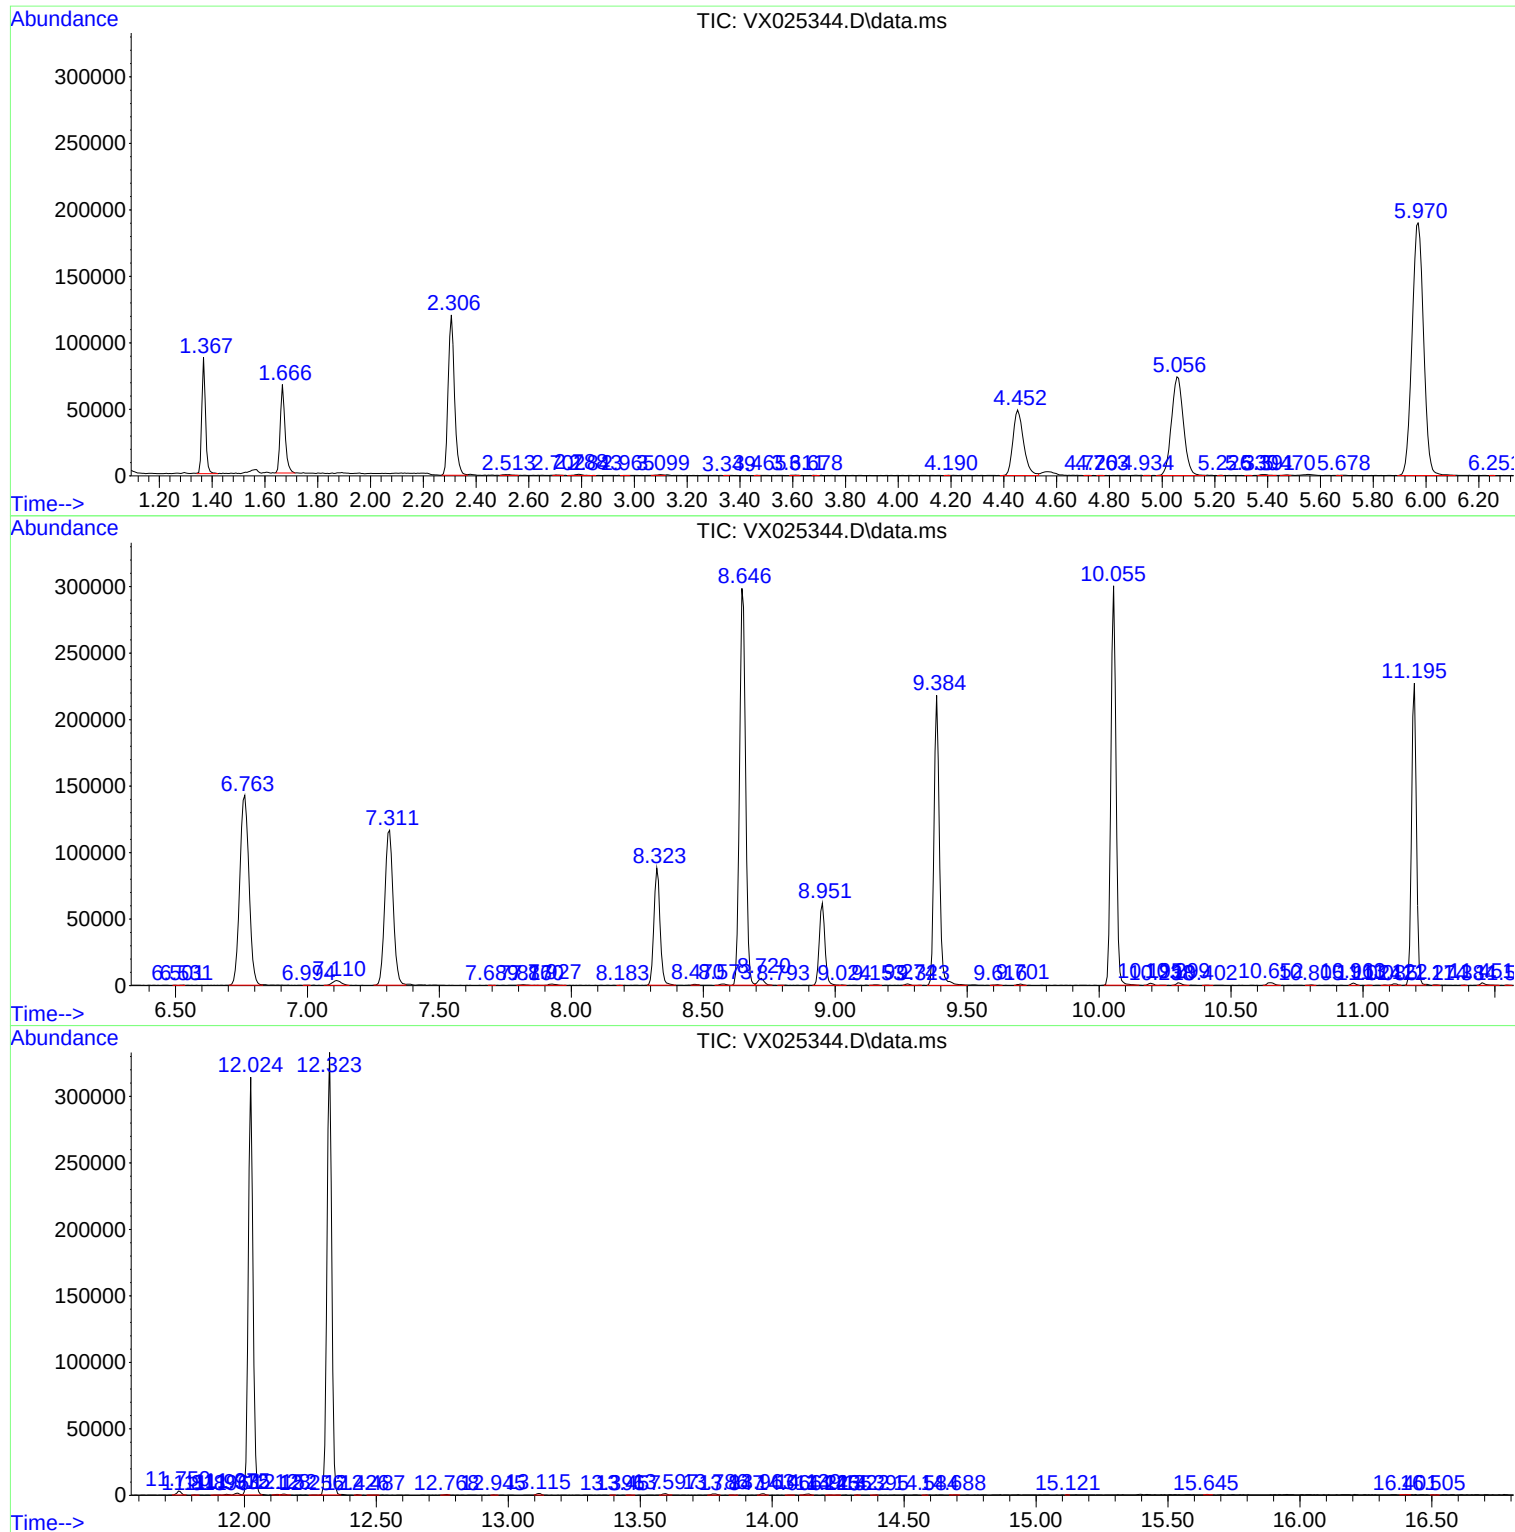

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
Data File : VX025344.D
Acq On : 26 Nov 2021 10:13
Operator : JC/MD
Sample : VX1126WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK642

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
Data File : VX025344.D
Acq On : 26 Nov 2021 10:13
Operator : JC/MD
Sample : VX1126WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK642

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc