

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
 Data File : VX025348.D
 Acq On : 26 Nov 2021 11:57
 Operator : JC/MD
 Sample : M4799-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025348.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rBV	72694	69559	12.96%	1.658%
2	1.660	90	94	105	rVB	57475	74752	13.93%	1.782%
3	2.307	194	200	211	rBV	100552	167978	31.31%	4.005%
4	2.435	220	221	224	rBV2	298	272	0.05%	0.006%
5	2.788	275	279	284	rVB3	596	893	0.17%	0.021%
6	2.947	299	305	312	rVB2	891	1911	0.36%	0.046%
7	3.008	312	315	316	rBV	159	172	0.03%	0.004%
8	3.532	397	401	402	rVV2	92	118	0.02%	0.003%
9	3.611	412	414	416	rVB2	158	124	0.02%	0.003%
10	3.745	434	436	438	rVB2	198	142	0.03%	0.003%
11	3.983	474	475	478	rBV	146	140	0.03%	0.003%
12	4.087	489	492	493	rBV2	125	138	0.03%	0.003%
13	4.343	532	534	537	rBV2	83	116	0.02%	0.003%
14	4.453	543	552	567	rBV	46442	130652	24.35%	3.115%
15	4.702	589	593	595	rBV2	118	115	0.02%	0.003%
16	4.843	612	616	620	rVB2	158	221	0.04%	0.005%
17	4.971	633	637	639	rBV2	119	121	0.02%	0.003%
18	5.062	639	652	667	rBV	70075	217304	40.50%	5.181%
19	5.245	678	682	686	rBV2	158	309	0.06%	0.007%
20	5.361	699	701	702	rBV2	198	143	0.03%	0.003%
21	5.556	724	733	742	rBV2	648	1840	0.34%	0.044%
22	5.794	769	772	775	rBV2	127	161	0.03%	0.004%
23	5.971	789	801	821	rBV2	178155	536575	100.00%	12.793%
24	6.160	830	832	834	rVB	151	117	0.02%	0.003%
25	6.257	847	848	851	rVB2	167	124	0.02%	0.003%
26	6.605	903	905	908	rVB	122	131	0.02%	0.003%
27	6.763	921	931	946	rBV	137183	324788	60.53%	7.744%
28	6.897	951	953	955	rVV2	184	186	0.03%	0.004%
29	6.922	955	957	959	rVB2	191	118	0.02%	0.003%
30	6.983	964	967	971	rBV	113	174	0.03%	0.004%
31	7.111	982	988	996	rVB3	3415	7120	1.33%	0.170%
32	7.165	996	997	999	rBV	134	123	0.02%	0.003%
33	7.312	1012	1021	1032	rBV	111769	245269	45.71%	5.848%
34	7.464	1043	1046	1047	rBV	141	127	0.02%	0.003%
35	7.482	1047	1049	1053	rVV3	227	335	0.06%	0.008%
36	7.537	1055	1058	1059	rBV2	131	120	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
 Data File : VX025348.D
 Acq On : 26 Nov 2021 11:57
 Operator : JC/MD
 Sample : M4799-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

37	7.665	1077	1079	1081	rVB	159	118	0.02%	0.003%
38	7.696	1081	1084	1086	rBV2	183	170	0.03%	0.004%
39	7.806	1100	1102	1109	rVB	338	452	0.08%	0.011%
40	7.879	1111	1114	1117	rBV2	144	199	0.04%	0.005%
41	7.928	1117	1122	1128	rBV4	914	1663	0.31%	0.040%
42	8.324	1181	1187	1198	rBV	80716	130807	24.38%	3.119%
43	8.434	1203	1205	1208	rBV	140	149	0.03%	0.004%
44	8.470	1208	1211	1216	rBV3	690	1009	0.19%	0.024%
45	8.574	1225	1228	1230	rBV3	148	158	0.03%	0.004%
46	8.647	1233	1240	1248	rBV	277115	439372	81.88%	10.476%
47	8.720	1248	1252	1261	rVB	3945	6140	1.14%	0.146%
48	8.952	1284	1290	1297	rBV	58690	85561	15.95%	2.040%
49	9.116	1314	1317	1321	rBV	77	138	0.03%	0.003%
50	9.330	1347	1352	1355	rBV	83	140	0.03%	0.003%
51	9.385	1355	1361	1375	rBV	209624	293928	54.78%	7.008%
52	9.537	1384	1386	1387	rBV	210	150	0.03%	0.004%
53	9.708	1410	1414	1418	rBV3	315	470	0.09%	0.011%
54	10.055	1465	1471	1480	rBV	286728	388697	72.44%	9.267%
55	10.189	1491	1493	1500	rVB3	251	347	0.06%	0.008%
56	10.305	1509	1512	1517	rVB2	507	618	0.12%	0.015%
57	10.555	1550	1553	1555	rVB2	104	139	0.03%	0.003%
58	10.622	1560	1564	1565	rBV	102	121	0.02%	0.003%
59	10.957	1618	1619	1621	rBV2	253	202	0.04%	0.005%
60	11.085	1638	1640	1642	rVB	208	187	0.03%	0.004%
61	11.122	1642	1646	1650	rBV	987	1131	0.21%	0.027%
62	11.195	1652	1658	1668	rBV	223986	285051	53.12%	6.796%
63	11.281	1670	1672	1674	rBV	297	233	0.04%	0.006%
64	11.305	1674	1676	1677	rBV2	125	126	0.02%	0.003%
65	11.378	1686	1688	1690	rVB	141	117	0.02%	0.003%
66	11.451	1696	1700	1704	rBV3	258	493	0.09%	0.012%
67	11.482	1704	1705	1708	rVV2	155	136	0.03%	0.003%
68	11.689	1738	1739	1742	rBV	103	116	0.02%	0.003%
69	11.750	1746	1749	1752	rBV3	1057	1246	0.23%	0.030%
70	11.848	1763	1765	1767	rVB2	169	161	0.03%	0.004%
71	11.933	1776	1779	1782	rVB2	423	368	0.07%	0.009%
72	12.024	1789	1794	1802	rBV	299128	369300	68.83%	8.805%
73	12.128	1807	1811	1812	rBV2	313	407	0.08%	0.010%
74	12.201	1819	1823	1824	rVB2	130	140	0.03%	0.003%
75	12.226	1824	1827	1830	rBV	116	121	0.02%	0.003%
76	12.323	1837	1843	1851	rVV	309421	396159	73.83%	9.445%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
 Data File : VX025348.D
 Acq On : 26 Nov 2021 11:57
 Operator : JC/MD
 Sample : M4799-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	12.421	1858	1859	1865	rBV2	191	263	0.05%	0.006%
78	12.469	1865	1867	1870	rBV2	118	118	0.02%	0.003%
79	12.762	1912	1915	1918	rVB2	368	432	0.08%	0.010%
80	12.823	1922	1925	1927	rBV2	112	121	0.02%	0.003%
81	12.981	1948	1951	1952	rBV2	110	118	0.02%	0.003%
82	13.414	2019	2022	2023	rBV2	103	116	0.02%	0.003%
83	13.433	2023	2025	2026	rBV	119	114	0.02%	0.003%
84	13.707	2067	2070	2073	rBV2	112	122	0.02%	0.003%
85	13.780	2080	2082	2087	rVB2	214	233	0.04%	0.006%
86	13.865	2094	2096	2098	rBV2	129	144	0.03%	0.003%
87	14.097	2130	2134	2135	rBV	158	133	0.02%	0.003%
88	14.134	2136	2140	2145	rVB2	1057	1393	0.26%	0.033%
89	14.268	2160	2162	2165	rBV	191	162	0.03%	0.004%
90	14.298	2165	2167	2170	rVB2	120	121	0.02%	0.003%
91	14.365	2176	2178	2181	rVB	153	138	0.03%	0.003%
92	14.396	2181	2183	2188	rBV2	202	304	0.06%	0.007%
93	14.445	2189	2191	2193	rBV	233	163	0.03%	0.004%
94	14.603	2215	2217	2219	rBV	118	117	0.02%	0.003%
95	14.853	2256	2258	2261	rVB	208	185	0.03%	0.004%
96	15.444	2352	2355	2356	rBV2	172	217	0.04%	0.005%
97	15.658	2388	2390	2391	rBV	298	176	0.03%	0.004%
98	16.072	2456	2458	2463	rBV	168	217	0.04%	0.005%
99	16.597	2542	2544	2547	rBV2	187	166	0.03%	0.004%
100	16.731	2564	2566	2568	rBV3	248	256	0.05%	0.006%




Sum of corrected areas: 4194257

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
Data File : VX025348.D
Acq On : 26 Nov 2021 11:57
Operator : JC/MD
Sample : M4799-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

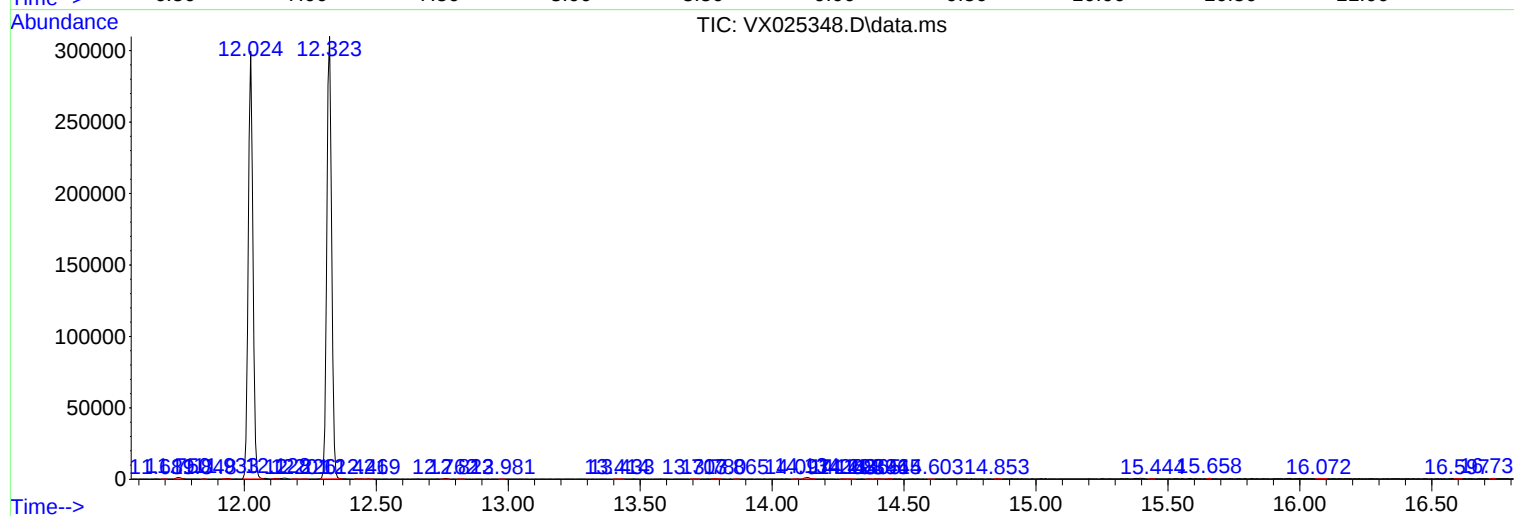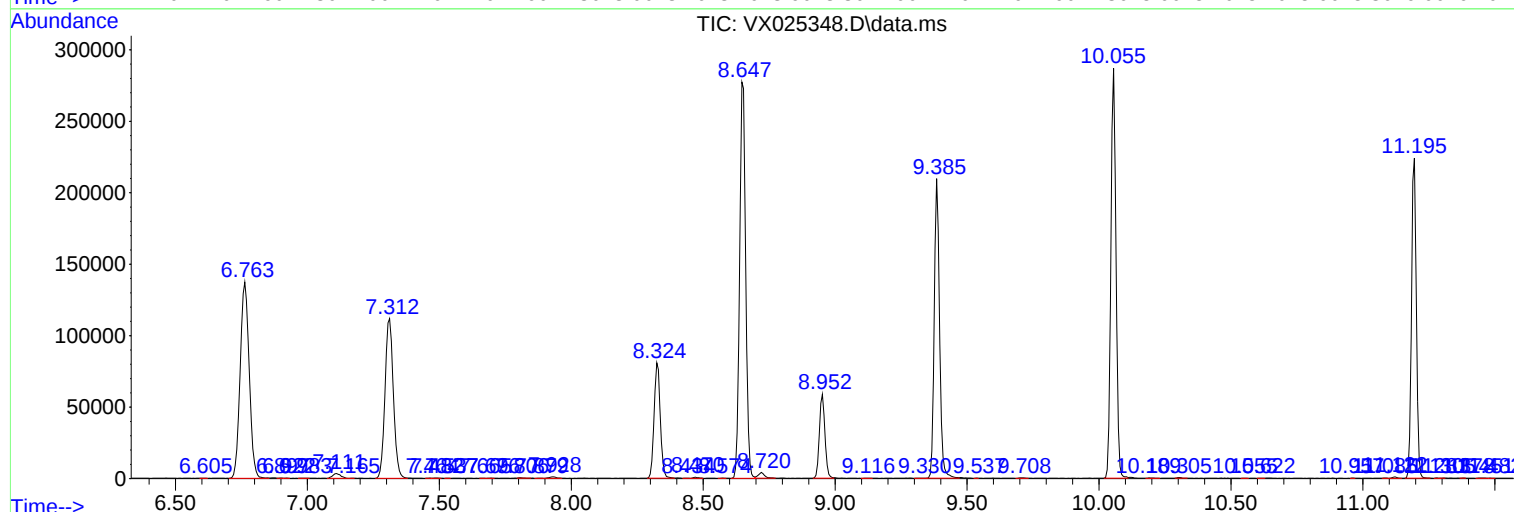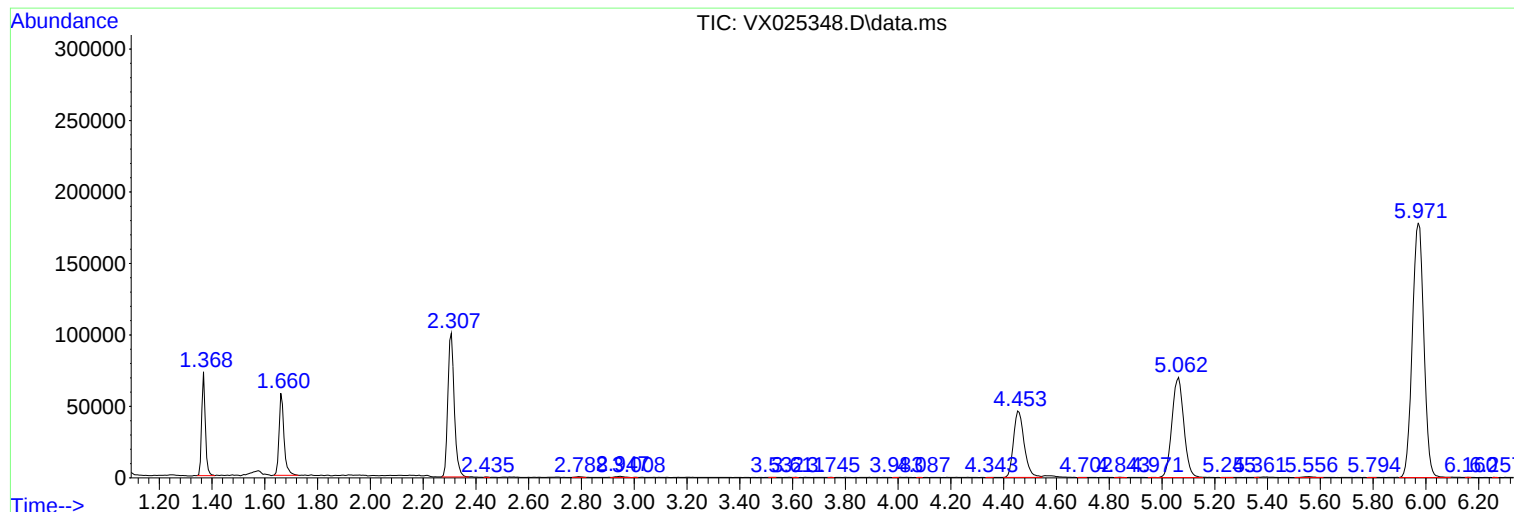

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
Data File : VX025348.D
Acq On : 26 Nov 2021 11:57
Operator : JC/MD
Sample : M4799-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
Data File : VX025348.D
Acq On : 26 Nov 2021 11:57
Operator : JC/MD
Sample : M4799-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc