

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
 Data File : VX025352.D
 Acq On : 26 Nov 2021 13:42
 Operator : JC/MD
 Sample : M4839-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025352.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	24	26	36	rVB2	2596	4482	0.84%	0.107%
2	1.368	42	46	53	rVB	75652	73722	13.85%	1.760%
3	1.660	90	94	107	rVB	56264	76047	14.29%	1.815%
4	2.306	193	200	212	rBV	107689	175903	33.06%	4.199%
5	2.508	232	233	238	rVB2	308	317	0.06%	0.008%
6	2.684	260	262	263	rBV	164	120	0.02%	0.003%
7	2.788	275	279	285	rVB3	669	1163	0.22%	0.028%
8	2.843	285	288	290	rBV2	169	218	0.04%	0.005%
9	2.940	301	304	305	rBV2	237	247	0.05%	0.006%
10	3.087	326	328	330	rBV2	177	150	0.03%	0.004%
11	3.196	343	346	347	rBV	146	138	0.03%	0.003%
12	3.605	411	413	418	rVV2	165	197	0.04%	0.005%
13	3.666	420	423	426	rBV2	138	200	0.04%	0.005%
14	3.855	450	454	455	rBV	135	145	0.03%	0.003%
15	4.105	491	495	496	rBV2	123	176	0.03%	0.004%
16	4.452	543	552	570	rBV	45370	128783	24.20%	3.074%
17	4.666	585	587	589	rBV2	206	196	0.04%	0.005%
18	4.739	597	599	602	rBV	106	116	0.02%	0.003%
19	4.971	636	637	639	rBV	181	117	0.02%	0.003%
20	5.062	639	652	667	rVV	69131	214132	40.24%	5.112%
21	5.166	667	669	672	rVB	273	209	0.04%	0.005%
22	5.202	673	675	678	rVB2	129	119	0.02%	0.003%
23	5.379	700	704	706	rBV3	162	266	0.05%	0.006%
24	5.556	727	733	740	rVB2	503	1134	0.21%	0.027%
25	5.629	740	745	746	rBV2	124	213	0.04%	0.005%
26	5.879	784	786	789	rVB	151	133	0.02%	0.003%
27	5.970	789	801	817	rBV2	178478	532141	100.00%	12.703%
28	6.403	869	872	873	rBV2	131	123	0.02%	0.003%
29	6.653	911	913	914	rBV2	139	120	0.02%	0.003%
30	6.763	920	931	944	rBV	142987	337335	63.39%	8.053%
31	6.897	951	953	955	rBV2	139	137	0.03%	0.003%
32	6.982	965	967	968	rBV	258	154	0.03%	0.004%
33	7.062	978	980	981	rBV2	143	129	0.02%	0.003%
34	7.110	981	988	995	rVV	2812	6347	1.19%	0.152%
35	7.312	1011	1021	1036	rBV	111170	242724	45.61%	5.794%
36	7.488	1045	1050	1052	rBV3	256	366	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
 Data File : VX025352.D
 Acq On : 26 Nov 2021 13:42
 Operator : JC/MD
 Sample : M4839-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	7.702	1081	1085	1087	rVB	154	244	0.05%	0.006%
38	7.799	1099	1101	1108	rVB2	253	421	0.08%	0.010%
39	7.927	1116	1122	1128	rBV6	742	1614	0.30%	0.039%
40	8.122	1152	1154	1157	rVB2	171	158	0.03%	0.004%
41	8.196	1162	1166	1170	rBV2	112	172	0.03%	0.004%
42	8.324	1180	1187	1198	rBV	77178	127793	24.01%	3.051%
43	8.464	1208	1210	1212	rBV3	578	667	0.13%	0.016%
44	8.561	1223	1226	1227	rVB2	153	118	0.02%	0.003%
45	8.574	1227	1228	1232	rBV2	213	218	0.04%	0.005%
46	8.653	1234	1241	1248	rVV	270698	436795	82.08%	10.427%
47	8.720	1249	1252	1262	rVB2	4161	6119	1.15%	0.146%
48	8.952	1284	1290	1301	rBV	58106	82032	15.42%	1.958%
49	9.275	1341	1343	1345	rBV	192	180	0.03%	0.004%
50	9.384	1355	1361	1372	rBV	199077	284042	53.38%	6.781%
51	9.707	1409	1414	1421	rVB2	696	1151	0.22%	0.027%
52	9.829	1433	1434	1437	rBV	165	129	0.02%	0.003%
53	9.915	1445	1448	1450	rBV	122	141	0.03%	0.003%
54	9.957	1453	1455	1457	rVB2	166	125	0.02%	0.003%
55	10.000	1460	1462	1465	rVV	145	178	0.03%	0.004%
56	10.055	1465	1471	1490	rVV	291327	399854	75.14%	9.545%
57	10.189	1491	1493	1498	rVB3	191	241	0.05%	0.006%
58	10.311	1509	1513	1518	rVB3	425	639	0.12%	0.015%
59	10.354	1518	1520	1525	rVB	127	188	0.04%	0.004%
60	10.756	1584	1586	1588	rVB2	140	145	0.03%	0.003%
61	10.780	1588	1590	1593	rBV	118	140	0.03%	0.003%
62	10.994	1622	1625	1626	rBV2	120	120	0.02%	0.003%
63	11.085	1637	1640	1643	rBV3	520	688	0.13%	0.016%
64	11.122	1643	1646	1649	rVB2	948	1205	0.23%	0.029%
65	11.195	1652	1658	1666	rBV	218424	273737	51.44%	6.535%
66	11.457	1698	1701	1702	rVV2	207	168	0.03%	0.004%
67	11.482	1702	1705	1706	rVV	299	231	0.04%	0.006%
68	11.506	1706	1709	1711	rVB2	213	237	0.04%	0.006%
69	11.750	1745	1749	1754	rVB3	1143	1368	0.26%	0.033%
70	11.847	1761	1765	1767	rBV2	168	157	0.03%	0.004%
71	11.933	1776	1779	1783	rVB3	677	697	0.13%	0.017%
72	12.024	1789	1794	1804	rVV	303872	374347	70.35%	8.936%
73	12.128	1808	1811	1813	rBV2	512	695	0.13%	0.017%
74	12.152	1813	1815	1820	rVB3	686	757	0.14%	0.018%
75	12.323	1837	1843	1850	rBV	303460	387880	72.89%	9.260%
76	12.427	1859	1860	1863	rBV	188	155	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
 Data File : VX025352.D
 Acq On : 26 Nov 2021 13:42
 Operator : JC/MD
 Sample : M4839-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	12.548	1878	1880	1883	rBV	154	137	0.03%	0.003%
78	12.652	1894	1897	1900	rBV2	116	172	0.03%	0.004%
79	12.695	1902	1904	1908	rVV2	132	124	0.02%	0.003%
80	12.762	1912	1915	1916	rBV	323	316	0.06%	0.008%
81	12.963	1944	1948	1953	rBV2	97	177	0.03%	0.004%
82	13.335	2008	2009	2014	rVB2	239	175	0.03%	0.004%
83	13.512	2036	2038	2039	rBV	196	125	0.02%	0.003%
84	13.786	2081	2083	2088	rBV	128	156	0.03%	0.004%
85	13.938	2106	2108	2112	rVB2	133	169	0.03%	0.004%
86	13.981	2112	2115	2118	rBV2	117	175	0.03%	0.004%
87	14.109	2132	2136	2137	rBV2	124	175	0.03%	0.004%
88	14.127	2137	2139	2146	rVB2	559	908	0.17%	0.022%
89	14.188	2146	2149	2150	rBV	106	133	0.02%	0.003%
90	14.304	2166	2168	2171	rBV2	161	242	0.05%	0.006%
91	14.402	2182	2184	2186	rBV2	153	158	0.03%	0.004%
92	14.420	2186	2187	2191	rVB2	254	203	0.04%	0.005%
93	14.463	2191	2194	2196	rBV	198	151	0.03%	0.004%
94	14.493	2196	2199	2200	rBV2	181	192	0.04%	0.005%
95	14.664	2225	2227	2230	rVB	142	160	0.03%	0.004%
96	14.731	2235	2238	2239	rBV2	145	140	0.03%	0.003%
97	15.085	2294	2296	2297	rBV2	179	143	0.03%	0.003%
98	15.243	2320	2322	2323	rBV2	145	122	0.02%	0.003%
99	16.133	2467	2468	2471	rBV	297	174	0.03%	0.004%
100	16.450	2518	2520	2522	rBV2	247	190	0.04%	0.005%

Sum of corrected areas: 4188982




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
Data File : VX025352.D
Acq On : 26 Nov 2021 13:42
Operator : JC/MD
Sample : M4839-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

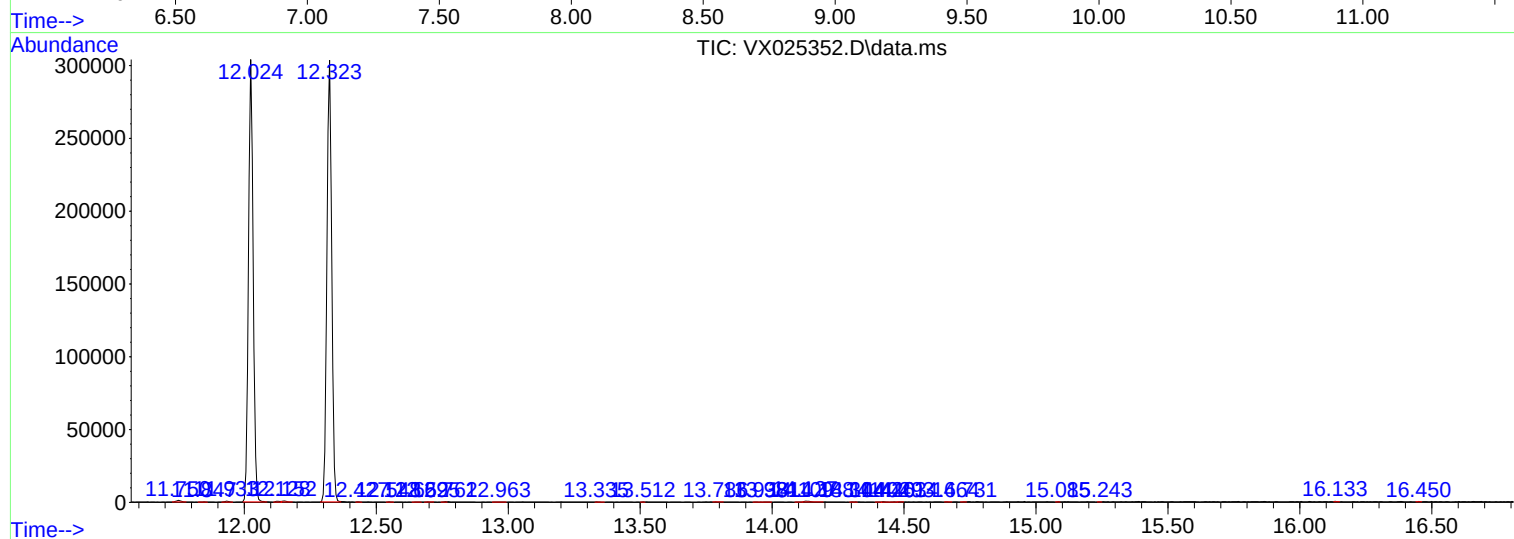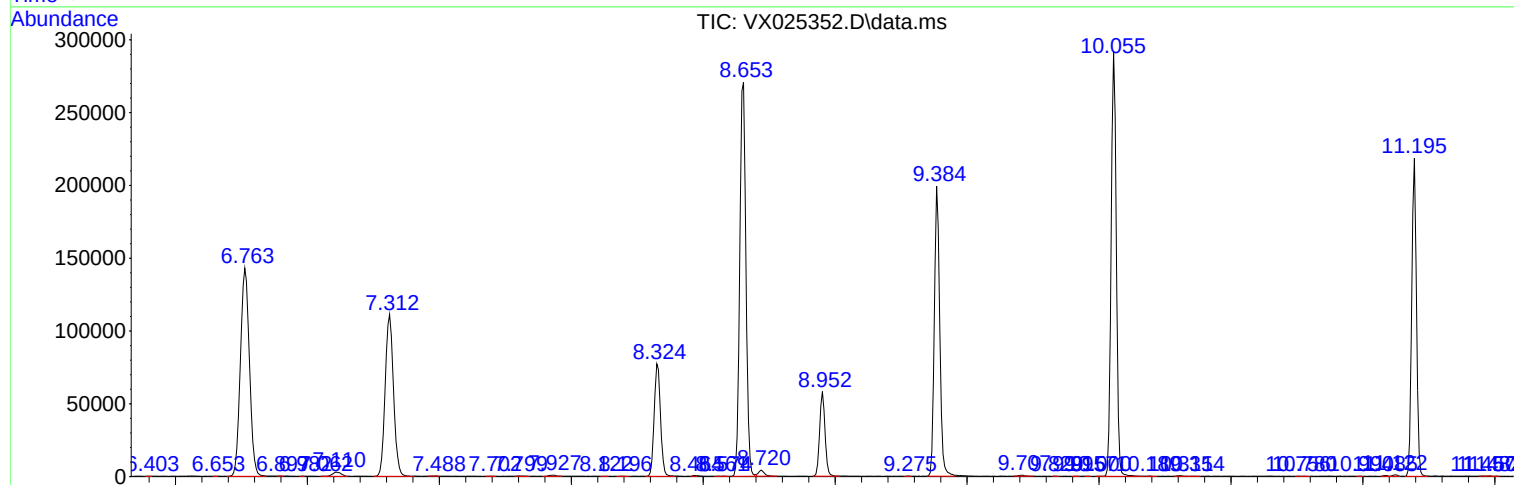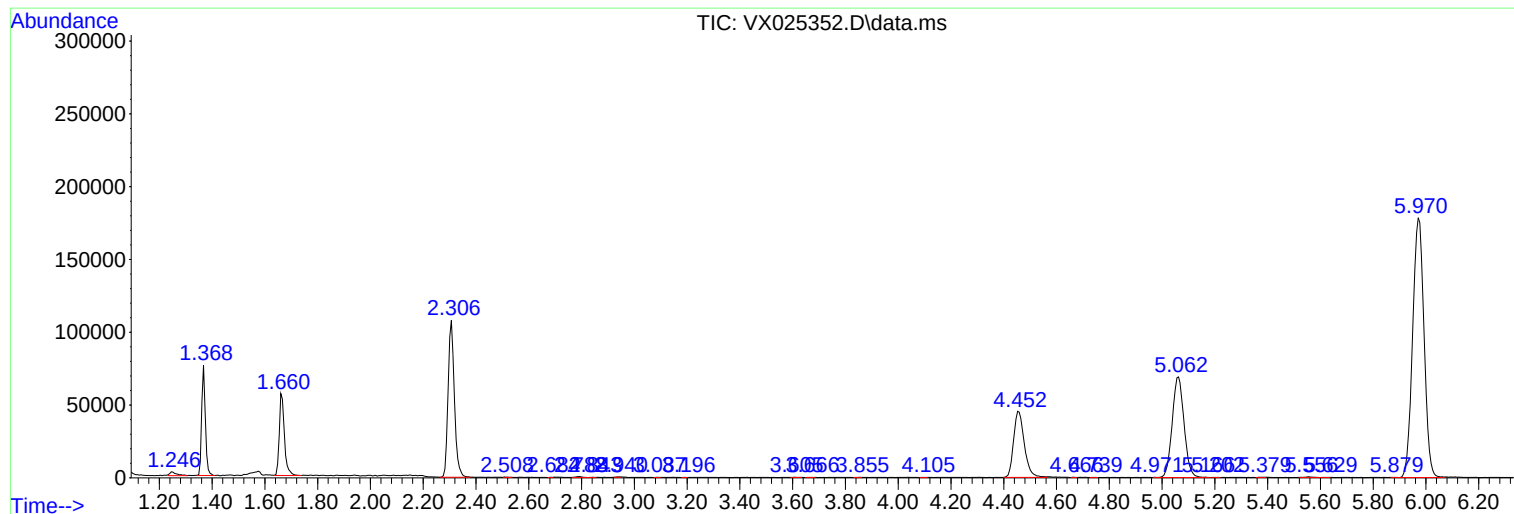

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
Data File : VX025352.D
Acq On : 26 Nov 2021 13:42
Operator : JC/MD
Sample : M4839-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
Data File : VX025352.D
Acq On : 26 Nov 2021 13:42
Operator : JC/MD
Sample : M4839-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc