

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
 Data File : VX025355.D
 Acq On : 26 Nov 2021 14:57
 Operator : JC/MD
 Sample : M4833-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025355.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	54	rVB	69665	68366	13.61%	1.726%
2	1.666	90	95	106	rVB	53981	73087	14.54%	1.846%
3	2.306	194	200	211	rBV	98793	162362	32.31%	4.100%
4	2.946	300	305	309	rBV3	317	713	0.14%	0.018%
5	3.202	344	347	348	rBV	113	111	0.02%	0.003%
6	3.336	366	369	371	rBV2	152	115	0.02%	0.003%
7	3.574	406	408	411	rBV2	143	170	0.03%	0.004%
8	3.922	461	465	466	rBV	106	154	0.03%	0.004%
9	4.159	502	504	508	rBV2	99	145	0.03%	0.004%
10	4.294	523	526	528	rBV2	123	117	0.02%	0.003%
11	4.458	544	553	569	rBV	45553	129854	25.84%	3.279%
12	5.062	640	652	671	rBV	66538	206900	41.17%	5.224%
13	5.336	693	697	699	rVB2	117	175	0.03%	0.004%
14	5.360	699	701	703	rBV	146	124	0.02%	0.003%
15	5.379	703	704	707	rVV2	205	195	0.04%	0.005%
16	5.409	707	709	712	rVB2	178	180	0.04%	0.005%
17	5.556	727	733	736	rBV	430	604	0.12%	0.015%
18	5.812	771	775	776	rBV2	120	121	0.02%	0.003%
19	5.866	781	784	786	rBV	164	169	0.03%	0.004%
20	5.970	789	801	818	rBV2	170016	502506	100.00%	12.689%
21	6.452	879	880	882	rVV	145	123	0.02%	0.003%
22	6.555	895	897	899	rVB2	165	146	0.03%	0.004%
23	6.586	899	902	903	rBV2	129	136	0.03%	0.003%
24	6.677	908	917	918	rBV2	98	216	0.04%	0.005%
25	6.763	922	931	947	rVV	132549	316338	62.95%	7.988%
26	6.958	962	963	966	rVB2	147	109	0.02%	0.003%
27	7.110	982	988	995	rVB2	3186	6657	1.32%	0.168%
28	7.311	1011	1021	1032	rBV	105932	230570	45.88%	5.822%
29	7.384	1032	1033	1035	rBV	237	178	0.04%	0.004%
30	7.470	1045	1047	1048	rBV	254	144	0.03%	0.004%
31	7.622	1069	1072	1074	rBV	105	114	0.02%	0.003%
32	7.701	1084	1085	1088	rBV	130	125	0.02%	0.003%
33	7.756	1092	1094	1097	rVV2	124	119	0.02%	0.003%
34	7.805	1098	1102	1110	rVV3	248	608	0.12%	0.015%
35	7.872	1110	1113	1114	rVV2	126	110	0.02%	0.003%
36	7.890	1114	1116	1118	rVV	98	108	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
 Data File : VX025355.D
 Acq On : 26 Nov 2021 14:57
 Operator : JC/MD
 Sample : M4833-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	7.933	1118	1123	1131	rVV3	746	1458	0.29%	0.037%
38	8.250	1173	1175	1177	rBV2	125	108	0.02%	0.003%
39	8.329	1181	1188	1198	rBV	73905	119762	23.83%	3.024%
40	8.470	1207	1211	1216	rVB3	661	940	0.19%	0.024%
41	8.653	1234	1241	1249	rBV	250545	403238	80.25%	10.182%
42	8.720	1249	1252	1259	rVV2	3727	5432	1.08%	0.137%
43	8.951	1284	1290	1301	rVV	53701	77323	15.39%	1.952%
44	9.091	1311	1313	1316	rBV2	126	151	0.03%	0.004%
45	9.146	1319	1322	1324	rBV2	105	134	0.03%	0.003%
46	9.183	1326	1328	1331	rBV	124	135	0.03%	0.003%
47	9.274	1339	1343	1344	rVB2	133	150	0.03%	0.004%
48	9.384	1356	1361	1373	rBV	200383	285357	56.79%	7.206%
49	9.707	1411	1414	1420	rVB3	329	521	0.10%	0.013%
50	9.811	1429	1431	1434	rVB	137	139	0.03%	0.004%
51	10.000	1459	1462	1465	rBV2	140	204	0.04%	0.005%
52	10.055	1465	1471	1487	rVV	282891	374802	74.59%	9.464%
53	10.171	1487	1490	1492	rVV	125	147	0.03%	0.004%
54	10.201	1493	1495	1497	rVB2	226	171	0.03%	0.004%
55	10.225	1497	1499	1504	rBV2	103	133	0.03%	0.003%
56	10.262	1504	1505	1508	rBV2	111	113	0.02%	0.003%
57	10.305	1508	1512	1515	rVB2	554	655	0.13%	0.017%
58	10.597	1558	1560	1563	rVB	185	151	0.03%	0.004%
59	10.640	1566	1567	1570	rVB	191	188	0.04%	0.005%
60	10.957	1618	1619	1622	rVB2	176	155	0.03%	0.004%
61	11.085	1639	1640	1642	rBV	217	146	0.03%	0.004%
62	11.122	1644	1646	1650	rVB3	632	724	0.14%	0.018%
63	11.195	1652	1658	1669	rVV	209458	267804	53.29%	6.762%
64	11.317	1676	1678	1680	rBV	121	120	0.02%	0.003%
65	11.433	1694	1697	1698	rBV2	129	140	0.03%	0.004%
66	11.451	1698	1700	1702	rBV2	139	123	0.02%	0.003%
67	11.500	1705	1708	1709	rBV2	169	173	0.03%	0.004%
68	11.719	1742	1744	1746	rBV	154	137	0.03%	0.003%
69	11.750	1746	1749	1754	rVB2	824	988	0.20%	0.025%
70	11.896	1771	1773	1776	rVB2	135	127	0.03%	0.003%
71	11.932	1776	1779	1782	rBV2	223	206	0.04%	0.005%
72	12.024	1789	1794	1802	rBV	283175	346196	68.89%	8.742%
73	12.134	1807	1812	1813	rBV2	295	418	0.08%	0.011%
74	12.152	1813	1815	1819	rVB2	512	482	0.10%	0.012%
75	12.323	1837	1843	1850	rBV	292788	363389	72.32%	9.176%
76	12.432	1859	1861	1863	rVB	126	129	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
 Data File : VX025355.D
 Acq On : 26 Nov 2021 14:57
 Operator : JC/MD
 Sample : M4833-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	12.487	1865	1870	1872	rBV2	138	215	0.04%	0.005%
78	12.603	1886	1889	1890	rBV	136	143	0.03%	0.004%
79	12.621	1890	1892	1896	rVB	190	141	0.03%	0.004%
80	12.749	1910	1913	1914	rBV	142	135	0.03%	0.003%
81	13.188	1982	1985	1987	rVB2	115	108	0.02%	0.003%
82	13.304	2001	2004	2006	rBV	113	147	0.03%	0.004%
83	13.353	2009	2012	2015	rBV	124	150	0.03%	0.004%
84	13.432	2023	2025	2028	rVB2	119	147	0.03%	0.004%
85	13.774	2075	2081	2084	rBV2	178	332	0.07%	0.008%
86	13.981	2113	2115	2118	rBV2	146	174	0.03%	0.004%
87	14.127	2134	2139	2146	rBV3	837	1387	0.28%	0.035%
88	14.560	2208	2210	2213	rBV2	159	201	0.04%	0.005%
89	14.664	2226	2227	2228	rBV	200	131	0.03%	0.003%
90	15.011	2282	2284	2285	rBV2	183	121	0.02%	0.003%
91	15.054	2289	2291	2292	rBV	103	106	0.02%	0.003%
92	15.261	2323	2325	2328	rVB3	281	210	0.04%	0.005%
93	15.292	2328	2330	2332	rBV	198	126	0.03%	0.003%
94	15.542	2369	2371	2372	rBV	255	150	0.03%	0.004%
95	15.779	2406	2410	2412	rBV	246	361	0.07%	0.009%
96	15.993	2443	2445	2447	rBV2	202	145	0.03%	0.004%
97	16.169	2472	2474	2477	rVB	198	162	0.03%	0.004%
98	16.261	2488	2489	2493	rBV2	209	256	0.05%	0.006%
99	16.493	2525	2527	2529	rBV2	222	249	0.05%	0.006%
100	16.749	2567	2569	2570	rBV	201	113	0.02%	0.003%


Sum of corrected areas: 3960248

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
Data File : VX025355.D
Acq On : 26 Nov 2021 14:57
Operator : JC/MD
Sample : M4833-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

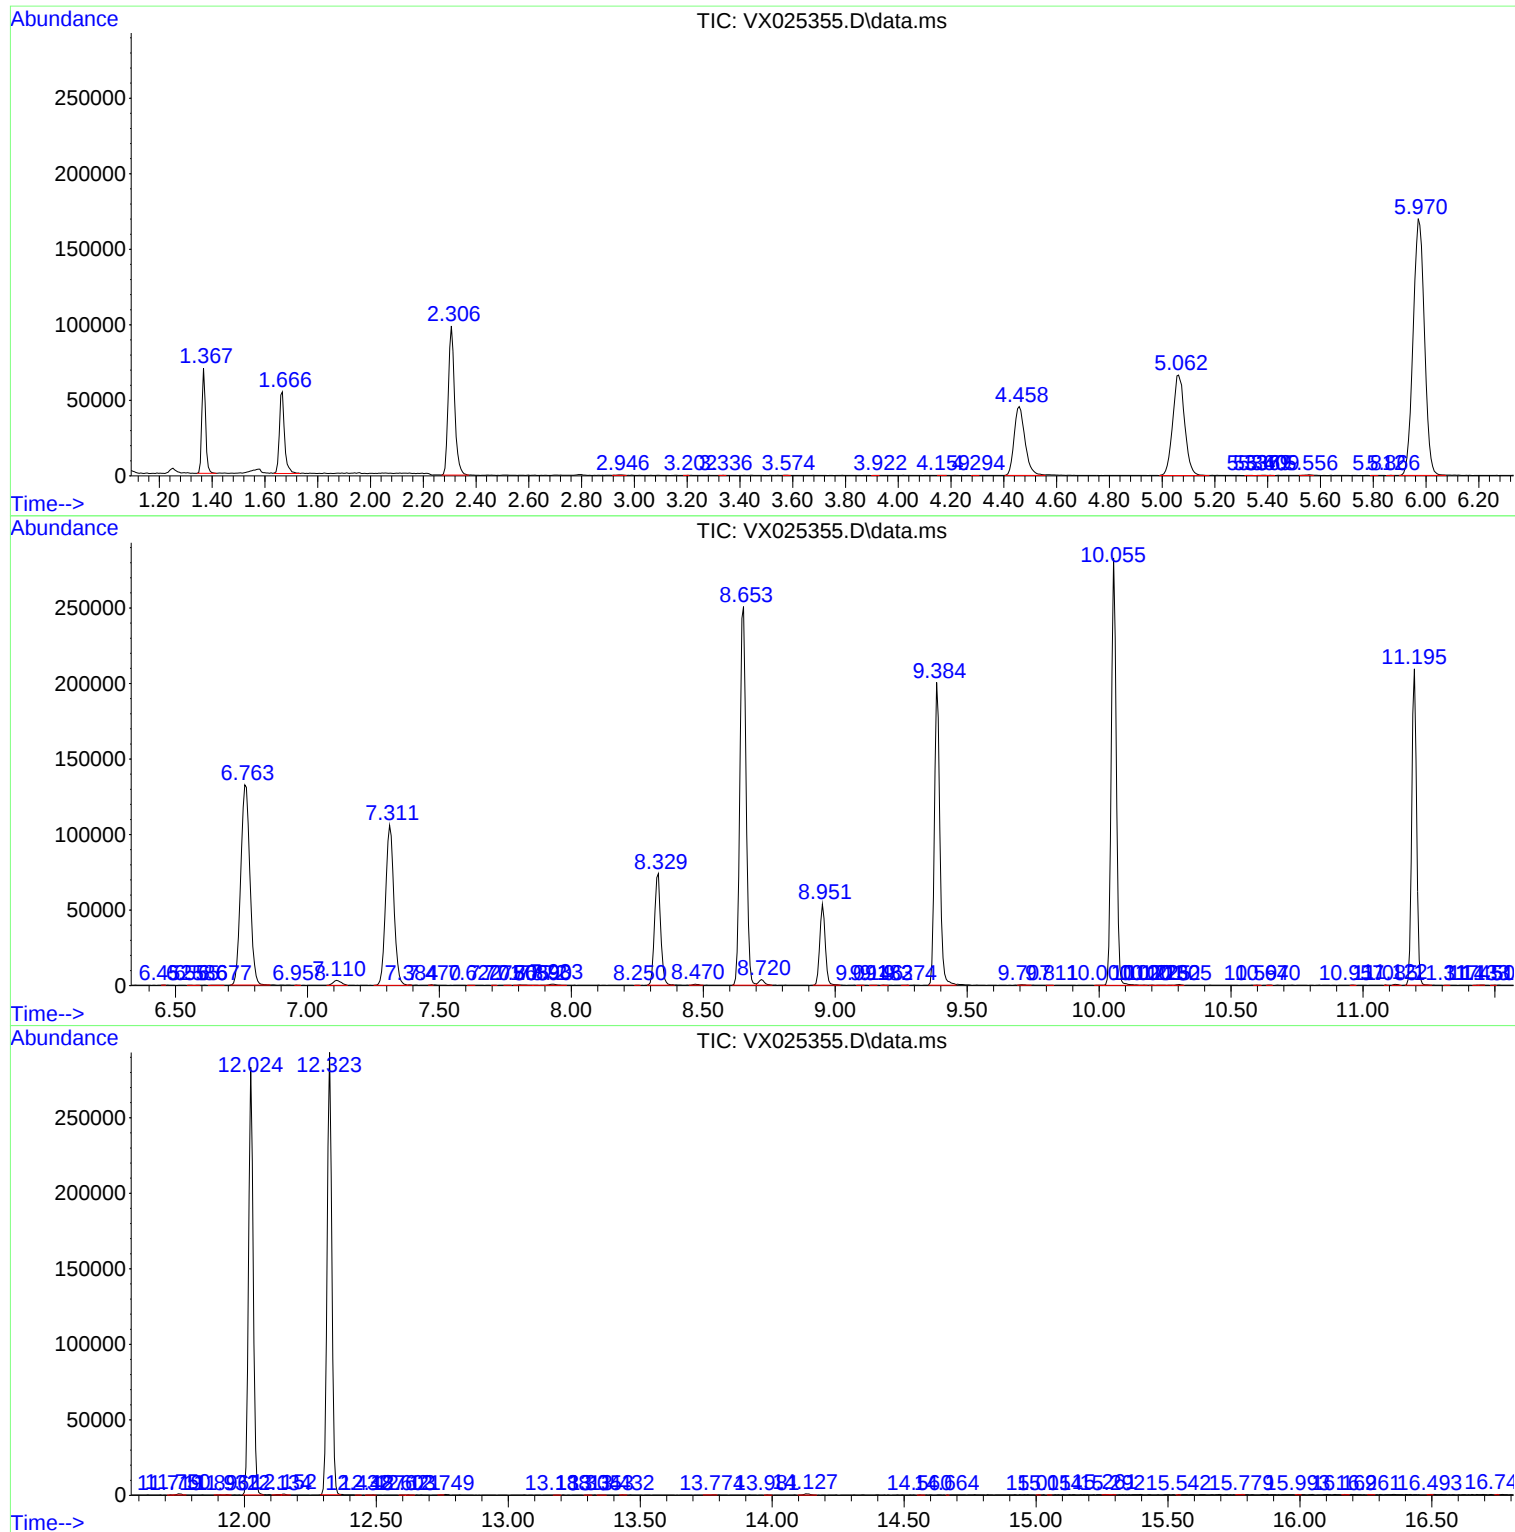

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
Data File : VX025355.D
Acq On : 26 Nov 2021 14:57
Operator : JC/MD
Sample : M4833-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
Data File : VX025355.D
Acq On : 26 Nov 2021 14:57
Operator : JC/MD
Sample : M4833-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc