
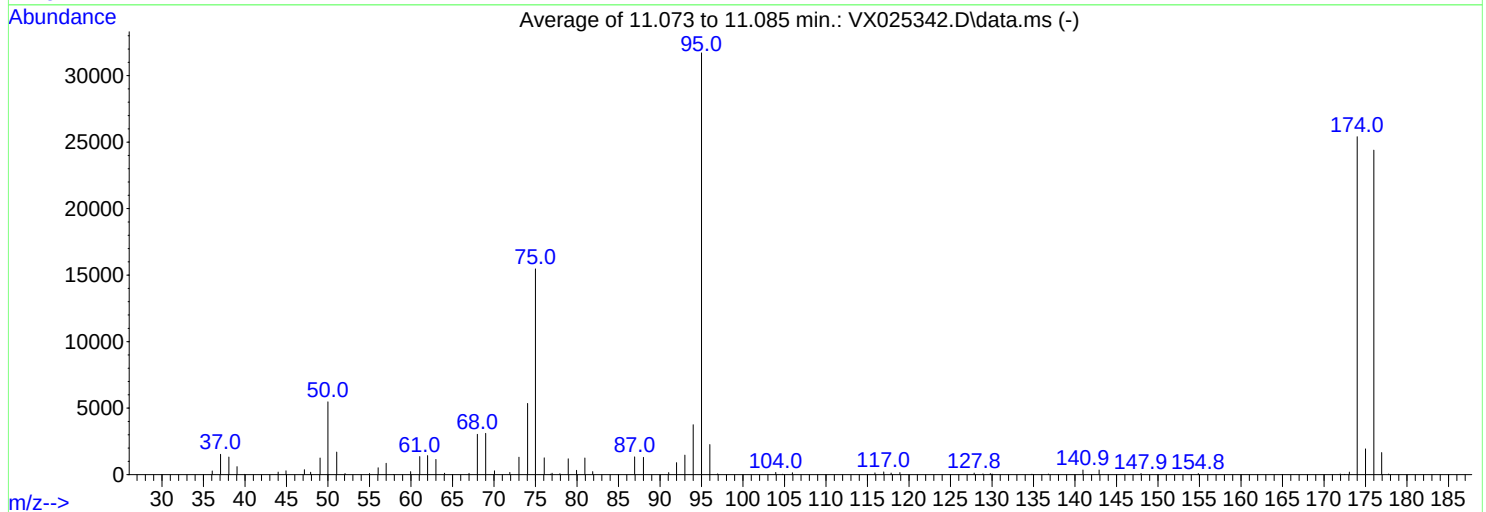


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112621\
 Data File : VX025342.D
 Acq On : 26 Nov 2021 09:10
 Operator : JC/MD
 Sample : BFB618
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB618

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis
 Last Update : Fri Nov 26 23:56:11 2021

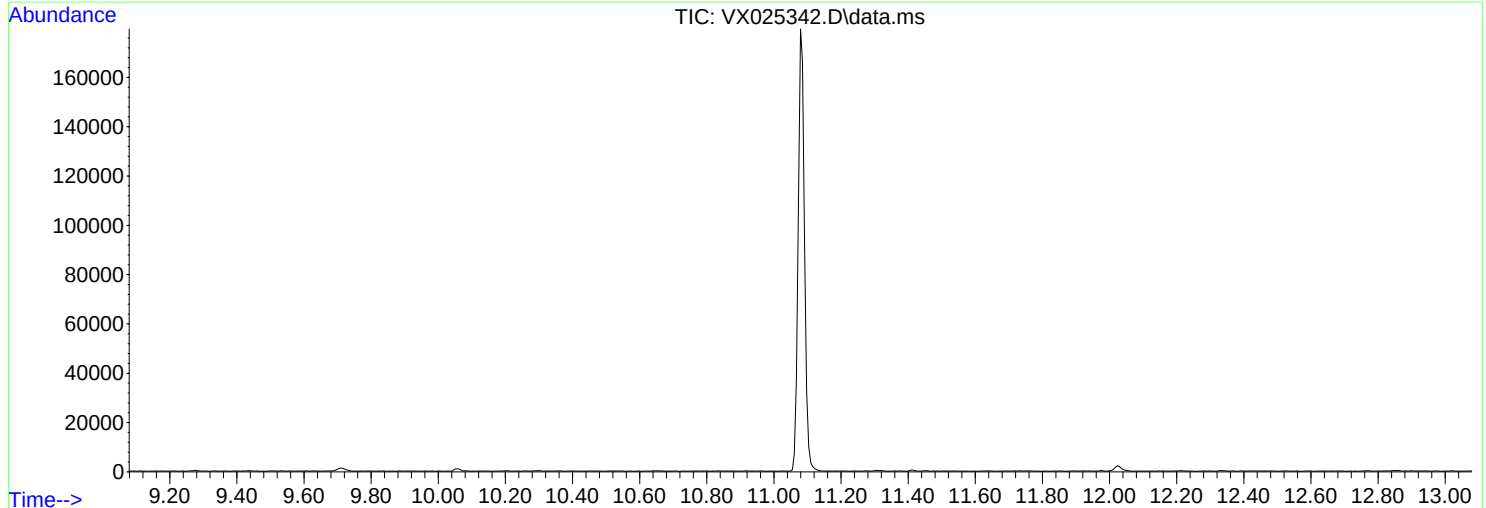

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	5470	PASS
75	95	30	80	48.8	15470	PASS
95	95	100	100	100.0	31712	PASS
96	95	5	9	7.1	2263	PASS
173	174	0.00	2	0.8	199	PASS
174	95	50	120	80.1	25410	PASS
175	174	5	9	7.6	1942	PASS
176	174	95	101	96.0	24399	PASS
177	176	5	9	6.8	1665	PASS

m/z	Abundance
36.10	299.0
37.10	1577.0
38.10	1330.0
39.10	509.0
40.00	222.0
44.00	385.0
45.00	275.0
47.20	370.0
47.80	158.0
49.00	1318.0
50.00	5560.0
51.10	1589.0
52.00	79.0
55.00	73.0
56.10	430.0
57.00	874.0
59.90	170.0
61.00	1284.0
62.00	1484.0
63.00	1304.0
64.00	103.0
67.00	82.0
68.00	3134.0
69.00	3233.0
70.00	317.0
71.90	186.0
73.00	1384.0
74.00	5565.0
75.00	16103.0
76.00	1182.0
77.00	151.0
77.90	80.0
78.90	1351.0
80.00	302.0
80.90	1398.0
81.90	269.0
87.00	1356.0
88.00	1325.0
91.00	205.0
92.00	935.0
93.00	1560.0
94.00	4161.0
95.00	33480.0
96.00	2460.0
96.90	61.0
104.00	166.0
104.80	55.0
106.00	158.0
115.90	152.0
117.00	208.0
117.90	155.0
119.00	165.0
127.90	128.0
128.80	74.0
130.00	138.0
134.80	60.0
136.80	78.0
140.90	389.0
142.90	361.0
148.00	147.0
154.90	88.0
172.00	66.0
173.00	221.0
174.00	30832.0
175.00	2223.0
176.00	28888.0
177.00	2032.0
177.80	75.0

Instrument :
MSVOA_X
ClientSampleId :
BFB618

m/z	Abundance
39.90	197.0
44.00	155.0

Instrument :
MSVOA_X
ClientSampleId :
BFB618

m/z	Abundance
36.10	161.0
37.00	1305.0
38.10	1121.0
39.00	607.0
40.00	221.0
44.00	300.0
45.00	269.0
47.10	300.0
48.10	120.0
49.10	961.0
50.00	4584.0
51.00	1318.0
52.00	82.0
55.00	61.0
56.00	476.0
57.00	655.0
59.90	211.0
61.00	1117.0
62.00	1040.0
63.00	793.0
64.10	98.0
67.00	60.0
68.00	2328.0
69.00	2642.0
70.10	238.0
71.90	149.0
73.00	1057.0
74.00	4109.0
75.00	11834.0
76.10	1083.0
76.80	121.0
79.00	904.0
80.00	262.0
80.90	929.0
82.00	181.0
86.90	1353.0
88.00	915.0
91.10	79.0
92.00	690.0
93.00	1142.0
94.00	2890.0
95.00	23744.0
96.00	1722.0
97.00	51.0
104.00	150.0
105.90	132.0
115.90	86.0
116.90	192.0
117.80	55.0
118.80	108.0
127.90	95.0
129.00	52.0
129.80	95.0
140.90	238.0
142.90	252.0
154.80	52.0
172.50	84.0
173.10	108.0
174.00	15765.0
175.00	1152.0
176.00	15164.0
176.90	940.0

Instrument :
MSVOA_X
ClientSampleId :
BFB618

m/z	Abundance
36.00	378.0
37.00	1715.0
38.00	1527.0
39.00	674.0
40.10	235.0
44.00	373.0
44.90	321.0
47.10	451.0
47.90	250.0
49.10	1491.0
50.00	6267.0
51.10	2178.0
52.10	103.0
55.00	138.0
56.10	655.0
57.00	1051.0
57.90	58.0
60.00	320.0
61.10	1695.0
62.00	1777.0
63.00	1320.0
64.10	141.0
67.00	139.0
68.00	3640.0
69.00	3437.0
70.10	318.0
71.90	163.0
73.00	1480.0
74.10	6402.0
75.00	18472.0
76.00	1519.0
77.00	177.0
78.00	158.0
78.90	1332.0
79.90	410.0
81.00	1431.0
81.80	254.0
86.90	1309.0
88.00	1652.0
91.00	184.0
92.00	1086.0
93.00	1702.0
94.00	4221.0
95.00	37912.0
96.00	2606.0
97.00	61.0
103.80	178.0
104.80	70.0
105.90	142.0
115.90	146.0
116.90	220.0
117.90	161.0
118.90	193.0
127.80	128.0
128.90	74.0
129.80	157.0
134.80	69.0
136.80	78.0
141.00	431.0
142.90	424.0
146.00	72.0
147.90	105.0
154.90	127.0
171.90	78.0
173.00	267.0
174.00	29632.0
175.00	2450.0
176.00	29144.0
177.00	2022.0
177.80	57.0

Instrument :
MSVOA_X
ClientSampleId :
BFB618