

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112624\
Data File : VX044011.D
Acq On : 26 Nov 2024 12:55
Operator : JC/MD
Sample : P4846-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-EVAL-01S-20241113

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Title : SW846 8260

Signal : TIC: VX044011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.605	68	85	86	rBV3	16521	62675	6.59%	1.347%
2	5.379	691	704	721	rBV2	82829	249072	26.19%	5.353%
3	5.544	721	731	744	rBV	124682	360643	37.92%	7.751%
4	5.952	786	798	812	rBV2	98152	269544	28.34%	5.793%
5	6.757	919	930	945	rBV	213982	520968	54.77%	11.197%
6	7.123	980	990	1007	rBV	424434	951129	100.00%	20.442%
7	8.647	1233	1240	1255	rBV	438881	701440	73.75%	15.076%
8	10.049	1465	1470	1481	rBV	421385	602555	63.35%	12.950%
9	11.079	1634	1639	1650	rBV	327395	426884	44.88%	9.175%
10	12.018	1788	1793	1805	rBV	399072	507848	53.39%	10.915%




Sum of corrected areas: 4652758

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112624\
Data File : VX044011.D
Acq On : 26 Nov 2024 12:55
Operator : JC/MD
Sample : P4846-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-EVAL-01S-20241113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

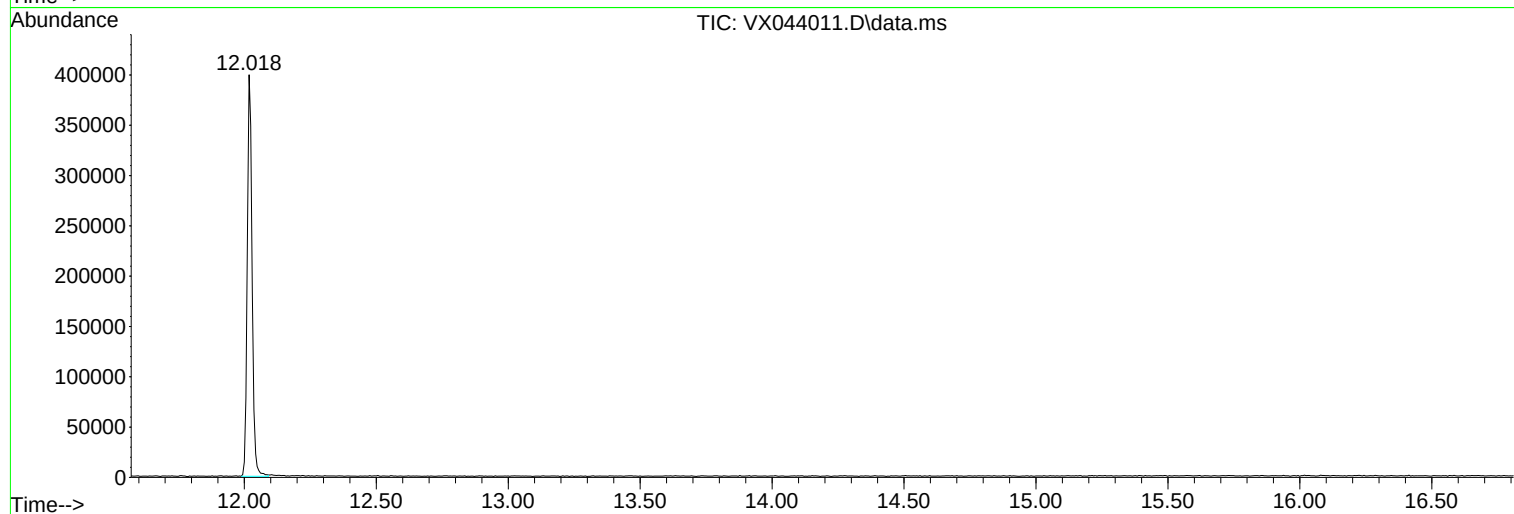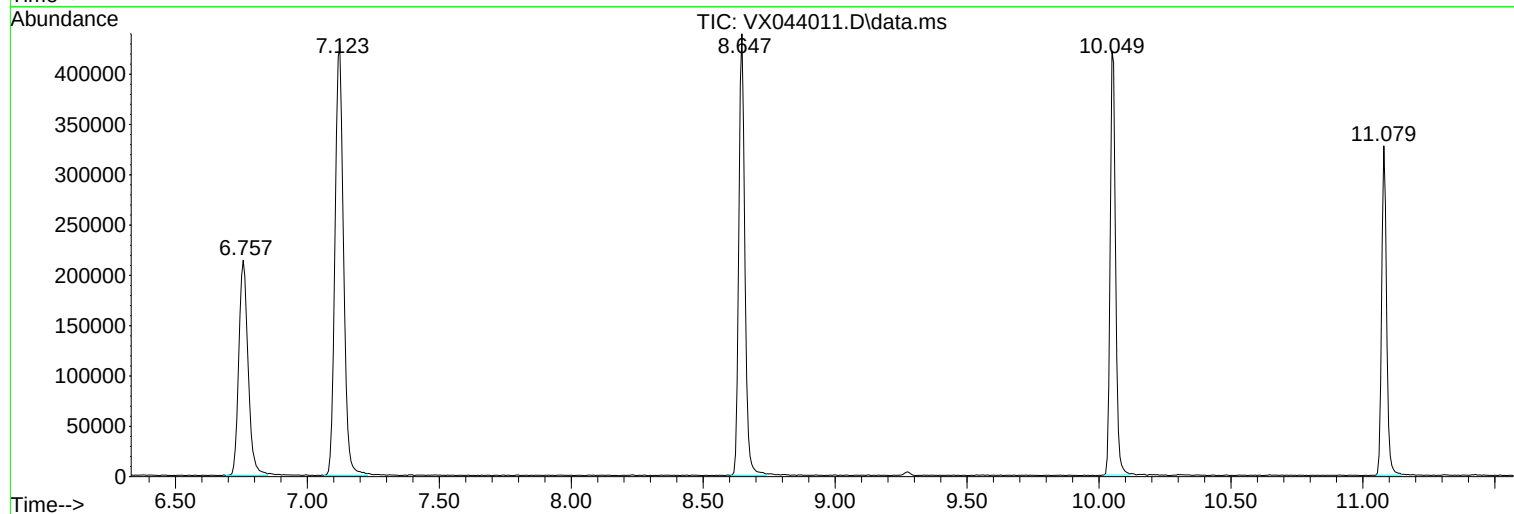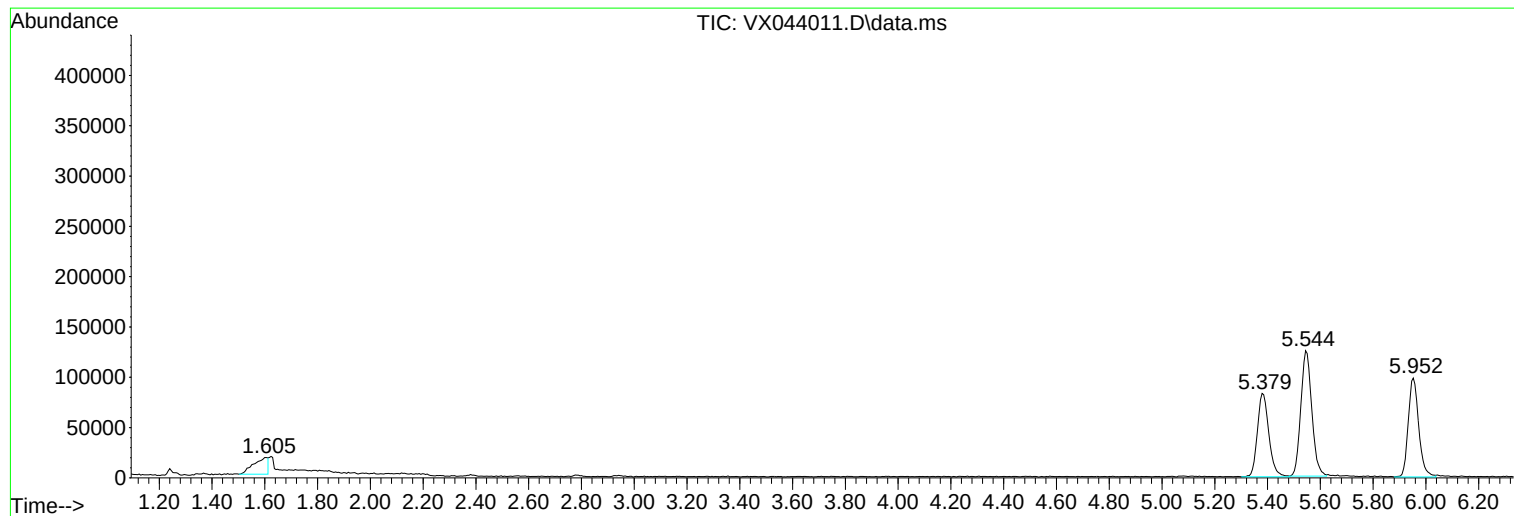

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112624\
Data File : VX044011.D
Acq On : 26 Nov 2024 12:55
Operator : JC/MD
Sample : P4846-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-EVAL-01S-20241113










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.605 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.605	8.69 ug/l	62675	Pentafluorobenzene	5.544

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2	-	[2-(2-Chloro-ethoxy)-ethoxy]-p...	216	C10H13ClO3	1000317-46-1	16
2	Propanoic acid, 2-chloro-, methy...	122	C4H7ClO2	073246-45-4	9		
3	Benzeneethanamine, 2-fluoro-.bet...	185	C9H12FN02	103439-07-2	9		
4	Ethyl hydrogen oxalate	118	C4H6O4	000617-37-8	9		
5	Topotecan	421	C23H23N3O5	1000131-70-7	9		

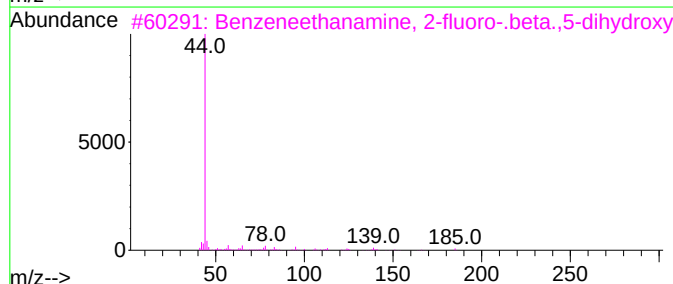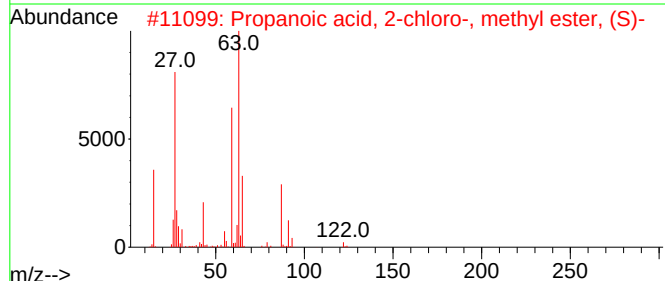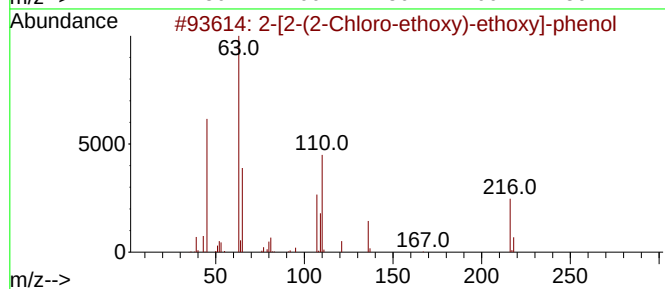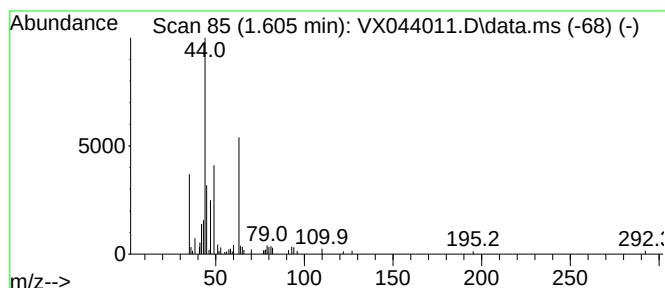

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112624\
Data File : VX044011.D
Acq On : 26 Nov 2024 12:55
Operator : JC/MD
Sample : P4846-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-MW-EVAL-01S-20241113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.605	1.605	8.7	ug/l	62675	1	5.544	360643	50.0