


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX112719\
Data File : VX013640.D
Acq On : 27 Nov 2019 09:15
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
Title : SW846 8260
Last Update : Tue Nov 26 15:53:00 2019

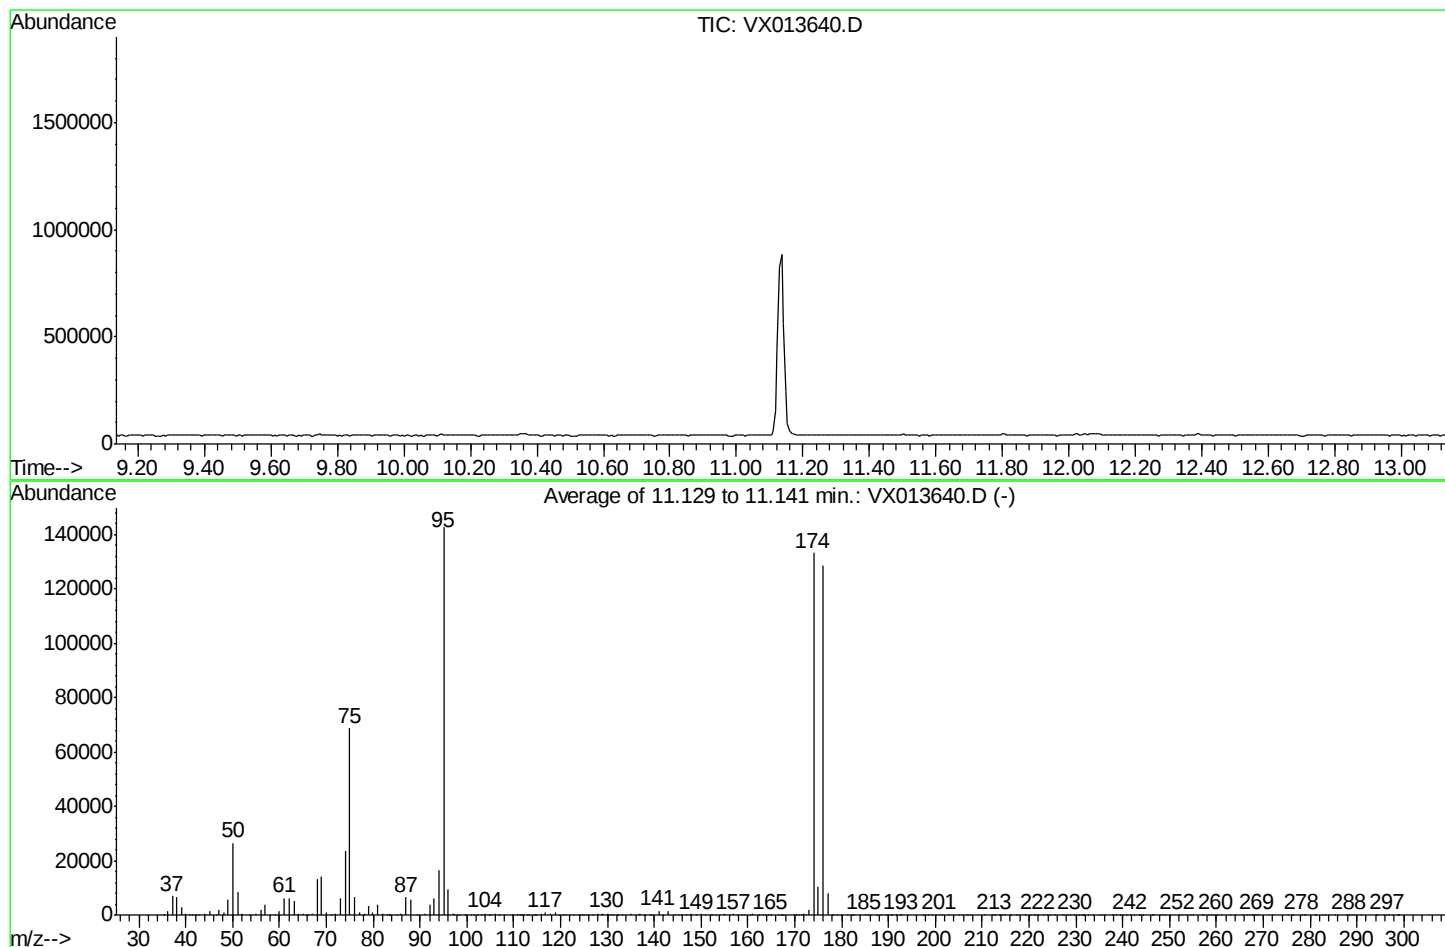

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	26462	PASS
75	95	30	60	48.1	68624	PASS
95	95	100	100	100.0	142530	PASS
96	95	5	9	6.5	9335	PASS
173	174	0.00	2	1.3	1708	PASS
174	95	50	100	93.3	133018	PASS
175	174	5	9	7.7	10242	PASS
176	174	95	101	96.8	128728	PASS
177	176	5	9	6.4	8230	PASS