


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX112719\
 Data File : VX013666.D
 Acq On : 27 Nov 2019 21:17
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
 Title : SW846 8260
 Last Update : Tue Nov 26 15:53:00 2019

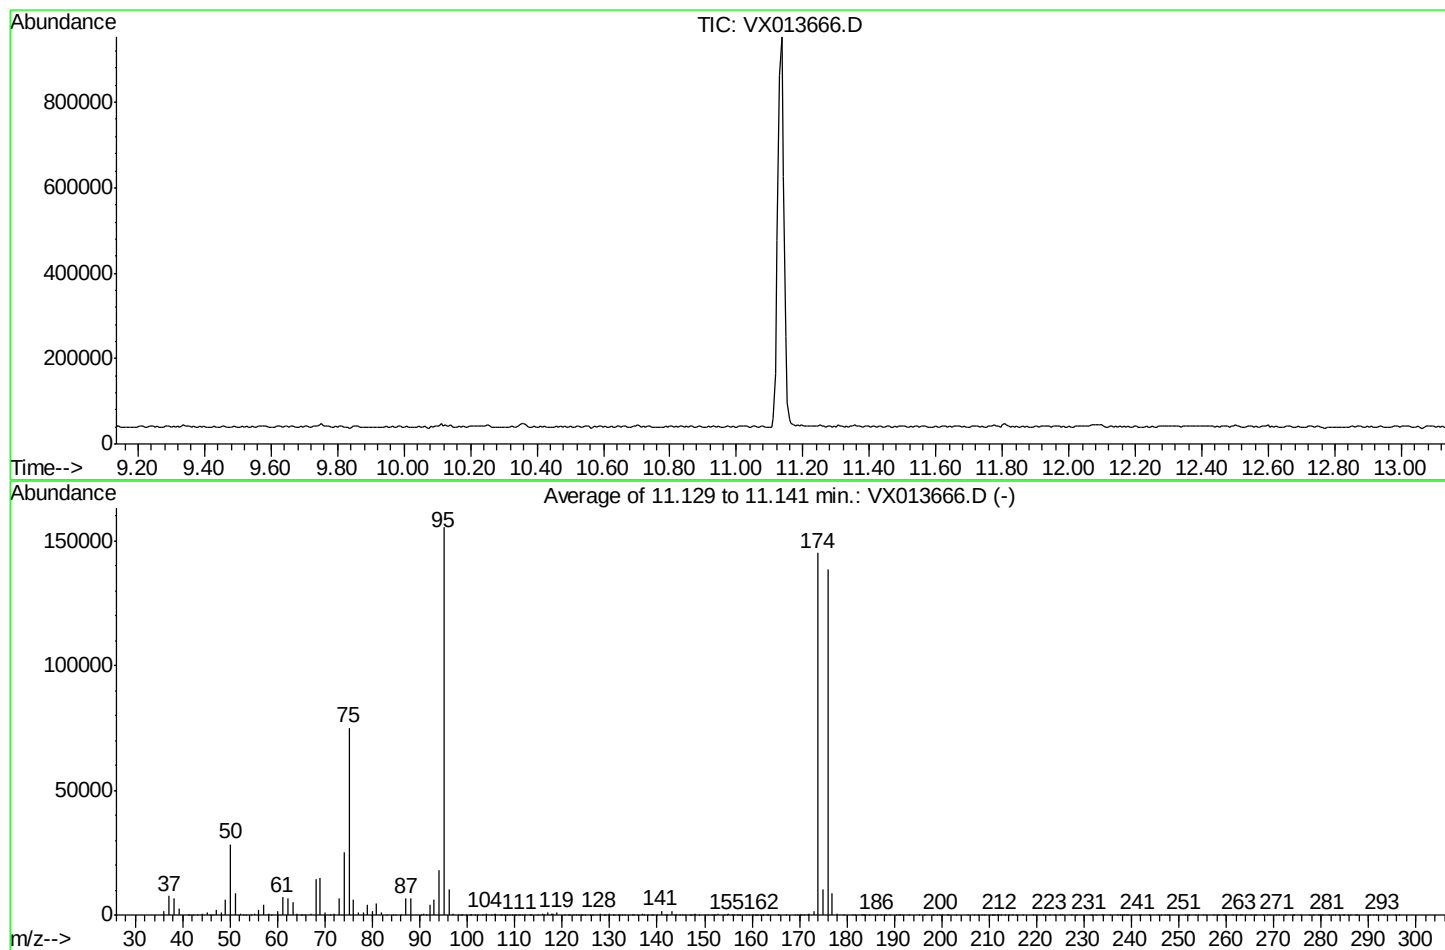

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	28394	PASS
75	95	30	60	48.2	74963	PASS
95	95	100	100	100.0	155465	PASS
96	95	5	9	6.6	10251	PASS
173	174	0.00	2	1.0	1515	PASS
174	95	50	100	93.4	145210	PASS
175	174	5	9	7.1	10262	PASS
176	174	95	101	95.5	138657	PASS
177	176	5	9	6.5	8988	PASS