
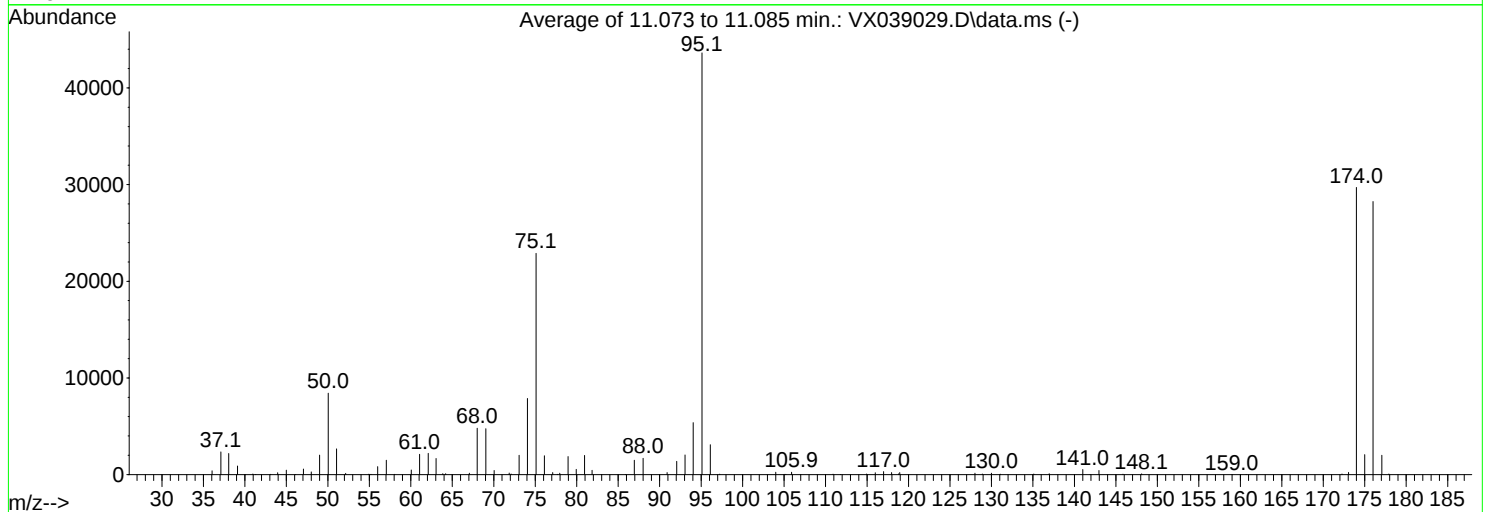


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112723\
Data File : VX039029.D
Acq On : 27 Nov 2023 09:52
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X112423W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Mon Nov 27 03:22:25 2023

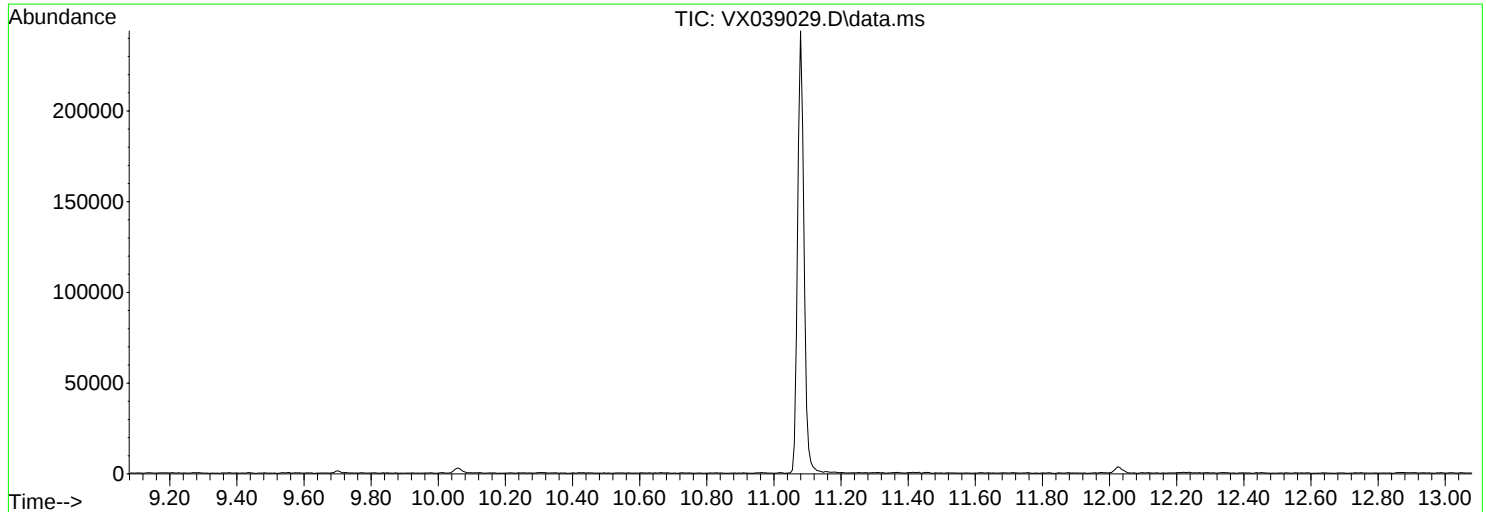

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	8419	PASS
75	95	30	60	52.5	22896	PASS
95	95	100	100	100.0	43627	PASS
96	95	5	9	7.1	3093	PASS
173	174	0.00	2	0.8	225	PASS
174	95	50	100	68.1	29701	PASS
175	174	5	9	7.0	2070	PASS
176	174	95	101	95.1	28253	PASS
177	176	5	9	7.1	2006	PASS