

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112724\
 Data File : VX044033.D
 Acq On : 27 Nov 2024 12:22
 Operator : JC/MD
 Sample : P5001-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 28 00:44:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 22 03:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	121169	50.000	ug/l	0.01
34) 1,4-Difluorobenzene	6.757	114	227299	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	203619	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	98952	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	102751	49.441	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	98.880%		
35) Dibromofluoromethane	5.385	113	51191	31.518	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	63.040%#		
50) Toluene-d8	8.647	98	280952	50.182	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	100.360%		
62) 4-Bromofluorobenzene	11.079	95	99073	51.996	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	104.000%		
Target Compounds						Qvalue
5) Bromomethane	1.599	94	219	0.207	ug/l #	56
6) Chloroethane	1.623	64	329	0.314	ug/l #	67
11) Tert butyl alcohol	3.001	59	526	1.577	ug/l #	73
16) Acetone	2.386	43	9871	10.341	ug/l	96
18) Methyl Acetate	2.703	43	1166	0.525	ug/l	100
20) Methylene Chloride	2.782	84	1077	0.665	ug/l #	79
25) 2-Butanone	4.605	43	1804	1.465	ug/l	90
27) cis-1,2-Dichloroethene	4.483	96	1948	1.093	ug/l	97
31) Cyclohexane	5.543	56	3354	1.448	ug/l #	44
36) 1,1-Dichloropropene	5.543	75	11603	5.733	ug/l #	44
38) Carbon Tetrachloride	5.537	117	13994	6.154	ug/l #	16
40) Benzene	6.031	78	64688	10.261	ug/l	98
49) 1,4-Dioxane	7.476	88	21	0.614	ug/l #	30
51) 4-Methyl-2-Pentanone	8.580	43	974	0.399	ug/l	92
52) Toluene	8.714	92	157506	41.742	ug/l	100
53) t-1,3-Dichloropropene	8.720	75	2026	0.907	ug/l #	1
67) Ethyl Benzene	10.189	91	964297	127.251	ug/l	98
68) m/p-Xylenes	10.299	106	176821	62.570	ug/l	97
69) o-Xylene	10.640	106	120204	43.565	ug/l	96
70) Styrene	10.640	104	9939	2.178	ug/l #	1
73) Isopropylbenzene	10.963	105	46801	6.153	ug/l	98
76) 1,2,3-Trichloropropane	11.378	75	3700	1.705	ug/l #	1
78) n-propylbenzene	11.305	91	10673	1.256	ug/l #	53
79) 2-Chlorotoluene	11.378	91	44504	8.285	ug/l #	44
80) 1,3,5-Trimethylbenzene	11.451	105	44141	7.054	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	56785	71.407	ug/l #	7
82) 4-Chlorotoluene	11.451	91	5040	0.831	ug/l #	46
83) tert-Butylbenzene	11.750	119	18805	3.032	ug/l #	42
84) 1,2,4-Trimethylbenzene	11.750	105	157988	25.358	ug/l	100
85) sec-Butylbenzene	11.750	105	157988	20.789	ug/l #	57
86) p-Isopropyltoluene	12.006	119	6789	1.100	ug/l #	74
89) n-Butylbenzene	12.237	91	310843	57.114	ug/l #	44
92) 1,2-Dibromo-3-Chloropr...	12.926	75	163	0.312	ug/l #	4
95) Naphthalene	13.780	128	12832701	1813.064	ug/l #	90

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112724\
Data File : VX044033.D
Acq On : 27 Nov 2024 12:22
Operator : JC/MD
Sample : P5001-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 28 00:44:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 22 03:45:52 2024
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112724\
Data File : VX044033.D
Acq On : 27 Nov 2024 12:22
Operator : JC/MD
Sample : P5001-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Nov 28 00:44:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 22 03:45:52 2024
Response via : Initial Calibration

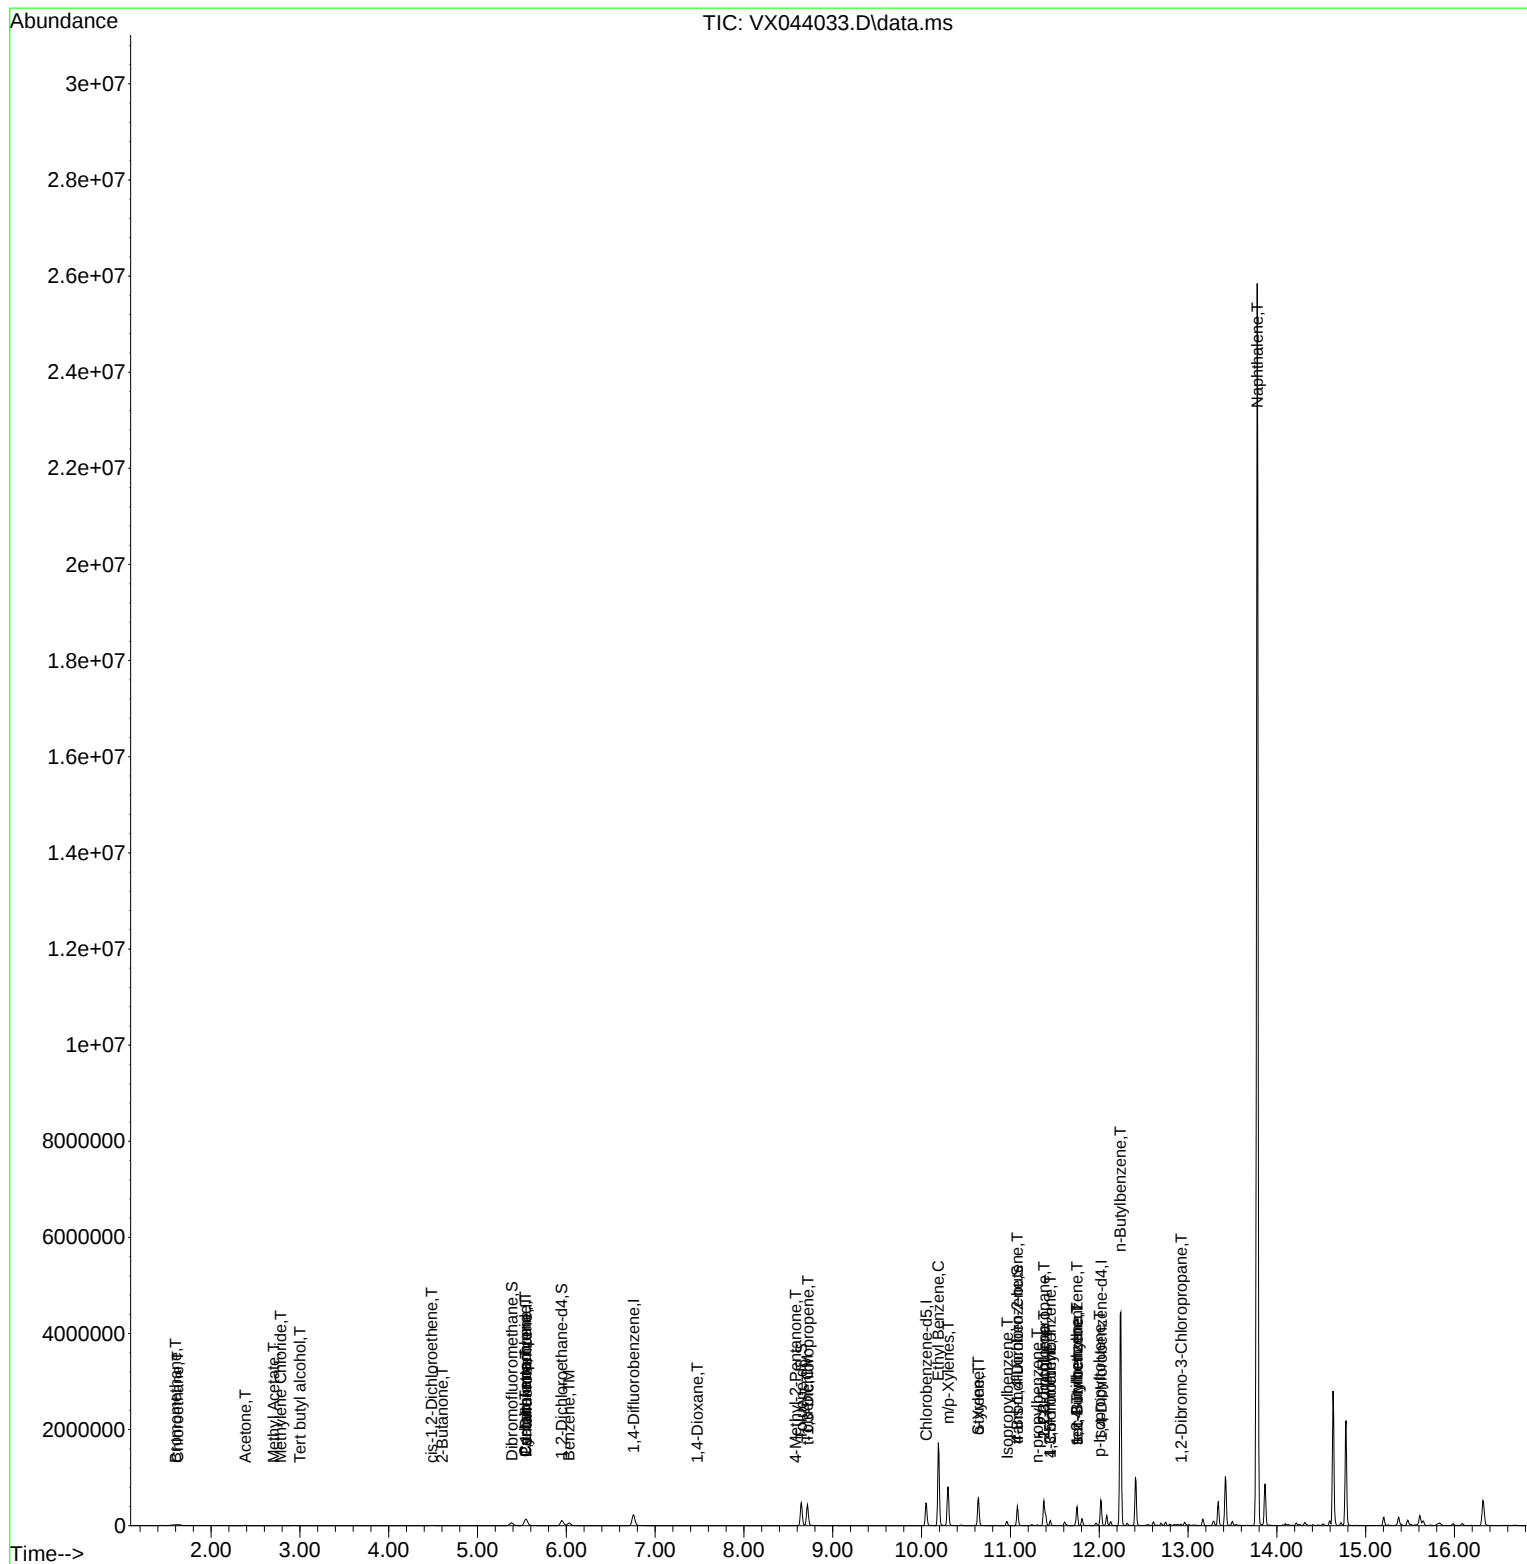






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.012 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:168 Resp: 121169
Ion Ratio Lower Upper
168 100
99 61.4 51.8 77.8



#5
Bromomethane
Concen: 0.207 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.006 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22


Tgt Ion: 94 Resp: 219
Ion Ratio Lower Upper
94 100
96 50.8 73.9 110.9#

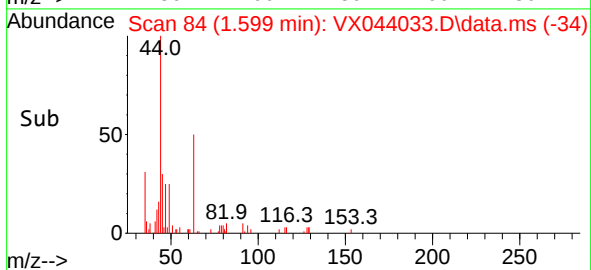



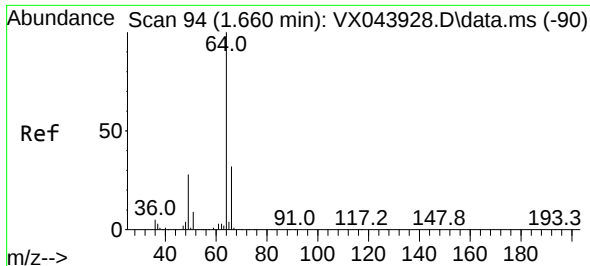


#6
Chloroethane
Concen: 0.314 ug/l
RT: 1.623 min Scan# 81
Delta R.T. -0.037 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22

Instrument :
MSVOA_X
ClientSampleId :



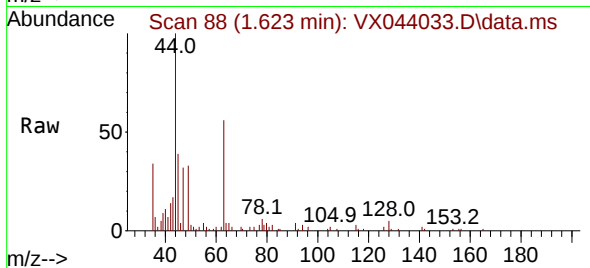



Tgt Ion: 64 Resp: 329
Ion Ratio Lower Upper
64 100
66 14.1 25.9 38.9#

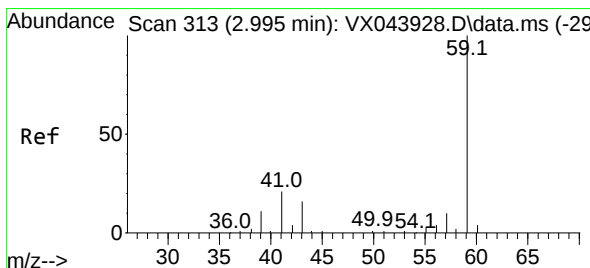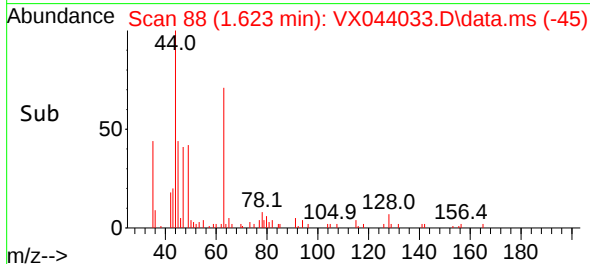

#11
Tert butyl alcohol
Concen: 1.577 ug/l
RT: 3.001 min Scan# 314
Delta R.T. 0.006 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22

Tgt Ion: 59 Resp: 526
Ion Ratio Lower Upper
59 100
57 0.0 7.9 11.9#


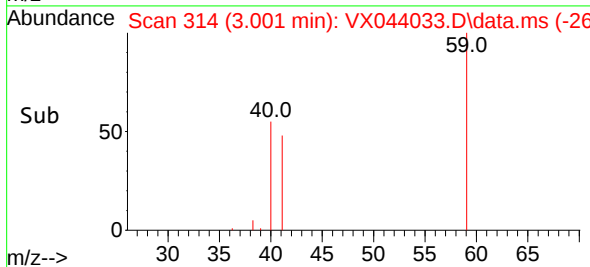

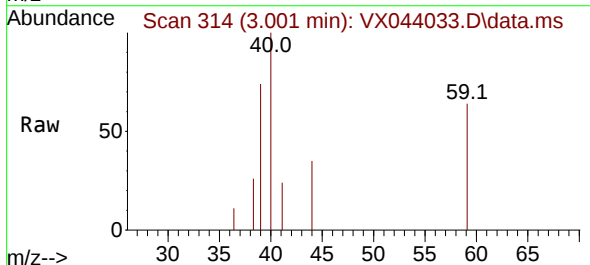




#16
Acetone
Concen: 10.341 ug/l
RT: 2.386 min Scan# 212
Delta R.T. 0.006 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 9871
Ion Ratio Lower Upper
43 100
58 30.6 22.7 34.1

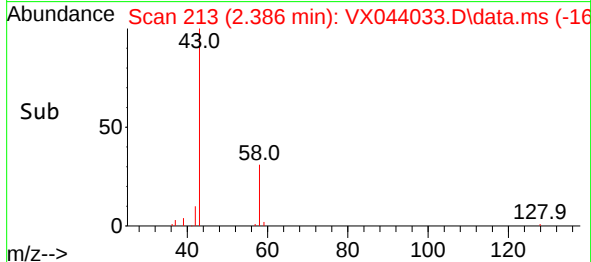

#18
Methyl Acetate
Concen: 0.525 ug/l
RT: 2.703 min Scan# 265
Delta R.T. -0.000 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22


Tgt Ion: 43 Resp: 1166
Ion Ratio Lower Upper
43 100
74 23.6 18.9 28.3

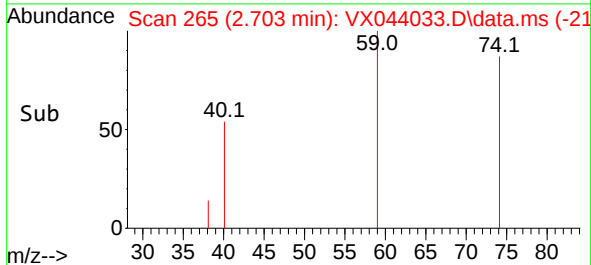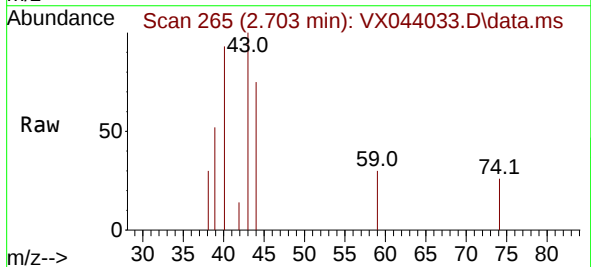






#20
Methylene Chloride
Concen: 0.665 ug/l
RT: 2.782 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:	84	Resp:	1077
Ion	Ratio	Lower	Upper
84	100		
49	102.9	102.7	154.1
51	30.3	31.7	47.5#
86	49.9	53.9	80.9#

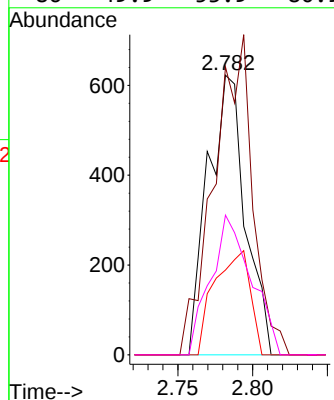

#25
2-Butanone
Concen: 1.465 ug/l
RT: 4.605 min Scan# 577
Delta R.T. 0.048 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22

Tgt Ion:	43	Resp:	1804
Ion	Ratio	Lower	Upper
43	100		
72	20.4	20.2	30.2

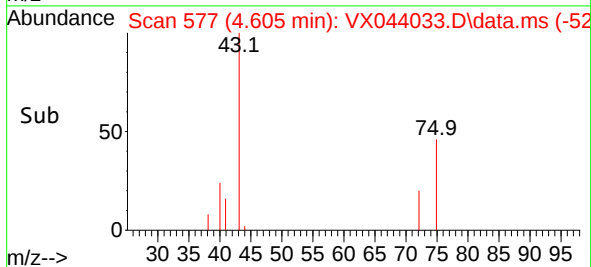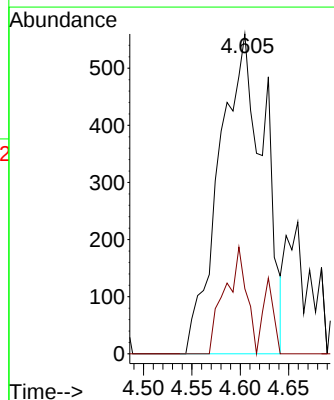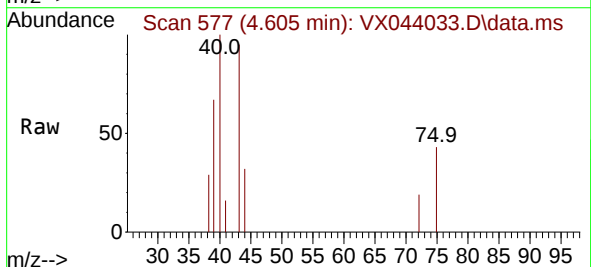



#27

cis-1,2-Dichloroethene

Concen: 1.093 ug/l

RT: 4.483 min Scan# 51

Delta R.T. 0.006 min


Lab File: VX044033.D

Acq: 27 Nov 2024 12:22

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 96 Resp: 1948

Ion Ratio Lower Upper

96 100

61 142.9 0.0 297.4

98 64.2 0.0 127.8



#31

Cyclohexane

Concen: 1.448 ug/l

RT: 5.543 min Scan# 731

Delta R.T. 0.085 min

Lab File: VX044033.D

Acq: 27 Nov 2024 12:22




Tgt Ion: 56 Resp: 3354


Ion Ratio Lower Upper

56 100

69 119.7 24.7 37.1#

84 102.2 68.7 103.1

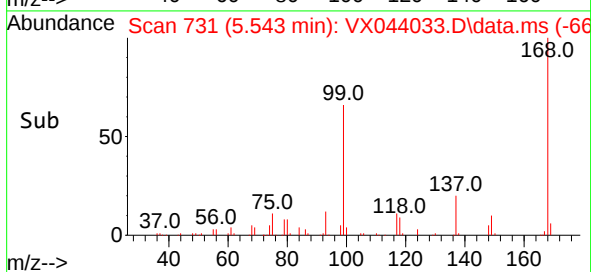



#33

1,2-Dichloroethane-d4

Concen: 49.441 ug/l

RT: 5.946 min Scan# 797

Delta R.T. -0.000 min

Lab File: VX044033.D

Acq: 27 Nov 2024 12:22

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 102751

Ion Ratio Lower Upper

65 100

67 49.4 0.0 100.8



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX044033.D

Acq: 27 Nov 2024 12:22




Tgt Ion: 114 Resp: 227299


Ion Ratio Lower Upper

114 100

63 21.3 0.0 44.0

88 15.8 0.0 32.4


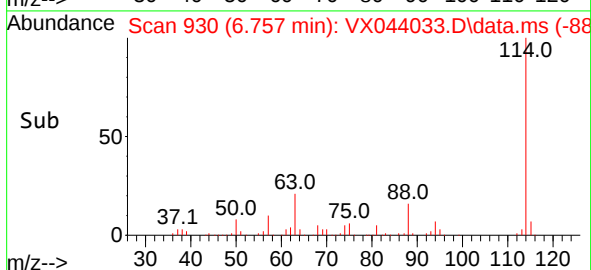






#35
Dibromofluoromethane
Concen: 31.518 ug/l
RT: 5.385 min Scan# 704
Delta R.T. 0.006 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:113 Resp: 51191
Ion Ratio Lower Upper
113 100
111 101.6 81.0 121.4
192 16.6 13.0 19.6

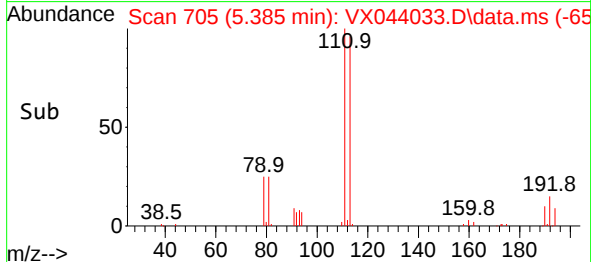

#36
1,1-Dichloropropene
Concen: 5.733 ug/l
RT: 5.543 min Scan# 731
Delta R.T. -0.134 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22


Tgt Ion: 75 Resp: 11603
Ion Ratio Lower Upper
75 100
110 3.3 17.4 52.2#
77 0.0 25.8 38.8#

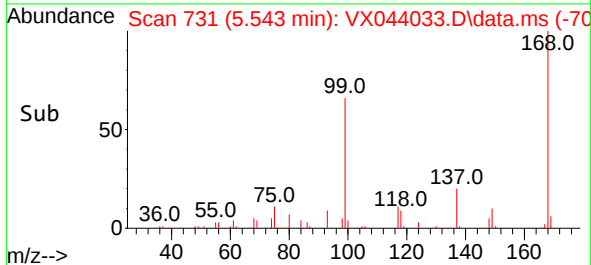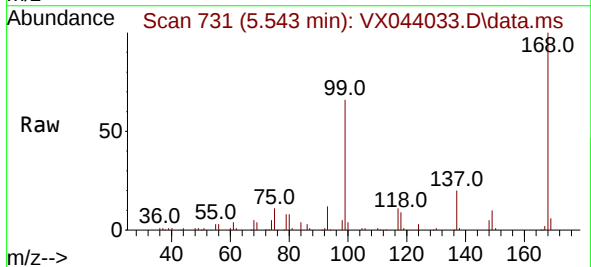






#38
Carbon Tetrachloride
Concen: 6.154 ug/l
RT: 5.537 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 13994
Ion Ratio Lower Upper
117 100
119 4.6 75.2 112.8#
121 0.0 24.5 36.7#



#40
Benzene
Concen: 10.261 ug/l
RT: 6.031 min Scan# 811
Delta R.T. 0.006 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22

Tgt Ion: 78 Resp: 64688
Ion Ratio Lower Upper
78 100
77 25.2 19.2 28.8

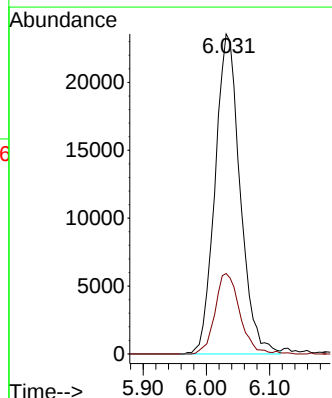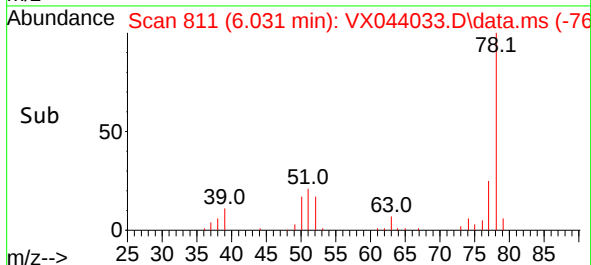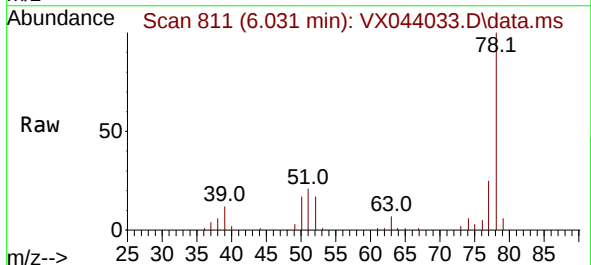

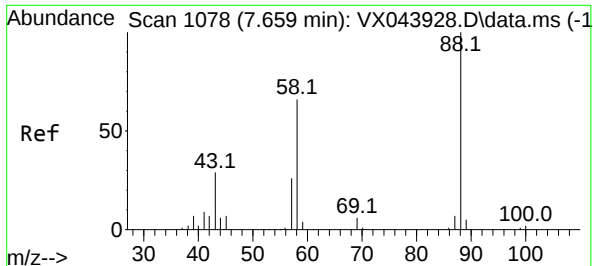

#49

1,4-Dioxane

Concen: 0.614 ug/l

RT: 7.476 min Scan# 1048

Delta R.T. -0.183 min

Lab File: VX044033.D

Acq: 27 Nov 2024 12:22

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 88 Resp: 21

Ion Ratio Lower Upper

88 100

43 0.0 26.8 40.2#

58 0.0 45.4 68.2#

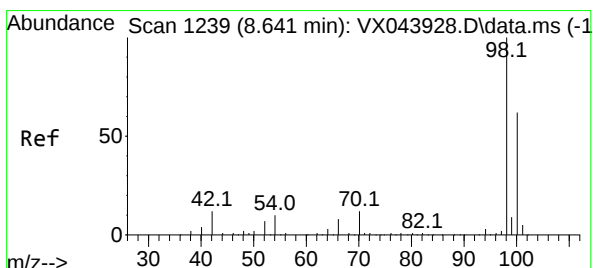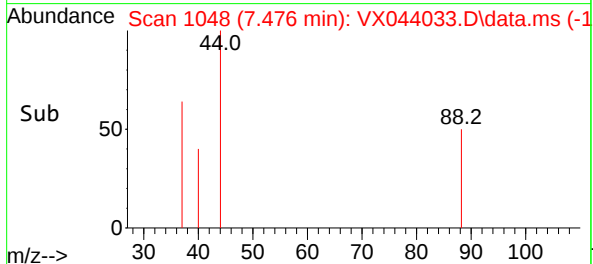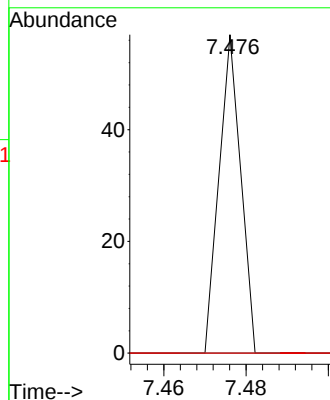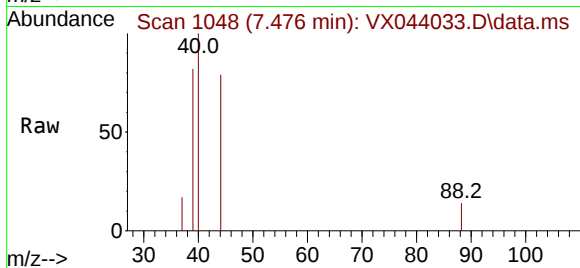

#50

Toluene-d8

Concen: 50.182 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.006 min

Lab File: VX044033.D




Acq: 27 Nov 2024 12:22


Tgt Ion: 98 Resp: 280952

Ion Ratio Lower Upper

98 100

100 65.0 52.6 79.0


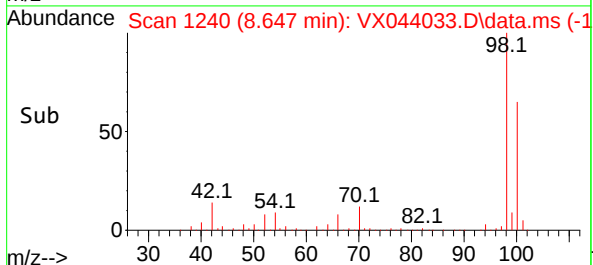
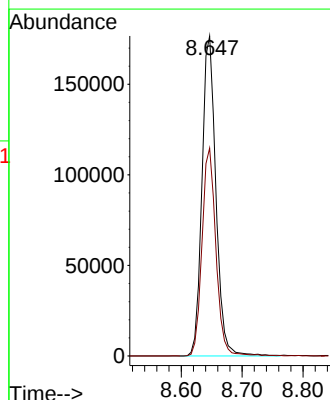
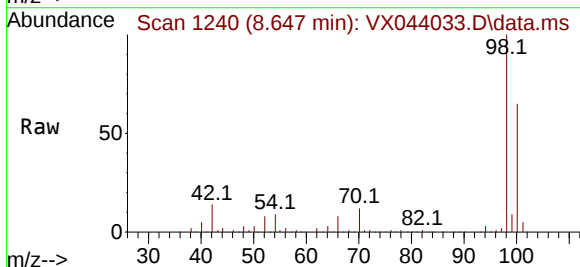


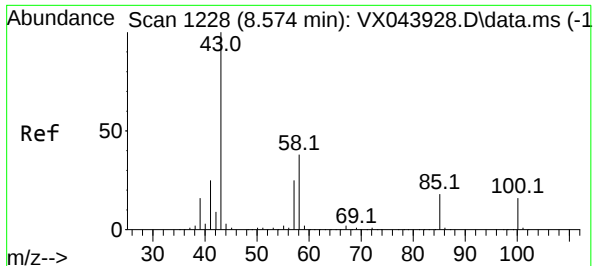

#51
4-Methyl-2-Pentanone
Concen: 0.399 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. 0.006 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 974
Ion Ratio Lower Upper
43 100
58 32.5 30.0 45.0

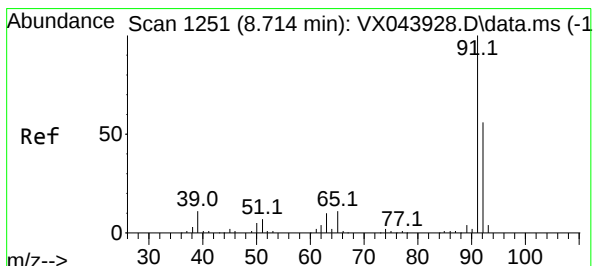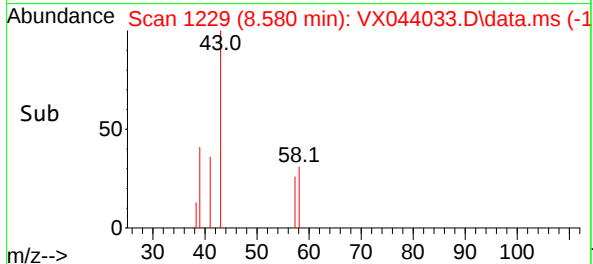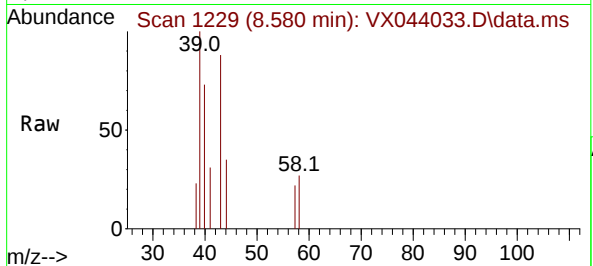

#52
Toluene
Concen: 41.742 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.000 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22

Tgt Ion: 92 Resp: 157506
Ion Ratio Lower Upper
92 100
91 175.0 139.7 209.5


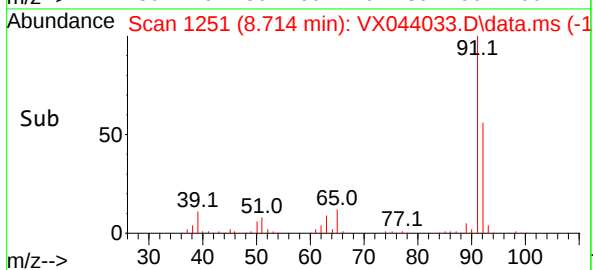

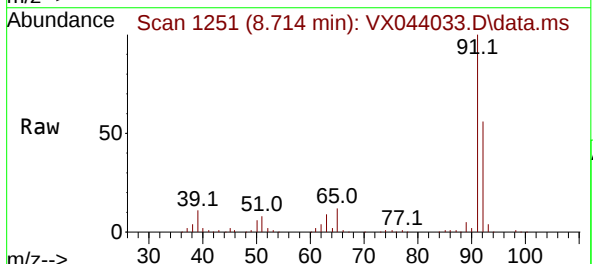




#53
t-1,3-Dichloropropene
Concen: 0.907 ug/l
RT: 8.720 min Scan# 11
Delta R.T. -0.256 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 2026
Ion Ratio Lower Upper
75 100
77 147.8 25.1 37.7#

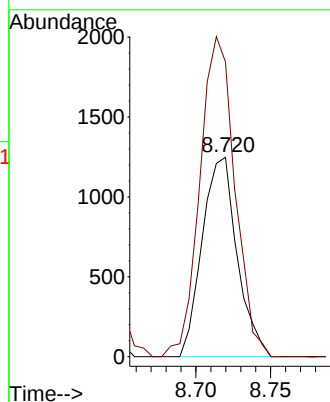

#62
4-Bromofluorobenzene
Concen: 51.996 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22


Tgt Ion: 95 Resp: 99073
Ion Ratio Lower Upper
95 100
174 73.6 0.0 150.4
176 72.6 0.0 146.0

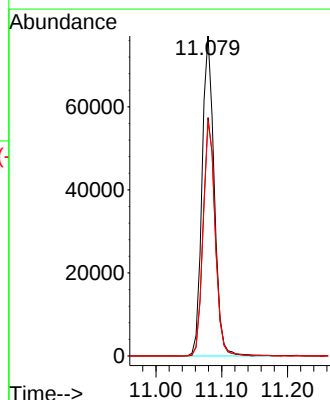






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1470
Delta R.T. 0.006 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 203619
Ion Ratio Lower Upper
117 100
82 54.5 46.4 69.6
119 30.5 24.6 37.0

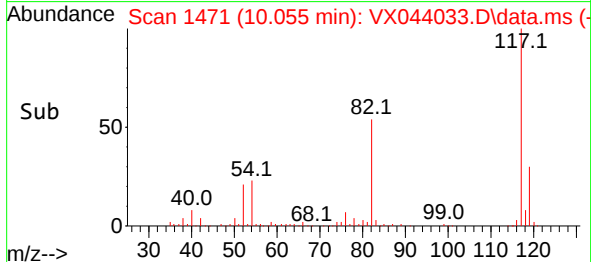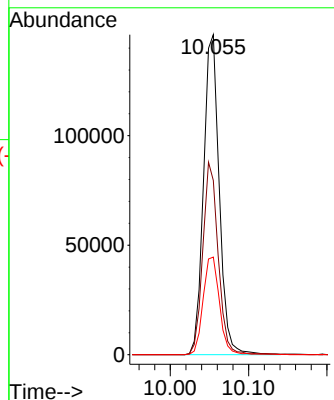

#67
Ethyl Benzene
Concen: 127.251 ug/l
RT: 10.189 min Scan# 1493
Delta R.T. -0.000 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22

Tgt Ion: 91 Resp: 964297
Ion Ratio Lower Upper
91 100
106 30.3 23.6 35.4


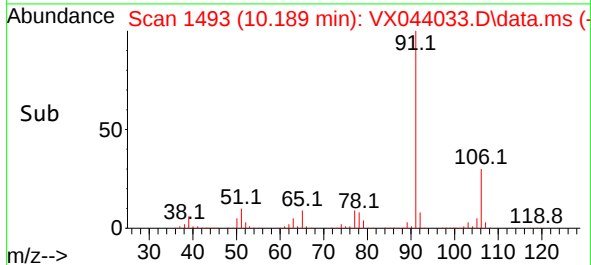
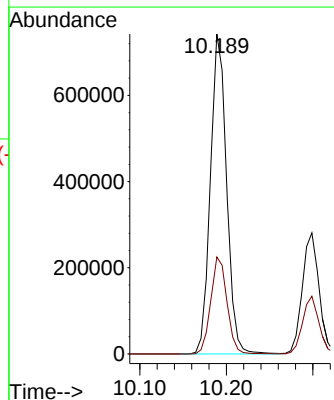
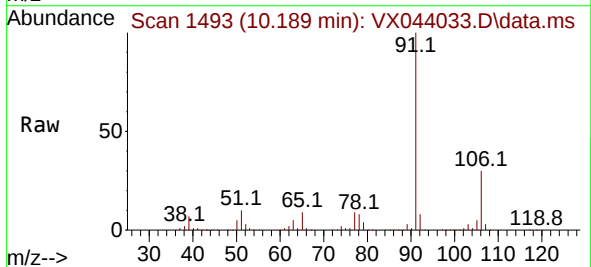




#68
m/p-Xylenes
Concen: 62.570 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 176821
Ion Ratio Lower Upper
106 100
91 214.7 168.1 252.1

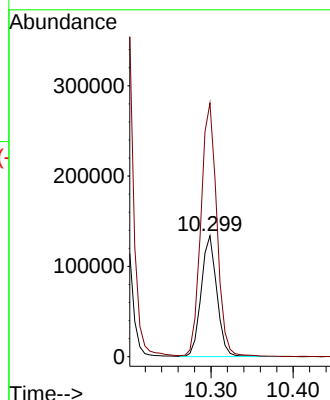

#69
o-Xylene
Concen: 43.565 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22

Tgt Ion:106 Resp: 120204
Ion Ratio Lower Upper
106 100
91 226.6 110.2 330.6

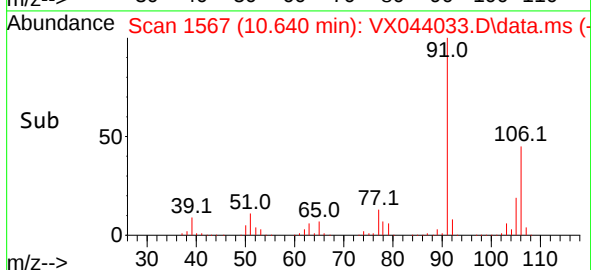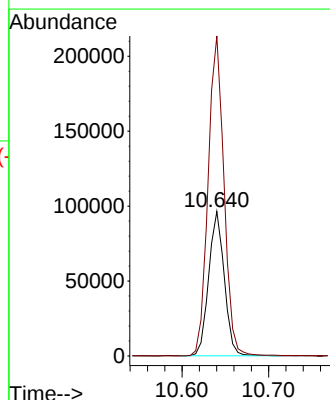

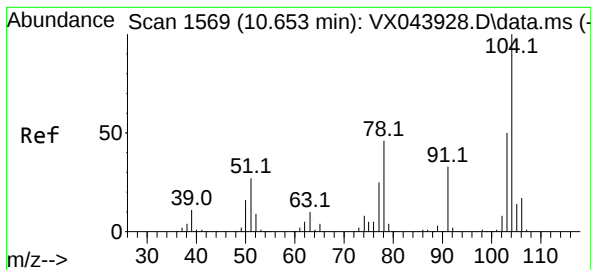

#70

Styrene

Concen: 2.178 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. -0.012 min

Lab File: VX044033.D

Acq: 27 Nov 2024 12:22

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:104 Resp: 9939

Ion Ratio Lower Upper

104 100

78 225.1 42.2 63.2#

103 193.5 44.7 67.1#

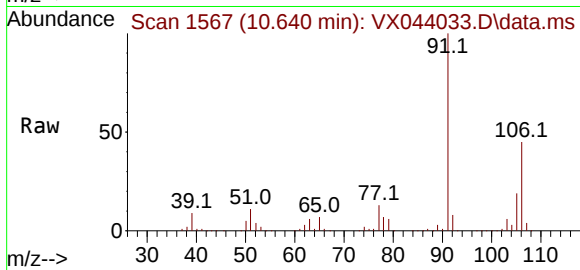

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX044033.D

Acq: 27 Nov 2024 12:22




Tgt Ion:152 Resp: 98952


Ion Ratio Lower Upper

152 100

115 61.9 45.4 136.2

150 157.0 0.0 353.0

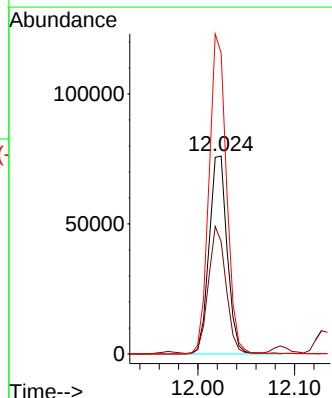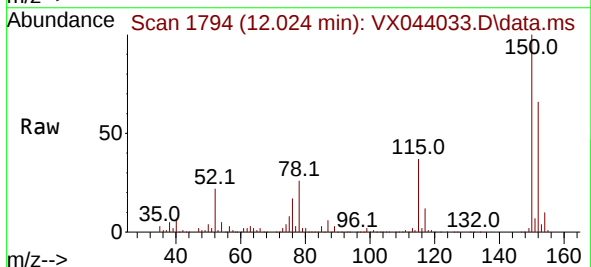



#73

Isopropylbenzene

Concen: 6.153 ug/l

RT: 10.963 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX044033.D

Acq: 27 Nov 2024 12:22

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 46801

Ion Ratio Lower Upper

105 100

120 24.7 13.0 38.9

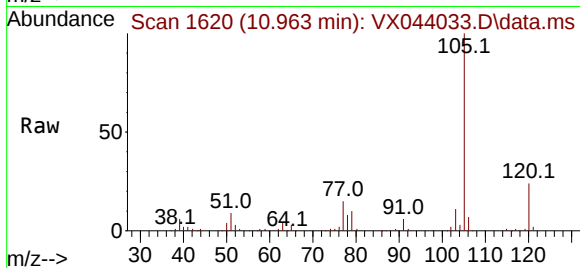

#76

1,2,3-Trichloropropane

Concen: 1.705 ug/l

RT: 11.378 min Scan# 1688

Delta R.T. 0.140 min

Lab File: VX044033.D




Acq: 27 Nov 2024 12:22


Tgt Ion: 75 Resp: 3700

Ion Ratio Lower Upper

75 100

77 1125.6 21.8 65.3#

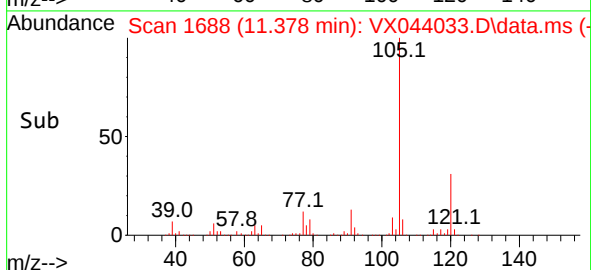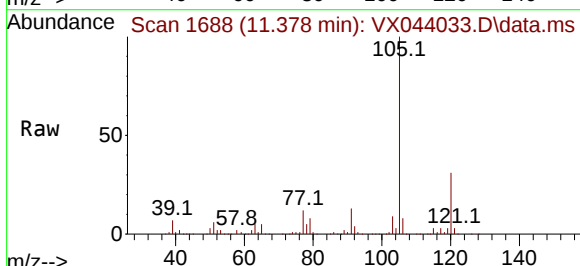

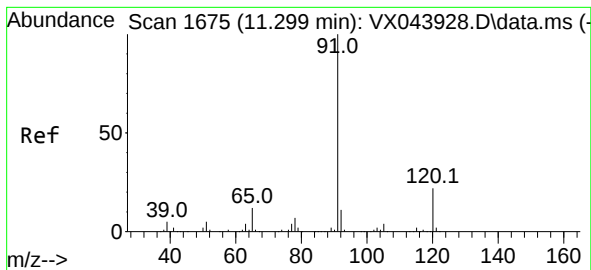

#78

n-propylbenzene

Concen: 1.256 ug/l

RT: 11.305 min Scan# 1675

Delta R.T. 0.006 min

Lab File: VX044033.D

Acq: 27 Nov 2024 12:22

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 10673

Ion Ratio Lower Upper

91 100

120 0.0 11.5 34.4#

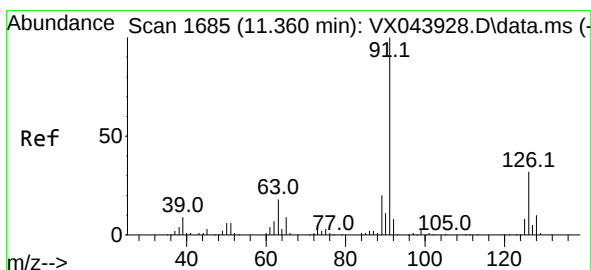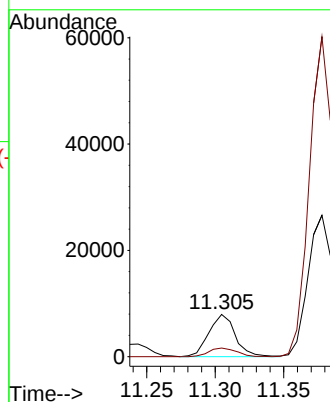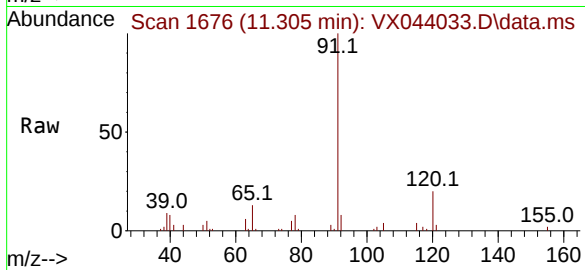

#79

2-Chlorotoluene

Concen: 8.285 ug/l

RT: 11.378 min Scan# 1688

Delta R.T. 0.018 min

Lab File: VX044033.D




Acq: 27 Nov 2024 12:22


Tgt Ion: 91 Resp: 44504

Ion Ratio Lower Upper

91 100

126 1.3 16.6 49.8#

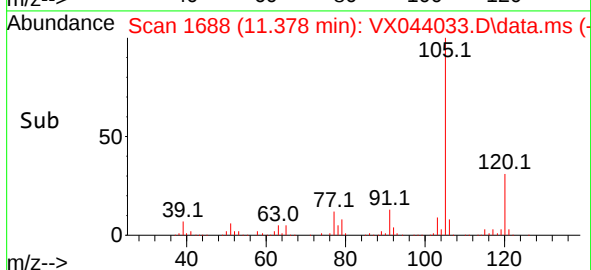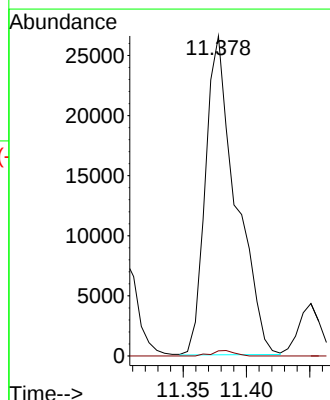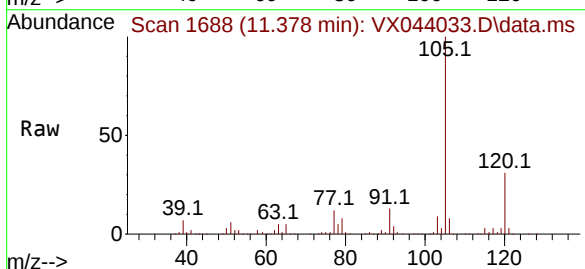



#80

1,3,5-Trimethylbenzene

Concen: 7.054 ug/l

RT: 11.451 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX044033.D

Acq: 27 Nov 2024 12:22

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 44141

Ion Ratio Lower Upper

105 100

120 45.5 23.3 69.8



#81

trans-1,4-Dichloro-2-butene

Concen: 71.407 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX044033.D

Acq: 27 Nov 2024 12:22




Tgt Ion: 75 Resp: 56785


Ion Ratio Lower Upper

75 100

53 0.0 86.7 130.1#

89 0.1 38.2 57.2#


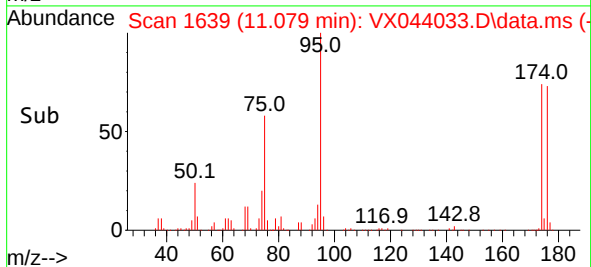

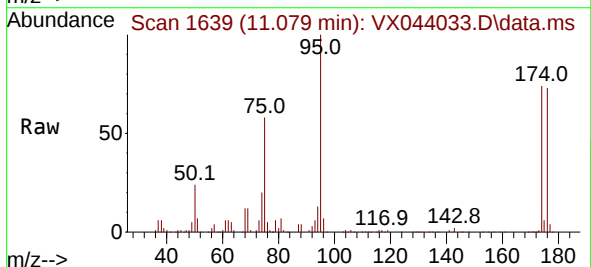




#82
4-Chlorotoluene
Concen: 0.831 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 5040
Ion Ratio Lower Upper
91 100
126 0.0 14.3 42.9#

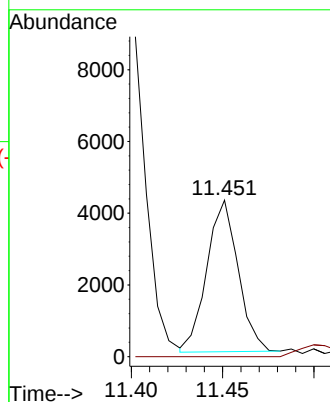

#83
tert-Butylbenzene
Concen: 3.032 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.036 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22

Tgt Ion: 119 Resp: 18805
Ion Ratio Lower Upper
119 100
91 109.5 31.0 93.0#
134 0.0 11.6 34.8#


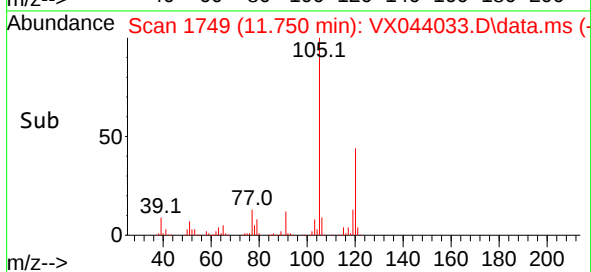
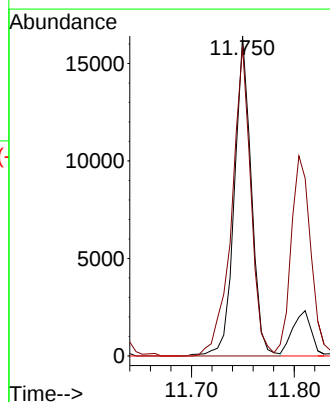





#84
1,2,4-Trimethylbenzene
Concen: 25.358 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 157988
Ion Ratio Lower Upper
105 100
120 43.6 21.9 65.7

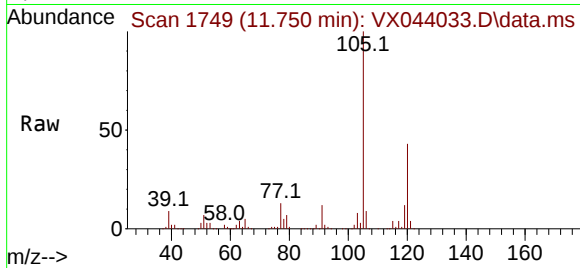

#85
sec-Butylbenzene
Concen: 20.789 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.141 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22

Tgt Ion:105 Resp: 157988
Ion Ratio Lower Upper
105 100
134 0.0 9.7 29.1#

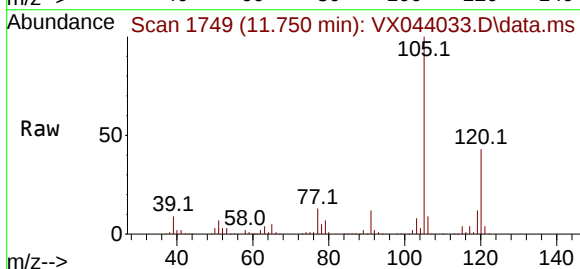



#86

p-Isopropyltoluene

Concen: 1.100 ug/l

RT: 12.006 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX044033.D

Acq: 27 Nov 2024 12:22

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:119 Resp: 6789

Ion Ratio Lower Upper

119 100

134 26.8 13.0 38.9

91 0.0 13.0 38.9#

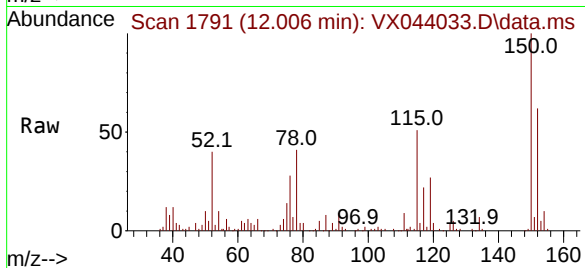

#89

n-Butylbenzene

Concen: 57.114 ug/l

RT: 12.237 min Scan# 1829

Delta R.T. -0.092 min

Lab File: VX044033.D

Acq: 27 Nov 2024 12:22




Tgt Ion: 91 Resp: 310843


Ion Ratio Lower Upper

91 100

92 9.7 26.6 79.8#


134 2.2 12.4 37.2#

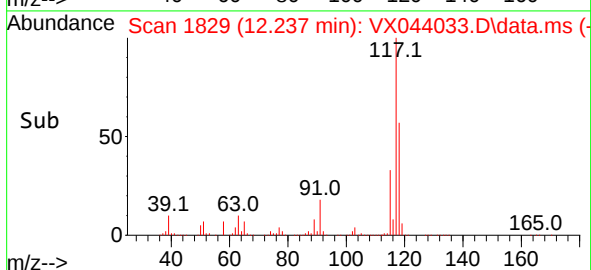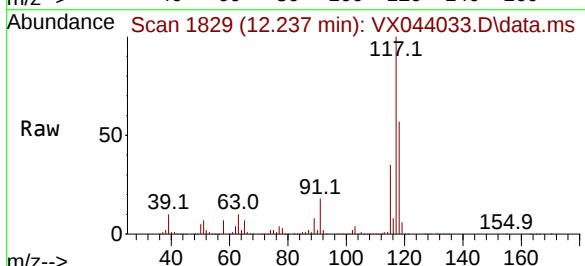






#92
1,2-Dibromo-3-Chloropropane
Concen: 0.312 ug/l
RT: 12.926 min Scan# 1944
Delta R.T. -0.012 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22

Instrument :
MSVOA_X
ClientSampleId :

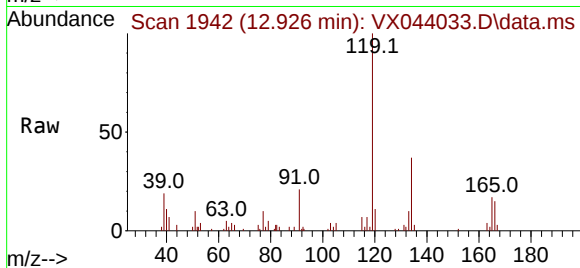

Tgt Ion: 75 Resp: 163
Ion Ratio Lower Upper
75 100
155 0.0 40.1 120.2#
157 0.0 49.6 149.0#



#95
Naphthalene
Concen: 1813.064 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX044033.D
Acq: 27 Nov 2024 12:22

Tgt Ion: 128 Resp: 12832701
Ion Ratio Lower Upper
128 100
127 16.6 10.2 15.2#
129 14.9 8.6 12.8#

