

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112724\
 Data File : VX044040.D
 Acq On : 27 Nov 2024 15:02
 Operator : JC/MD
 Sample : P5001-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 28 00:49:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 22 03:45:52 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	113725	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	222916	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	203256	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	88732	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	101660	52.118	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 104.240%	
35) Dibromofluoromethane	5.379	113	52838	33.172	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 66.340%#	
50) Toluene-d8	8.647	98	277165	50.479	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 100.960%	
62) 4-Bromofluorobenzene	11.079	95	99567	53.283	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 106.560%	
Target Compounds						
					Qvalue	
4) Vinyl Chloride	1.374	62	733	0.455	ug/l	98
5) Bromomethane	1.599	94	365	0.368	ug/l #	34
11) Tert butyl alcohol	2.983	59	185	0.591	ug/l #	73
16) Acetone	2.380	43	15950	17.804	ug/l	95
17) Carbon Disulfide	2.508	76	754	0.279	ug/l #	76
18) Methyl Acetate	2.703	43	919	0.440	ug/l #	79
20) Methylene Chloride	2.788	84	1447	0.952	ug/l	87
25) 2-Butanone	4.580	43	3135	2.712	ug/l #	84
27) cis-1,2-Dichloroethene	4.483	96	7515	4.494	ug/l	91
29) Tetrahydrofuran	5.044	42	835	1.178	ug/l #	49
31) Cyclohexane	5.544	56	3269	1.504	ug/l #	46
36) 1,1-Dichloropropene	5.544	75	10667	5.374	ug/l #	51
37) Ethyl Acetate	4.580	43	3135	1.272	ug/l #	69
38) Carbon Tetrachloride	5.544	117	13619	6.106	ug/l #	19
40) Benzene	6.044	78	4679	0.757	ug/l	90
44) Trichloroethene	7.129	130	657	0.375	ug/l	60
51) 4-Methyl-2-Pentanone	8.580	43	954	0.399	ug/l #	64
52) Toluene	8.720	92	2524	0.682	ug/l	88
67) Ethyl Benzene	10.195	91	24818	3.281	ug/l	99
68) m/p-Xylenes	10.299	106	3684	1.306	ug/l	97
69) o-Xylene	10.640	106	3325	1.207	ug/l	95
73) Isopropylbenzene	10.963	105	2233	0.327	ug/l	94
76) 1,2,3-Trichloropropane	11.079	75	57336	29.465	ug/l #	34
79) 2-Chlorotoluene	11.384	91	1181	0.245	ug/l #	45
80) 1,3,5-Trimethylbenzene	11.451	105	2447	0.436	ug/l	96
81) trans-1,4-Dichloro-2-b...	11.079	75	57336	80.404	ug/l #	7
84) 1,2,4-Trimethylbenzene	11.750	105	7482	1.339	ug/l	99
85) sec-Butylbenzene	11.750	105	7482	1.098	ug/l #	57
90) Hexachloroethane	12.408	117	1525	1.620	ug/l #	18
92) 1,2-Dibromo-3-Chloropr...	12.945	75	98	0.209	ug/l #	4
95) Naphthalene	13.774	128	824849	129.961	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112724\
Data File : VX044040.D
Acq On : 27 Nov 2024 15:02
Operator : JC/MD
Sample : P5001-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 28 00:49:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 22 03:45:52 2024
Response via : Initial Calibration




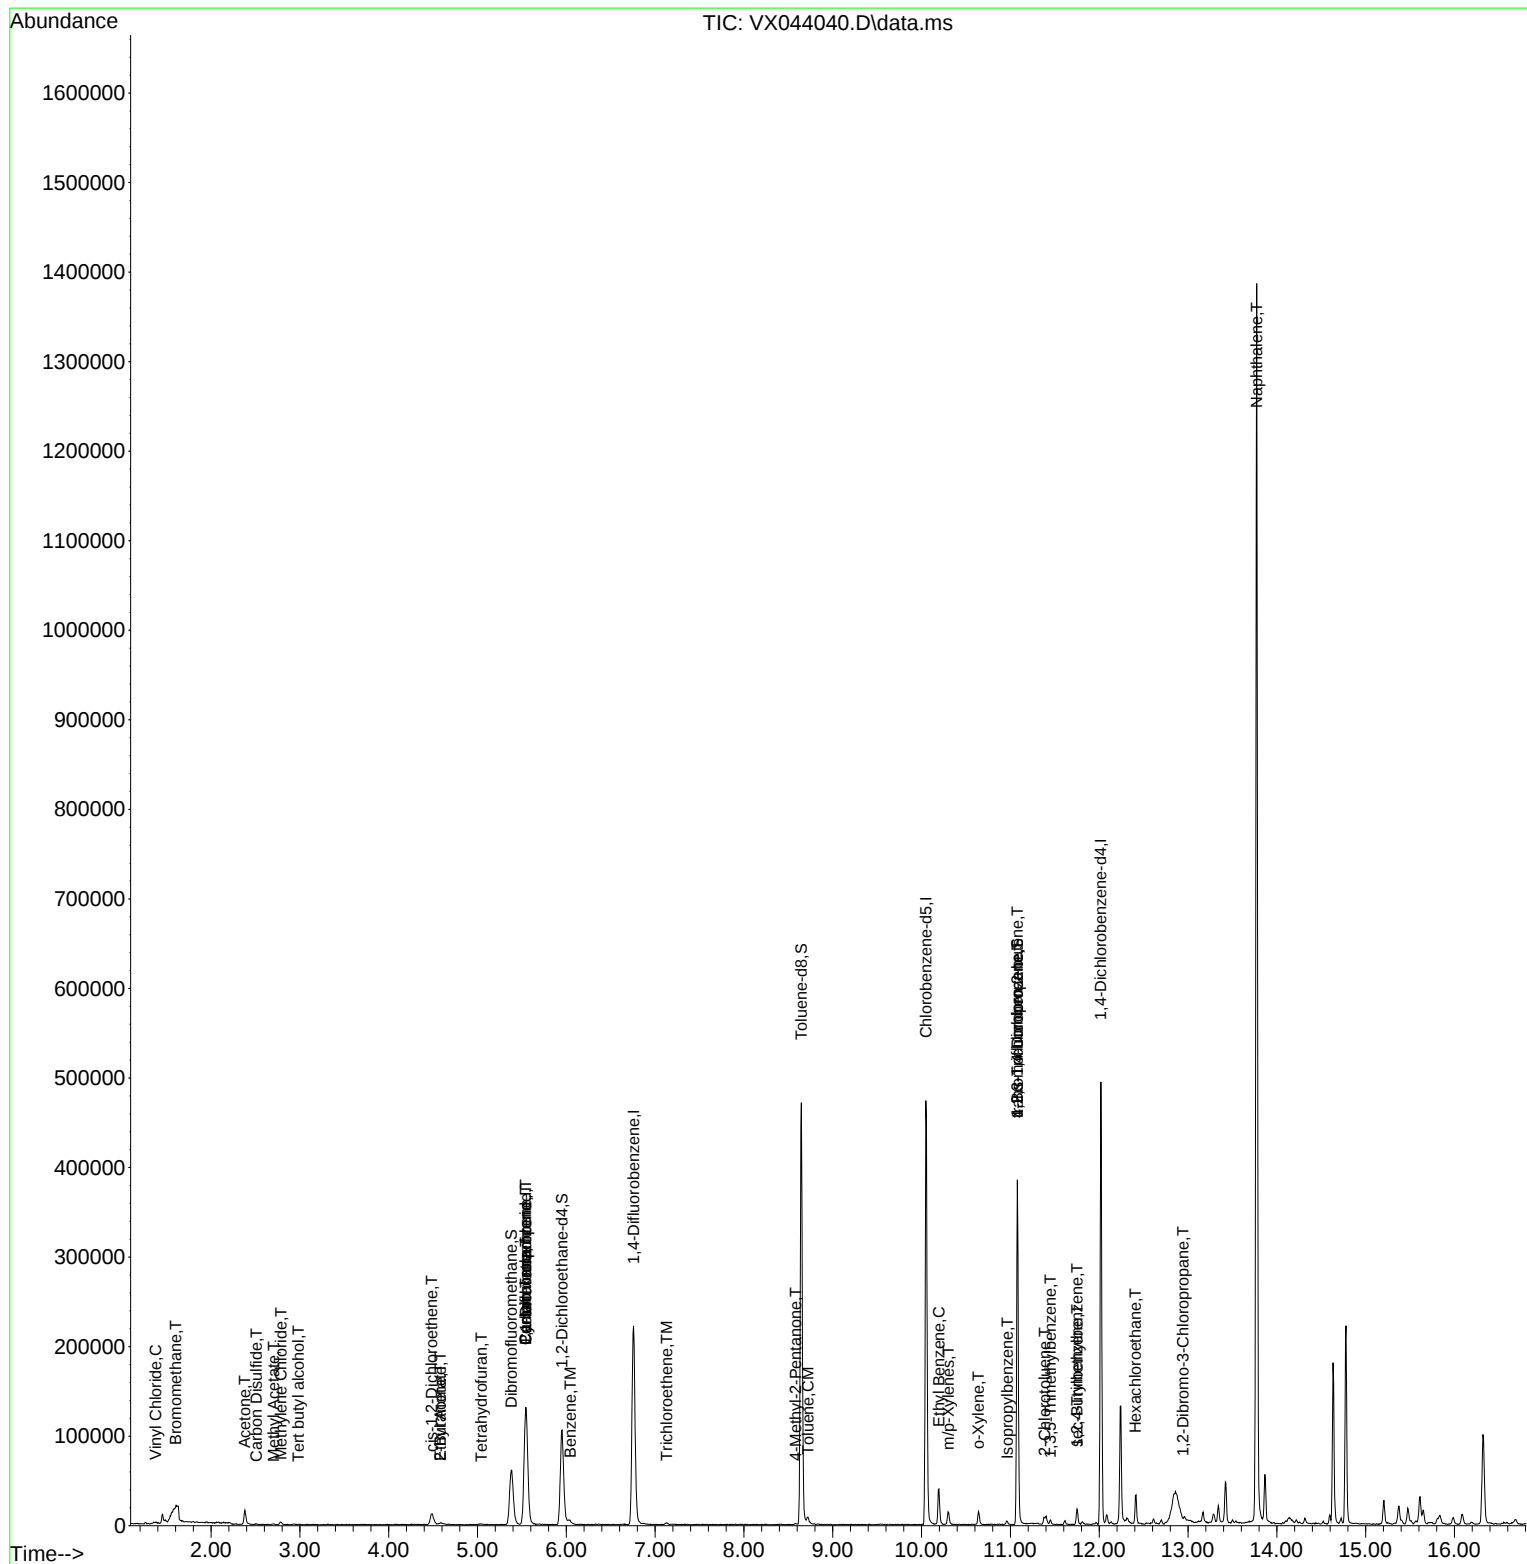




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 113725
Ion Ratio Lower Upper
168 100
99 71.8 51.8 77.8

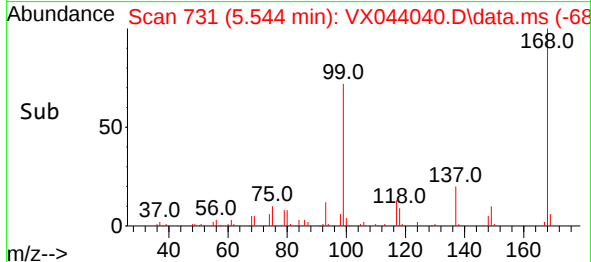

#4
Vinyl Chloride
Concen: 0.455 ug/l
RT: 1.374 min Scan# 47
Delta R.T. -0.000 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02

Tgt Ion: 62 Resp: 733
Ion Ratio Lower Upper
62 100
64 31.8 26.2 39.4




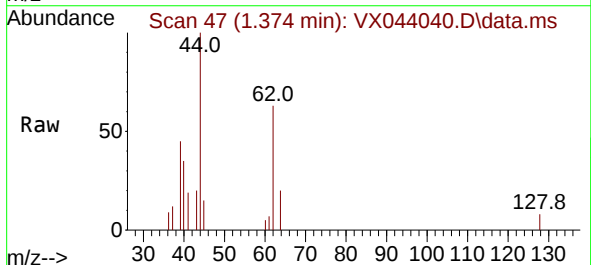


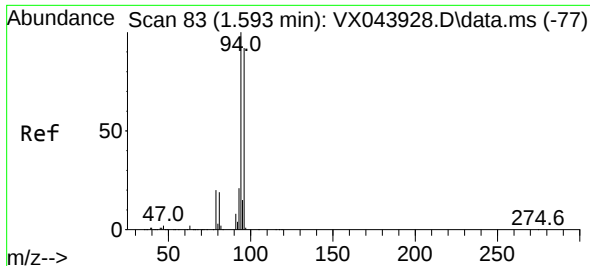

#5
Bromomethane
Concen: 0.368 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.006 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02




Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 94 Resp: 365
Ion Ratio Lower Upper
94 100
96 28.9 73.9 110.9#

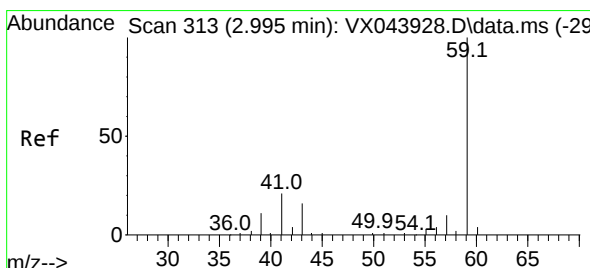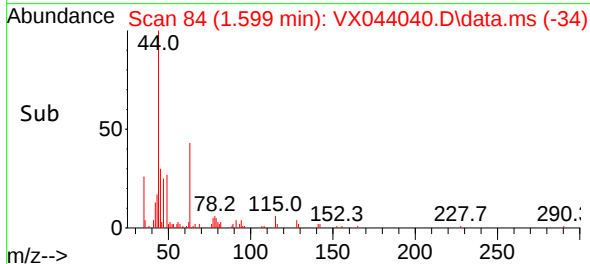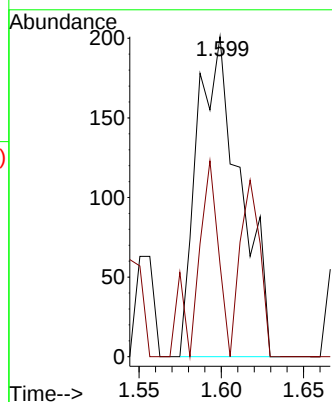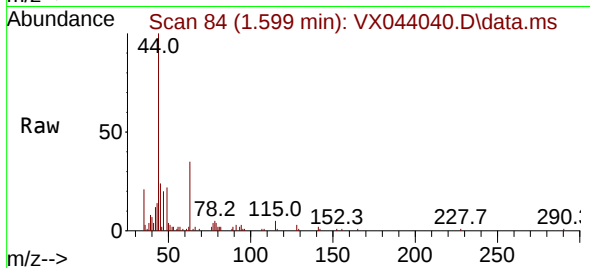

#11
Tert butyl alcohol
Concen: 0.591 ug/l
RT: 2.983 min Scan# 311
Delta R.T. -0.012 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02

Tgt Ion: 59 Resp: 185
Ion Ratio Lower Upper
59 100
57 0.0 7.9 11.9#


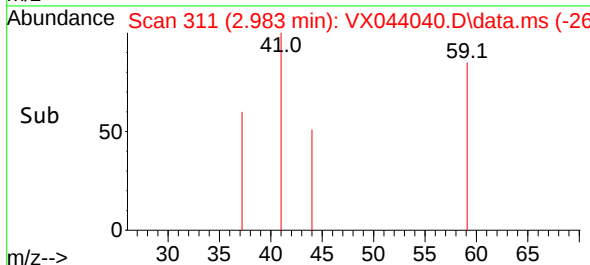

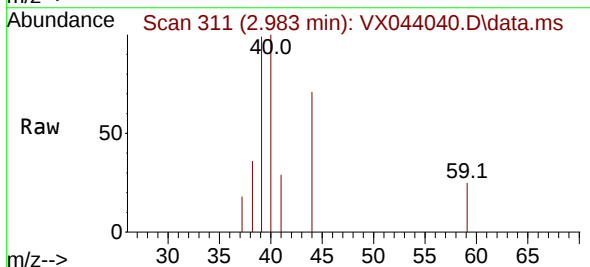




#16
Acetone
Concen: 17.804 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 15950
Ion Ratio Lower Upper
43 100
58 26.0 22.7 34.1

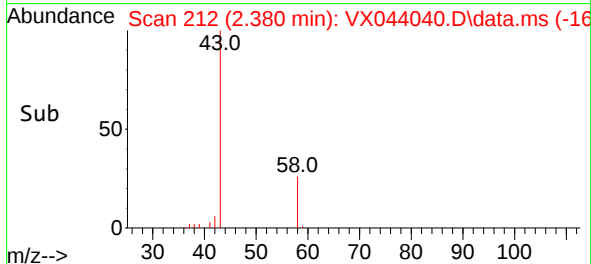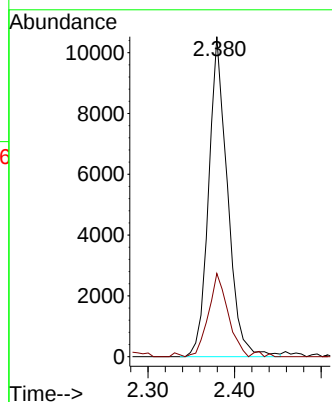

#17
Carbon Disulfide
Concen: 0.279 ug/l
RT: 2.508 min Scan# 233
Delta R.T. 0.006 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02

Tgt Ion: 76 Resp: 754
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.6#



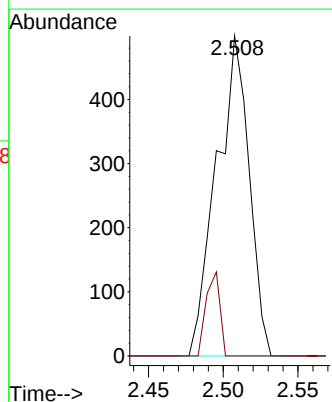





#18
Methyl Acetate
Concen: 0.440 ug/l
RT: 2.703 min Scan# 218
Delta R.T. -0.000 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 919
Ion Ratio Lower Upper
43 100
74 13.5 18.9 28.3#

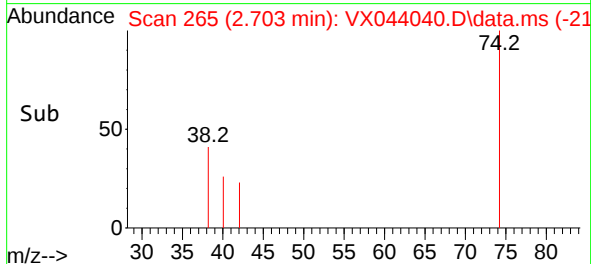

#20
Methylene Chloride
Concen: 0.952 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.006 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02

Tgt Ion: 84 Resp: 1447
Ion Ratio Lower Upper
84 100
49 145.6 102.7 154.1
51 38.4 31.7 47.5
86 56.0 53.9 80.9









#25
2-Butanone
Concen: 2.712 ug/l
RT: 4.580 min Scan# 51
Delta R.T. 0.024 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 3135
Ion Ratio Lower Upper
43 100
72 17.2 20.2 30.2#

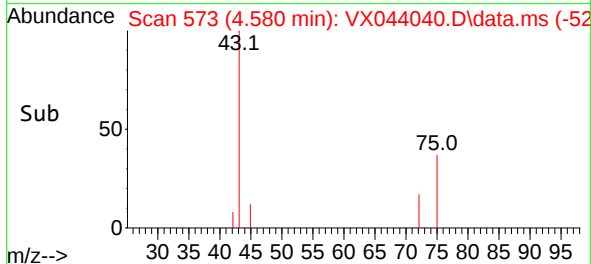

#27
cis-1,2-Dichloroethene
Concen: 4.494 ug/l
RT: 4.483 min Scan# 557
Delta R.T. 0.006 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02

Tgt Ion: 96 Resp: 7515
Ion Ratio Lower Upper
96 100
61 133.0 0.0 297.4
98 64.8 0.0 127.8





#29

Tetrahydrofuran

Concen: 1.178 ug/l

RT: 5.044 min Scan# 642

Delta R.T. 0.042 min

Lab File: VX044040.D

Acq: 27 Nov 2024 15:02

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 42 Resp: 835

Ion Ratio Lower Upper

42 100

72 14.1 36.4 54.6#

71 7.5 33.4 50.0#

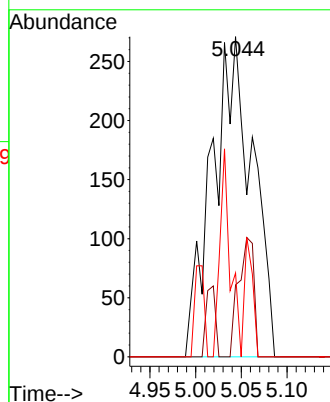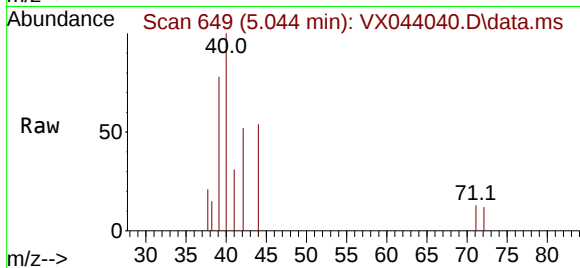

#31

Cyclohexane

Concen: 1.504 ug/l

RT: 5.544 min Scan# 731

Delta R.T. 0.085 min

Lab File: VX044040.D

Acq: 27 Nov 2024 15:02




Tgt Ion: 56 Resp: 3269


Ion Ratio Lower Upper

56 100

69 137.3 24.7 37.1#

84 89.2 68.7 103.1




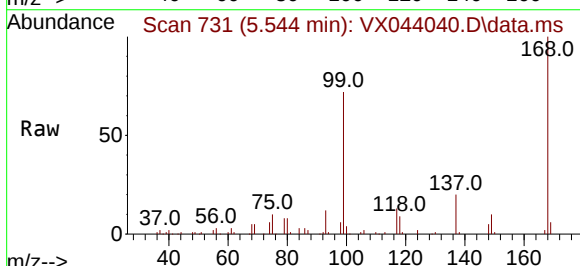


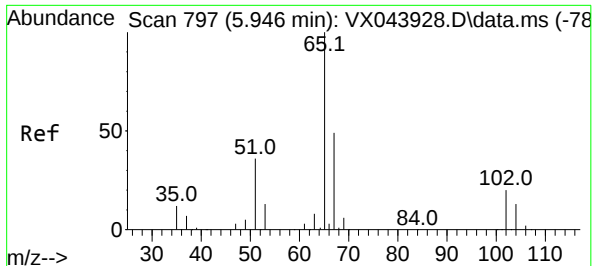

#33
 1,2-Dichloroethane-d4
 Concen: 52.118 ug/l
 RT: 5.952 min Scan# 797
 Delta R.T. 0.006 min
 Lab File: VX044040.D
 Acq: 27 Nov 2024 15:02




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 65 Resp: 101660
 Ion Ratio Lower Upper
 65 100
 67 49.6 0.0 100.8

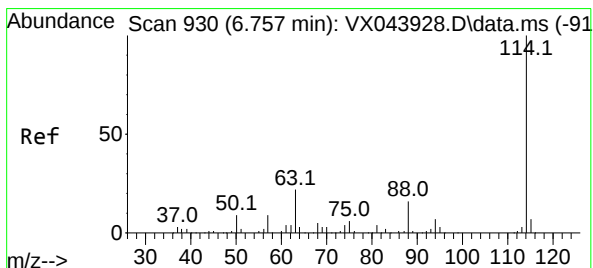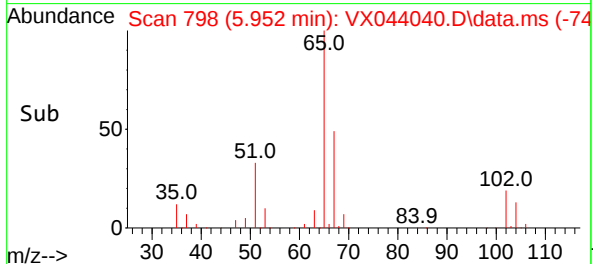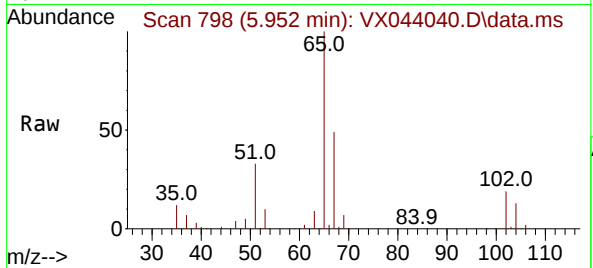

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 930
 Delta R.T. -0.000 min
 Lab File: VX044040.D
 Acq: 27 Nov 2024 15:02

Tgt Ion: 114 Resp: 222916
 Ion Ratio Lower Upper
 114 100
 63 21.6 0.0 44.0
 88 16.1 0.0 32.4


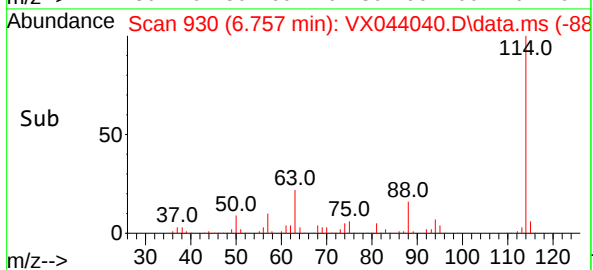

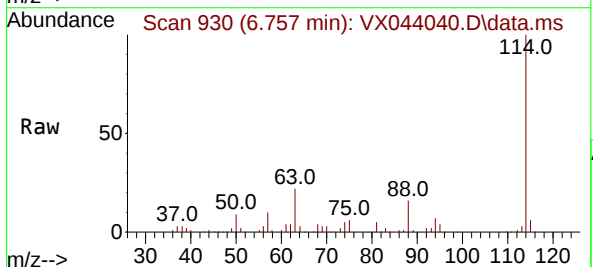


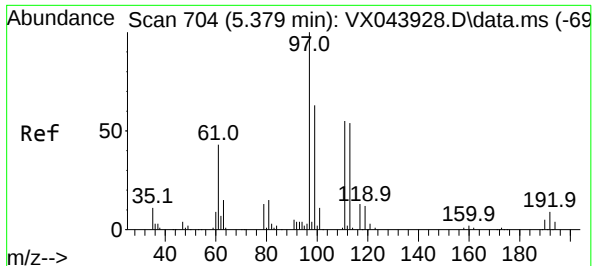

#35
Dibromofluoromethane
Concen: 33.172 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:113 Resp: 52838
Ion Ratio Lower Upper
113 100
111 102.8 81.0 121.4
192 16.6 13.0 19.6

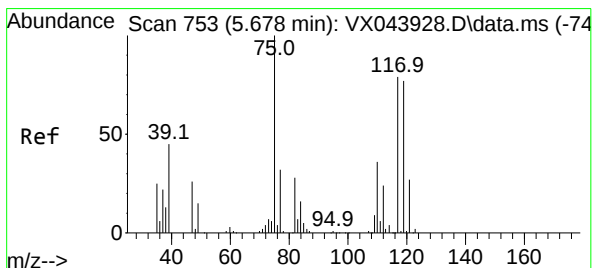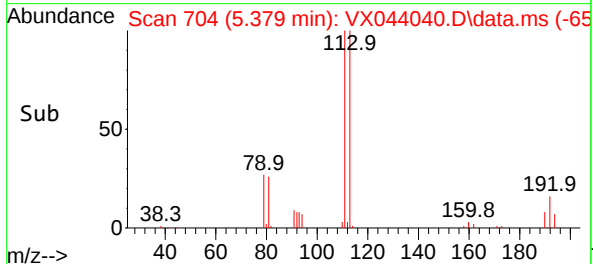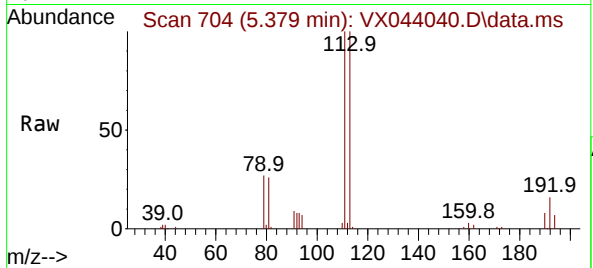

#36
1,1-Dichloropropene
Concen: 5.374 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.134 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02


Tgt Ion: 75 Resp: 10667
Ion Ratio Lower Upper
75 100
110 11.5 17.4 52.2#
77 0.0 25.8 38.8#

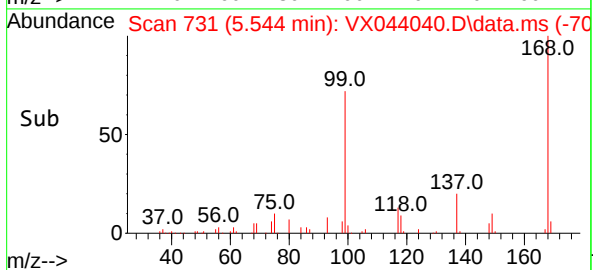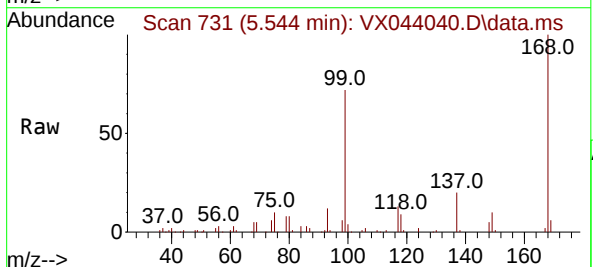






#37
Ethyl Acetate
Concen: 1.272 ug/l
RT: 4.580 min Scan# 51
Delta R.T. -0.128 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 43 Resp: 3135
Ion Ratio Lower Upper
43 100
61 0.0 10.7 16.1#
70 0.0 8.0 12.0#



#38
Carbon Tetrachloride
Concen: 6.106 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.122 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02

Tgt Ion: 117 Resp: 13619
Ion Ratio Lower Upper
117 100
119 7.3 75.2 112.8#
121 0.0 24.5 36.7#

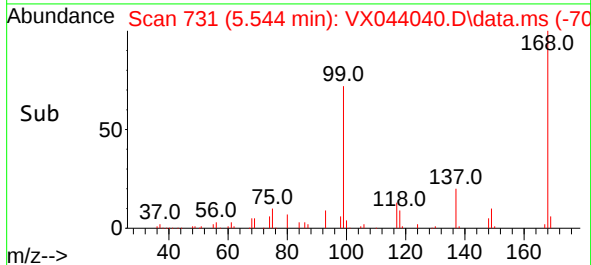

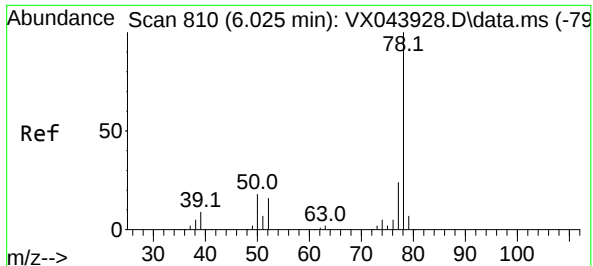

#40

Benzene

Concen: 0.757 ug/l

RT: 6.044 min Scan# 810

Delta R.T. 0.018 min

Lab File: VX044040.D

Acq: 27 Nov 2024 15:02

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 78 Resp: 4679

Ion Ratio Lower Upper

78 100

77 19.2 19.2 28.8

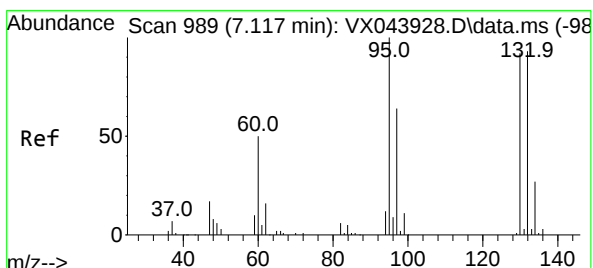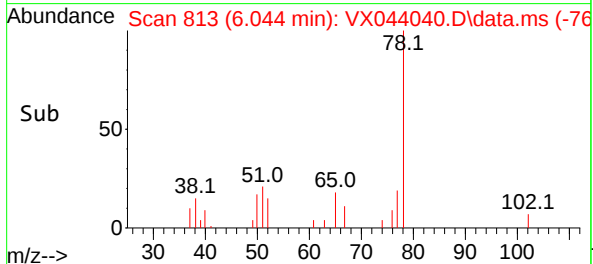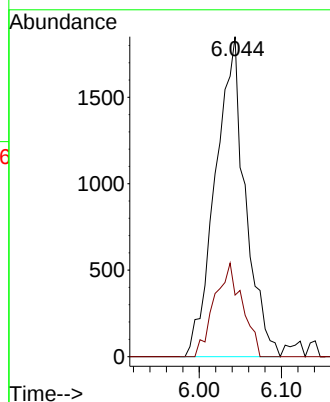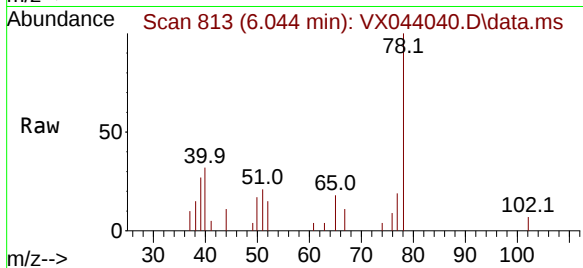

#44

Trichloroethene

Concen: 0.375 ug/l

RT: 7.129 min Scan# 991

Delta R.T. 0.012 min

Lab File: VX044040.D




Acq: 27 Nov 2024 15:02


Tgt Ion:130 Resp: 657

Ion Ratio Lower Upper

130 100

95 67.0 0.0 217.8


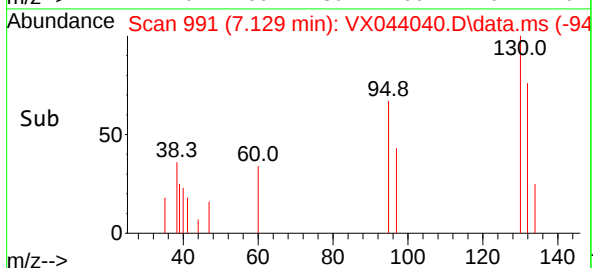

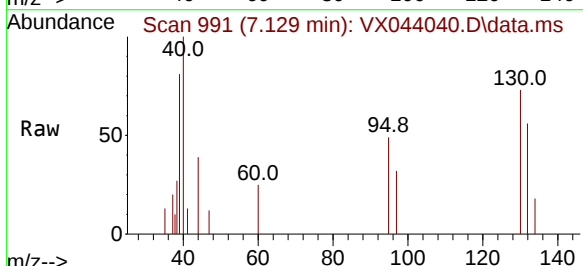


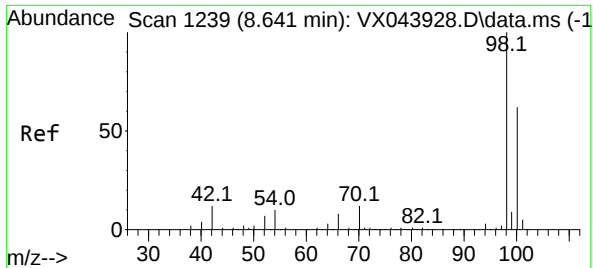

#50
Toluene-d8
Concen: 50.479 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 277165
Ion Ratio Lower Upper
98 100
100 64.1 52.6 79.0

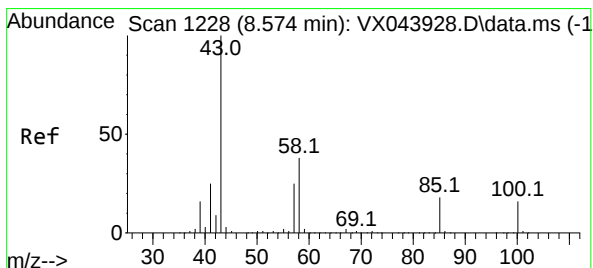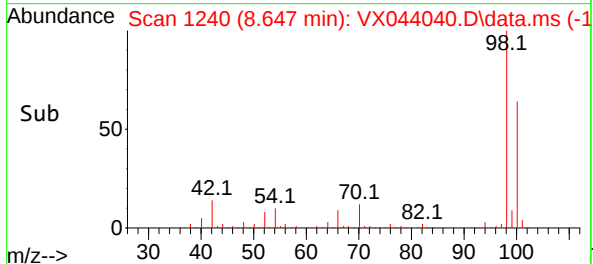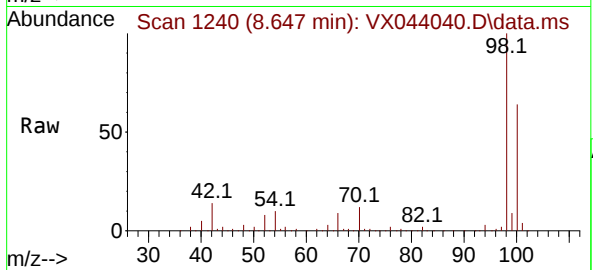

#51
4-Methyl-2-Pentanone
Concen: 0.399 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. 0.006 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02

Tgt Ion: 43 Resp: 954
Ion Ratio Lower Upper
43 100
58 15.8 30.0 45.0#


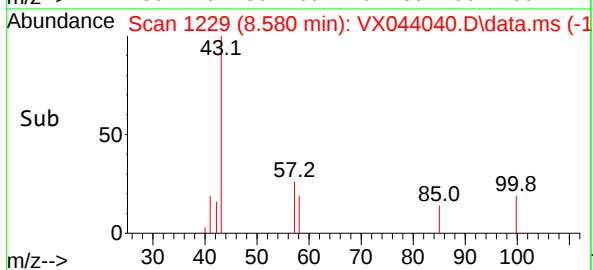
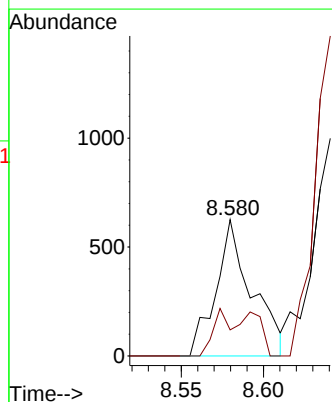
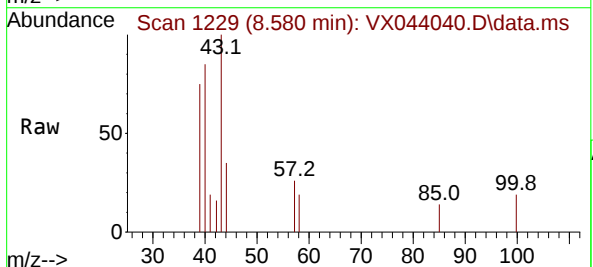




#52
Toluene
Concen: 0.682 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 92 Resp: 2524
Ion Ratio Lower Upper
92 100
91 192.0 139.7 209.5

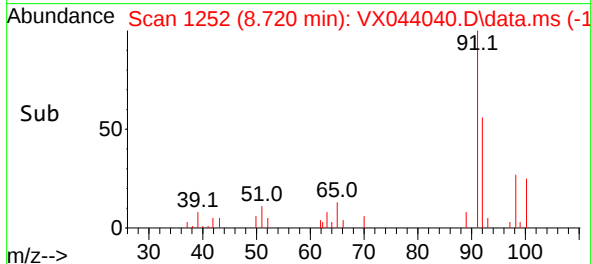

#62
4-Bromofluorobenzene
Concen: 53.283 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02

Tgt Ion: 95 Resp: 99567
Ion Ratio Lower Upper
95 100
174 70.8 0.0 150.4
176 69.1 0.0 146.0









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 203256
Ion Ratio Lower Upper
117 100
82 59.1 46.4 69.6
119 32.9 24.6 37.0

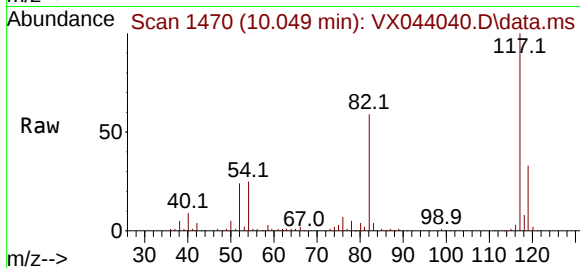

#67
Ethyl Benzene
Concen: 3.281 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.006 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02

Tgt Ion: 91 Resp: 24818
Ion Ratio Lower Upper
91 100
106 30.0 23.6 35.4




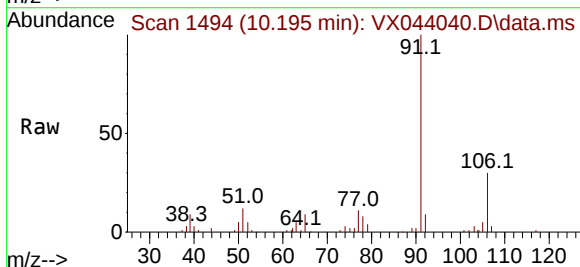




#68
m/p-Xylenes
Concen: 1.306 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 3684
Ion Ratio Lower Upper
106 100
91 205.1 168.1 252.1

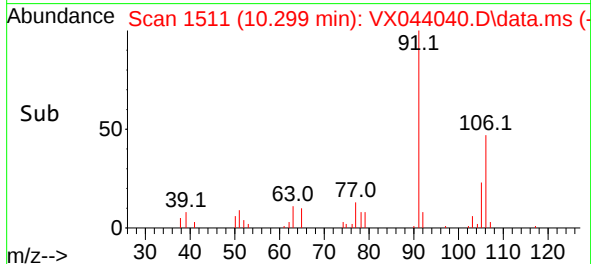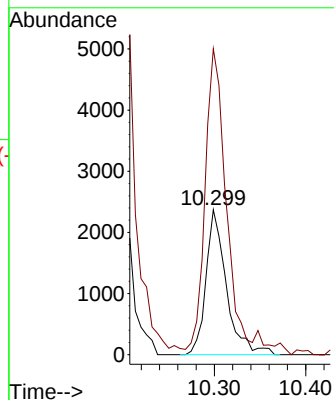

#69
o-Xylene
Concen: 1.207 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02

Tgt Ion:106 Resp: 3325
Ion Ratio Lower Upper
106 100
91 212.7 110.2 330.6

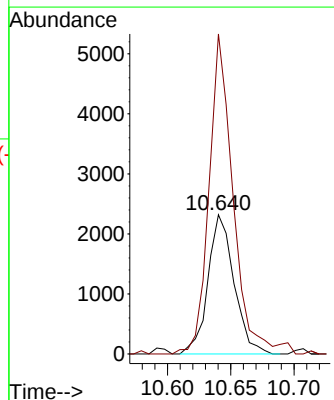



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX044040.D

Acq: 27 Nov 2024 15:02

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:152 Resp: 88732

Ion Ratio Lower Upper

152 100

115 66.5 45.4 136.2

150 159.4 0.0 353.0

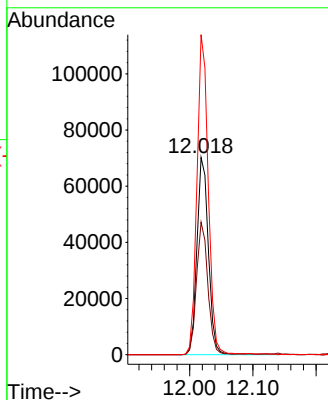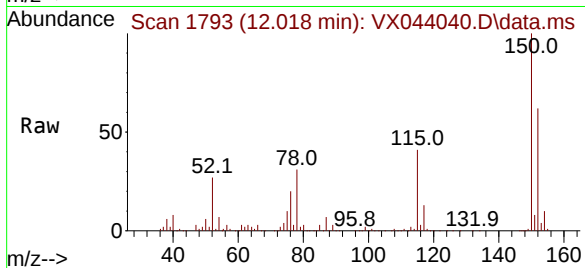

#73

Isopropylbenzene

Concen: 0.327 ug/l

RT: 10.963 min Scan# 1620

Delta R.T. 0.006 min

Lab File: VX044040.D




Acq: 27 Nov 2024 15:02


Tgt Ion:105 Resp: 2233

Ion Ratio Lower Upper

105 100

120 22.9 13.0 38.9



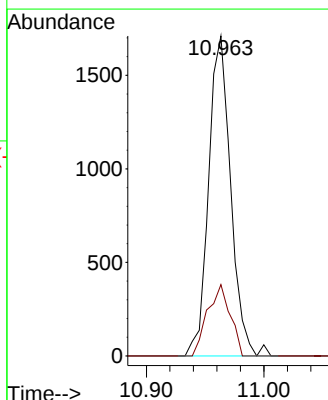
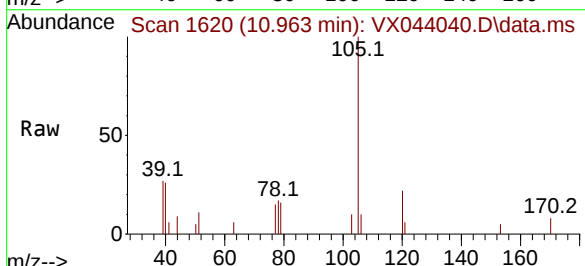




#76
1,2,3-Trichloropropane
Concen: 29.465 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 57336
Ion Ratio Lower Upper
75 100
77 1.2 21.8 65.3#

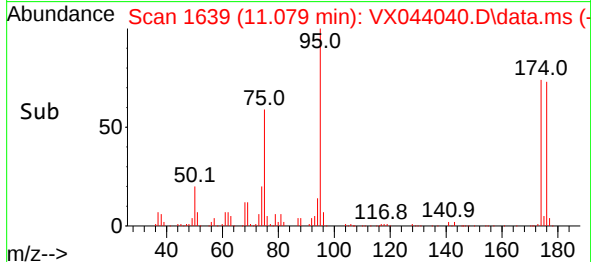

#79
2-Chlorotoluene
Concen: 0.245 ug/l
RT: 11.384 min Scan# 1689
Delta R.T. 0.024 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02

Tgt Ion: 91 Resp: 1181
Ion Ratio Lower Upper
91 100
126 2.3 16.6 49.8#

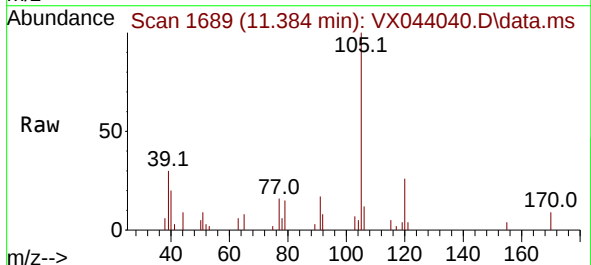



#80

1,3,5-Trimethylbenzene

Concen: 0.436 ug/l

RT: 11.451 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX044040.D

Acq: 27 Nov 2024 15:02

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 2447

Ion Ratio Lower Upper

105 100

120 44.1 23.3 69.8

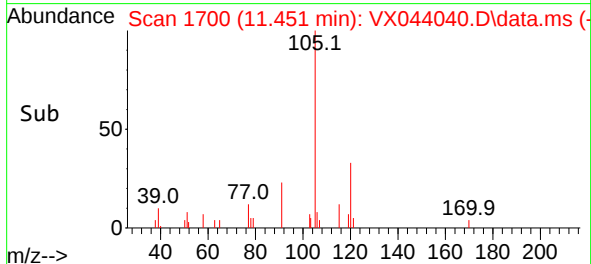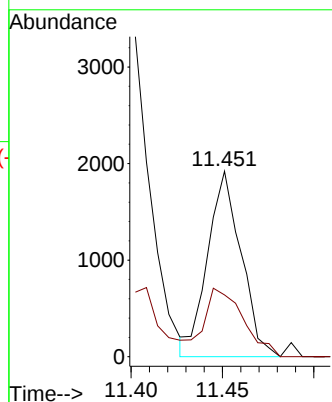

#81

trans-1,4-Dichloro-2-butene

Concen: 80.404 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX044040.D

Acq: 27 Nov 2024 15:02




Tgt Ion: 75 Resp: 57336


Ion Ratio Lower Upper

75 100

53 0.0 86.7 130.1#

89 0.1 38.2 57.2#

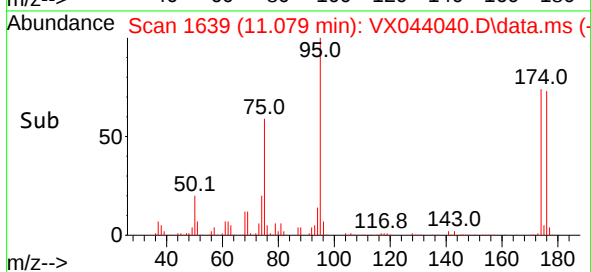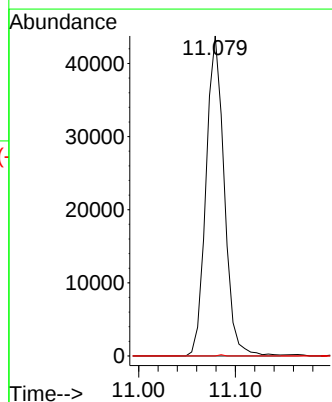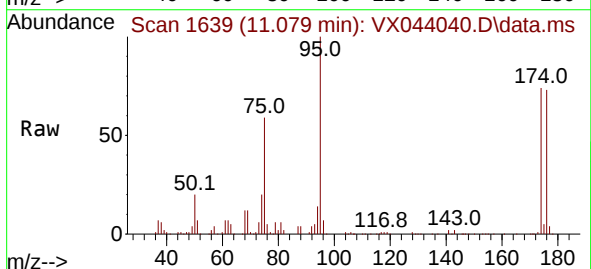



#84

1,2,4-Trimethylbenzene

Concen: 1.339 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX044040.D

Acq: 27 Nov 2024 15:02

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 7482

Ion Ratio Lower Upper

105 100

120 44.7 21.9 65.7

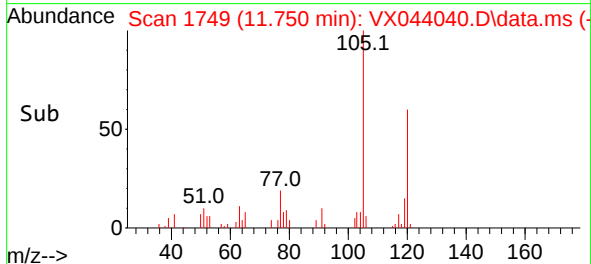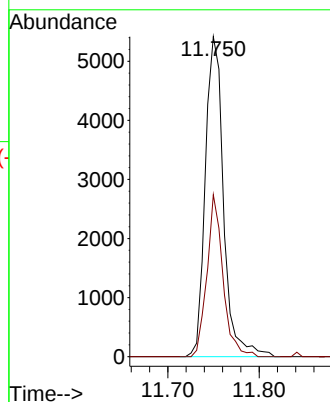

#85

sec-Butylbenzene

Concen: 1.098 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.140 min

Lab File: VX044040.D




Acq: 27 Nov 2024 15:02


Tgt Ion:105 Resp: 7482

Ion Ratio Lower Upper

105 100

134 0.0 9.7 29.1#




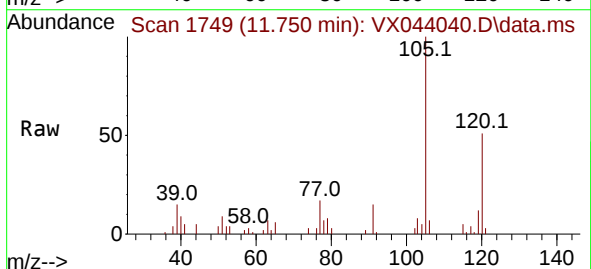




#90
Hexachloroethane
Concen: 1.620 ug/l
RT: 12.408 min Scan# 117
Delta R.T. -0.128 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 1525
Ion Ratio Lower Upper
117 100
201 0.0 32.4 97.0#

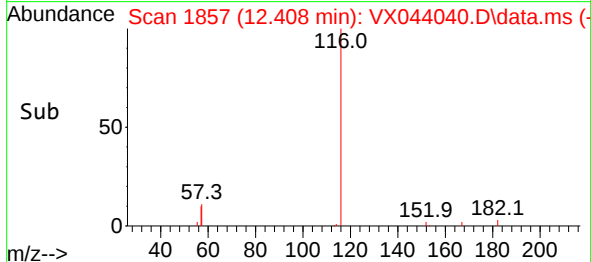

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.209 ug/l
RT: 12.945 min Scan# 1945
Delta R.T. 0.006 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02


Tgt Ion: 75 Resp: 98
Ion Ratio Lower Upper
75 100
155 0.0 40.1 120.2#
157 0.0 49.6 149.0#

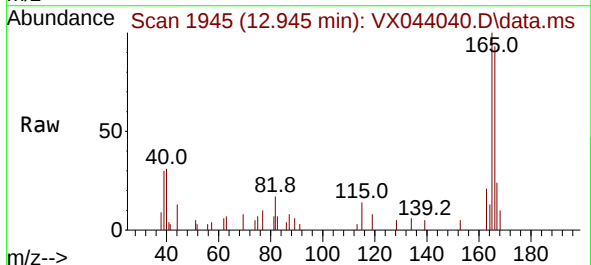



#95
Naphthalene
Concen: 129.961 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX044040.D
Acq: 27 Nov 2024 15:02

Instrument :
MSVOA_X
ClientSampleId :



Tgt Ion:128 Resp: 824849
Ion Ratio Lower Upper
128 100
127 13.1 10.2 15.2
129 11.1 8.6 12.8

