



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112724\
Data File : VX044023.D
Acq On : 27 Nov 2024 07:52
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Title : SW846 8260
Last Update : Fri Nov 22 03:45:52 2024

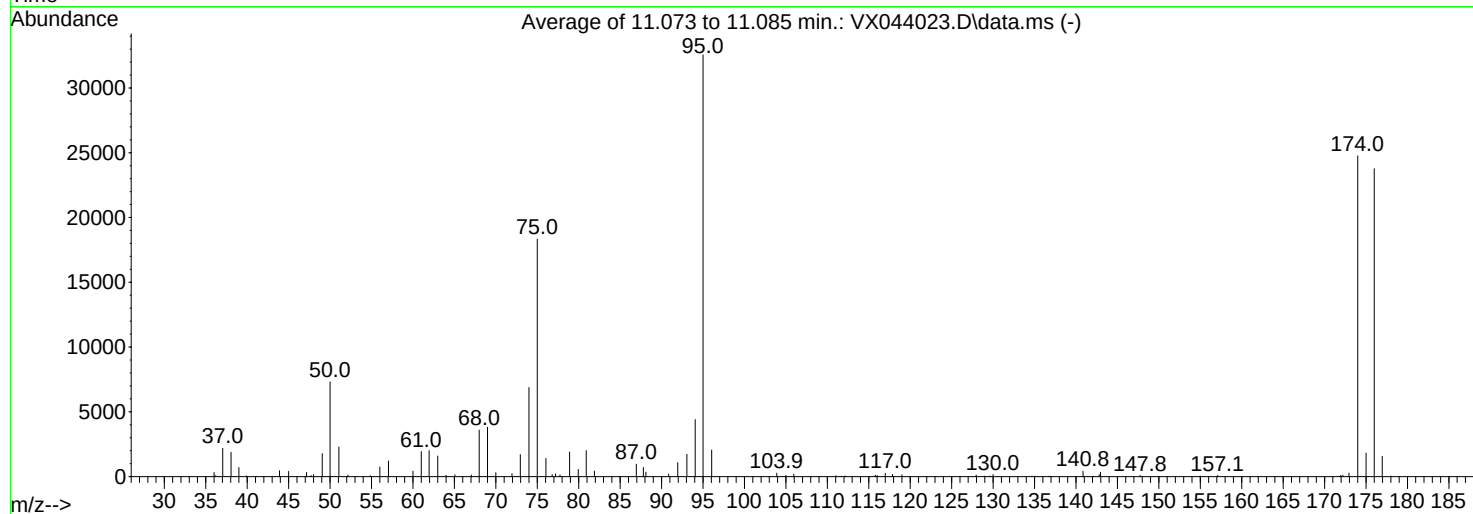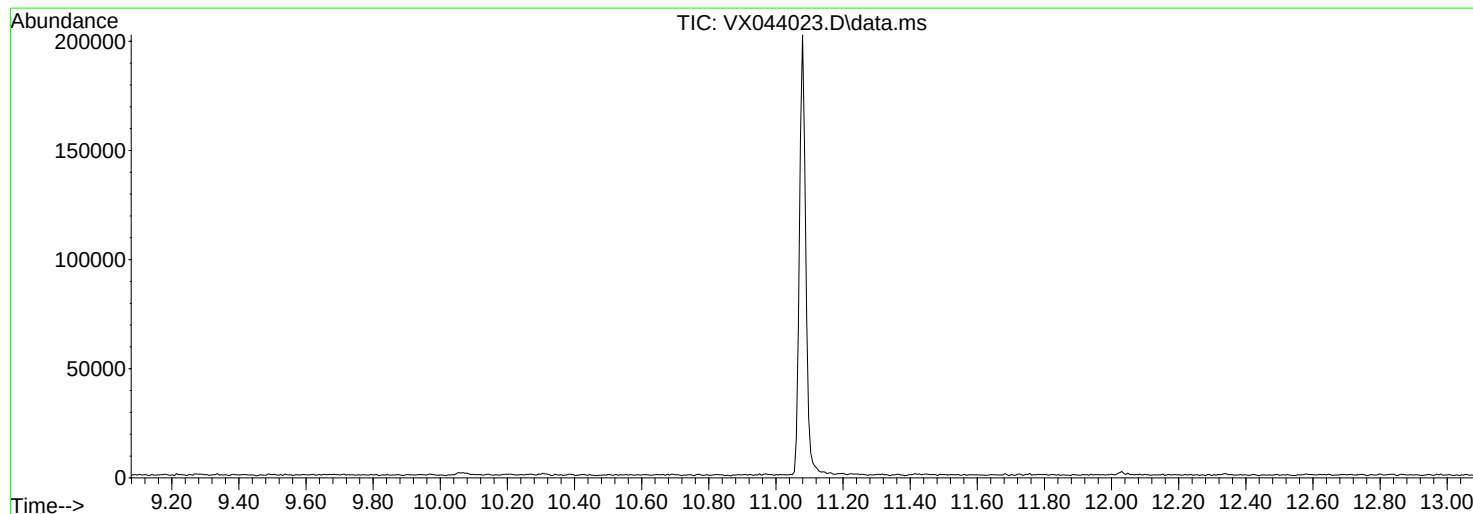

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.5	7314	PASS
75	95	30	60	56.3	18335	PASS
95	95	100	100	100.0	32555	PASS
96	95	5	9	6.3	2051	PASS
173	174	0.00	2	1.1	266	PASS
174	95	50	100	76.1	24760	PASS
175	174	5	9	7.3	1810	PASS
176	174	95	101	96.0	23773	PASS
177	176	5	9	6.6	1572	PASS