


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX112918\
Data File : VX006208.D
Acq On : 29 Nov 2018 13:03
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
Title : SW846 8260
Last Update : Fri Nov 30 03:55:33 2018

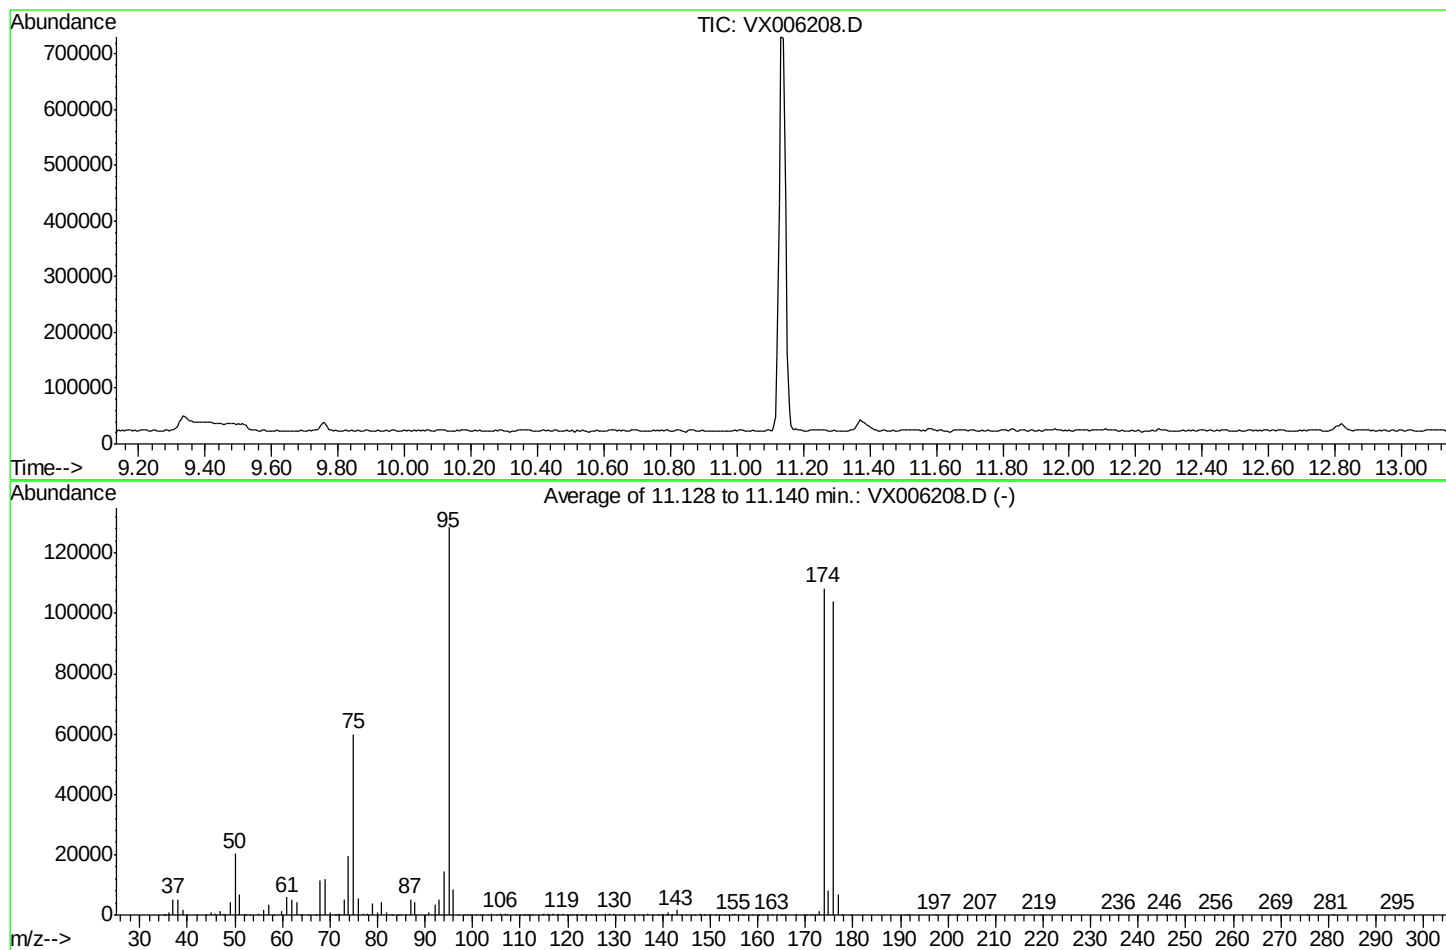

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	20240	PASS
75	95	30	60	46.6	59874	PASS
95	95	100	100	100.0	128523	PASS
96	95	5	9	6.5	8369	PASS
173	174	0.00	2	1.1	1177	PASS
174	95	50	100	84.3	108378	PASS
175	174	5	9	7.3	7899	PASS
176	174	95	101	95.7	103770	PASS
177	176	5	9	6.4	6623	PASS