
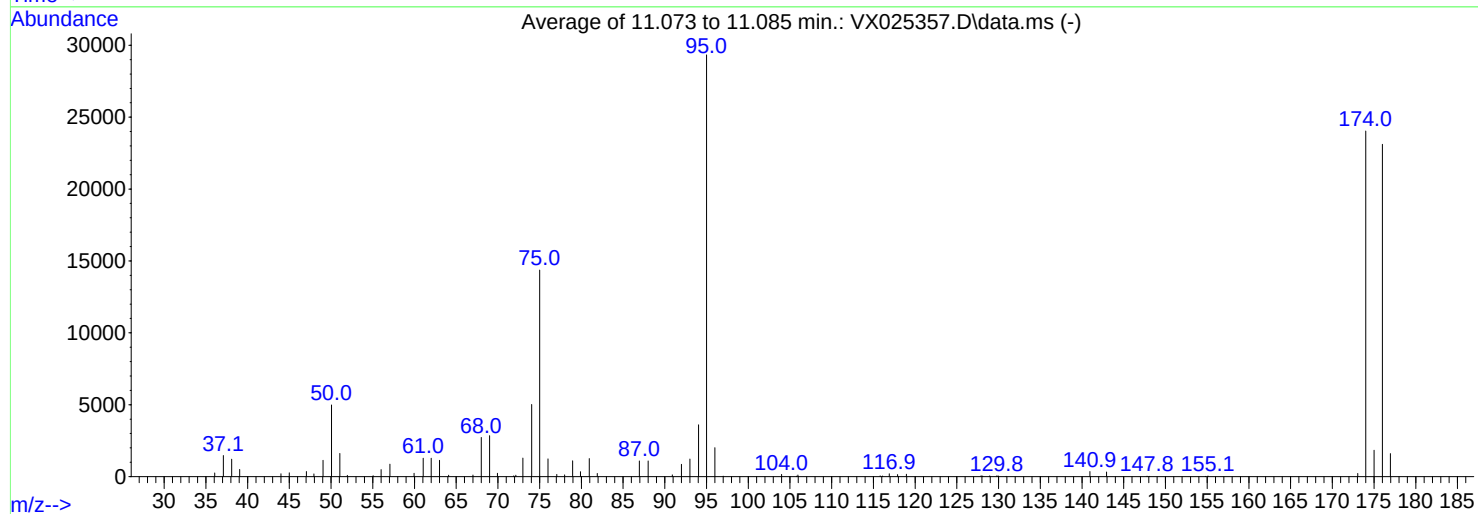


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112921\
Data File : VX025357.D
Acq On : 29 Nov 2021 09:54
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Title : SW846 8260
Last Update : Wed Nov 17 15:36:16 2021

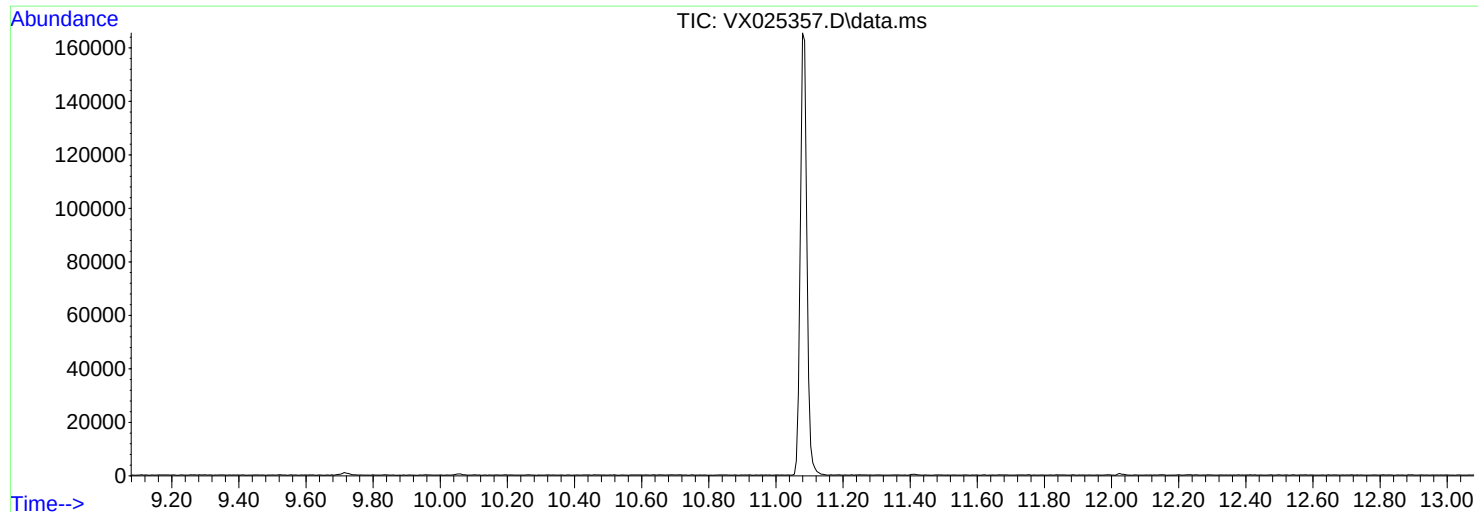

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	4984	PASS
75	95	30	60	49.0	14361	PASS
95	95	100	100	100.0	29333	PASS
96	95	5	9	6.9	2012	PASS
173	174	0.00	2	0.9	222	PASS
174	95	50	100	82.0	24039	PASS
175	174	5	9	7.6	1831	PASS
176	174	95	101	96.1	23113	PASS
177	176	5	9	6.9	1606	PASS