

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112922\
 Data File : VX033110.D
 Acq On : 29 Nov 2022 12:16
 Operator : JC/MD
 Sample : N5786-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Quant Time: Nov 30 01:01:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 22 13:58:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	125835	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	203844	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	178746	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	81029	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	69311	56.795	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	113.580%
35) Dibromofluoromethane	5.385	113	55449	48.250	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.500%
50) Toluene-d8	8.647	98	185587	53.839	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	107.680%
62) 4-Bromofluorobenzene	11.079	95	72825	48.242	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	96.480%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112922\
Data File : VX033110.D
Acq On : 29 Nov 2022 12:16
Operator : JC/MD
Sample : N5786-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Time: Nov 30 01:01:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 22 13:58:46 2022
Response via : Initial Calibration




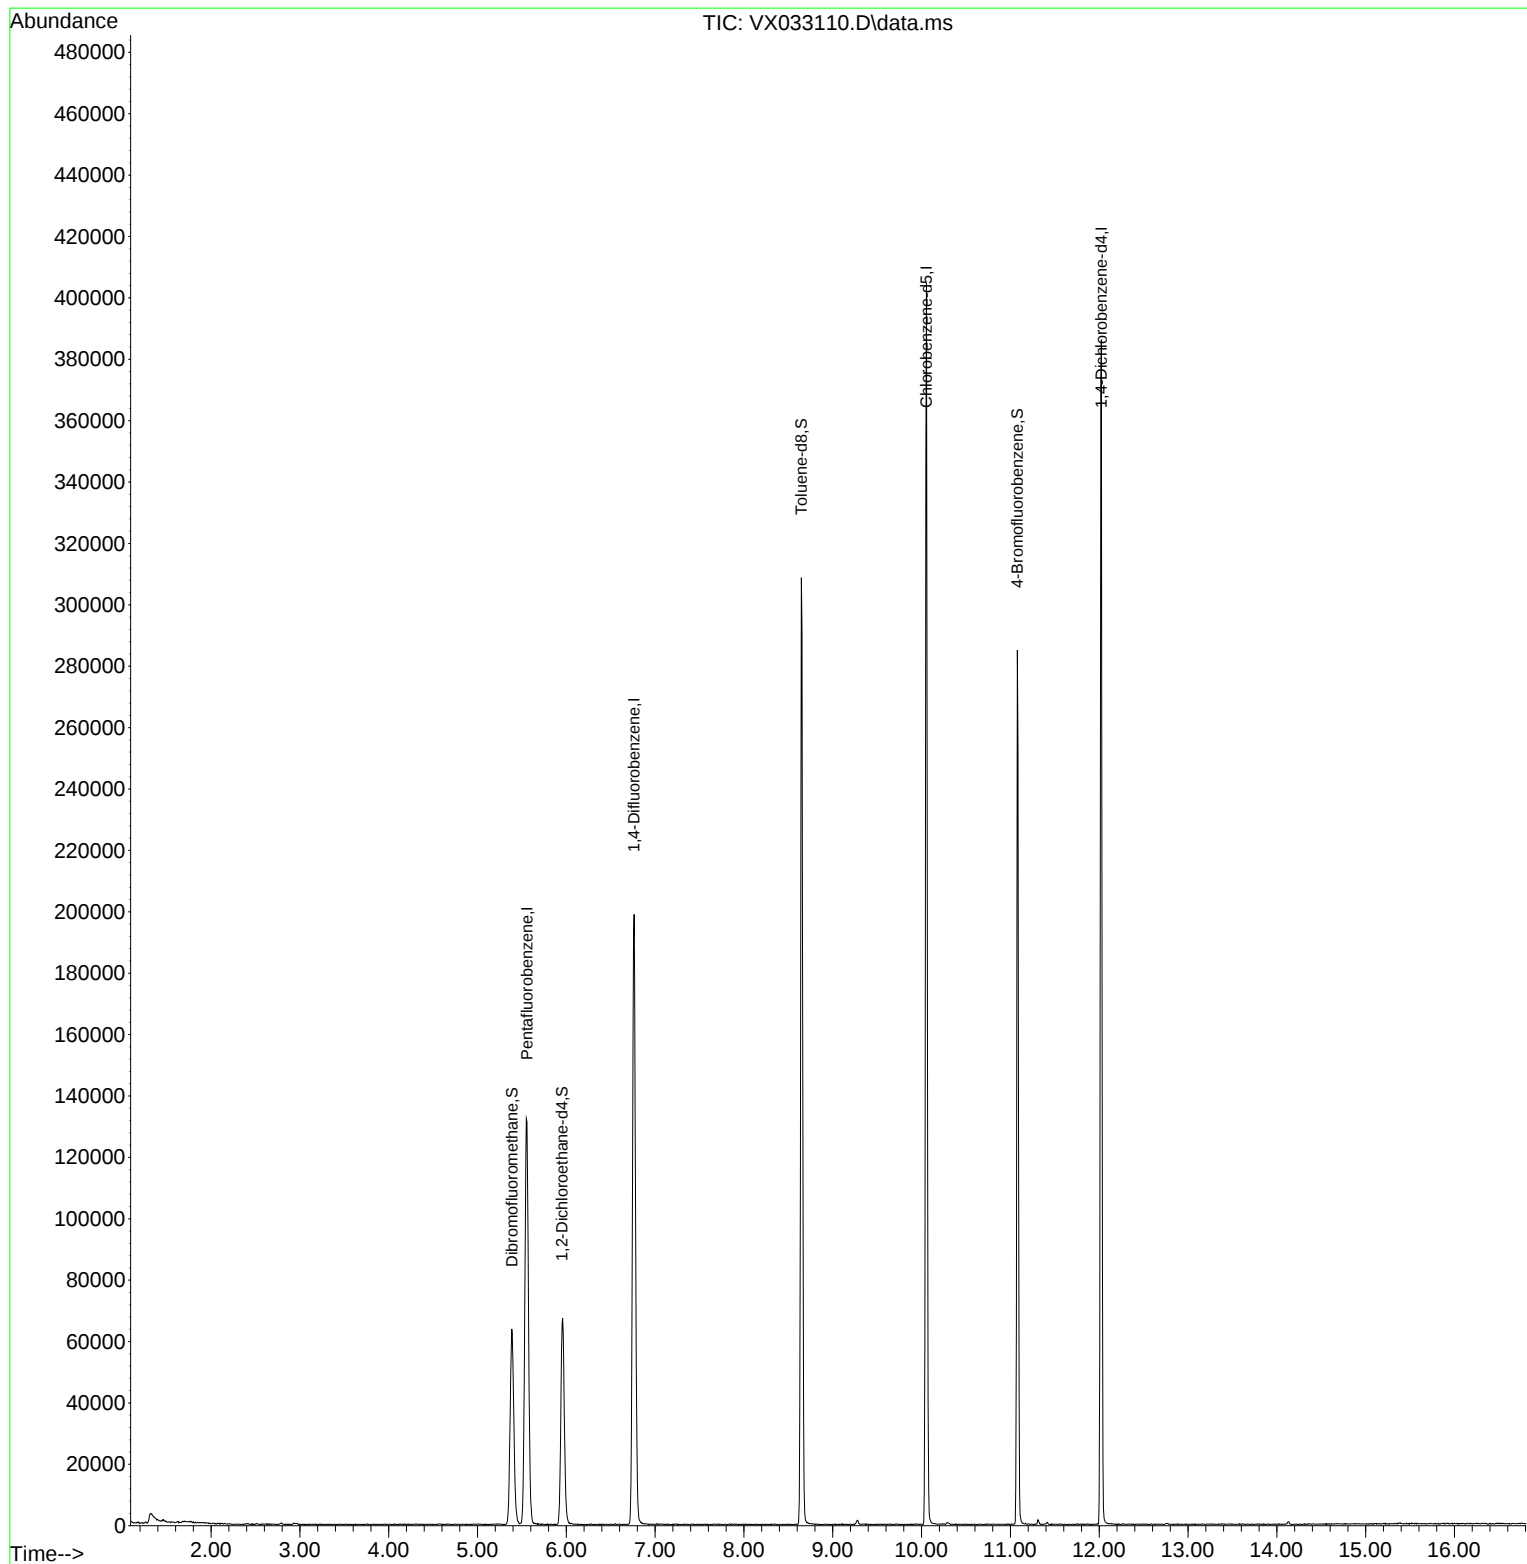


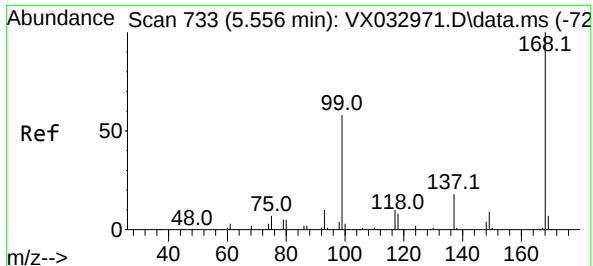

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.000 min
Lab File: VX033110.D
Acq: 29 Nov 2022 12:16




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:168 Resp: 125835
Ion Ratio Lower Upper
168 100
99 59.2 46.1 69.1

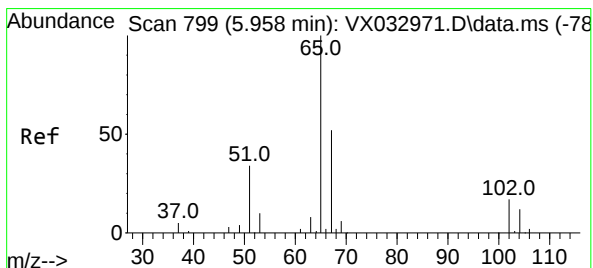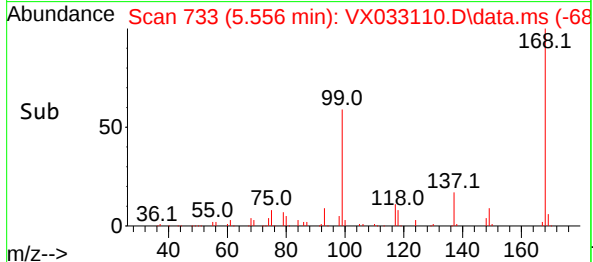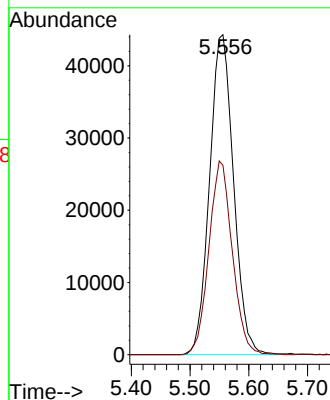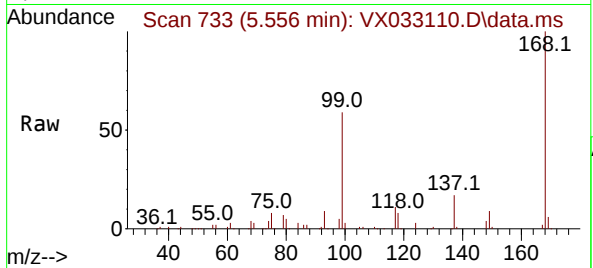

#33
1,2-Dichloroethane-d4
Concen: 56.795 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX033110.D
Acq: 29 Nov 2022 12:16

Tgt Ion: 65 Resp: 69311
Ion Ratio Lower Upper
65 100
67 50.9 0.0 101.8


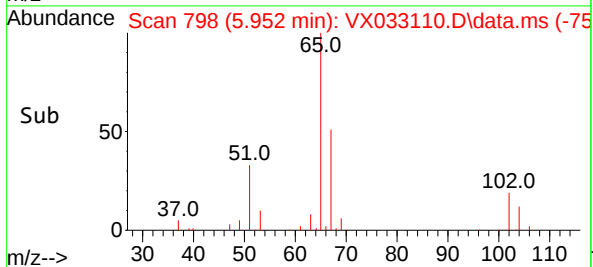
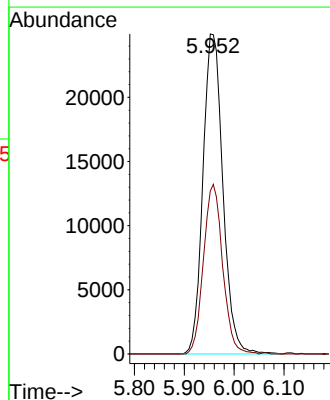
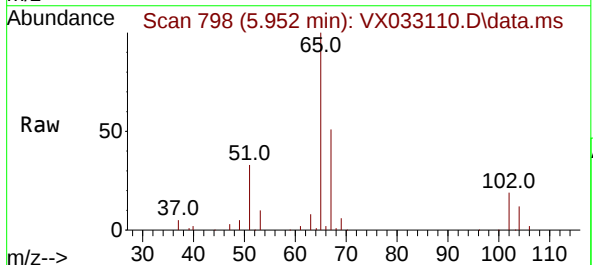


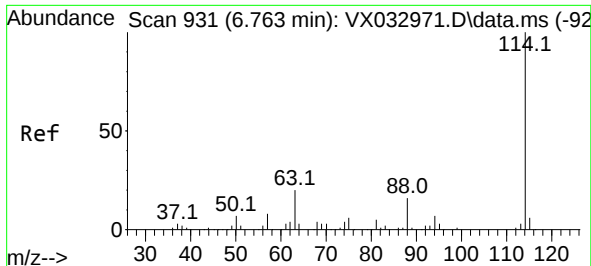

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX033110.D
Acq: 29 Nov 2022 12:16




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:114 Resp: 203844
Ion Ratio Lower Upper
114 100
63 19.2 0.0 41.6
88 15.2 0.0 33.4

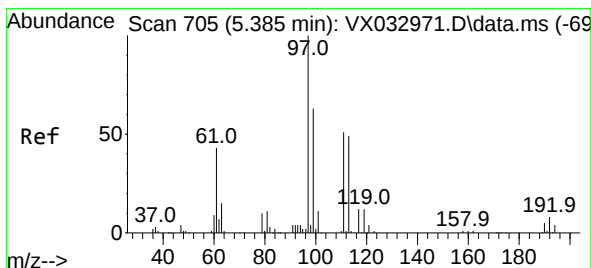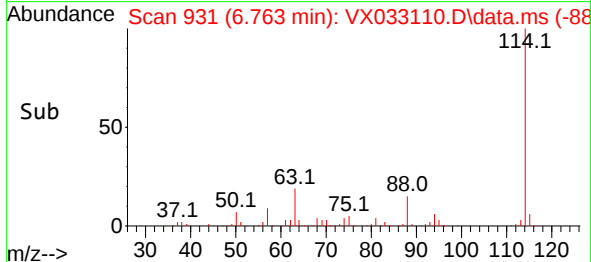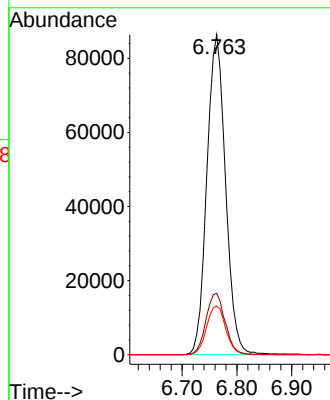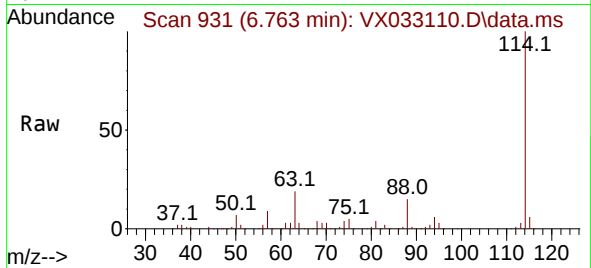

#35
Dibromofluoromethane
Concen: 48.250 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX033110.D
Acq: 29 Nov 2022 12:16

Tgt Ion:113 Resp: 55449
Ion Ratio Lower Upper
113 100
111 99.9 82.4 123.6
192 18.9 15.4 23.2


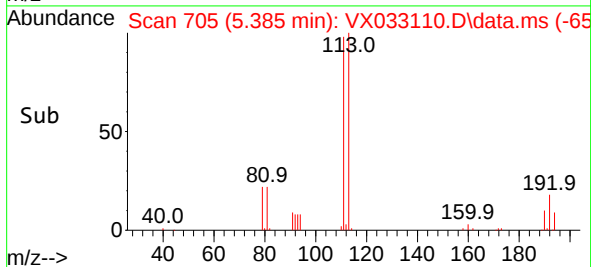
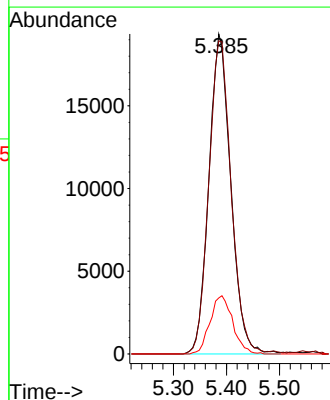
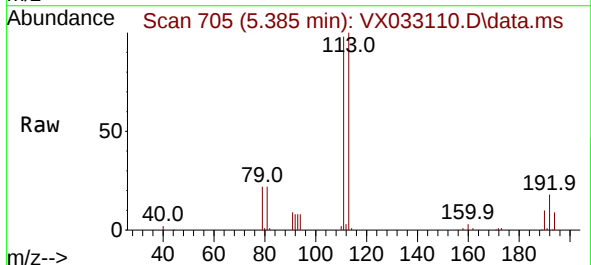


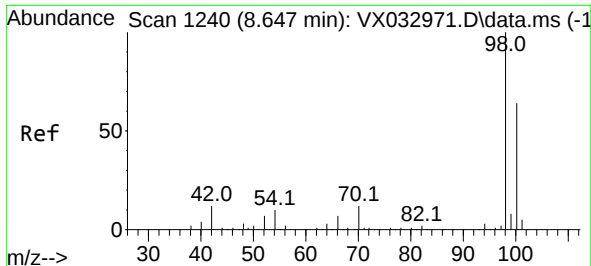

#50
Toluene-d8
Concen: 53.839 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX033110.D
Acq: 29 Nov 2022 12:16




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion: 98 Resp: 185587
Ion Ratio Lower Upper
98 100
100 63.6 50.9 76.3

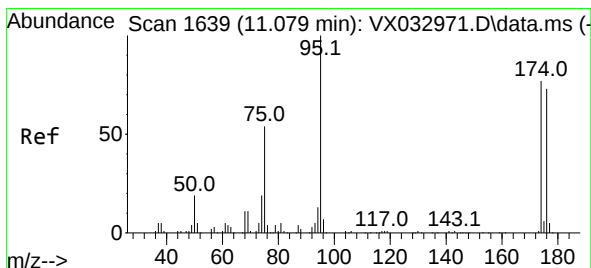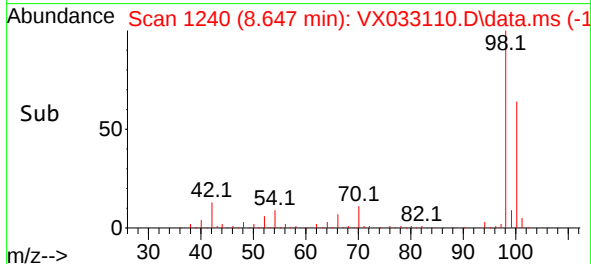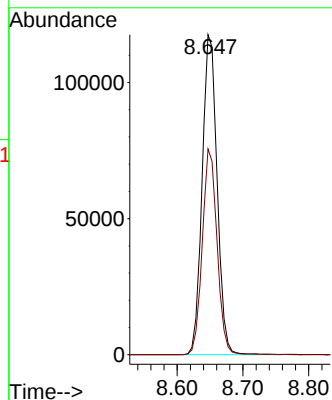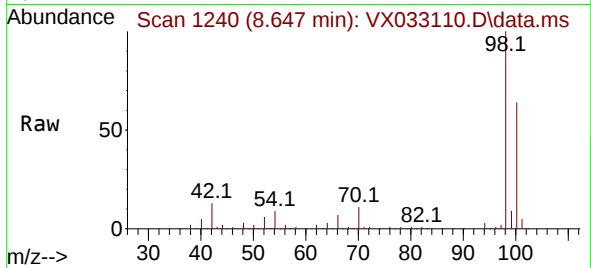

#62
4-Bromofluorobenzene
Concen: 48.242 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX033110.D
Acq: 29 Nov 2022 12:16

Tgt Ion: 95 Resp: 72825
Ion Ratio Lower Upper
95 100
174 79.8 0.0 164.0
176 78.8 0.0 154.4


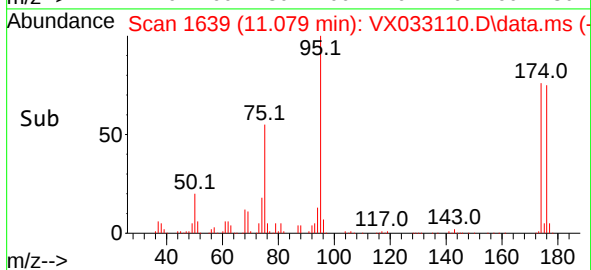
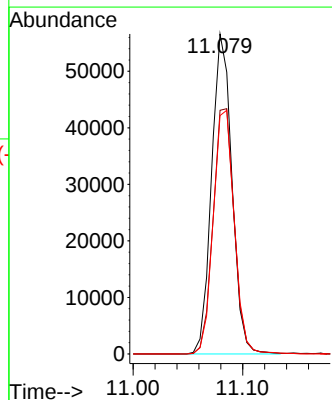
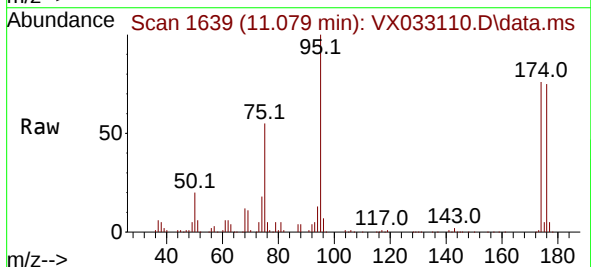


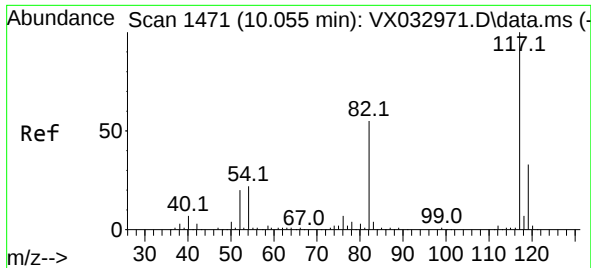

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX033110.D
Acq: 29 Nov 2022 12:16

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Tgt Ion:117 Resp: 178746
Ion Ratio Lower Upper
117 100
82 54.3 44.3 66.5
119 32.2 25.7 38.5

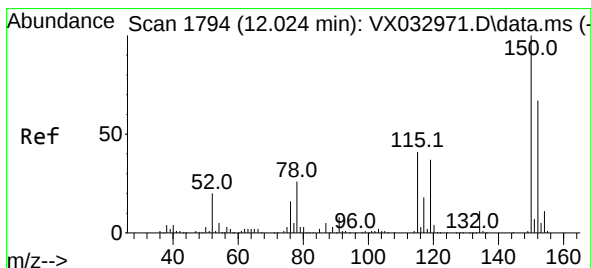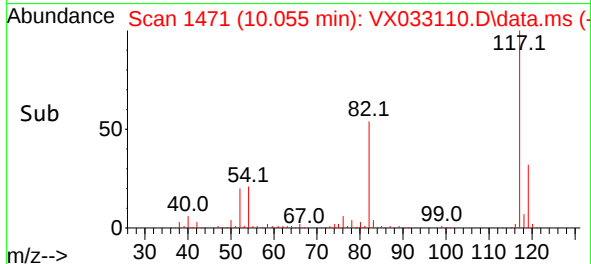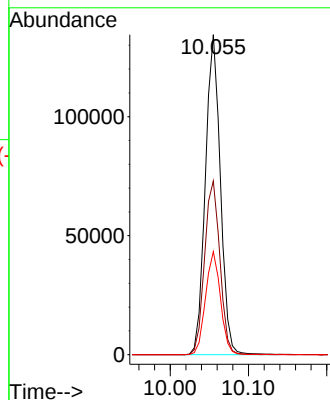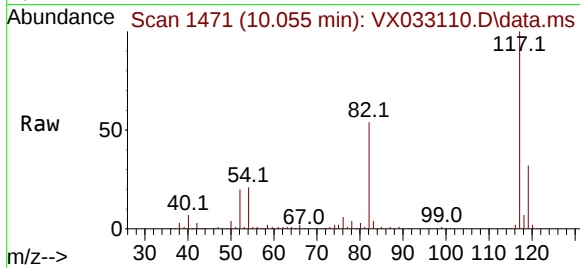

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX033110.D
Acq: 29 Nov 2022 12:16

Tgt Ion:152 Resp: 81029
Ion Ratio Lower Upper
152 100
115 60.8 44.0 132.0
150 159.2 0.0 351.8

