

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112922\
 Data File : VX033114.D
 Acq On : 29 Nov 2022 13:47
 Operator : JC/MD
 Sample : N5741-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-37

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Title : SW846 8260

Signal : TIC: VX033114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	30	35	42	rBV2	11094	37543	6.81%	1.098%
2	2.428	210	220	229	rVB	19358	34690	6.29%	1.015%
3	2.983	300	311	324	rBV2	13847	46949	8.52%	1.373%
4	3.111	324	332	347	rVB2	53280	124489	22.58%	3.642%
5	3.764	429	439	448	rVB2	4163	11544	2.09%	0.338%
6	4.306	521	528	530	rBV2	3197	5911	1.07%	0.173%
7	5.385	693	705	721	rBV	64727	188300	34.16%	5.508%
8	5.550	722	732	746	rVB2	135522	383696	69.60%	11.224%
9	5.958	788	799	809	rBV	68646	182168	33.04%	5.329%
10	6.044	809	813	822	rVB3	5283	12494	2.27%	0.365%
11	6.763	920	931	943	rBV	202074	481361	87.32%	14.081%
12	8.647	1234	1240	1251	rBV	314923	492856	89.40%	14.417%
13	9.458	1366	1373	1378	rBV2	6166	10331	1.87%	0.302%
14	10.055	1465	1471	1481	rBV	405757	551275	100.00%	16.126%
15	11.079	1634	1639	1650	rBV	267317	336887	61.11%	9.855%
16	12.024	1788	1794	1803	rBV	411714	517978	93.96%	15.152%




Sum of corrected areas: 3418472

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112922\
Data File : VX033114.D
Acq On : 29 Nov 2022 13:47
Operator : JC/MD
Sample : N5741-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

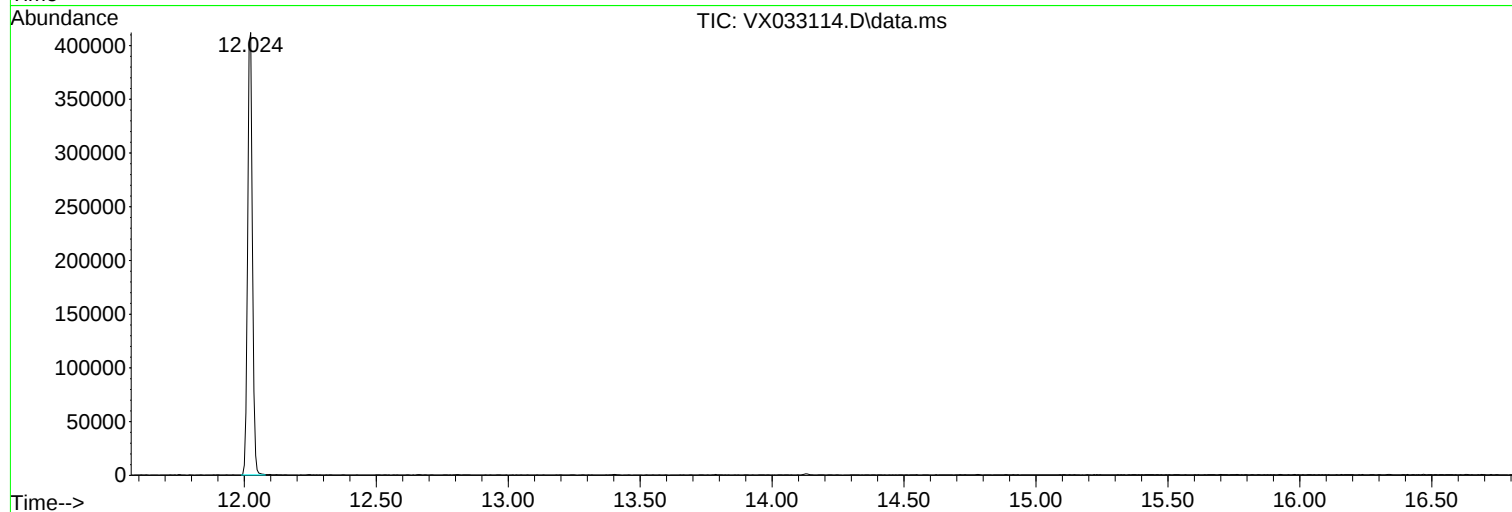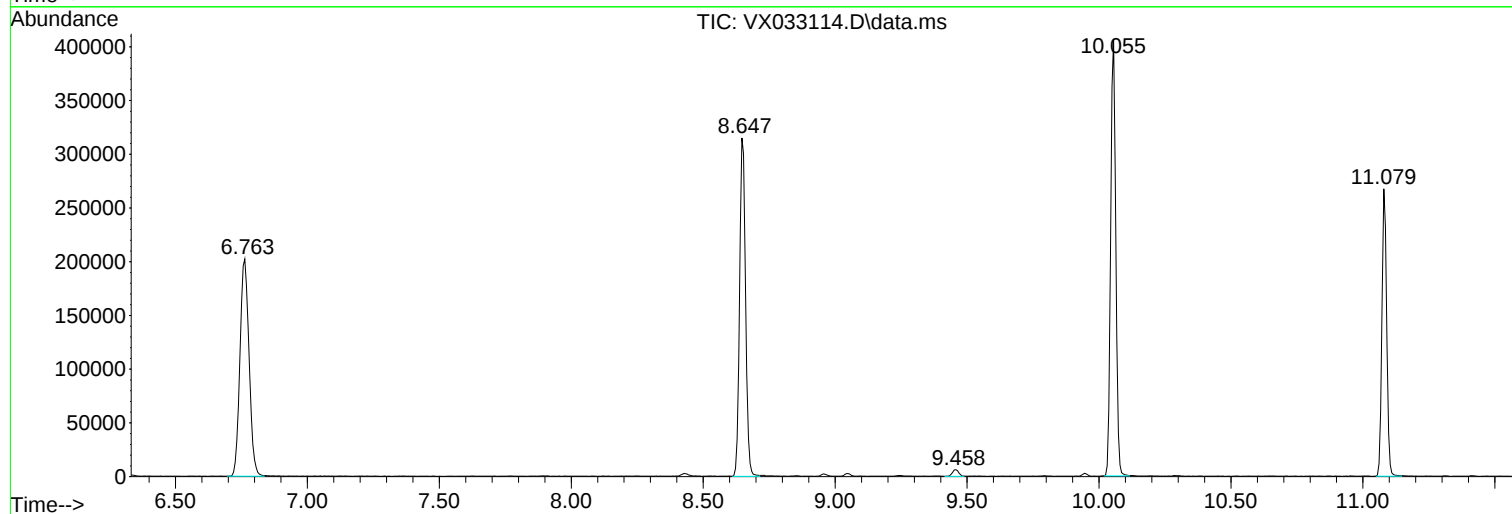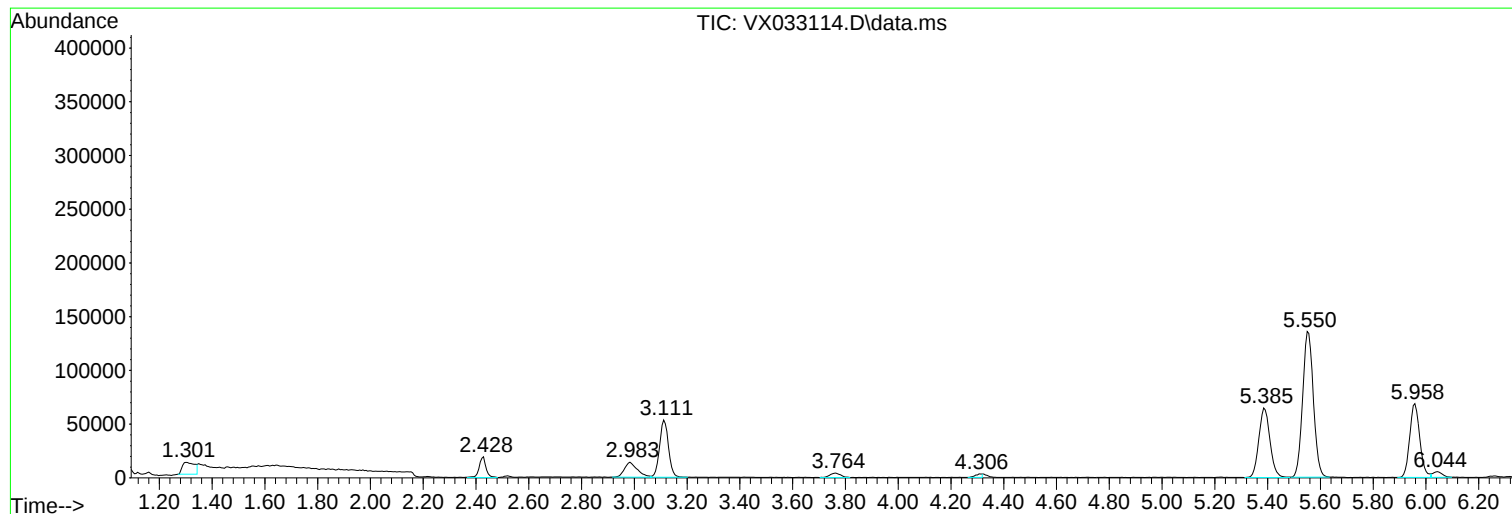

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112922\
Data File : VX033114.D
Acq On : 29 Nov 2022 13:47
Operator : JC/MD
Sample : N5741-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112922\
Data File : VX033114.D
Acq On : 29 Nov 2022 13:47
Operator : JC/MD
Sample : N5741-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc