
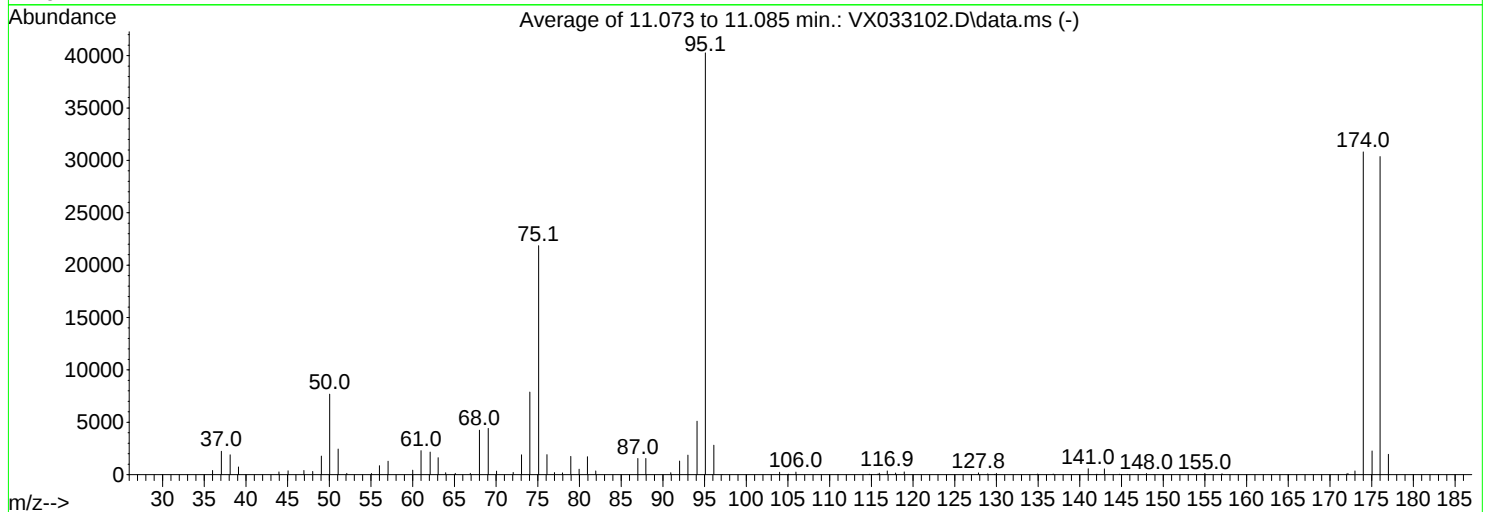


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112922\
Data File : VX033102.D
Acq On : 29 Nov 2022 08:45
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Title : SW846 8260
Last Update : Tue Nov 22 13:58:46 2022

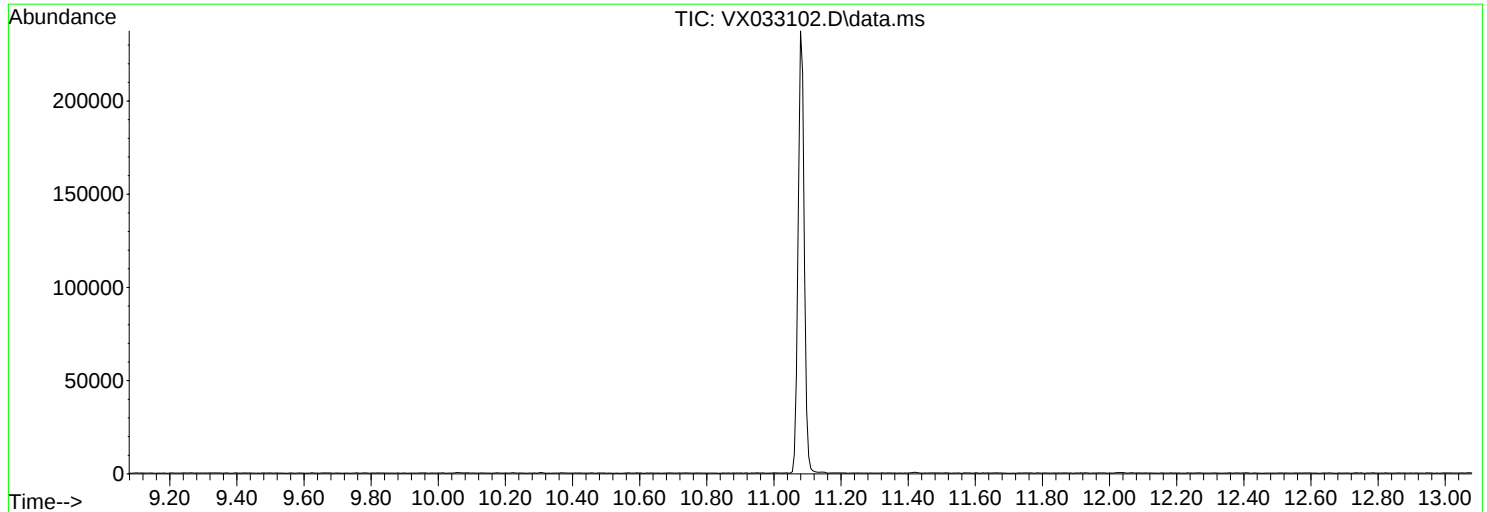

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	7691	PASS
75	95	30	60	54.3	21853	PASS
95	95	100	100	100.0	40267	PASS
96	95	5	9	7.0	2817	PASS
173	174	0.00	2	1.1	353	PASS
174	95	50	100	76.5	30816	PASS
175	174	5	9	7.3	2263	PASS
176	174	95	101	98.6	30371	PASS
177	176	5	9	6.4	1943	PASS