


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX113018\
Data File : VX006216.D
Acq On : 30 Nov 2018 08:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
Title : SW846 8260
Last Update : Fri Nov 30 03:55:33 2018

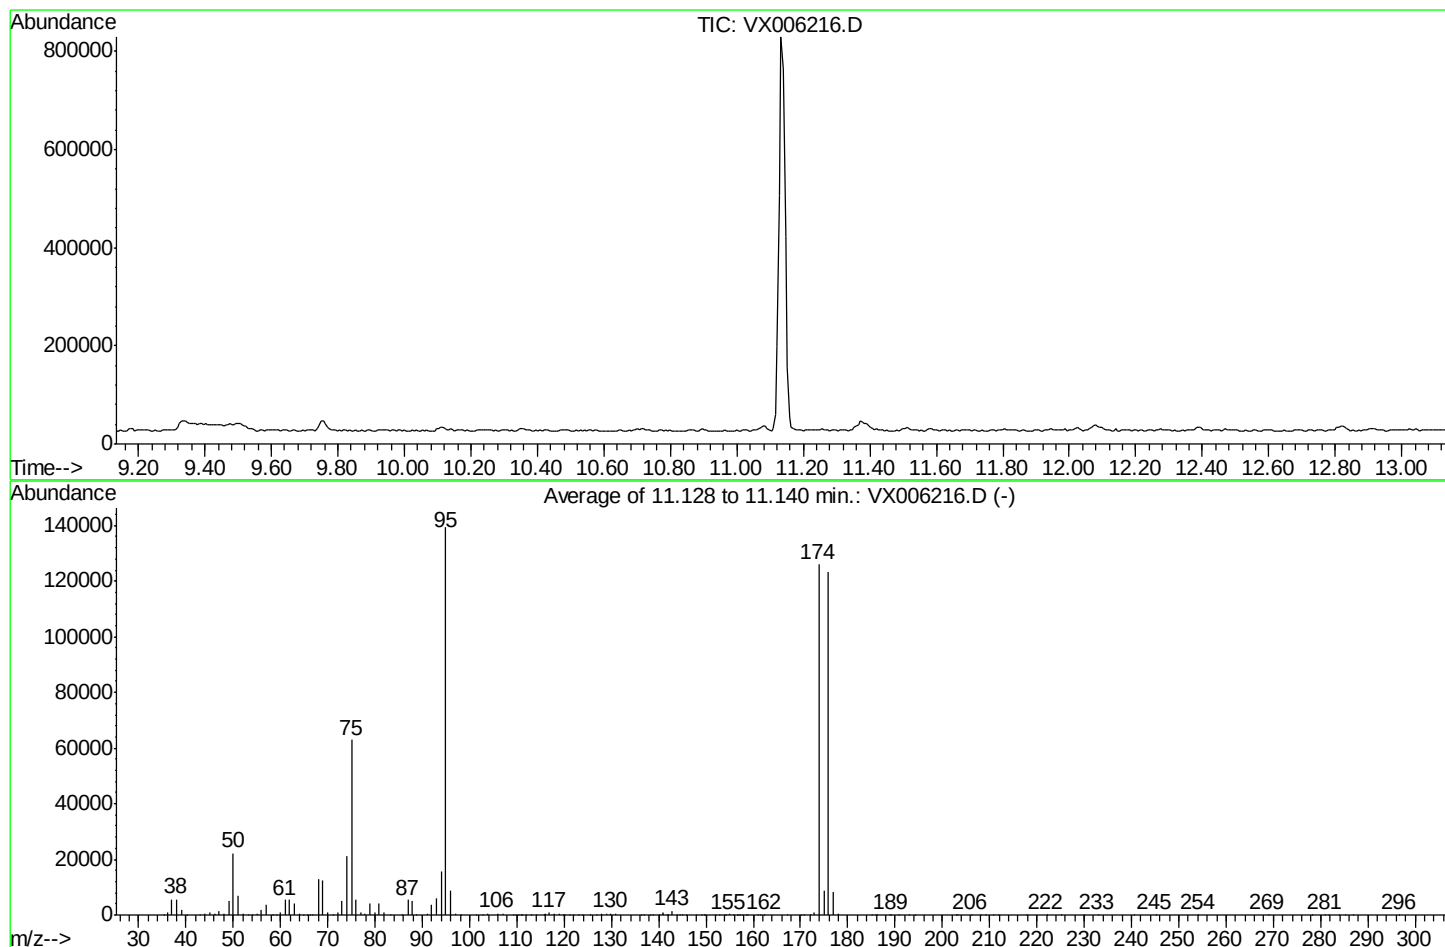

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	22318	PASS
75	95	30	60	45.1	62907	PASS
95	95	100	100	100.0	139340	PASS
96	95	5	9	6.3	8789	PASS
173	174	0.00	2	0.9	1073	PASS
174	95	50	100	90.4	125896	PASS
175	174	5	9	6.8	8561	PASS
176	174	95	101	97.8	123136	PASS
177	176	5	9	6.7	8248	PASS