

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX113022\
Data File : VX033142.D
Acq On : 30 Nov 2022 19:10
Operator : JC/MD
Sample : N5815-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-08

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M

Title : SW846 8260

Signal : TIC: VX033142.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.752	105	109	115	rVB2	5085	6805	1.21%	0.216%
2	5.391	694	706	720	rBV	63014	184576	32.74%	5.855%
3	5.550	720	732	748	rVV	135507	386491	68.56%	12.260%
4	5.958	787	799	816	rBV	68134	180782	32.07%	5.735%
5	6.763	921	931	951	rBV2	205503	489675	86.86%	15.534%
6	8.647	1234	1240	1250	rBV	309975	479484	85.06%	15.210%
7	10.055	1465	1471	1486	rBV	414321	563720	100.00%	17.883%
8	11.079	1634	1639	1649	rBV	259532	334772	59.39%	10.620%
9	12.024	1788	1794	1802	rBV	413722	526041	93.32%	16.687%




Sum of corrected areas: 3152346

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX113022\
Data File : VX033142.D
Acq On : 30 Nov 2022 19:10
Operator : JC/MD
Sample : N5815-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

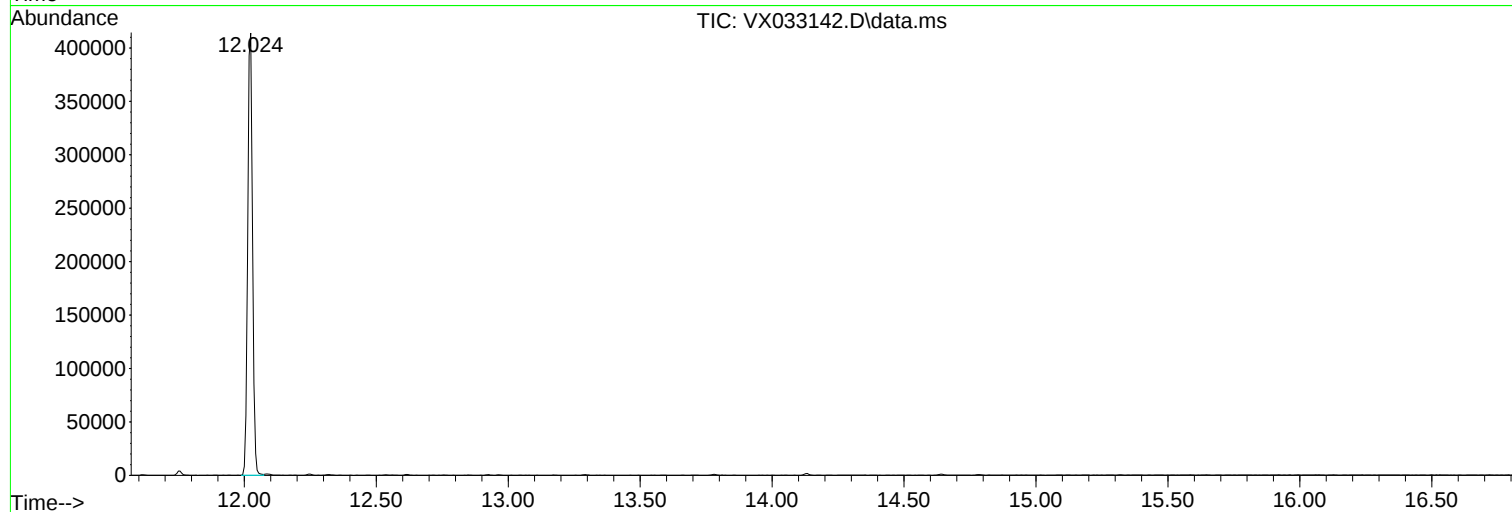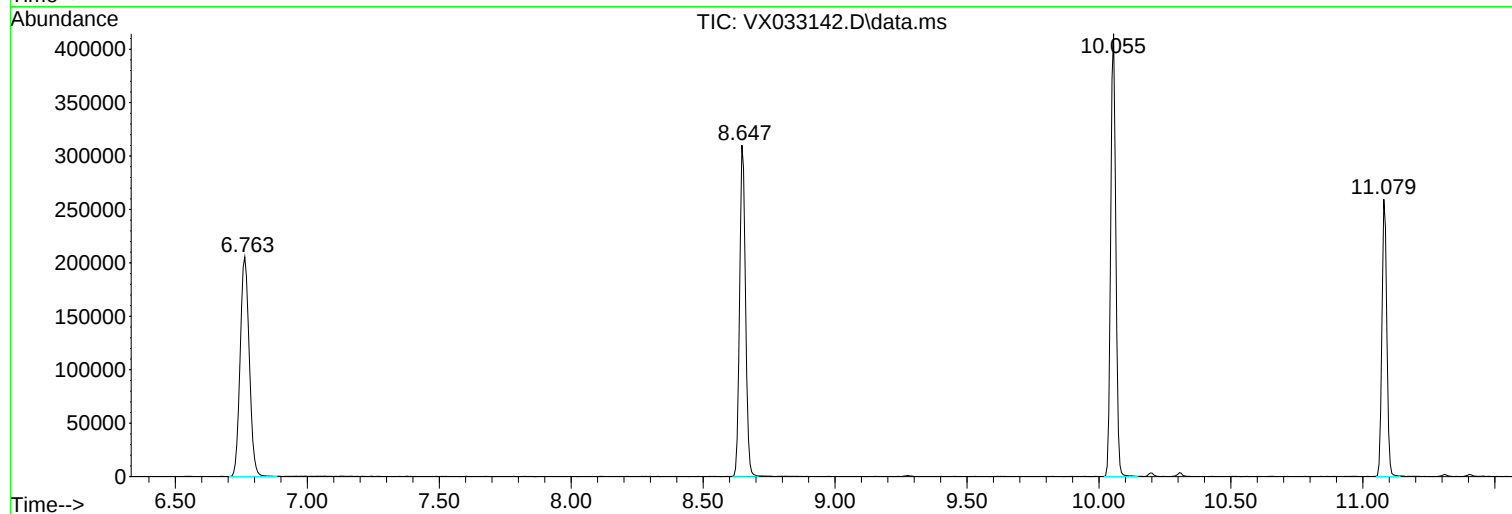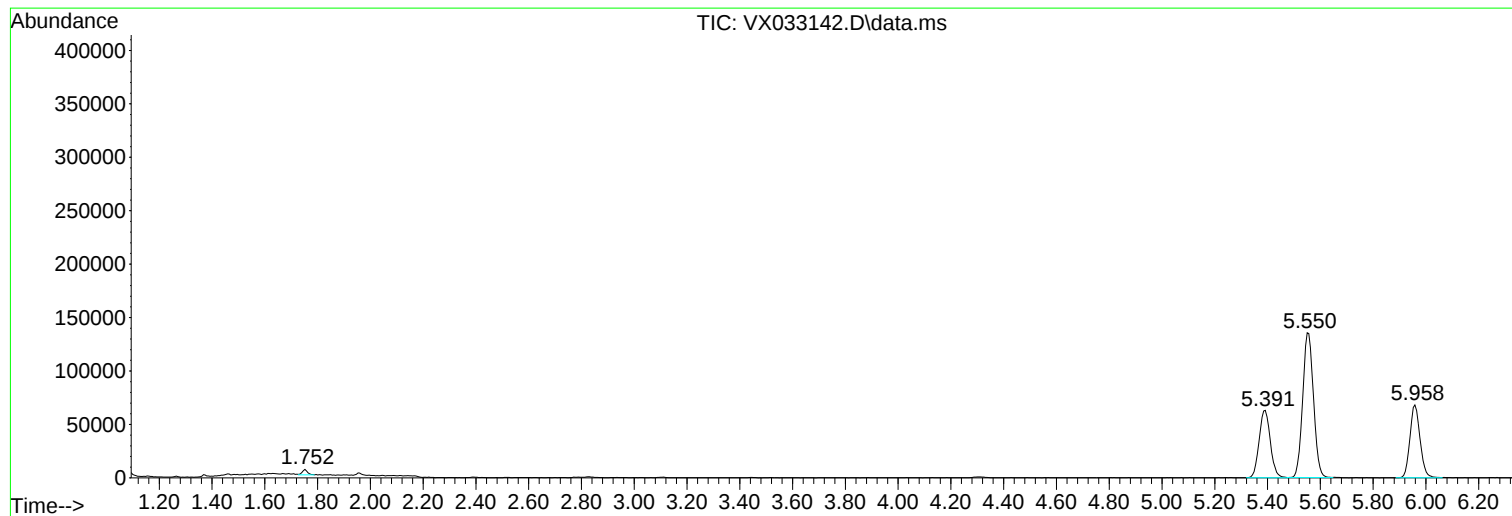

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX113022\
Data File : VX033142.D
Acq On : 30 Nov 2022 19:10
Operator : JC/MD
Sample : N5815-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX113022\
Data File : VX033142.D
Acq On : 30 Nov 2022 19:10
Operator : JC/MD
Sample : N5815-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc