


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX113023\
Data File : VX039058.D
Acq On : 30 Nov 2023 08:22
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X112423W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Mon Nov 27 03:22:25 2023

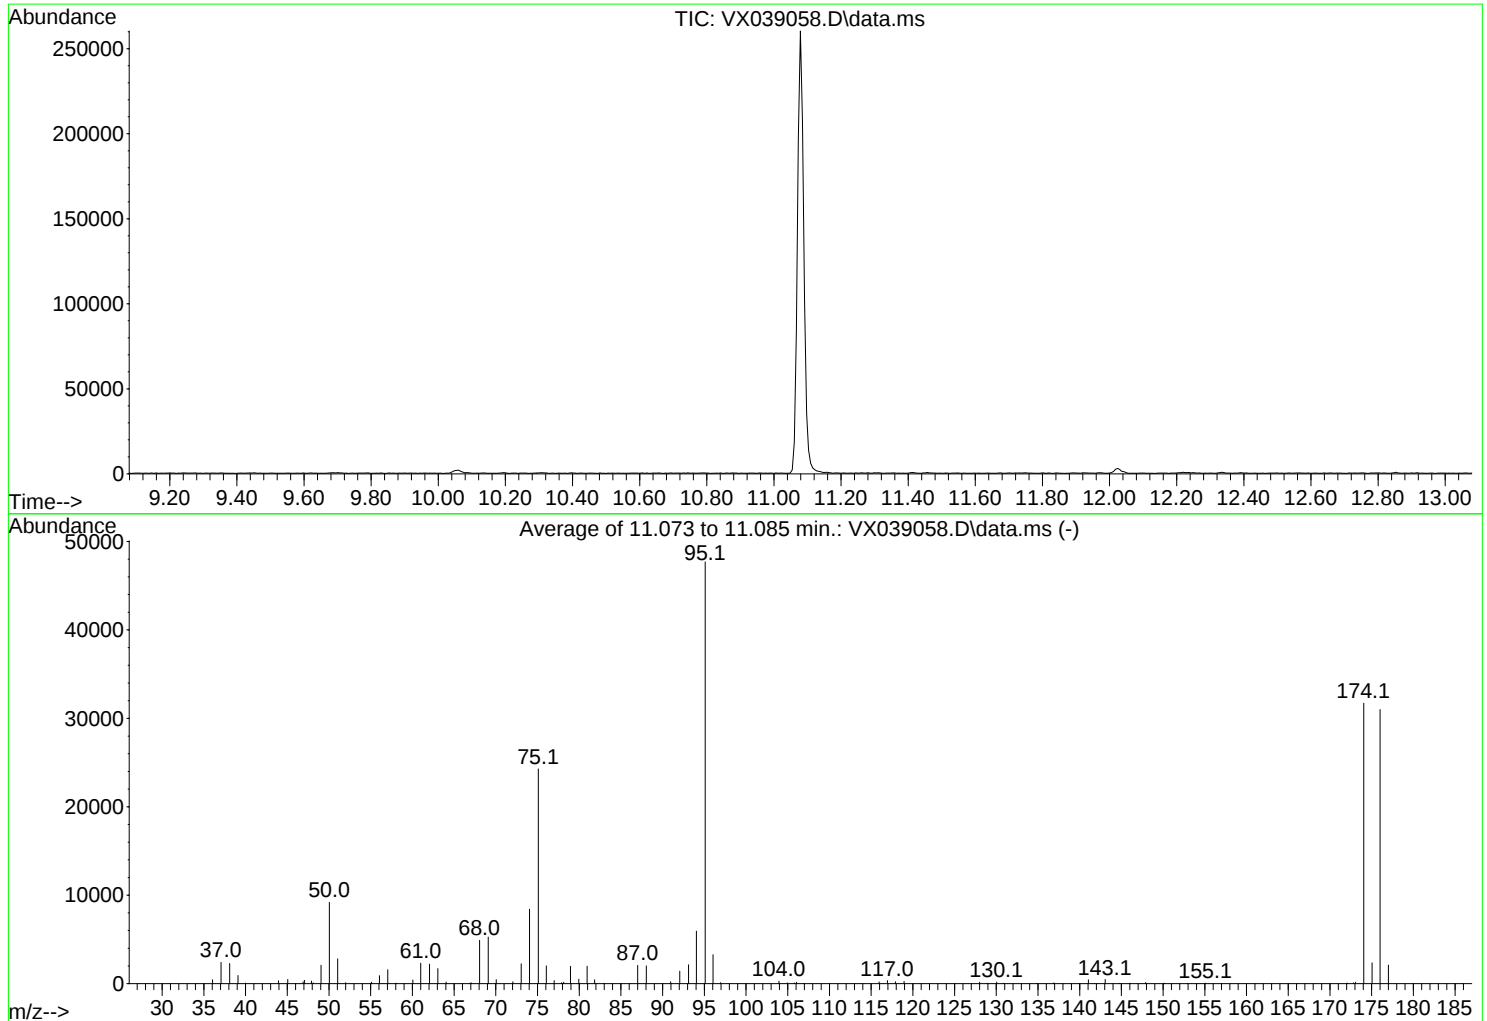

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	9197	PASS
75	95	30	60	50.9	24280	PASS
95	95	100	100	100.0	47701	PASS
96	95	5	9	6.9	3272	PASS
173	174	0.00	2	0.5	169	PASS
174	95	50	100	66.5	31715	PASS
175	174	5	9	7.4	2344	PASS
176	174	95	101	97.7	30992	PASS
177	176	5	9	6.8	2093	PASS