

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX120120\
 Data File : VX019693.D
 Acq On : 01 Dec 2020 14:24
 Operator : JC/MD
 Sample : PB133320ZHE#06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB133320ZHE#06

Quant Time: Dec 02 02:12:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 21 01:57:45 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	290378	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	483093	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	423831	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	179062	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.03	65	185391	49.24	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	98.48%
35) Dibromofluoromethane	5.46	113	146262	48.23	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	96.46%
50) Toluene-d8	8.70	98	580434	49.26	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	98.52%
62) 4-Bromofluorobenzene	11.12	95	193911	45.74	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	91.48%

Target Compounds


				Qvalue	
6) Chloroethane	1.69	64	2043	Below Cal	# 43
11) Tert butyl alcohol	3.00	59	4242	5.953	ug/l # 73
13) Acrolein	2.26	56	287	0.599	ug/l # 70
16) Acetone	2.43	43	11094	7.620	ug/l 98
18) Methyl Acetate	2.75	43	2445	1.311	ug/l 99
20) Methylene Chloride	2.83	84	22728	6.245	ug/l 98
25) 2-Butanone	4.64	43	8126	3.715	ug/l 97
29) Tetrahydrofuran	5.10	42	1961	1.405	ug/l # 70
31) Cyclohexane	5.62	56	5689	1.162	ug/l # 1
36) 1,1-Dichloropropene	5.62	75	21916	4.839	ug/l # 49
37) Ethyl Acetate	4.64	43	8126	1.911	ug/l # 67
38) Carbon Tetrachloride	5.63	117	28254	6.445	ug/l # 17
43) Isopropyl Acetate	6.42	43	32964	4.612	ug/l 99
48) Methyl methacrylate	7.65	41	7940	2.372	ug/l # 9
49) 1,4-Dioxane	7.85	88	311	4.092	ug/l # 1
51) 4-Methyl-2-Pentanone	8.59	43	100082	24.013	ug/l # 46
54) cis-1,3-Dichloropropene	8.59	75	53523	9.816	ug/l # 58
57) 1,3-Dichloropropane	9.52	76	28780	4.958	ug/l # 44
59) 2-Hexanone	9.52	43	337836	106.878	ug/l # 48
70) Styrene	10.70	104	242	1.669	ug/l # 77
74) N-amyl acetate	10.80	43	1697	0.366	ug/l # 43
76) 1,2,3-Trichloropropane	11.12	75	94017	24.059	ug/l # 37
80) 1,3,5-Trimethylbenzene	11.49	105	2087	0.201	ug/l 99
81) trans-1,4-Dichloro-2-buten	11.12	75	94017	63.714	ug/l # 12
95) Naphthalene	13.81	128	452	2.211	ug/l # 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX120120\
Data File : VX019693.D
Acq On : 01 Dec 2020 14:24
Operator : JC/MD
Sample : PB133320ZHE#06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB133320ZHE#06

Quant Time: Dec 02 02:12:23 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 21 01:57:45 2020
Response via : Initial Calibration

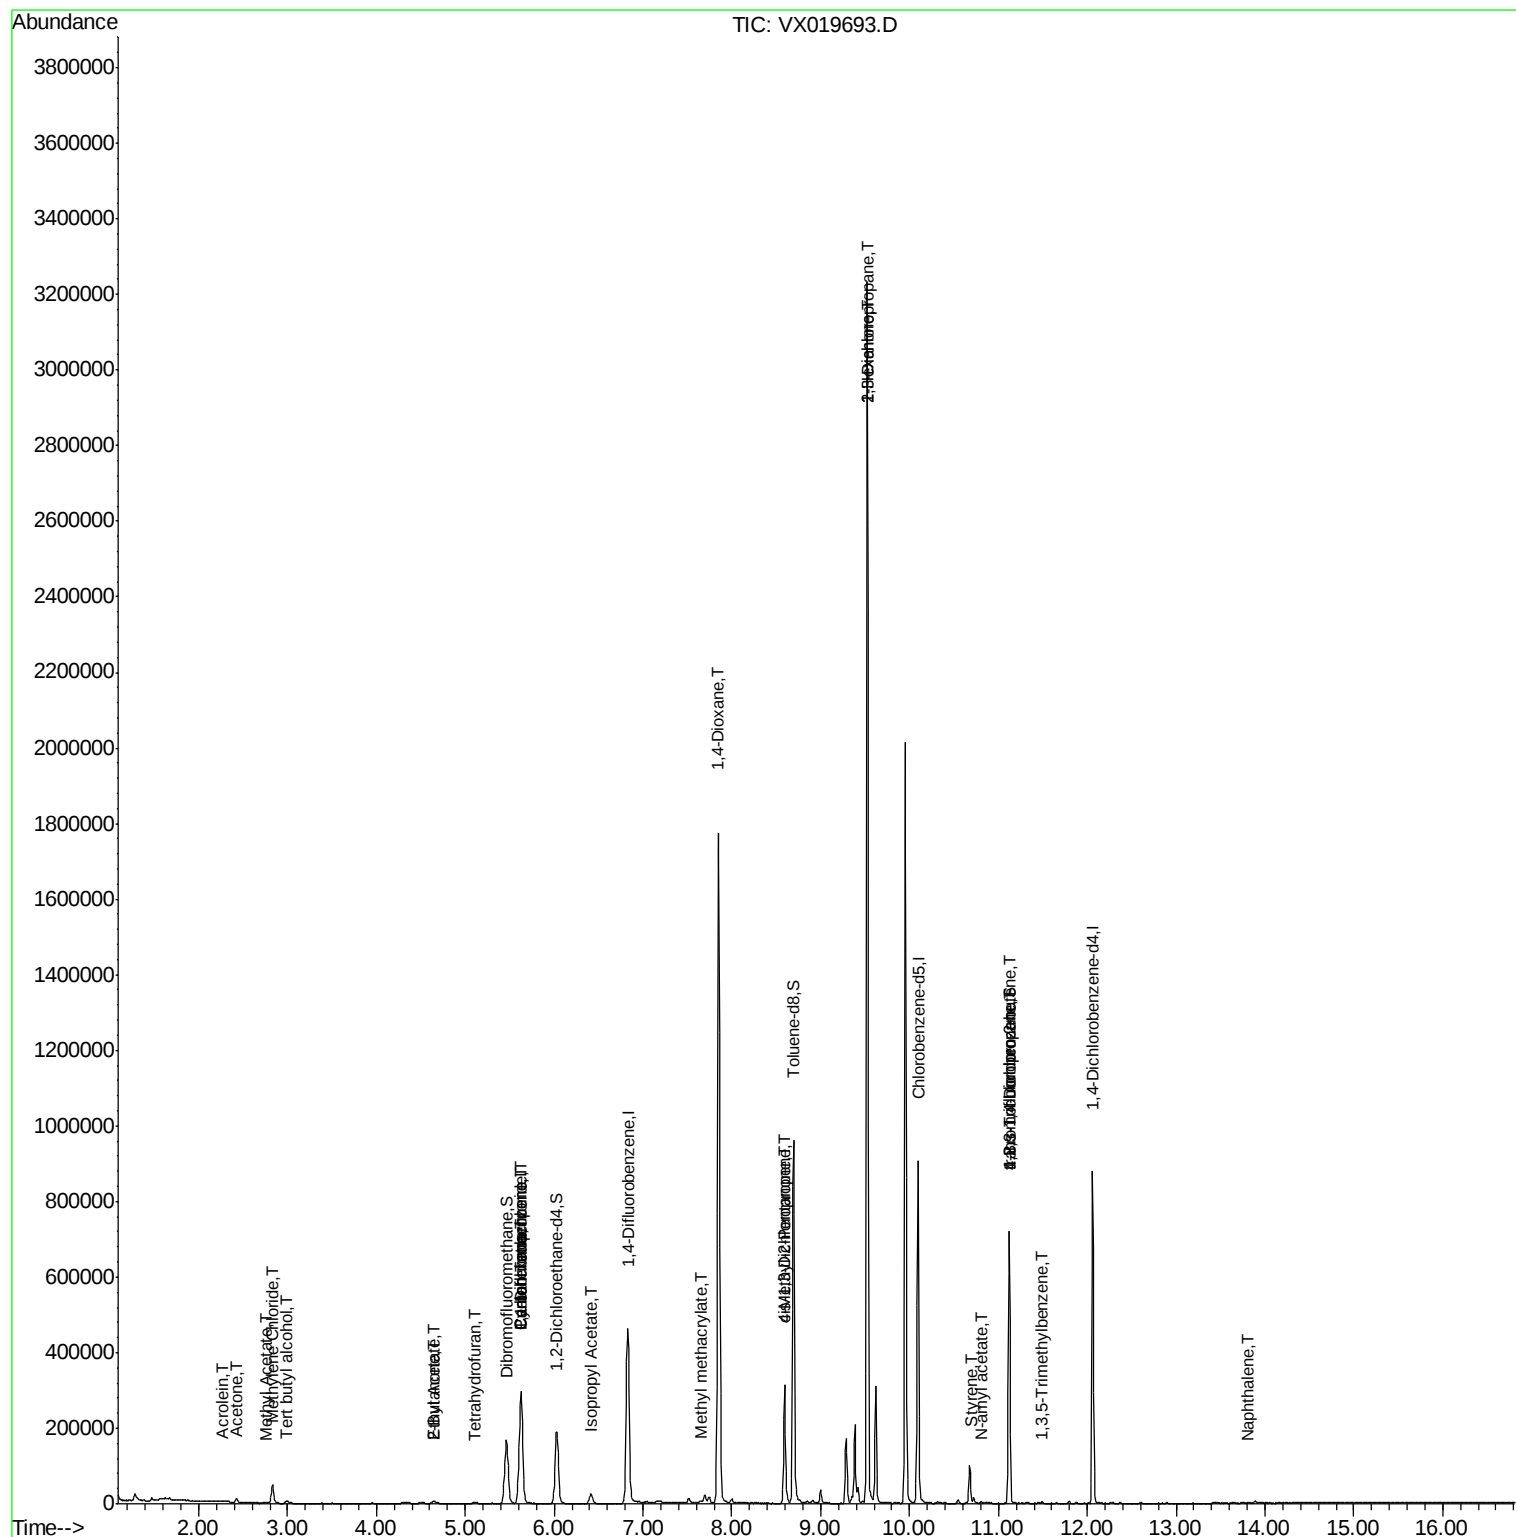



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.00 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24

Instrument :

MSVOA_X

ClientSampleId :


PB133320ZHE#06

Tot Ion:168 Resp: 290378

Ion Ratio Lower Upper




168 100

99 58.2 45.8 68.6

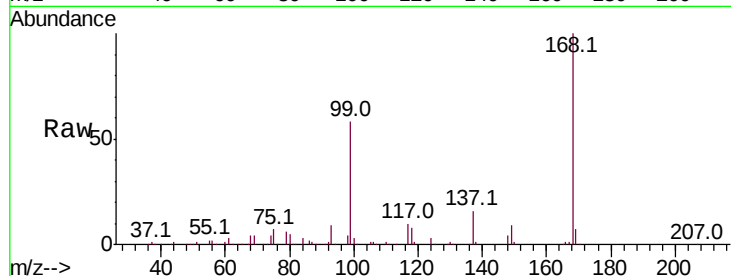

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

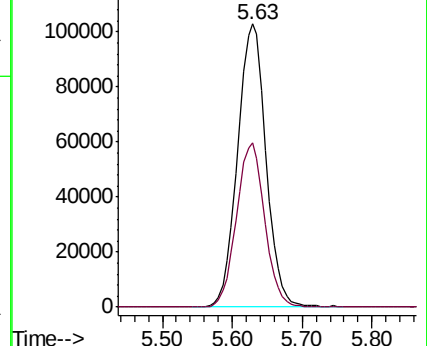

#6

Chloroethane

Concen: Below Cal

RT: 1.69 min Scan# 99

Delta R.T. 0.00 min

Lab File: VX019693.D


Acq: 01 Dec 2020 14:24

Tgt Ion: 64 Resp: 2043

Ion Ratio Lower Upper



64 100


66 1.3 27.1 40.7#



Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0

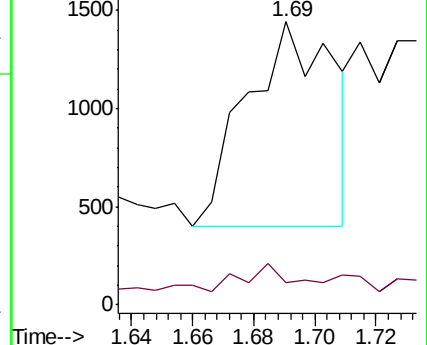

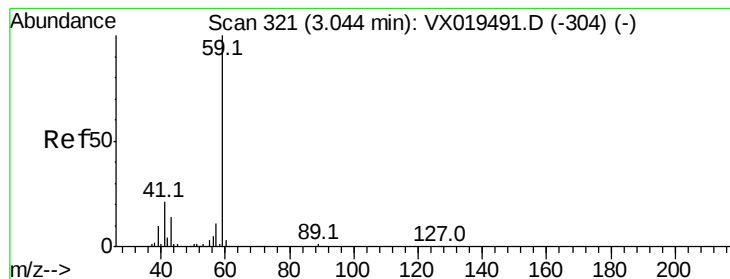

#11

Tert butyl alcohol

Concen: 5.953 ug/l

RT: 3.00 min Scan# 313

Delta R.T. -0.05 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24

Instrument :

MSVOA_X

ClientSampleId :


PB133320ZHE#06

Tot Ion: 59 Resp: 4242

Ion Ratio Lower Upper




59 100

57 0.0 7.9 11.9#

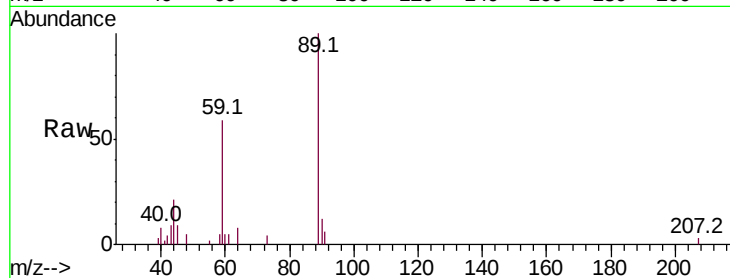

Abundance Ion 59.00 (58.70 to 59.70): VX0

Ion 57.00 (56.70 to 57.70): VX0

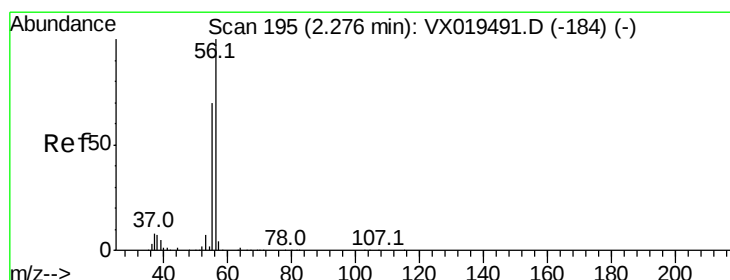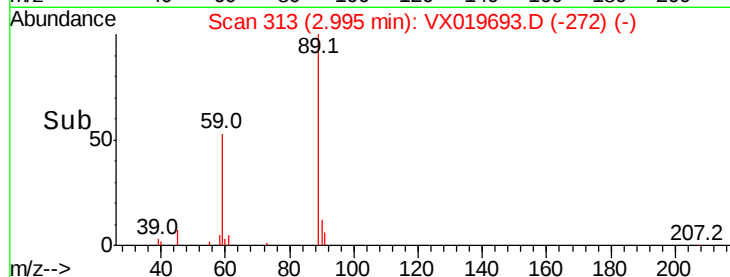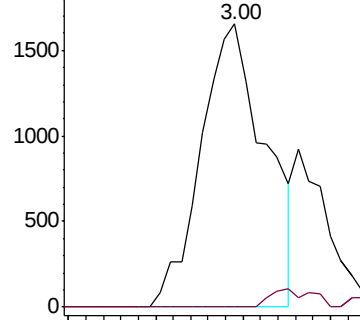

#13

Acrolein

Concen: 0.599 ug/l

RT: 2.26 min Scan# 193

Delta R.T. -0.01 min

Lab File: VX019693.D


Acq: 01 Dec 2020 14:24

Tgt Ion: 56 Resp: 287

Ion Ratio Lower Upper



56 100


55 45.3 55.5 83.3#

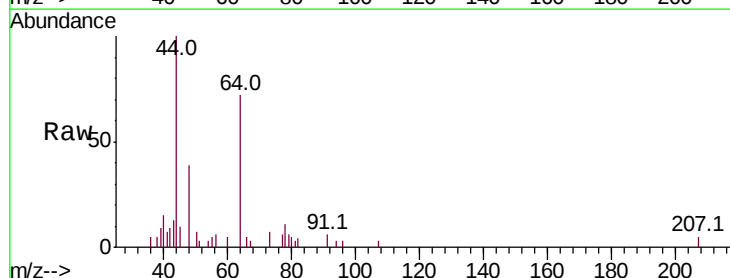

Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

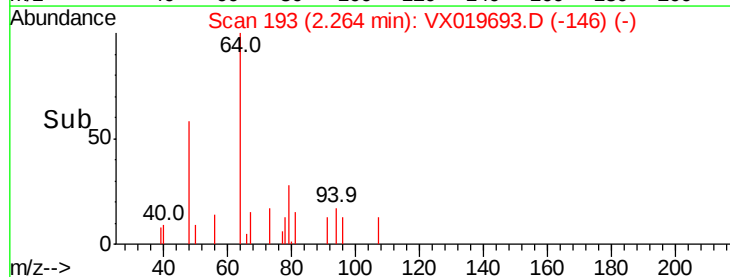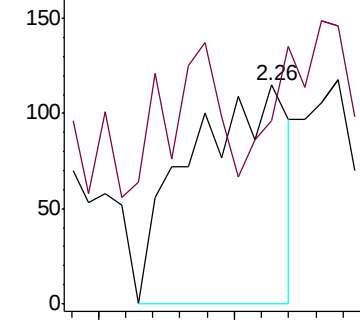



#16

Acetone

Concen: 7.620 ug/l

RT: 2.43 min Scan# 220

Delta R.T. -0.00 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24

Instrument :

MSVOA_X

ClientSampleId :





PB133320ZHE#06

Tot Ion: 43 Resp: 11094

Ion Ratio Lower Upper

43 100

58 35.5 27.4 41.2

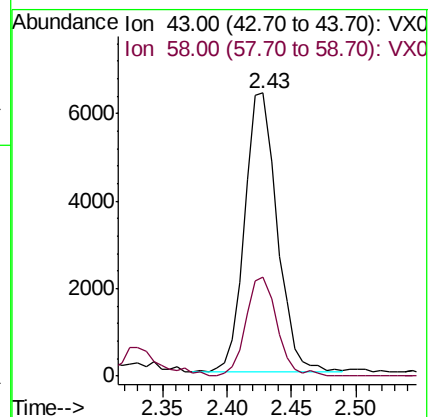

#18

Methyl Acetate

Concen: 1.311 ug/l

RT: 2.75 min Scan# 273

Delta R.T. 0.00 min

Lab File: VX019693.D




Acq: 01 Dec 2020 14:24


Tgt Ion: 43 Resp: 2445

Ion Ratio Lower Upper

43 100

74 27.5 22.2 33.4



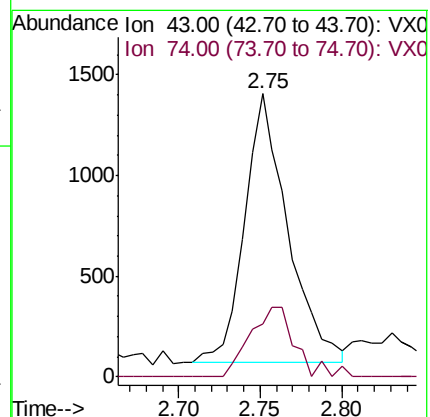





#20
Methvlene Chloride
Concen: 6.245 ug/l
RT: 2.83 min Scan# 286
Delta R.T. -0.00 min
Lab File: VX019693.D
Acq: 01 Dec 2020 14:24




Instrument :
MSVOA_X
ClientSampleId :
PB133320ZHE#06


Tot Ion: 84 Resp: 22728
Ion Ratio Lower Upper
84 100
49 110.4 88.5 132.7
51 33.2 28.0 42.0
86 62.4 53.0 79.4

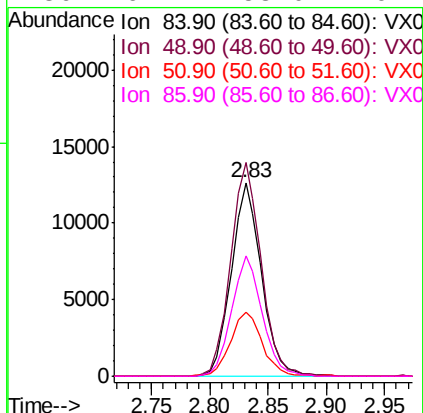

#25
2-Butanone
Concen: 3.715 ug/l
RT: 4.64 min Scan# 583
Delta R.T. -0.00 min
Lab File: VX019693.D
Acq: 01 Dec 2020 14:24

Tgt Ion: 43 Resp: 8126
Ion Ratio Lower Upper
43 100
72 31.7 24.0 36.0


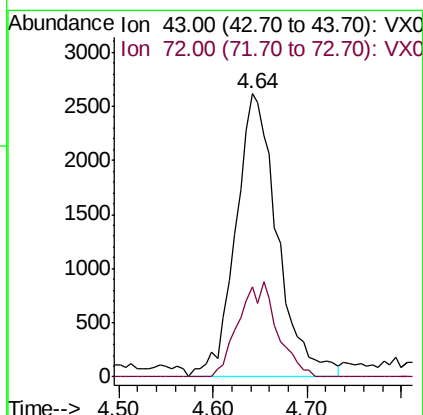




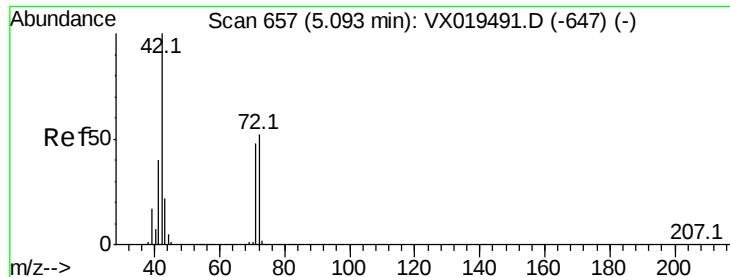

#29
Tetrahydrofuran
Concen: 1.405 ug/l
RT: 5.10 min Scan# 659
Delta R.T. 0.01 min
Lab File: VX019693.D
Acq: 01 Dec 2020 14:24




Instrument :
MSVOA_X
ClientSampleId :
PB133320ZHE#06


Tot Ion: 42 Resp: 1961
Ion Ratio Lower Upper
42 100
72 23.4 42.6 63.8#
71 37.6 39.0 58.6#

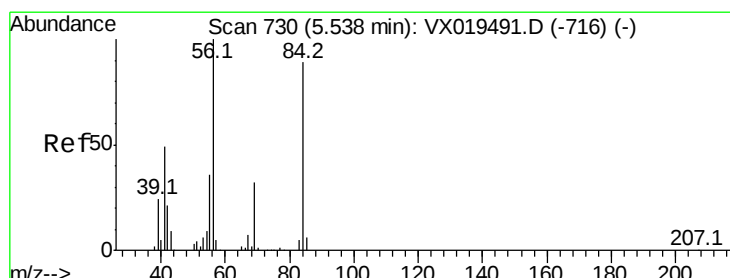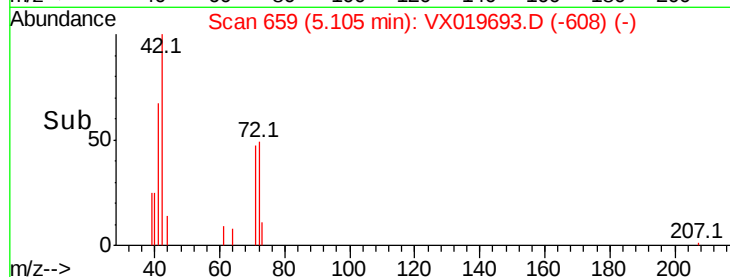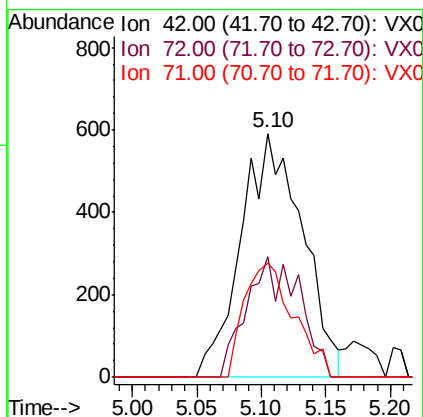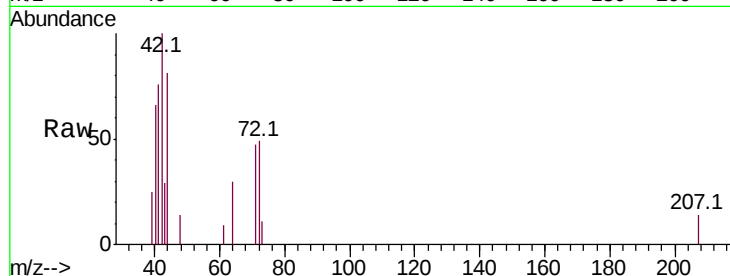

#31
Cyclohexane
Concen: 1.162 ug/l
RT: 5.62 min Scan# 744
Delta R.T. 0.09 min
Lab File: VX019693.D
Acq: 01 Dec 2020 14:24

Tgt Ion: 56 Resp: 5689
Ion Ratio Lower Upper
56 100
69 193.3 25.5 38.3#
84 155.3 71.1 106.7#

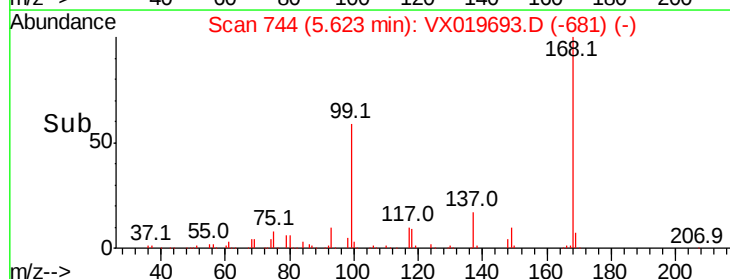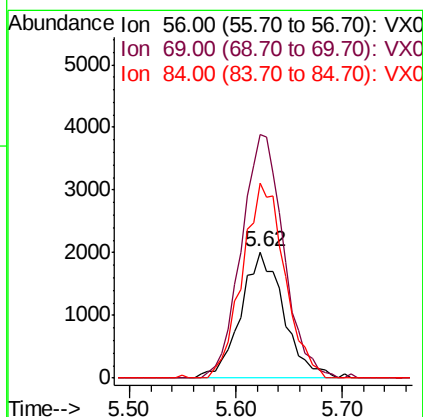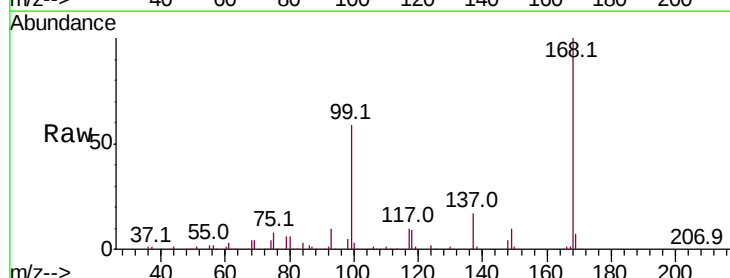



#33

1,2-Dichloroethane-d4

Concen: 49.241 ug/l

RT: 6.03 min Scan# 811

Delta R.T. -0.00 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24

Instrument :

MSVOA_X

ClientSampleId :


PB133320ZHE#06

Tot Ion: 65 Resp: 185391

Ion Ratio Lower Upper

65 100

67 52.6 0.0 105.0

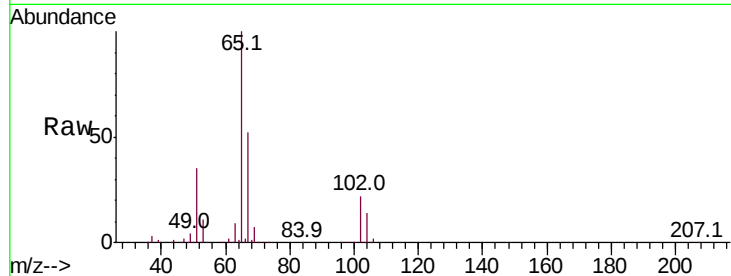

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.03

80000

60000



40000

20000

0

5.90 6.00 6.10 6.20

Time-->



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24


Tgt Ion:114 Resp: 483093

Ion Ratio Lower Upper

114 100

63 19.8 0.0 38.8

88 16.0 0.0 31.6



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

6.83

250000

200000

150000


100000


50000

0

6.80 7.00

Time-->





#35

Dibromofluoromethane

Concen: 48.233 ug/l

RT: 5.46 min Scan# 717

Delta R.T. -0.01 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24

Instrument :

MSVOA_X

ClientSampleId :

PB133320ZHE#06


Tot Ion:113 Resp: 146262

Ion Ratio Lower Upper

113 100

111 103.4 81.5 122.3




192 20.5 16.2 24.2



Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

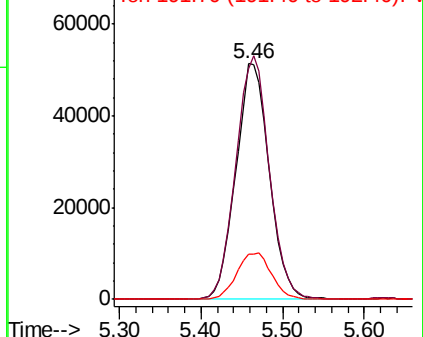

#36

1,1-Dichloropropene

Concen: 4.839 ug/l

RT: 5.62 min Scan# 744

Delta R.T. -0.14 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24


Tgt Ion: 75 Resp: 21916

Ion Ratio Lower Upper

75 100

110 8.5 18.1 54.3#



77 0.0 24.2 36.4#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0




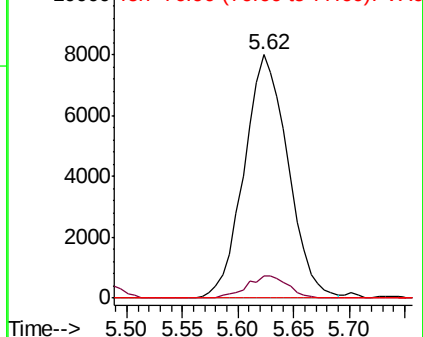




#37
Ethyl Acetate
Concen: 1.911 ug/l
RT: 4.64 min Scan# 583
Delta R.T. -0.15 min
Lab File: VX019693.D
Acq: 01 Dec 2020 14:24




Instrument :
MSVOA_X
ClientSampleId :
PB133320ZHE#06


Tot Ion: 43 Resp: 8126
Ion Ratio Lower Upper
43 100
61 1.3 12.7 19.1#
70 0.0 10.2 15.2#

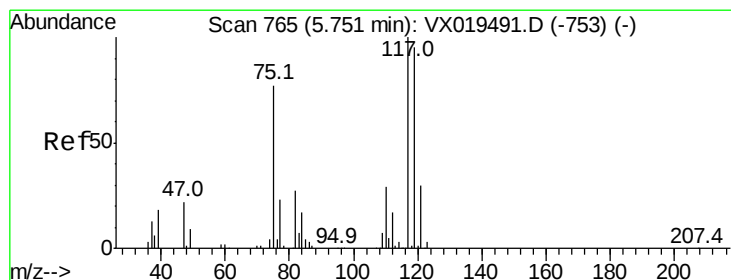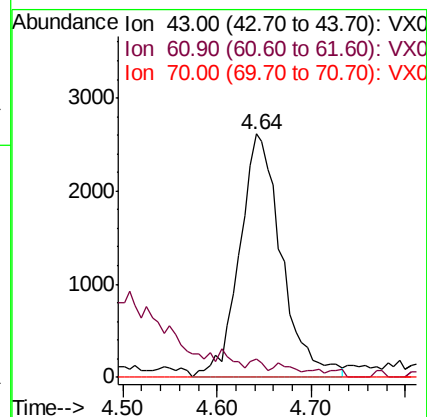

#38
Carbon Tetrachloride
Concen: 6.445 ug/l
RT: 5.63 min Scan# 745
Delta R.T. -0.12 min
Lab File: VX019693.D
Acq: 01 Dec 2020 14:24

Tgt Ion: 117 Resp: 28254
Ion Ratio Lower Upper
117 100
119 5.4 75.9 113.9#
121 0.0 24.0 36.0#

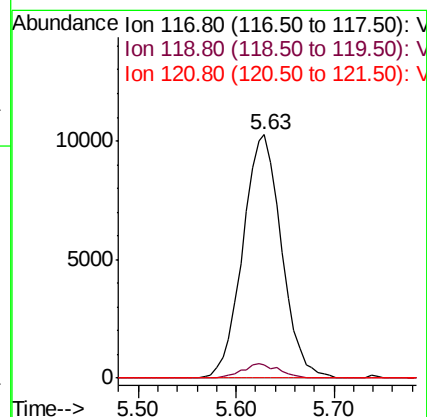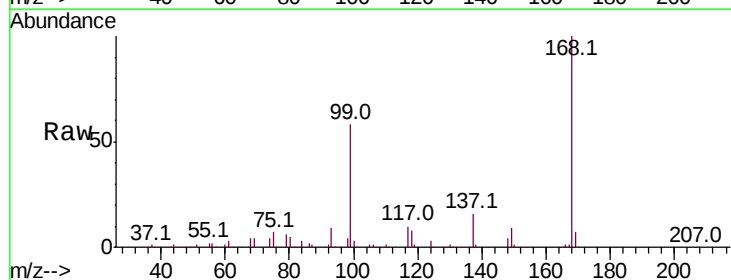



#43

Isopropyl Acetate

Concen: 4.612 ug/l

RT: 6.42 min Scan# 874

Delta R.T. -0.00 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24

Instrument :

MSVOA_X

ClientSampleId :

PB133320ZHE#06


Tot Ion: 43 Resp: 32964

Ion Ratio Lower Upper

43 100

61 22.9 18.2 27.2




87 15.0 12.6 18.8

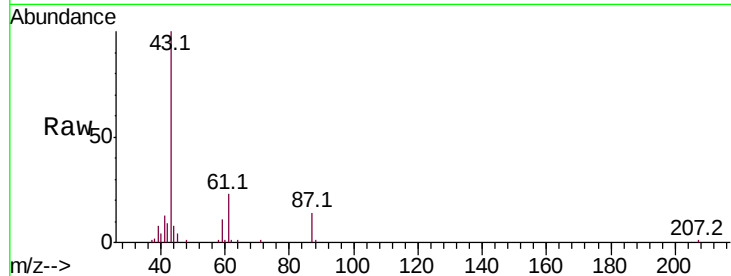

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

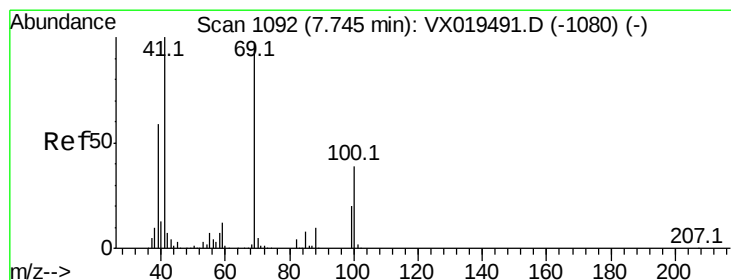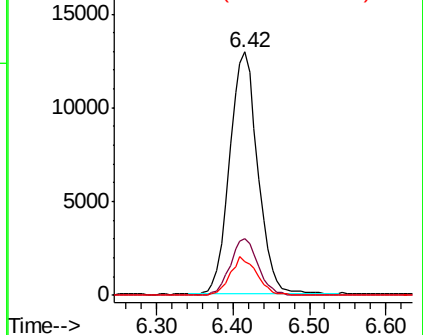

#48

Methyl methacrylate

Concen: 2.372 ug/l

RT: 7.65 min Scan# 1077

Delta R.T. -0.09 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24


Tgt Ion: 41 Resp: 7940

Ion Ratio Lower Upper

41 100

69 0.0 77.0 115.6#



39 0.0 45.6 68.4#




Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

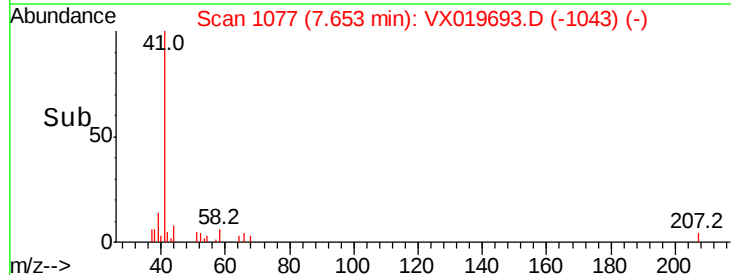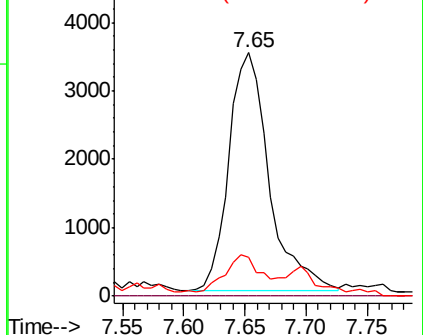



#49

1,4-Dioxane

Concen: 4.092 ug/l

RT: 7.85 min Scan# 1109

Delta R.T. 0.13 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24

Instrument :

MSVOA_X

ClientSampleId :

PB133320ZHE#06


Tot Ion: 88 Resp: 311

Ion Ratio Lower Upper

88 100

43 508370.1 23.8 35.6#




58 2599.0 54.2 81.2#

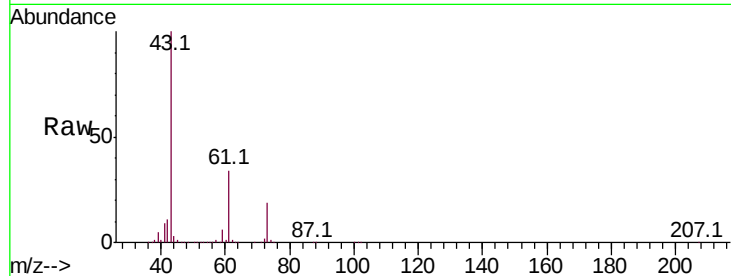

Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

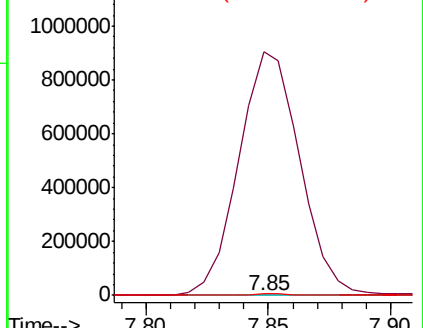

#50

Toluene-d8

Concen: 49.258 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX019693.D


Acq: 01 Dec 2020 14:24

Tgt Ion: 98 Resp: 580434

Ion Ratio Lower Upper



98 100


100 65.3 52.4 78.6



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

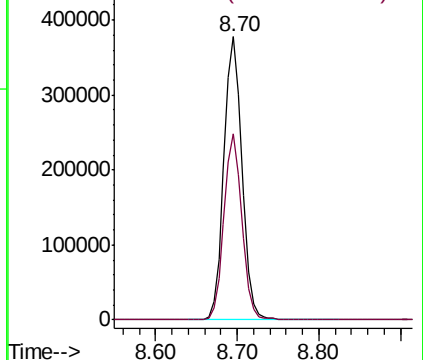



#51

4-Methyl-2-Pentanone

Concen: 24.013 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. -0.03 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24

Instrument :

MSVOA_X

ClientSampleId :





PB133320ZHE#06

Tot Ion: 43 Resp: 100082

Ion Ratio Lower Upper

43 100

58 9.2 35.1 52.7#

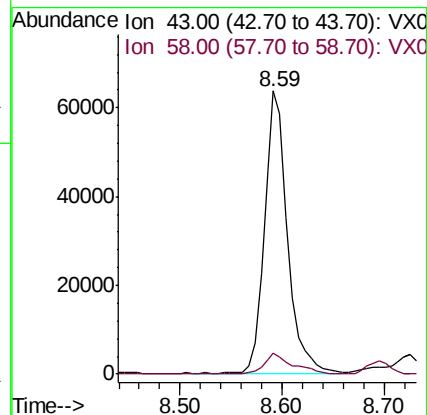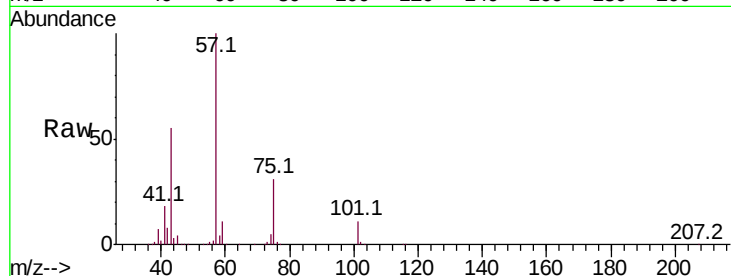

#54

cis-1,3-Dichloropropene

Concen: 9.816 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. 0.18 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24




Tgt Ion: 75 Resp: 53523


Ion Ratio Lower Upper

75 100

77 0.4 25.8 38.6#

39 23.8 34.6 51.8#

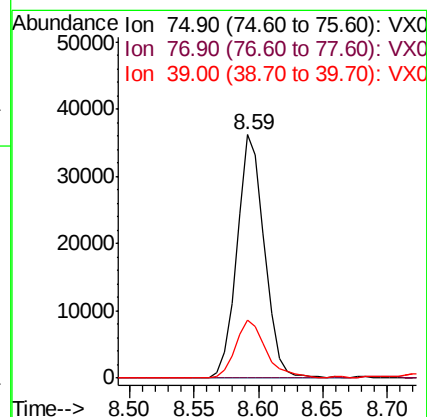



#57

1,3-Dichloropropane

Concen: 4.958 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.17 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24

Instrument :

MSVOA_X

ClientSampleId :


PB133320ZHE#06

Tot Ion: 76 Resp: 28780

Ion Ratio Lower Upper

76 100

78 0.7 25.7 38.5#

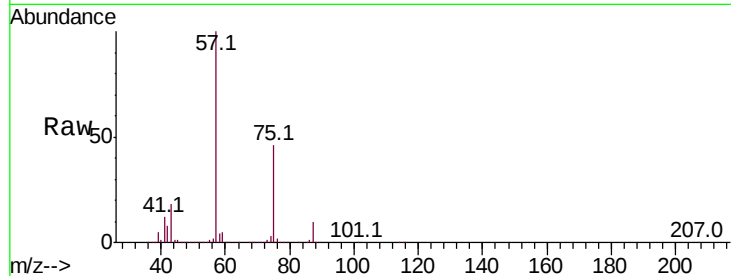

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

25000

20000

15000



10000

5000

0

9.45 9.50 9.55 9.60

Time-->

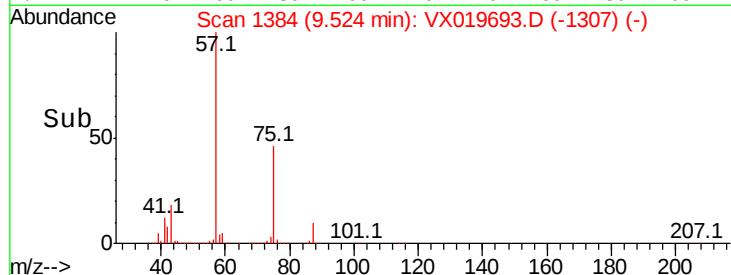

#59

2-Hexanone

Concen: 106.878 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.05 min

Lab File: VX019693.D


Acq: 01 Dec 2020 14:24

Tgt Ion: 43 Resp: 337836

Ion Ratio Lower Upper

43 100

58 21.1 30.6 91.6#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

300000

250000

200000

150000


100000


50000

0

9.45 9.50 9.55 9.60

Time-->



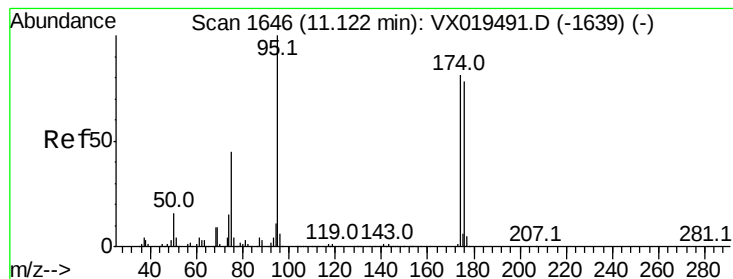

#62

4-Bromofluorobenzene

Concen: 45.739 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24

Instrument :

MSVOA_X

ClientSampleId :

PB133320ZHE#06


Tot Ion: 95 Resp: 193911

Ion Ratio Lower Upper

95 100

174 76.4 0.0 156.2




176 74.8 0.0 151.4

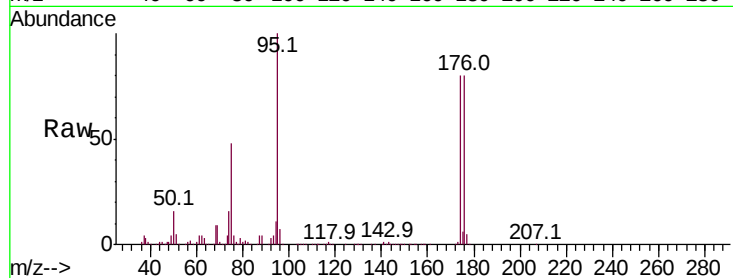

Abundance Ion 94.90 (94.60 to 95.60): VX019491.D (-1639) (-)

Ion 173.80 (173.50 to 174.50): VX019491.D (-1639) (-)

Ion 175.80 (175.50 to 176.50): VX019491.D (-1639) (-)

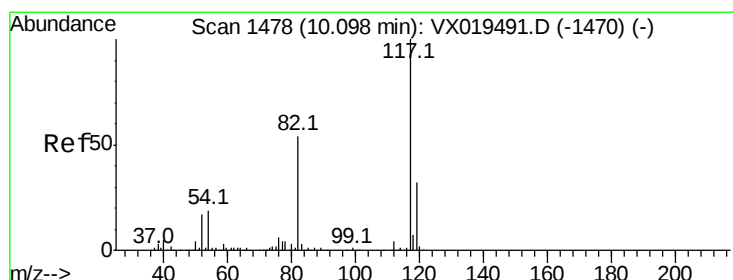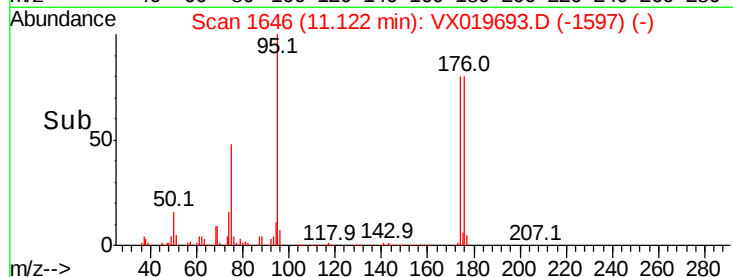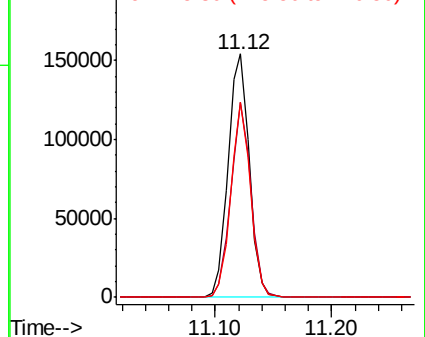

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24


Tgt Ion: 117 Resp: 423831

Ion Ratio Lower Upper

117 100

82 52.9 43.0 64.4



119 31.6 25.6 38.4

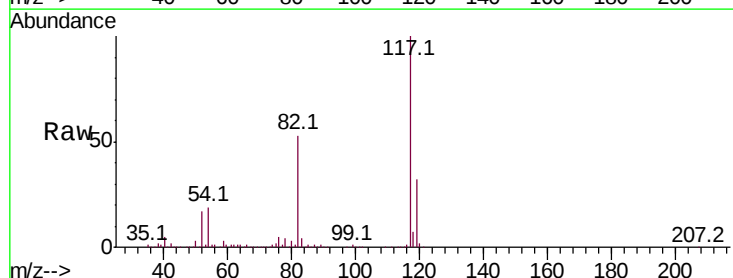


Abundance Ion 116.90 (116.60 to 117.60): VX019491.D (-1470) (-)

Ion 82.00 (81.70 to 82.70): VX019491.D (-1470) (-)

Ion 118.90 (118.60 to 119.60): VX019491.D (-1470) (-)



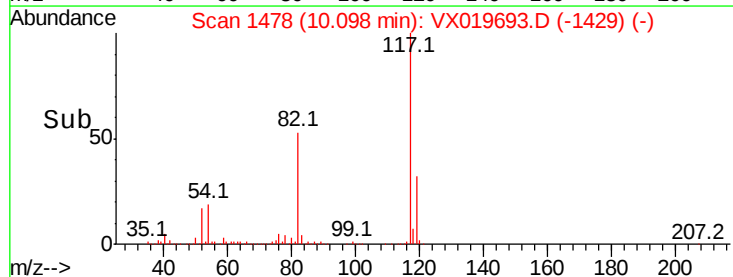
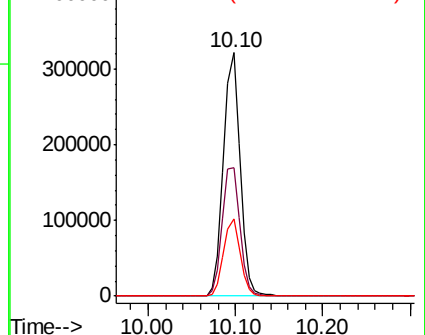




#70
Stvrene
Concen: 1.669 ug/l
RT: 10.70 min Scan# 1576
Delta R.T. 0.00 min
Lab File: VX019693.D
Acq: 01 Dec 2020 14:24




Instrument :
MSVOA_X
ClientSampleId :
PB133320ZHE#06


Tot Ion:104 Resp: 242
Ion Ratio Lower Upper
104 100
78 53.7 39.5 59.3
103 27.7 43.6 65.4#

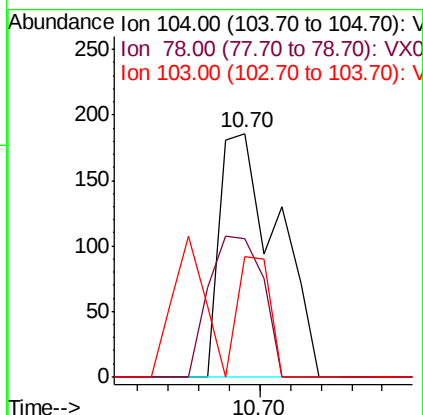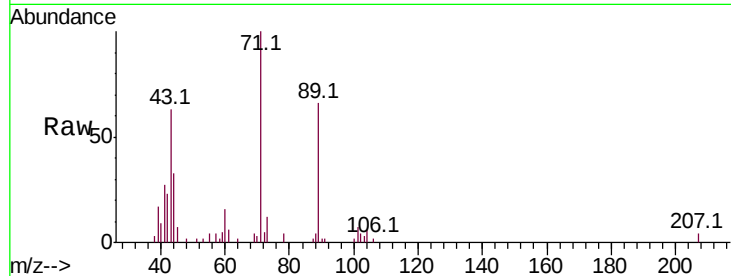

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX019693.D
Acq: 01 Dec 2020 14:24

Tgt Ion:152 Resp: 179062
Ion Ratio Lower Upper
152 100
115 58.5 41.8 125.4
150 155.0 0.0 348.2

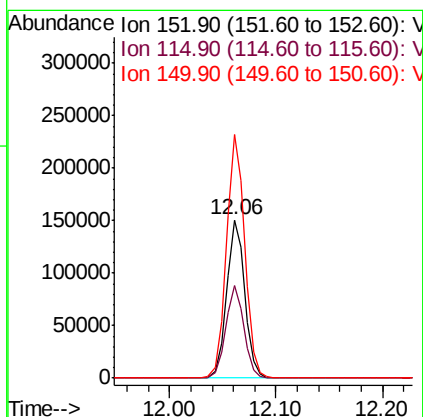

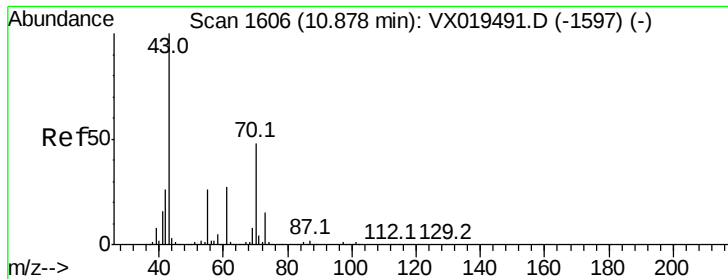

#74

N-amvl acetate

Concen: 0.366 ug/l

RT: 10.80 min Scan# 1594

Delta R.T. -0.07 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24

Instrument :

MSVOA_X

ClientSampleId :

PB133320ZHE#06

Tot Ion: 43 Resp: 1697


Ion Ratio Lower Upper

43 100

70 0.0 39.7 59.5#

55 10.9 21.8 32.6#

61 0.0 22.2 33.4#



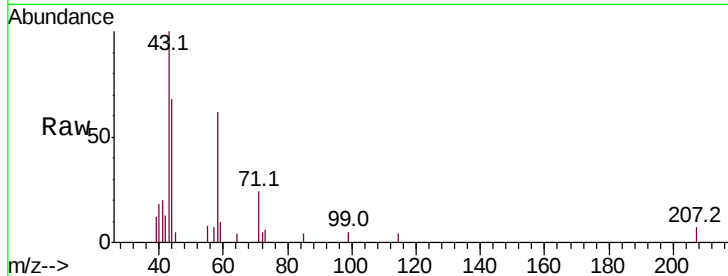


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

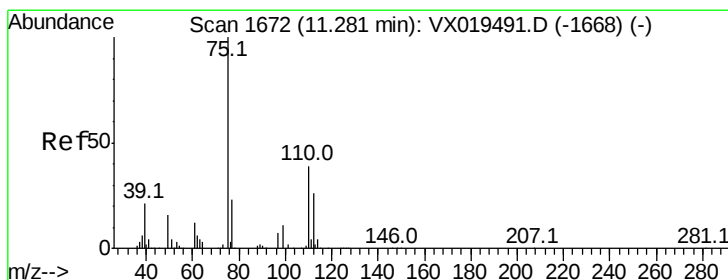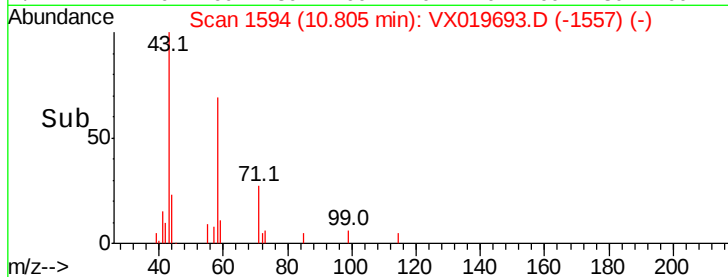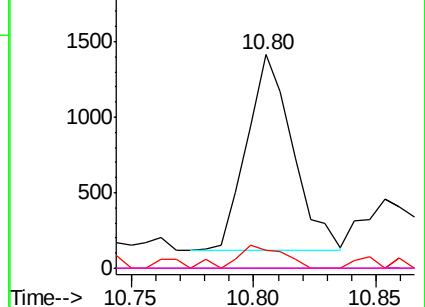

#76

1,2,3-Trichloropropane

Concen: 24.059 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX019693.D


Acq: 01 Dec 2020 14:24

Tgt Ion: 75 Resp: 94017

Ion Ratio Lower Upper



75 100


77 1.3 20.0 60.0#

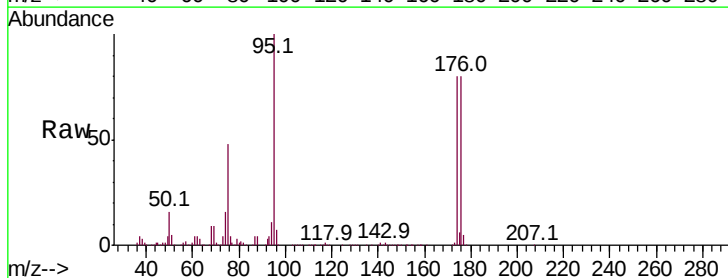

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0



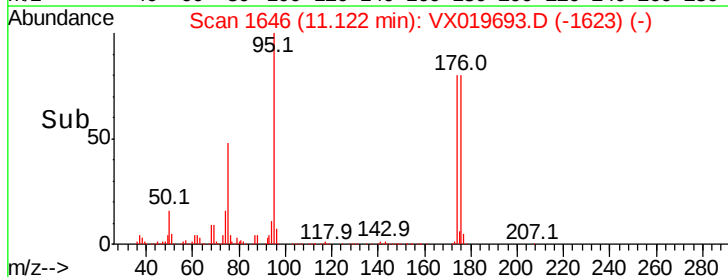
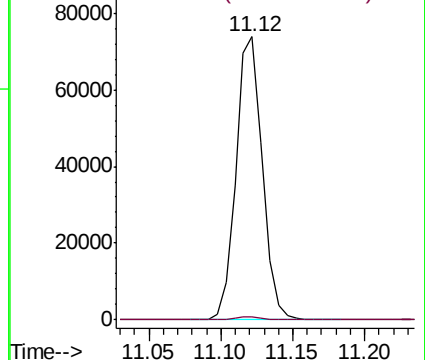


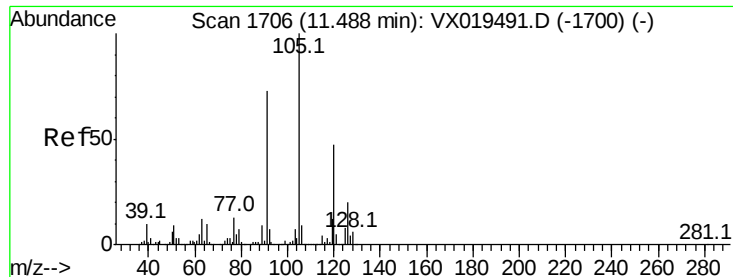

#80
 1,3,5-Trimethylbenzene
 Concen: 0.201 ug/l
 RT: 11.49 min Scan# 1706
 Delta R.T. -0.00 min
 Lab File: VX019693.D
 Acq: 01 Dec 2020 14:24




Instrument :
 MSVOA_X
 ClientSampleId :
 PB133320ZHE#06


Tot Ion:105 Resp: 2087
 Ion Ratio Lower Upper
 105 100
 120 48.7 24.1 72.3

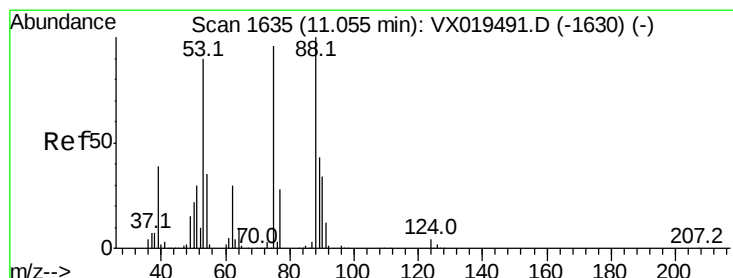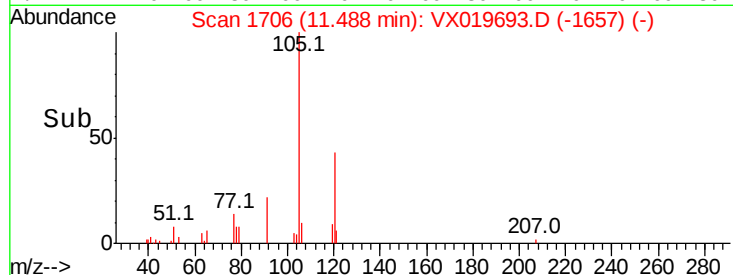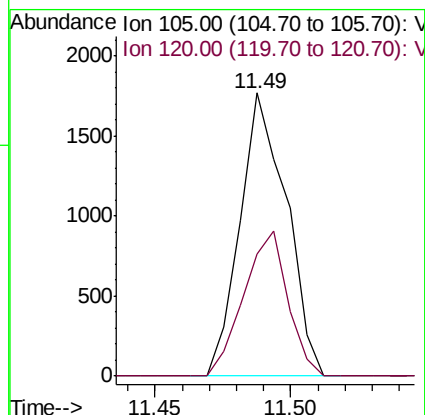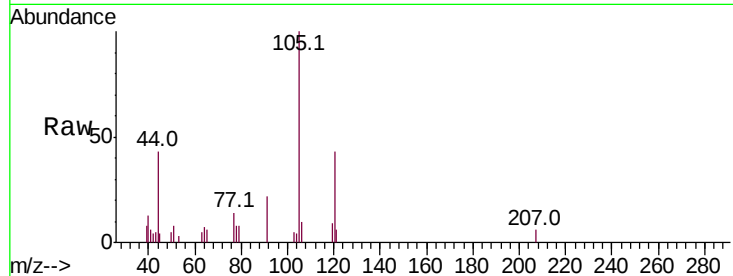

#81
 trans-1,4-Dichloro-2-butene
 Concen: 63.714 ug/l
 RT: 11.12 min Scan# 1646
 Delta R.T. 0.07 min
 Lab File: VX019693.D
 Acq: 01 Dec 2020 14:24

Tgt Ion: 75 Resp: 94017
 Ion Ratio Lower Upper
 75 100
 53 0.0 73.9 110.9#
 89 0.0 37.3 55.9#

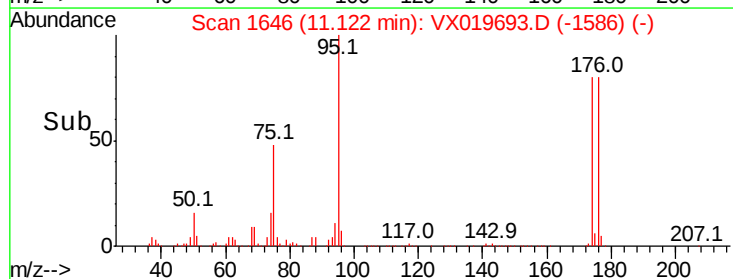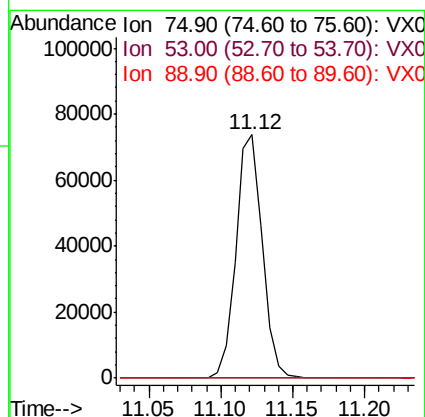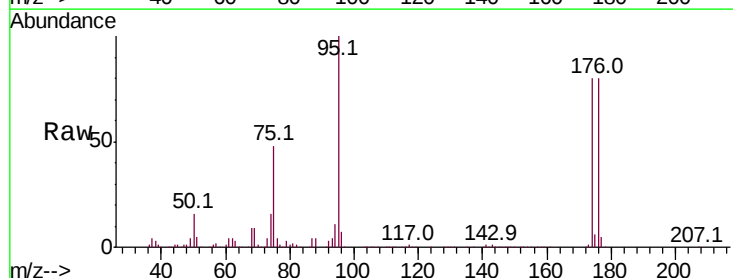

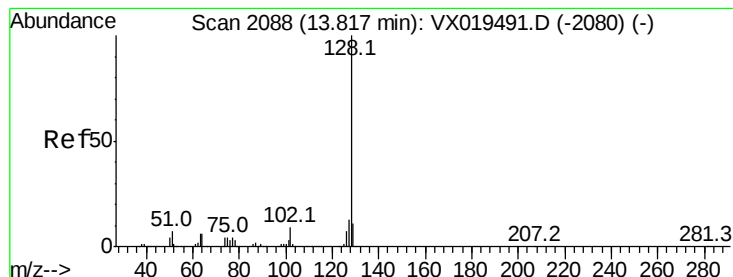

#95

Naphthalene

Concen: 2.211 ug/l

RT: 13.81 min Scan# 2087

Delta R.T. -0.01 min

Lab File: VX019693.D

Acq: 01 Dec 2020 14:24

Instrument :

MSVOA_X

ClientSampleId :

PB133320ZHE#06


Tot Ion:128 Resp: 452

Ion Ratio Lower Upper

128 100

127 0.0 10.3 15.5#

129 0.0 8.7 13.1#

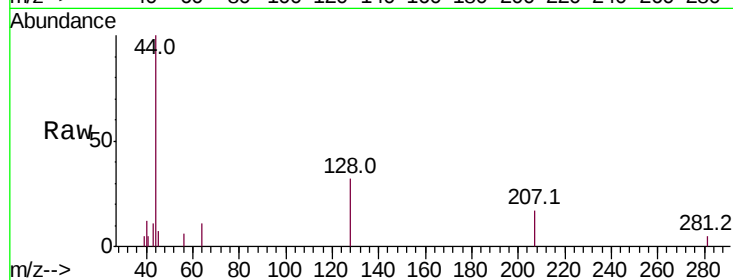

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

