

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX120120\
 Data File : VX019694.D
 Acq On : 01 Dec 2020 14:47
 Operator : JC/MD
 Sample : PB133320ZHE#07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB133320ZHE#07

Quant Time: Dec 02 02:12:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 21 01:57:45 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	286106	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	478552	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	422018	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	155839	50.00	ug/l	0.00

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4		6.03	65	181054	48.81	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	97.62%	
35) Dibromofluoromethane		5.46	113	144701	48.17	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	96.34%	
50) Toluene-d8		8.70	98	576332	49.37	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	98.74%	
62) 4-Bromofluorobenzene		11.12	95	185959	44.28	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	88.56%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.62	94	492	0.378	ug/l	94
6) Chloroethane	1.70	64	1610	Below Cal	#	51
11) Tert butyl alcohol	2.99	59	4151	5.913	ug/l #	73
13) Acrolein	2.25	56	116	0.246	ug/l #	3
16) Acetone	2.43	43	10837	7.554	ug/l	96
18) Methyl Acetate	2.75	43	3106	1.506	ug/l	93
20) Methylene Chloride	2.83	84	23333	6.507	ug/l	97
25) 2-Butanone	4.65	43	8380	3.889	ug/l	98
29) Tetrahydrofuran	5.10	42	1971	1.433	ug/l #	65
31) Cyclohexane	5.62	56	5536	1.147	ug/l #	1
36) 1,1-Dichloropropene	5.62	75	22316	4.974	ug/l #	49
38) Carbon Tetrachloride	5.62	117	27763	6.393	ug/l #	17
43) Isopropyl Acetate	6.42	43	34107	4.817	ug/l	99
48) Methyl methacrylate	7.65	41	8244	2.486	ug/l #	9
49) 1,4-Dioxane	7.85	88	319	4.237	ug/l #	1
51) 4-Methyl-2-Pentanone	8.59	43	102057	24.719	ug/l #	46
54) cis-1,3-Dichloropropene	8.59	75	55004	10.183	ug/l #	59
57) 1,3-Dichloropropane	9.52	76	29066	5.055	ug/l #	44
59) 2-Hexanone	9.52	43	345372	110.299	ug/l #	47
70) Styrene	10.69	104	187	1.664	ug/l #	48
74) N-amyl acetate	10.80	43	1780	0.441	ug/l #	47
76) 1,2,3-Trichloropropane	11.12	75	90262	26.540	ug/l #	38
80) 1,3,5-Trimethylbenzene	11.49	105	1948	0.215	ug/l	99
81) trans-1,4-Dichloro-2-buten	11.12	75	90262	69.848	ug/l #	12
95) Naphthalene	13.82	128	403	2.212	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX120120\
Data File : VX019694.D
Acq On : 01 Dec 2020 14:47
Operator : JC/MD
Sample : PB133320ZHE#07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB133320ZHE#07

Quant Time: Dec 02 02:12:34 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 21 01:57:45 2020
Response via : Initial Calibration

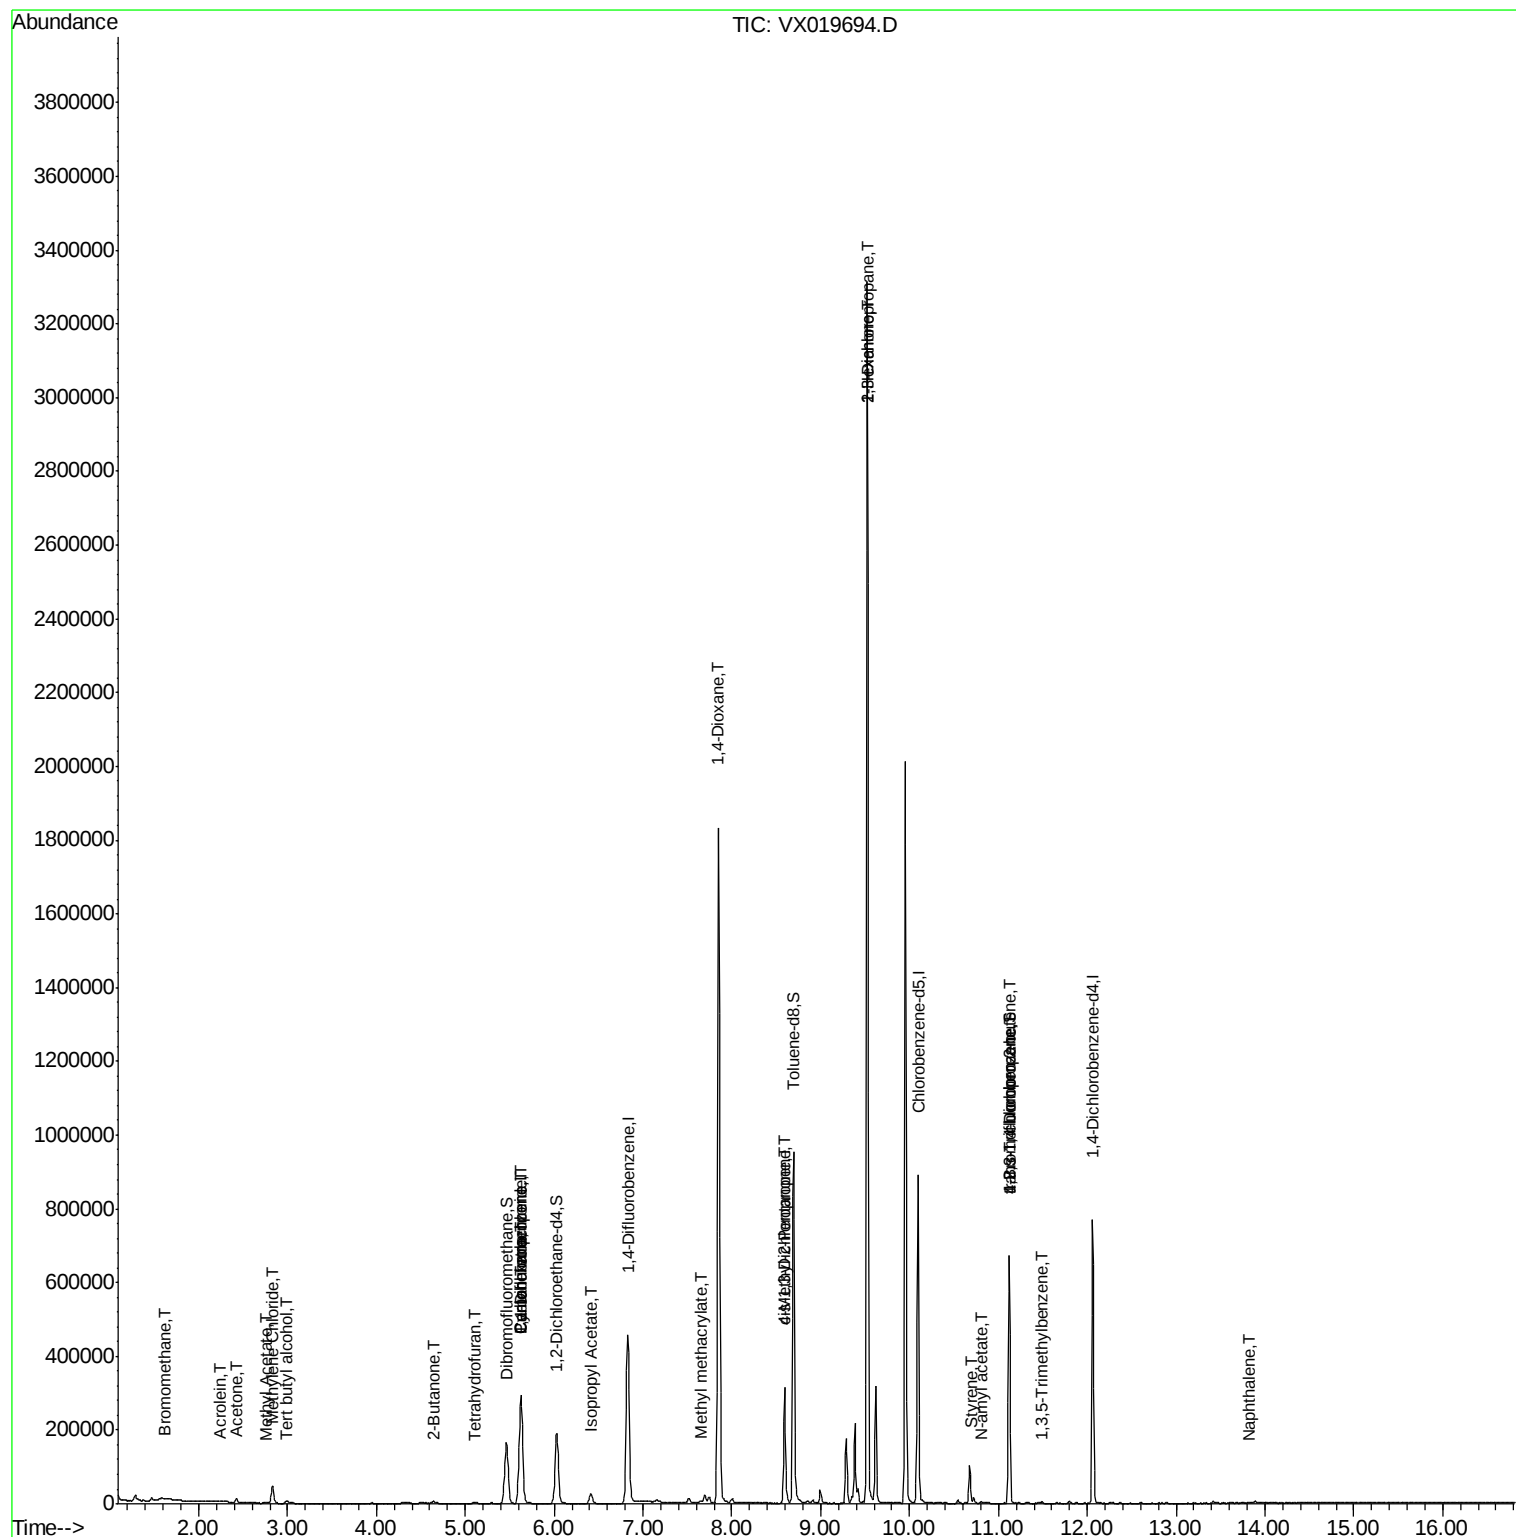



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.00 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47

Instrument :

MSVOA_X

ClientSampleId :


PB133320ZHE#07

Tot Ion:168 Resp: 286106

Ion Ratio Lower Upper

168 100

99 56.4 45.8 68.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

120000

100000

80000

60000

40000



20000

0

5.50 5.60 5.70 5.80

5.63

Time-->



#5

Bromomethane

Concen: 0.378 ug/l

RT: 1.62 min Scan# 88

Delta R.T. 0.01 min

Lab File: VX019694.D


Acq: 01 Dec 2020 14:47

Tgt Ion: 94 Resp: 492

Ion Ratio Lower Upper

94 100

96 100.0 75.6 113.4



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

300

250

200

150

100


50


0

1.60 1.65

1.62

Time-->



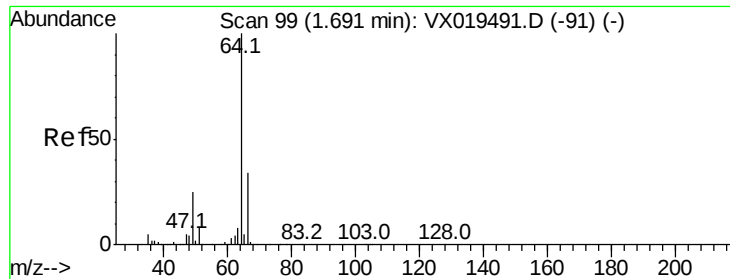

#6

Chloroethane

Concen: Below Cal

RT: 1.70 min Scan# 101

Delta R.T. 0.01 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47

Instrument :

MSVOA_X

ClientSampleId :





PB133320ZHE#07

Tot Ion: 64 Resp: 1610

Ion Ratio Lower Upper

64 100

66 5.7 27.1 40.7#

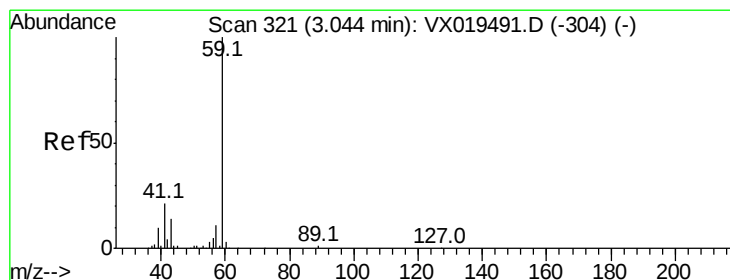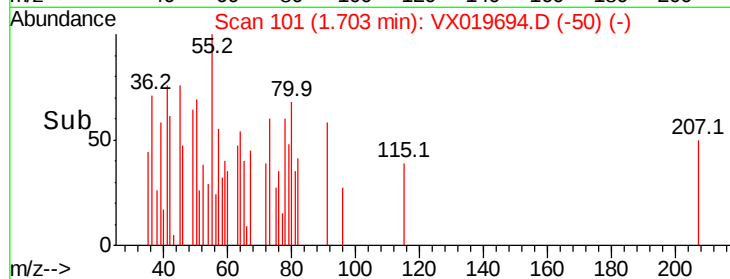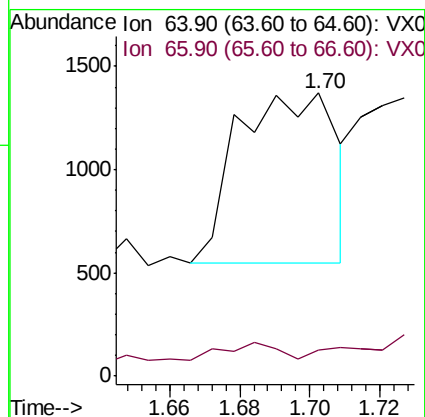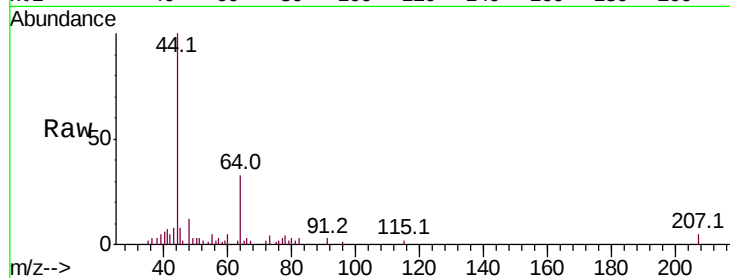

#11

Tert butyl alcohol

Concen: 5.913 ug/l

RT: 2.99 min Scan# 312

Delta R.T. -0.06 min

Lab File: VX019694.D




Acq: 01 Dec 2020 14:47


Tgt Ion: 59 Resp: 4151

Ion Ratio Lower Upper

59 100

57 0.0 7.9 11.9#

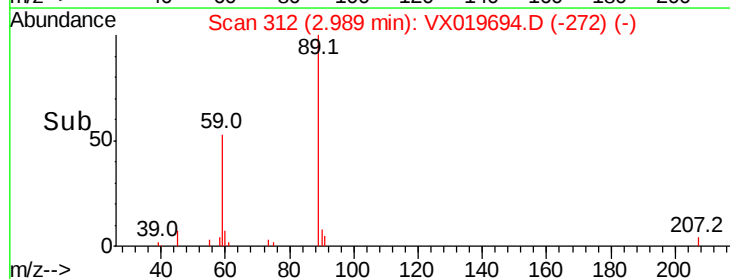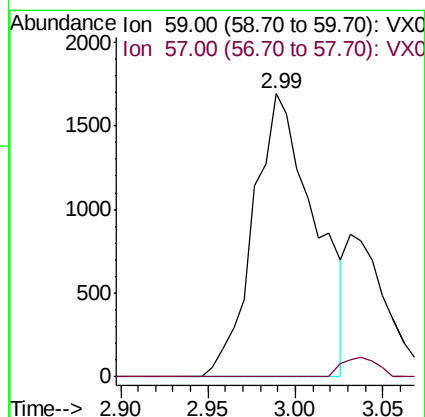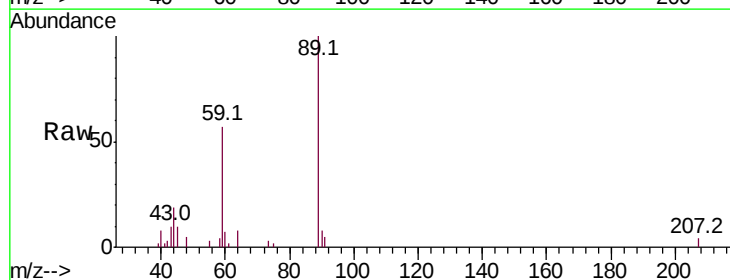



#13

Acrolein

Concen: 0.246 ug/l

RT: 2.25 min Scan# 191

Delta R.T. -0.02 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47

Instrument :

MSVOA_X

ClientSampleId :





PB133320ZHE#07

Tot Ion: 56 Resp: 116

Ion Ratio Lower Upper

56 100

55 148.3 55.5 83.3#

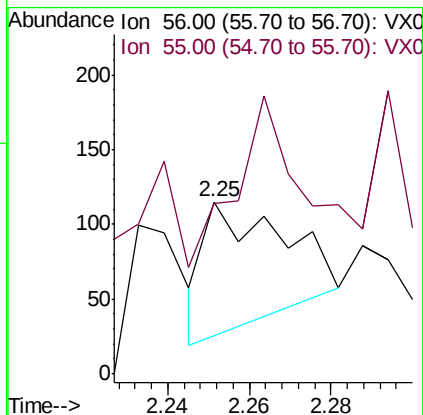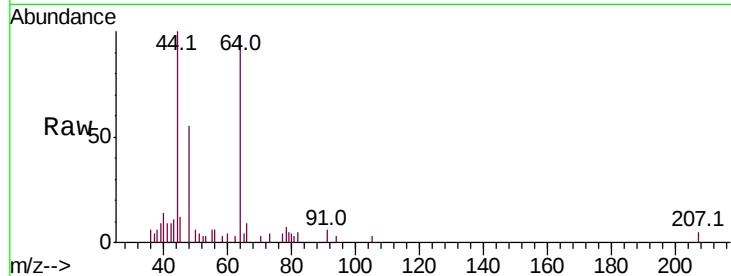

#16

Acetone

Concen: 7.554 ug/l

RT: 2.43 min Scan# 220

Delta R.T. -0.00 min

Lab File: VX019694.D




Acq: 01 Dec 2020 14:47


Tgt Ion: 43 Resp: 10837

Ion Ratio Lower Upper

43 100

58 36.3 27.4 41.2



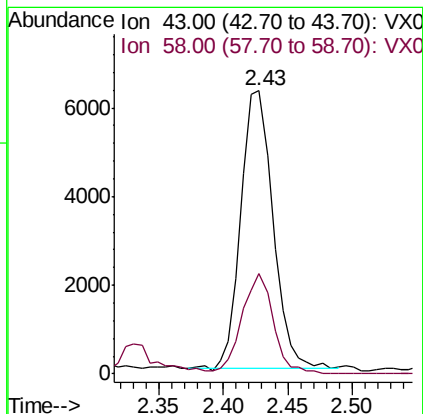





#18
Methyl Acetate
Concen: 1.506 ug/l
RT: 2.75 min Scan# 273
Delta R.T. 0.00 min
Lab File: VX019694.D
Acq: 01 Dec 2020 14:47




Instrument :
MSVOA_X
ClientSampleId :
PB133320ZHE#07


Tot Ion: 43 Resp: 3106
Ion Ratio Lower Upper
43 100
74 24.1 22.2 33.4

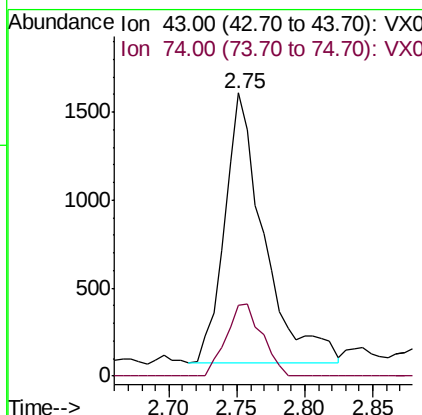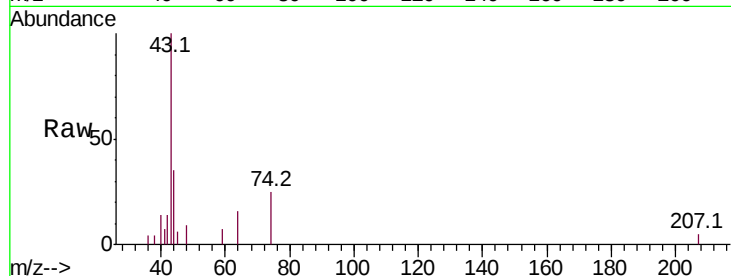

#20
Methylene Chloride
Concen: 6.507 ug/l
RT: 2.83 min Scan# 286
Delta R.T. -0.00 min
Lab File: VX019694.D
Acq: 01 Dec 2020 14:47

Tgt Ion: 84 Resp: 23333
Ion Ratio Lower Upper
84 100
49 109.0 88.5 132.7
51 32.8 28.0 42.0
86 62.5 53.0 79.4

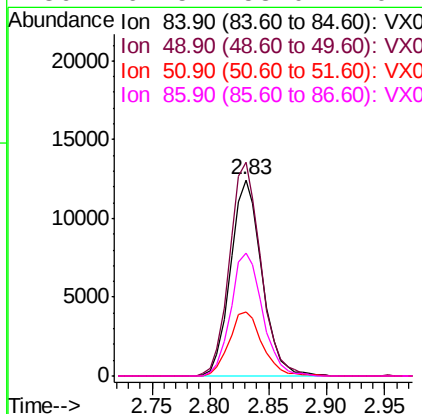



#25

2-Butanone

Concen: 3.889 ug/l

RT: 4.65 min Scan# 584

Delta R.T. 0.01 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47

Instrument :

MSVOA_X

ClientSampleId :





PB133320ZHE#07

Tot Ion: 43 Resp: 8380

Ion Ratio Lower Upper

43 100

72 29.1 24.0 36.0

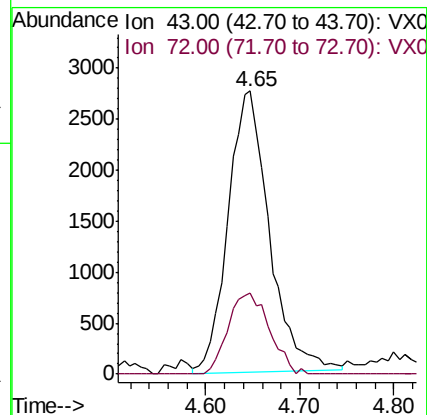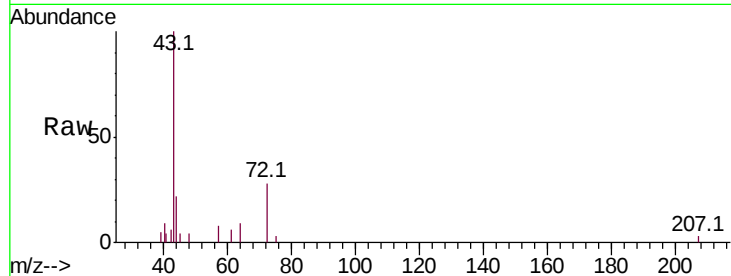

#29

Tetrahydrofuran

Concen: 1.433 ug/l

RT: 5.10 min Scan# 659

Delta R.T. 0.01 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47




Tgt Ion: 42 Resp: 1971


Ion Ratio Lower Upper

42 100

72 36.6 42.6 63.8#

71 15.9 39.0 58.6#



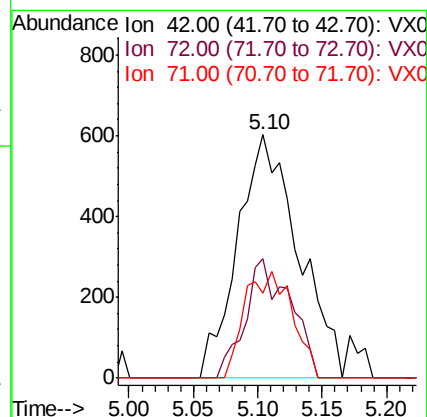



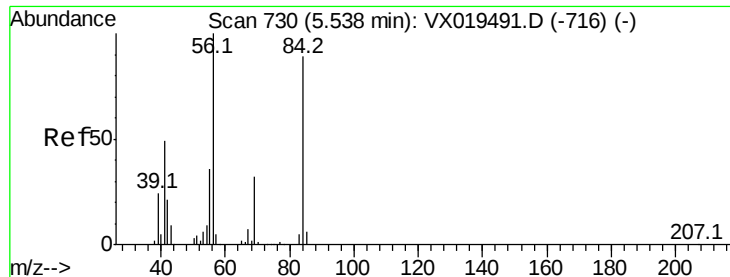

#31
Cyclohexane
Concen: 1.147 ug/l
RT: 5.62 min Scan# 743
Delta R.T. 0.08 min
Lab File: VX019694.D
Acq: 01 Dec 2020 14:47




Instrument :
MSVOA_X
ClientSampleId :
PB133320ZHE#07


Tot Ion: 56 Resp: 5536
Ion Ratio Lower Upper
56 100
69 186.0 25.5 38.3#
84 132.9 71.1 106.7#

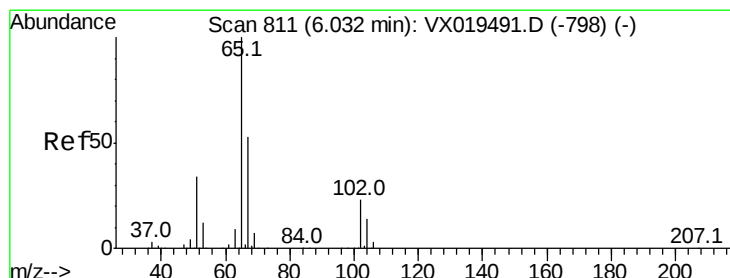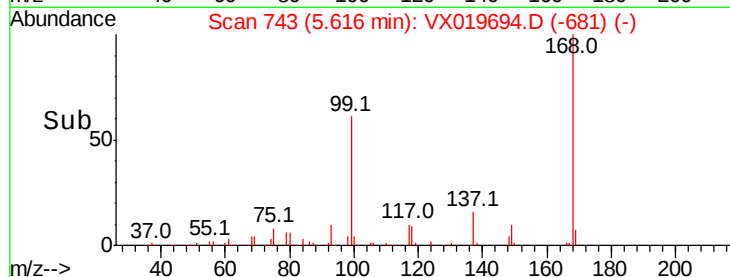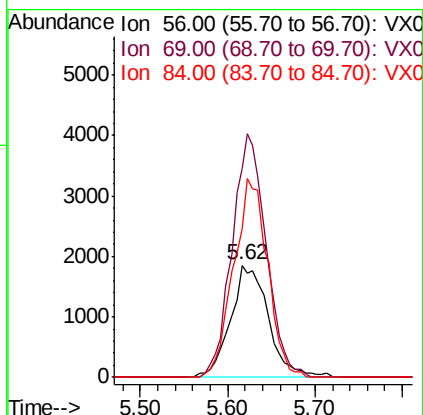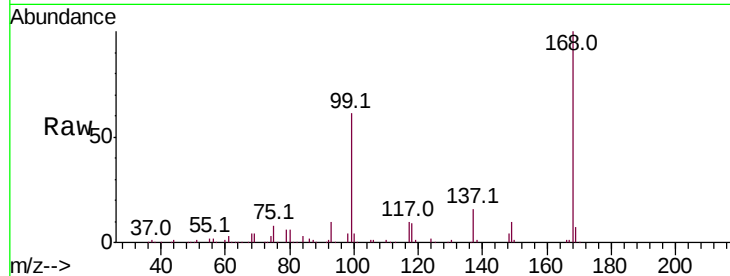

#33
1,2-Dichloroethane-d4
Concen: 48.807 ug/l
RT: 6.03 min Scan# 811
Delta R.T. -0.00 min
Lab File: VX019694.D
Acq: 01 Dec 2020 14:47

Tgt Ion: 65 Resp: 181054
Ion Ratio Lower Upper
65 100
67 53.0 0.0 105.0

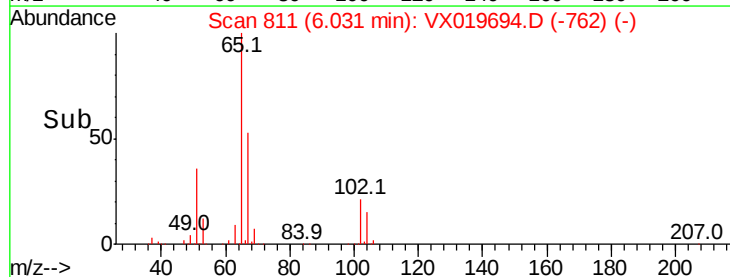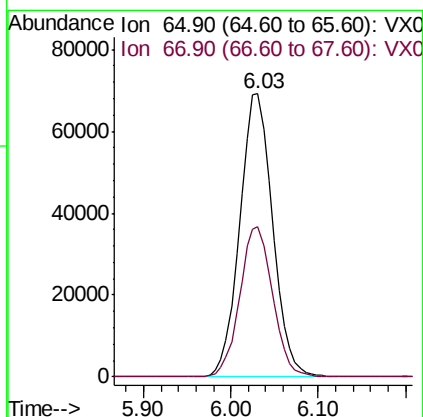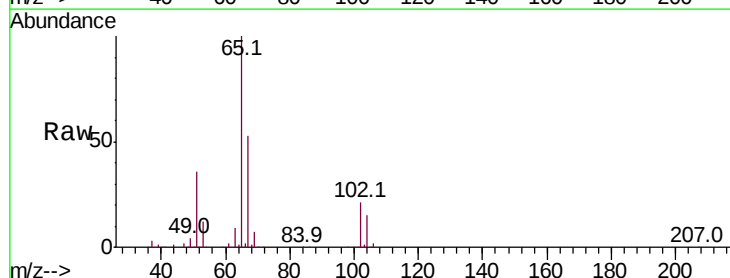



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47

Instrument :

MSVOA_X

ClientSampleId :

PB133320ZHE#07


Tot Ion:114 Resp: 478552

Ion Ratio Lower Upper

114 100

63 19.8 0.0 38.8




88 16.2 0.0 31.6



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

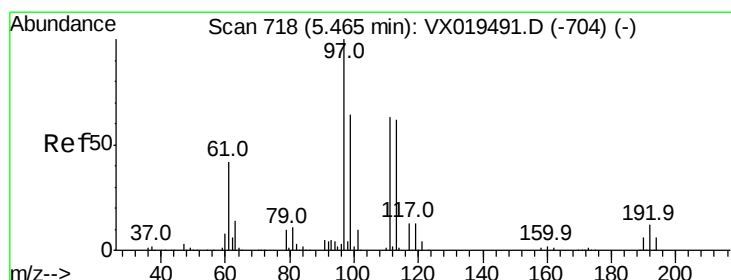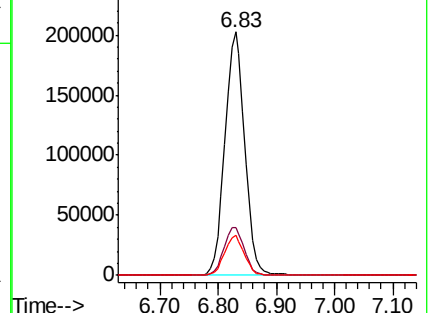

#35

Dibromofluoromethane

Concen: 48.172 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47


Tgt Ion:113 Resp: 144701

Ion Ratio Lower Upper

113 100

111 102.9 81.5 122.3



192 20.4 16.2 24.2




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



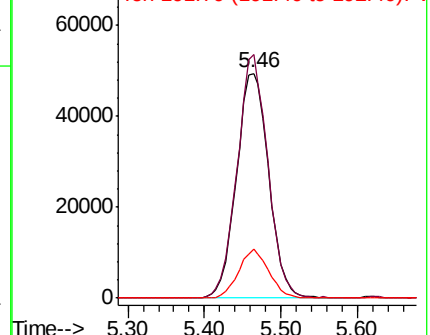





#36
 1,1-Dichloropropene
 Concen: 4.974 ug/l
 RT: 5.62 min Scan# 744
 Delta R.T. -0.14 min
 Lab File: VX019694.D
 Acq: 01 Dec 2020 14:47




Instrument :
 MSVOA_X
 ClientSampleId :
 PB133320ZHE#07


Tot Ion: 75 Resp: 22316
 Ion Ratio Lower Upper
 75 100
 110 8.7 18.1 54.3#
 77 0.0 24.2 36.4#

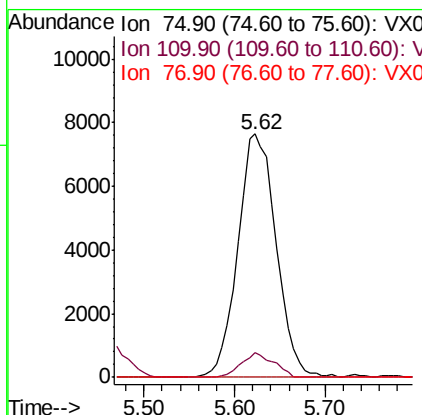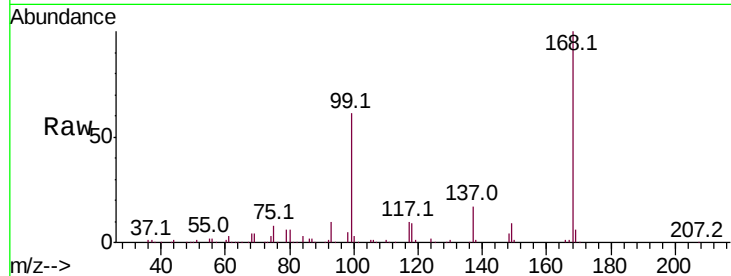

#38
 Carbon Tetrachloride
 Concen: 6.393 ug/l
 RT: 5.62 min Scan# 744
 Delta R.T. -0.13 min
 Lab File: VX019694.D
 Acq: 01 Dec 2020 14:47

Tgt Ion: 117 Resp: 27763
 Ion Ratio Lower Upper
 117 100
 119 5.7 75.9 113.9#
 121 0.0 24.0 36.0#

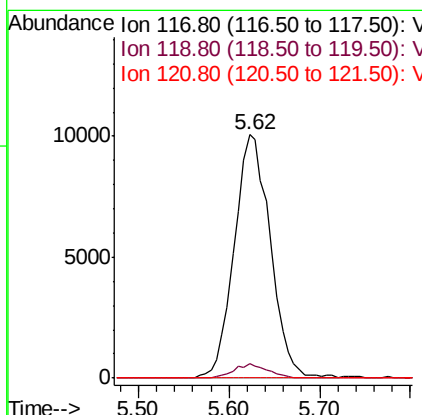



#43

Isopropyl Acetate

Concen: 4.817 ug/l

RT: 6.42 min Scan# 874

Delta R.T. -0.00 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47

Instrument :

MSVOA_X

ClientSampleId :

PB133320ZHE#07


Tot Ion: 43 Resp: 34107

Ion Ratio Lower Upper

43 100

61 22.1 18.2 27.2




87 15.3 12.6 18.8

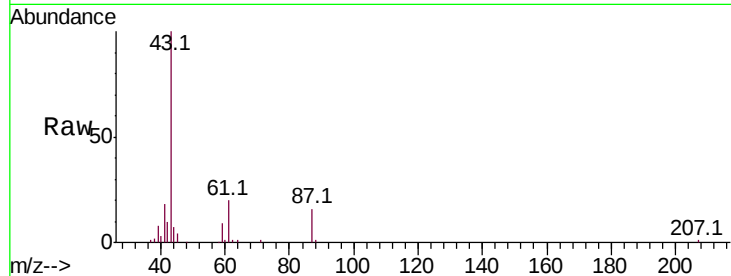

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

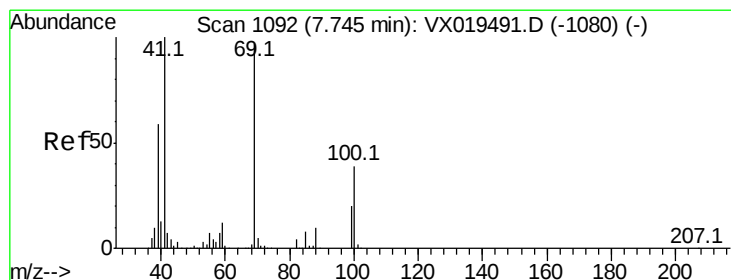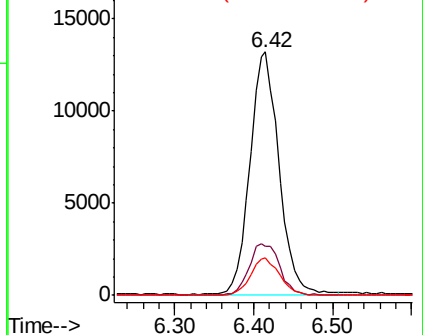

#48

Methyl methacrylate

Concen: 2.486 ug/l

RT: 7.65 min Scan# 1077

Delta R.T. -0.09 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47


Tgt Ion: 41 Resp: 8244

Ion Ratio Lower Upper

41 100

69 0.0 77.0 115.6#



39 0.0 45.6 68.4#




Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

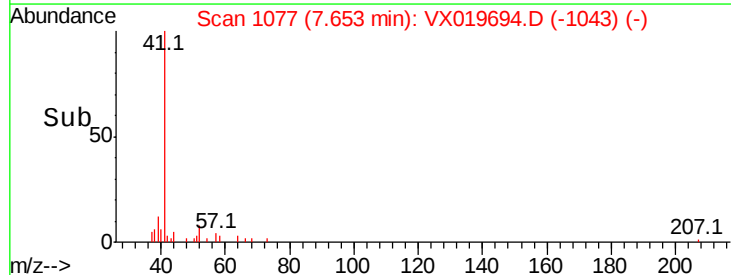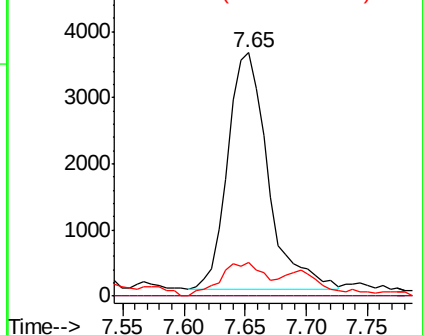



#49

1,4-Dioxane

Concen: 4.237 ug/l

RT: 7.85 min Scan# 1110

Delta R.T. 0.13 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47

Instrument :

MSVOA_X

ClientSampleId :

PB133320ZHE#07


Tot Ion: 88 Resp: 319

Ion Ratio Lower Upper

88 100

43 512379.9 23.8 35.6#




58 2506.9 54.2 81.2#

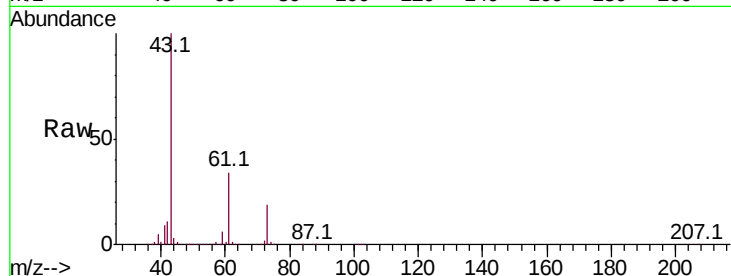

Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

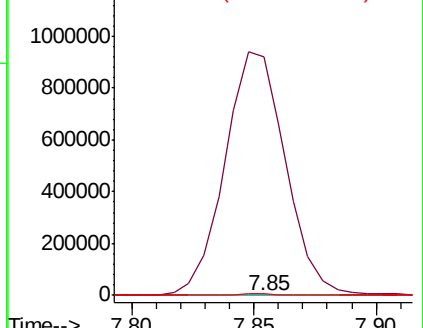

#50

Toluene-d8

Concen: 49.374 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX019694.D


Acq: 01 Dec 2020 14:47

Tgt Ion: 98 Resp: 576332

Ion Ratio Lower Upper



98 100


100 66.5 52.4 78.6



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

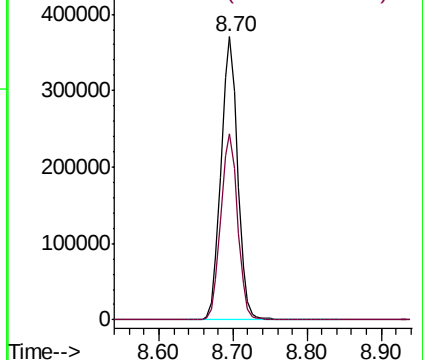



#51

4-Methyl-2-Pentanone

Concen: 24.719 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. -0.03 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47

Instrument :

MSVOA_X

ClientSampleId :





PB133320ZHE#07

Tot Ion: 43 Resp: 102057

Ion Ratio Lower Upper

43 100

58 9.2 35.1 52.7#

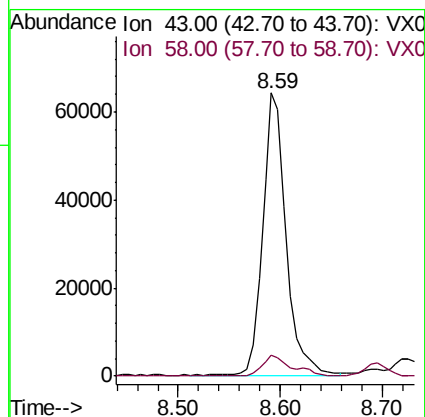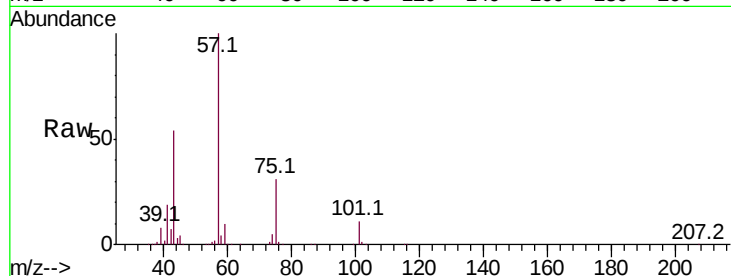

#54

cis-1,3-Dichloropropene

Concen: 10.183 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. 0.18 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47




Tgt Ion: 75 Resp: 55004


Ion Ratio Lower Upper

75 100

77 0.5 25.8 38.6#

39 24.7 34.6 51.8#

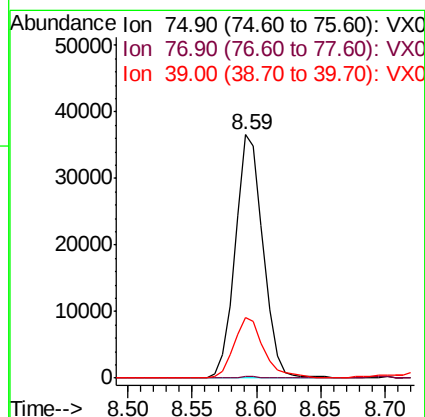



#57

1,3-Dichloropropane

Concen: 5.055 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.17 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47

Instrument :

MSVOA_X

ClientSampleId :





PB133320ZHE#07

Tot Ion: 76 Resp: 29066

Ion Ratio Lower Upper

76 100

78 0.6 25.7 38.5#

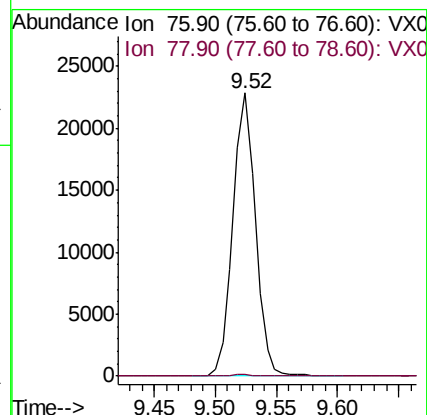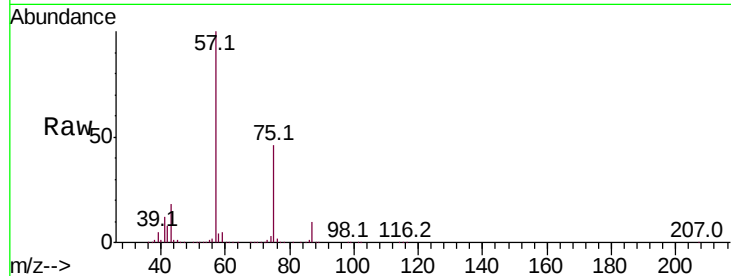

#59

2-Hexanone

Concen: 110.299 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.05 min

Lab File: VX019694.D




Acq: 01 Dec 2020 14:47


Tgt Ion: 43 Resp: 345372

Ion Ratio Lower Upper

43 100

58 21.0 30.6 91.6#

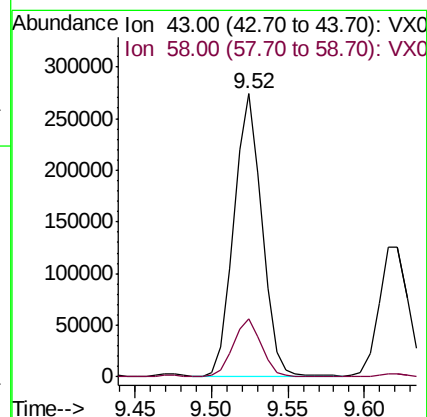

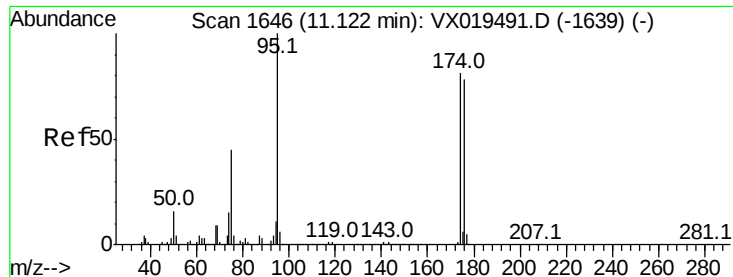

#62

4-Bromofluorobenzene

Concen: 44.279 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47

Instrument :

MSVOA_X

ClientSampleId :

PB133320ZHE#07


Tot Ion: 95 Resp: 185959

Ion Ratio Lower Upper

95 100

174 76.1 0.0 156.2

176 72.0 0.0 151.4



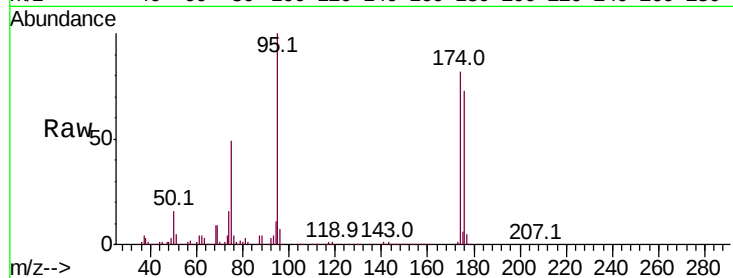


Abundance Ion 94.90 (94.60 to 95.60): VX019491.D (-1639) (-)

200000

Ion 173.80 (173.50 to 174.50): VX019491.D (-1639) (-)

Ion 175.80 (175.50 to 176.50): VX019491.D (-1639) (-)

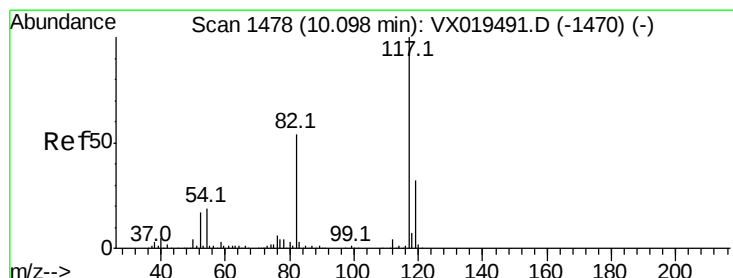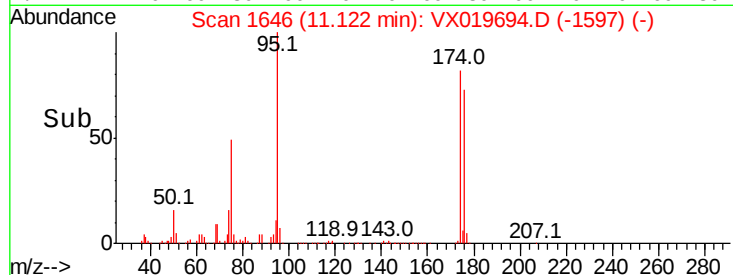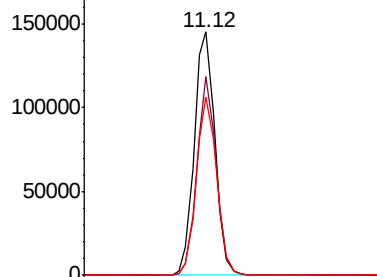

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47


Tgt Ion: 117 Resp: 422018

Ion Ratio Lower Upper

117 100

82 54.3 43.0 64.4

119 32.7 25.6 38.4


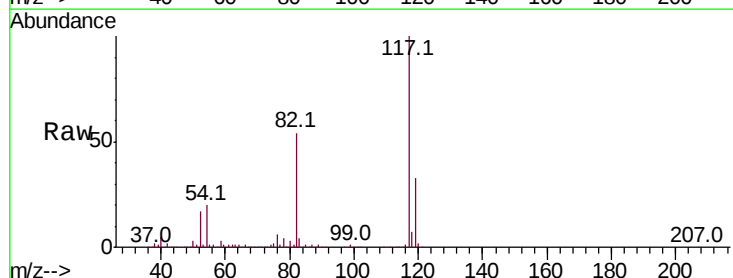



Abundance Ion 116.90 (116.60 to 117.60): VX019491.D (-1470) (-)

400000

Ion 82.00 (81.70 to 82.70): VX019491.D (-1470) (-)

Ion 118.90 (118.60 to 119.60): VX019491.D (-1470) (-)



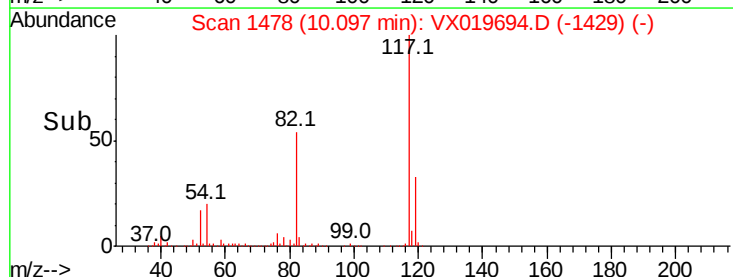
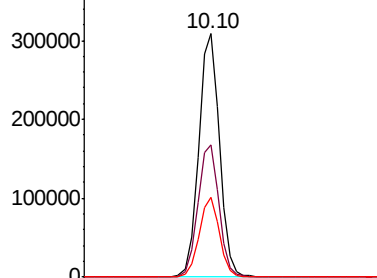




#70
Stvrene
Concen: 1.664 ug/l
RT: 10.69 min Scan# 1576
Delta R.T. -0.00 min
Lab File: VX019694.D
Acq: 01 Dec 2020 14:47




Instrument :
MSVOA_X
ClientSampleId :
PB133320ZHE#07


Tot Ion:104 Resp: 187
Ion Ratio Lower Upper
104 100
78 71.7 39.5 59.3#
103 104.3 43.6 65.4#

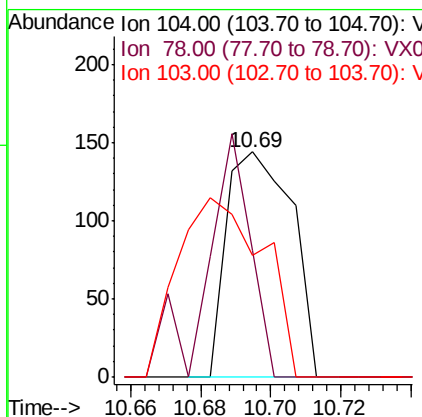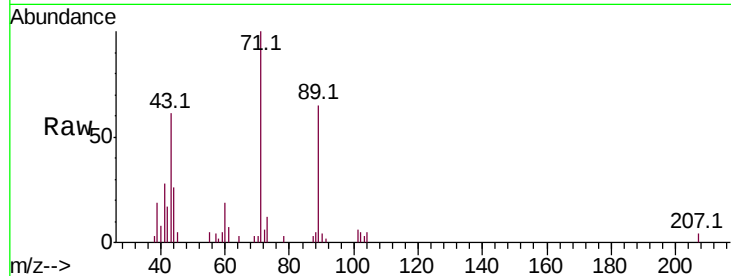

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX019694.D
Acq: 01 Dec 2020 14:47

Tgt Ion:152 Resp: 155839
Ion Ratio Lower Upper
152 100
115 60.6 41.8 125.4
150 159.1 0.0 348.2

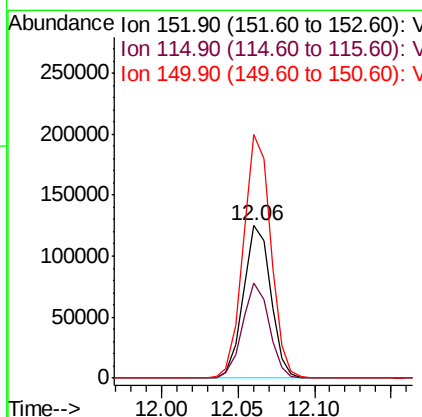



#74

N-amvl acetate

Concen: 0.441 ug/l

RT: 10.80 min Scan# 1594

Delta R.T. -0.07 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47

Instrument :

MSVOA_X

ClientSampleId :

PB133320ZHE#07

Tot Ion: 43 Resp: 1780


Ion Ratio Lower Upper

43 100

70 0.0 39.7 59.5#

55 17.0 21.8 32.6#

61 0.0 22.2 33.4#






Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

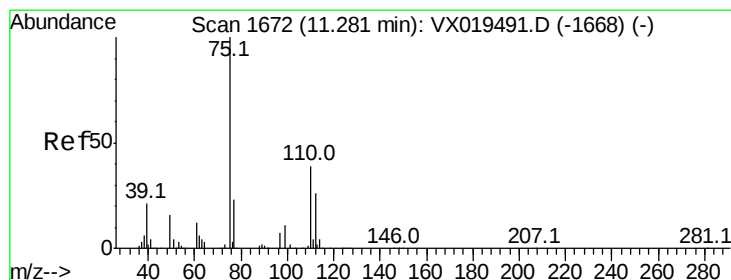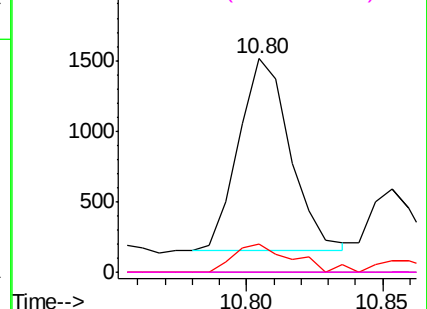

#76

1,2,3-Trichloropropane

Concen: 26.540 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX019694.D


Acq: 01 Dec 2020 14:47

Tgt Ion: 75 Resp: 90262

Ion Ratio Lower Upper



75 100


77 1.4 20.0 60.0#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

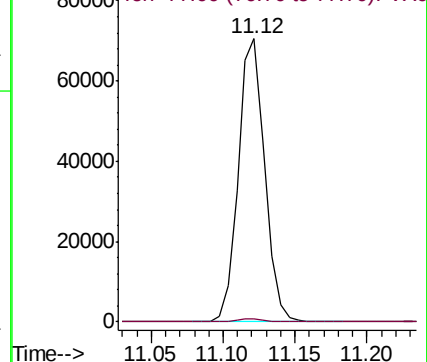

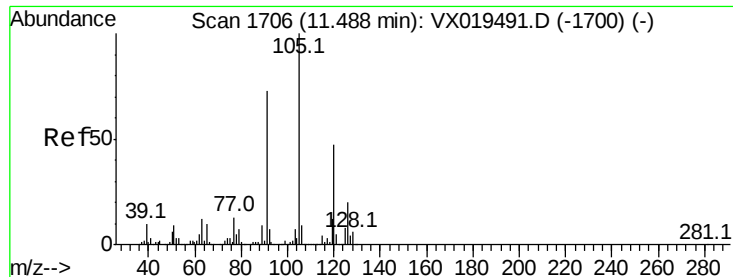

#80

1,3,5-Trimethylbenzene

Concen: 0.215 ug/l

RT: 11.49 min Scan# 1707

Delta R.T. 0.01 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47

Instrument :

MSVOA_X

ClientSampleId :





PB133320ZHE#07

Tot Ion:105 Resp: 1948

Ion Ratio Lower Upper

105 100

120 49.1 24.1 72.3

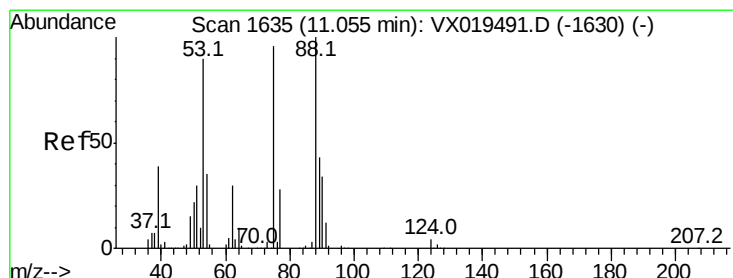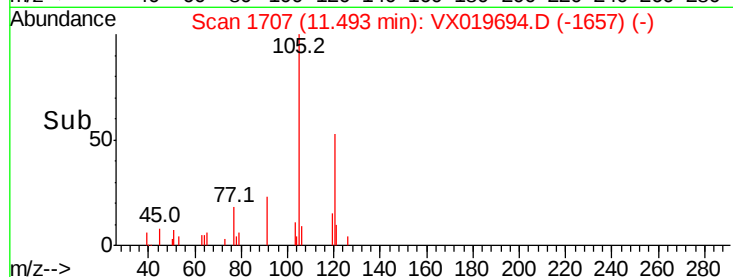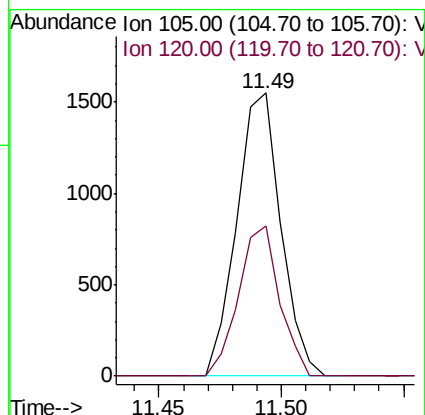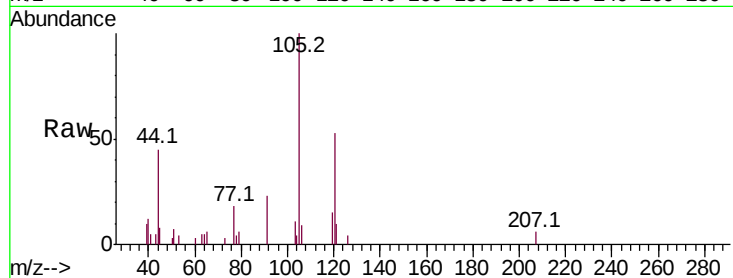

#81

trans-1,4-Dichloro-2-butene

Concen: 69.848 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.07 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47




Tgt Ion: 75 Resp: 90262


Ion Ratio Lower Upper

75 100

53 0.0 73.9 110.9#

89 0.0 37.3 55.9#

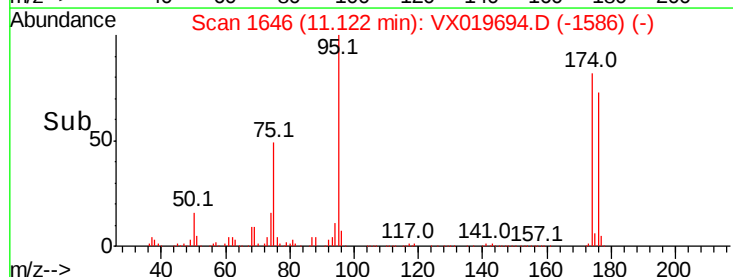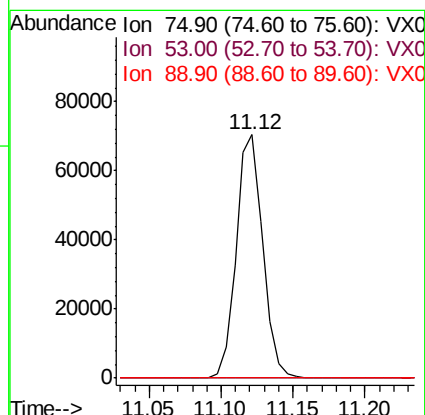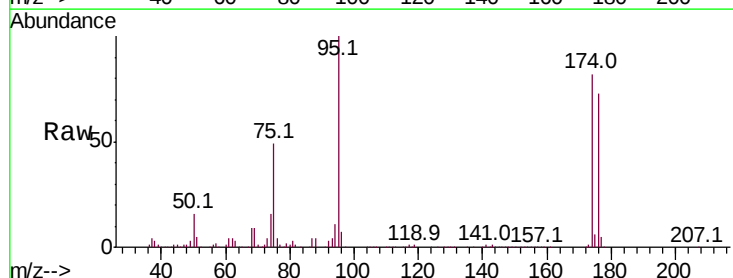

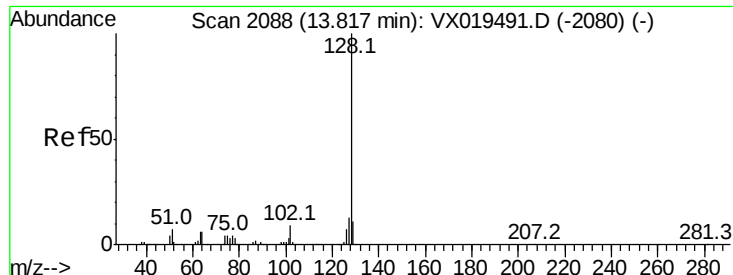

#95

Naphthalene

Concen: 2.212 ug/l

RT: 13.82 min Scan# 2088

Delta R.T. 0.00 min

Lab File: VX019694.D

Acq: 01 Dec 2020 14:47

Instrument :

MSVOA_X

ClientSampleId :

PB133320ZHE#07


Tot Ion:128 Resp: 403

Ion Ratio Lower Upper

128 100

127 0.0 10.3 15.5#

129 0.0 8.7 13.1#

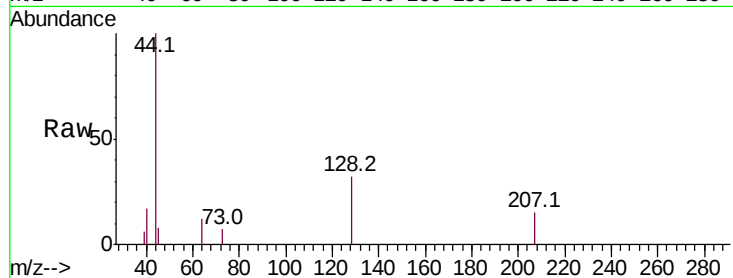

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

