

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX120120\
 Data File : VX019698.D
 Acq On : 01 Dec 2020 16:21
 Operator : JC/MD
 Sample : L4910-08
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PAV-B47-113020-12-12.75


Quant Time: Dec 02 02:13:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 21 01:57:45 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	295567	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	497208	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	438577	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	174386	50.00	ug/l	0.00

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4		6.03	65	187717	48.98	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	97.96%	
35) Dibromofluoromethane		5.46	113	150147	48.11	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	96.22%	
50) Toluene-d8		8.70	98	594489	49.02	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	98.04%	
62) 4-Bromofluorobenzene		11.12	95	198944	45.59	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	91.18%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.62	94	444	0.330	ug/l	93
6) Chloroethane	1.69	64	119	Below Cal	#	42
11) Tert butyl alcohol	3.03	59	4710	6.494	ug/l #	93
13) Acrolein	2.28	56	212	0.435	ug/l #	57
16) Acetone	2.42	43	17315	11.683	ug/l	98
17) Carbon Disulfide	2.54	76	1836	0.233	ug/l #	95
18) Methyl Acetate	2.76	43	2441	1.298	ug/l	97
20) Methylene Chloride	2.83	84	20960	5.659	ug/l	98
25) 2-Butanone	4.64	43	13447	6.040	ug/l	97
29) Tetrahydrofuran	5.12	42	2089	1.471	ug/l #	79
30) Chloroform	5.17	83	1262	0.207	ug/l	94
31) Cyclohexane	5.62	56	5860	1.176	ug/l #	1
36) 1,1-Dichloropropene	5.62	75	22022	4.724	ug/l #	50
37) Ethyl Acetate	4.64	43	13749	3.142	ug/l #	65
38) Carbon Tetrachloride	5.62	117	28893	6.404	ug/l #	16
43) Isopropyl Acetate	6.41	43	31552	4.289	ug/l	99
48) Methyl methacrylate	7.65	41	7225	2.097	ug/l #	9
49) 1,4-Dioxane	7.85	88	240	3.068	ug/l #	1
51) 4-Methyl-2-Pentanone	8.59	43	80314	18.723	ug/l #	46
54) cis-1,3-Dichloropropene	8.59	75	43640	7.776	ug/l #	61
57) 1,3-Dichloropropane	9.52	76	17268	2.891	ug/l #	44
59) 2-Hexanone	9.52	43	207893	63.902	ug/l #	48
70) Styrene	10.69	104	196	1.664	ug/l #	83
76) 1,2,3-Trichloropropane	11.12	75	96984	25.484	ug/l #	37
81) trans-1,4-Dichloro-2-buten	11.12	75	96984	67.236	ug/l #	12
95) Naphthalene	13.82	128	11670	3.046	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.00 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21

Instrument :

MSVOA_X

ClientSampleId :


PAV-B47-113020-12-12.75

Tot Ion:168 Resp: 295567

Ion Ratio Lower Upper

168 100

99 56.0 45.8 68.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

120000

100000

80000



60000

40000

20000

0

Time-->

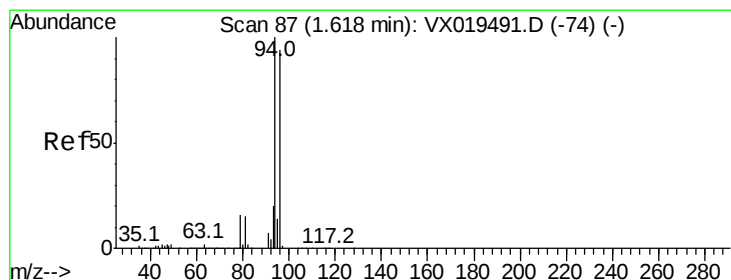

#5

Bromomethane

Concen: 0.330 ug/l

RT: 1.62 min Scan# 88

Delta R.T. 0.01 min

Lab File: VX019698.D


Acq: 01 Dec 2020 16:21

Tgt Ion: 94 Resp: 444

Ion Ratio Lower Upper

94 100

96 87.9 75.6 113.4

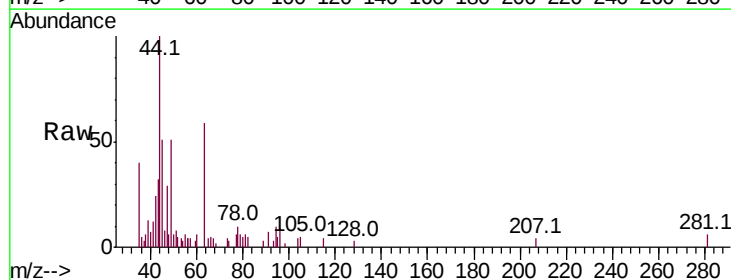

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.62

250

200


150


100

50

0

Time-->



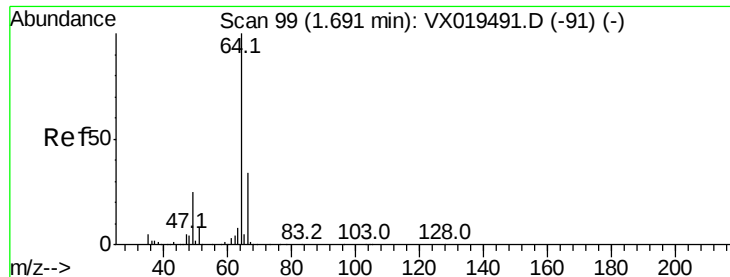

#6

Chloroethane

Concen: Below Cal

RT: 1.69 min Scan# 99

Delta R.T. 0.00 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21

Instrument :

MSVOA_X

ClientSampleId :


PAV-B47-113020-12-12.75

Tot Ion: 64 Resp: 119




Ion Ratio Lower Upper

64 100

66 0.9 27.1 40.7#

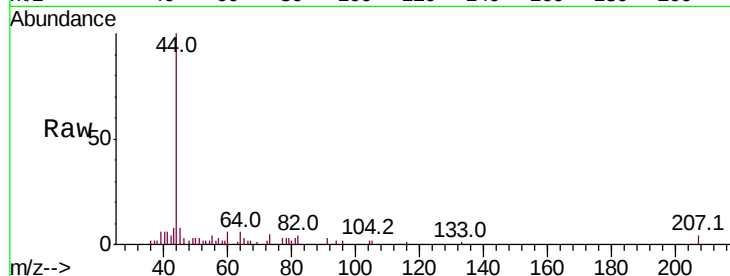

Abundance Ion 63.90 (63.60 to 64.60): VX0

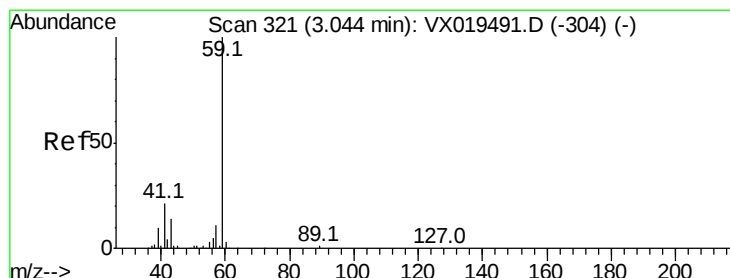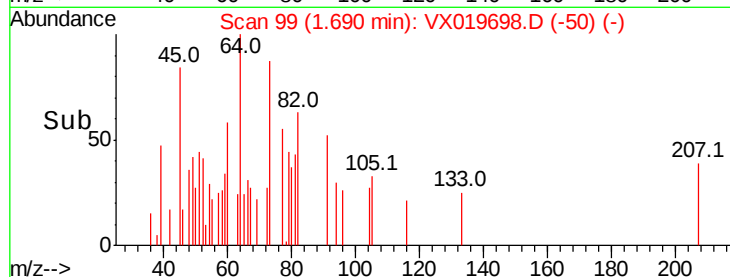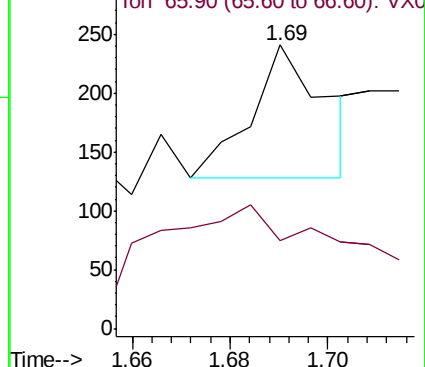

#11

Tert butyl alcohol

Concen: 6.494 ug/l

RT: 3.03 min Scan# 319

Delta R.T. -0.01 min

Lab File: VX019698.D


Acq: 01 Dec 2020 16:21

Tgt Ion: 59 Resp: 4710



Ion Ratio Lower Upper


59 100

57 7.2 7.9 11.9#

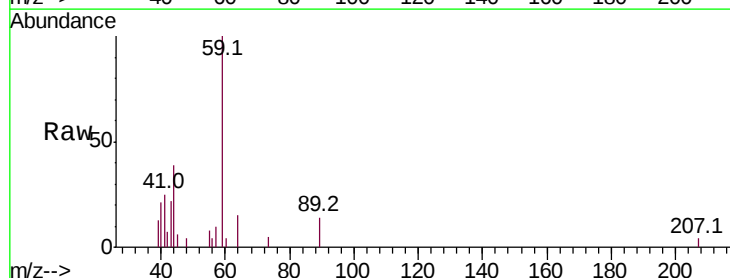

Abundance Ion 59.00 (58.70 to 59.70): VX0

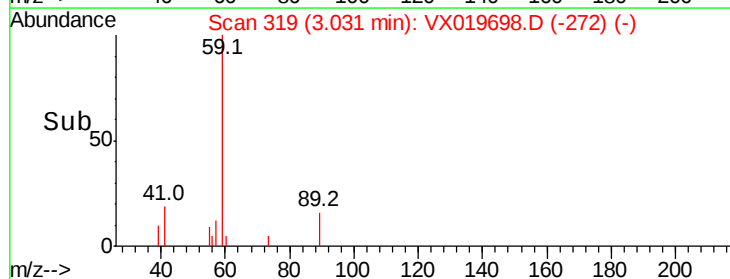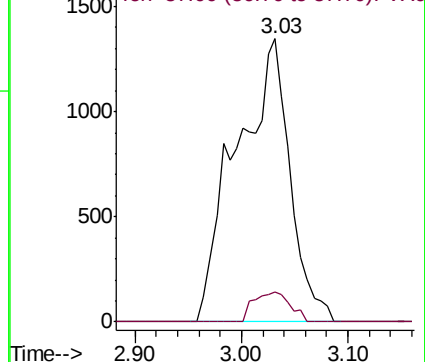

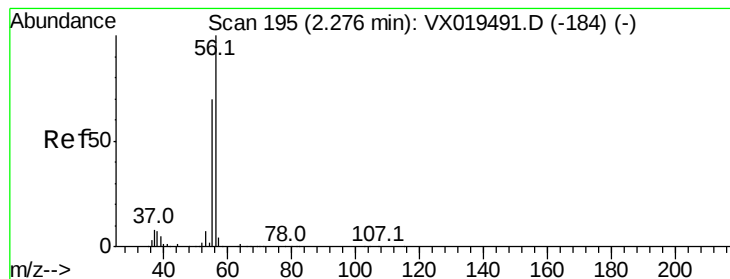

#13

Acrolein

Concen: 0.435 ug/l

RT: 2.28 min Scan# 195

Delta R.T. -0.00 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21

Instrument :

MSVOA_X

ClientSampleId :





PAV-B47-113020-12-12.75

Tot Ion: 56 Resp: 212

Ion Ratio Lower Upper

56 100

55 34.0 55.5 83.3#

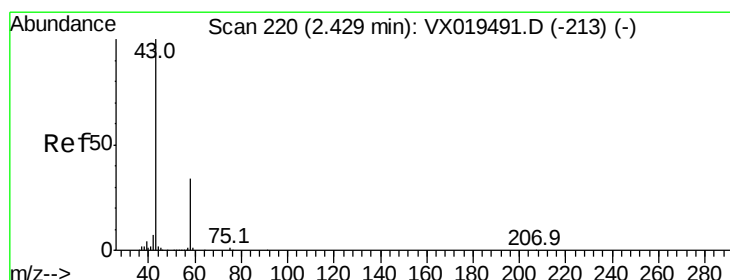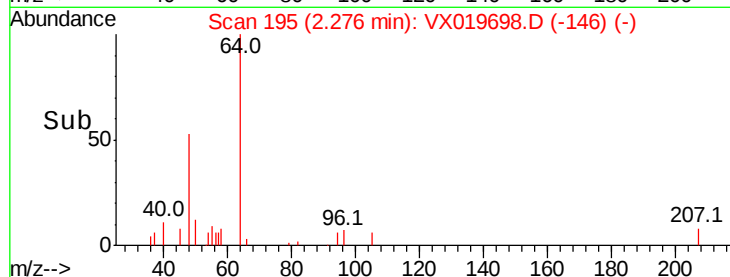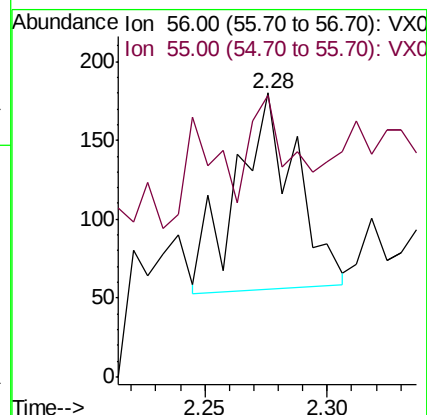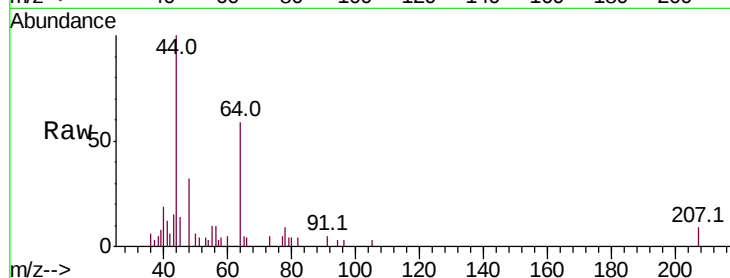

#16

Acetone

Concen: 11.683 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.01 min

Lab File: VX019698.D




Acq: 01 Dec 2020 16:21


Tgt Ion: 43 Resp: 17315

Ion Ratio Lower Upper

43 100

58 33.2 27.4 41.2

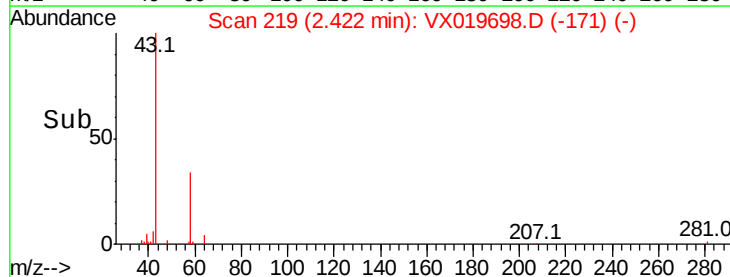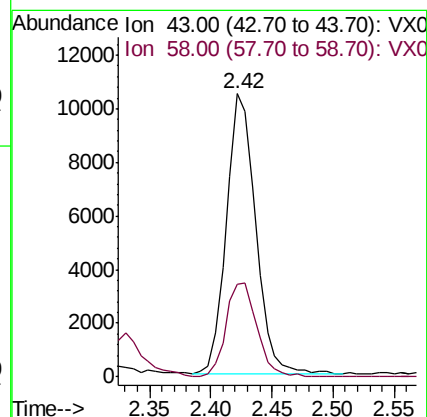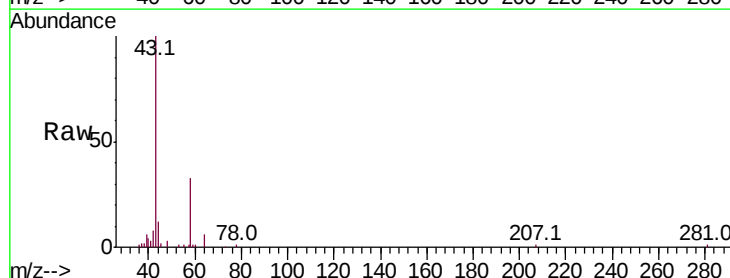

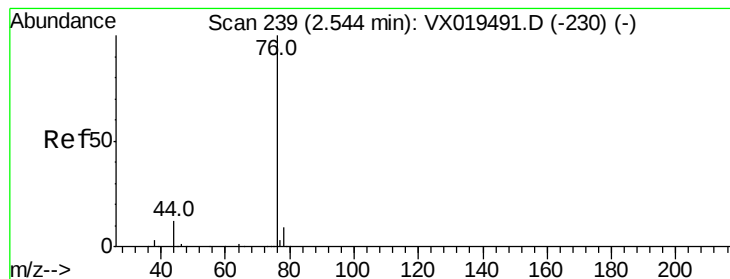

#17

Carbon Disulfide

Concen: 0.233 ug/l

RT: 2.54 min Scan# 239

Delta R.T. -0.00 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21

Instrument :

MSVOA_X

ClientSampleId :


PAV-B47-113020-12-12.75

Tot Ion: 76 Resp: 1836

Ion Ratio Lower Upper

76 100

78 10.9 7.2 10.8#

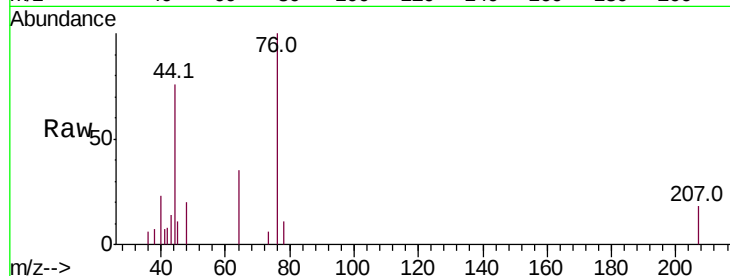

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

2.54

1200

1000

800

600

400

200



0

Time-->

2.50

2.55

2.60

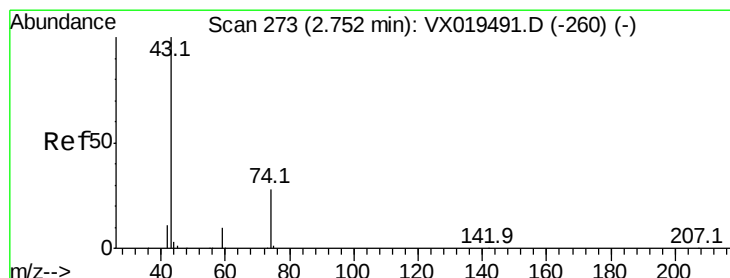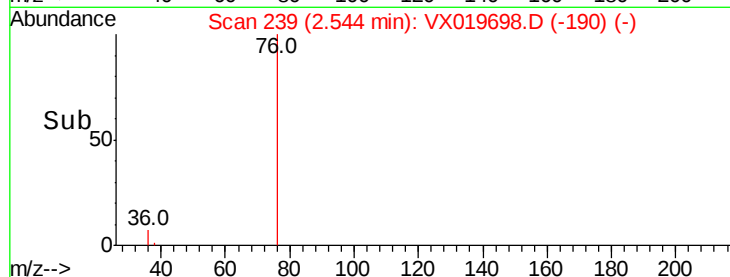

#18

Methyl Acetate

Concen: 1.298 ug/l

RT: 2.76 min Scan# 274

Delta R.T. 0.01 min

Lab File: VX019698.D


Acq: 01 Dec 2020 16:21

Tgt Ion: 43 Resp: 2441

Ion Ratio Lower Upper

43 100

74 26.3 22.2 33.4

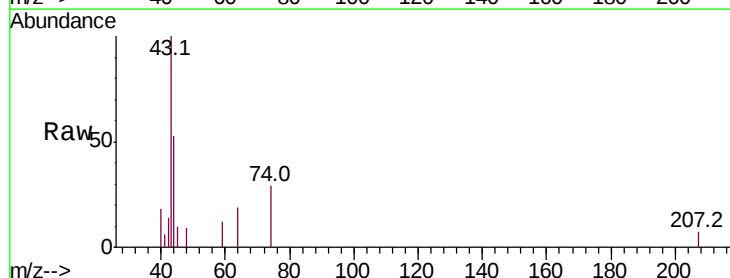

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0

2.76

1000

500

0

Time-->


2.65


2.70

2.75

2.80

2.85




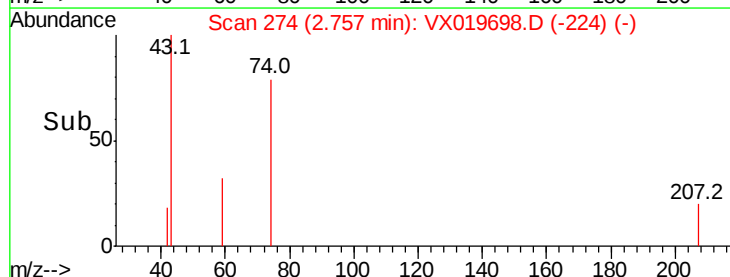




#20
Methvlene Chloride
Concen: 5.659 ug/l
RT: 2.83 min Scan# 286
Delta R.T. -0.00 min
Lab File: VX019698.D
Acq: 01 Dec 2020 16:21




Instrument :
MSVOA_X
ClientSampleId :
PAV-B47-113020-12-12.75


Tot Ion:	84	Resp:	20960
Ion	Ratio	Lower	Upper
84	100		
49	108.6	88.5	132.7
51	37.4	28.0	42.0
86	66.6	53.0	79.4

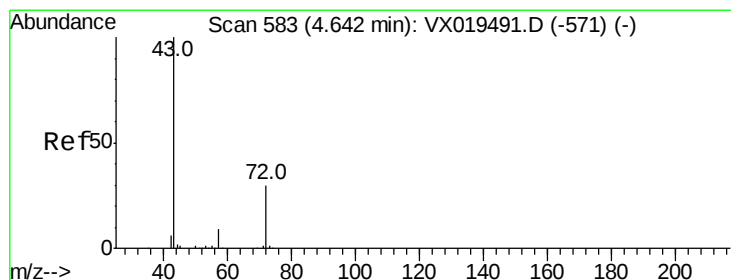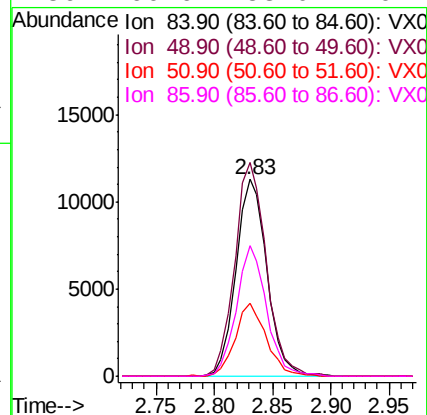

#25
2-Butanone
Concen: 6.040 ug/l
RT: 4.64 min Scan# 583
Delta R.T. -0.00 min
Lab File: VX019698.D
Acq: 01 Dec 2020 16:21

Tgt Ion:	43	Resp:	13447
Ion	Ratio	Lower	Upper
43	100		
72	31.5	24.0	36.0

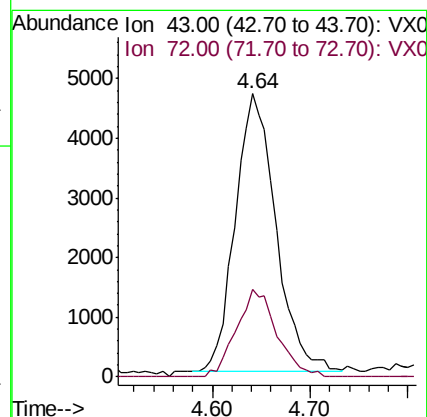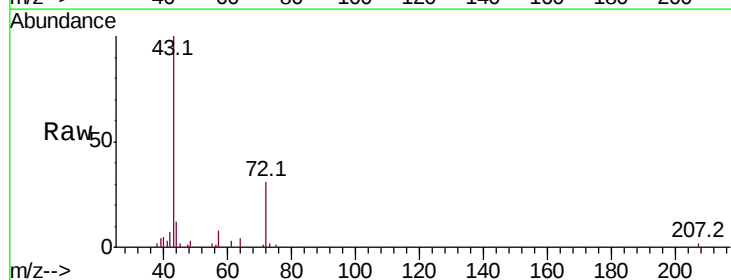



#29

Tetrahydrofuran

Concen: 1.471 ug/l

RT: 5.12 min Scan# 662

Delta R.T. 0.03 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21

Instrument :

MSVOA_X

ClientSampleId :

PAV-B47-113020-12-12.75


Tot Ion: 42 Resp: 2089

Ion Ratio Lower Upper

42 100

72 40.0 42.6 63.8#

71 33.1 39.0 58.6#



Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0



5.12

400

200

0

Time-->

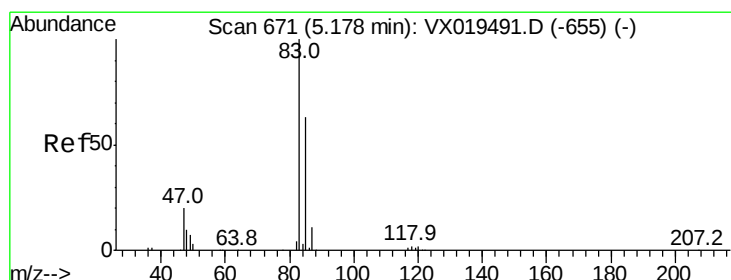

#30

Chloroform

Concen: 0.207 ug/l

RT: 5.17 min Scan# 670

Delta R.T. -0.01 min

Lab File: VX019698.D


Acq: 01 Dec 2020 16:21

Tgt Ion: 83 Resp: 1262

Ion Ratio Lower Upper

83 100

85 67.8 50.5 75.7



Abundance Ion 82.90 (82.60 to 83.60): VX0

Ion 84.90 (84.60 to 85.60): VX0

5.17


400


200

100

0

Time-->









#31
Cyclohexane
Concen: 1.176 ug/l
RT: 5.62 min Scan# 744
Delta R.T. 0.08 min
Lab File: VX019698.D
Acq: 01 Dec 2020 16:21




Instrument :
MSVOA_X
ClientSampleId :
PAV-B47-113020-12-12.75


Tot Ion: 56 Resp: 5860
Ion Ratio Lower Upper
56 100
69 175.7 25.5 38.3#
84 155.4 71.1 106.7#

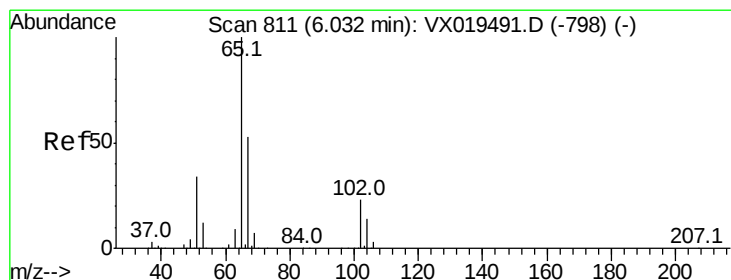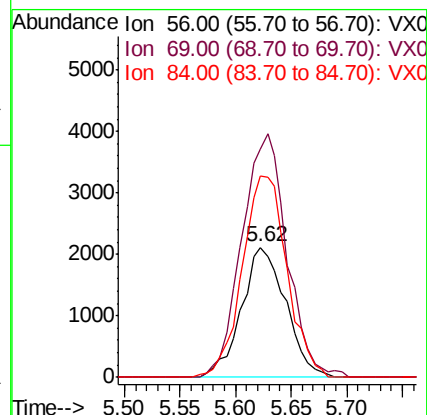

#33
1,2-Dichloroethane-d4
Concen: 48.983 ug/l
RT: 6.03 min Scan# 811
Delta R.T. -0.00 min
Lab File: VX019698.D
Acq: 01 Dec 2020 16:21

Tgt Ion: 65 Resp: 187717
Ion Ratio Lower Upper
65 100
67 52.6 0.0 105.0

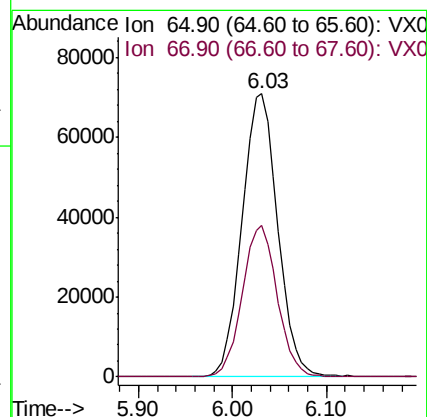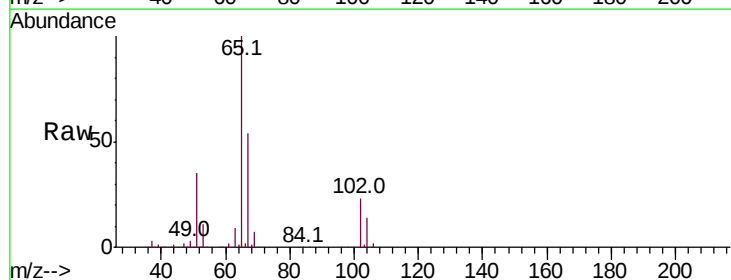

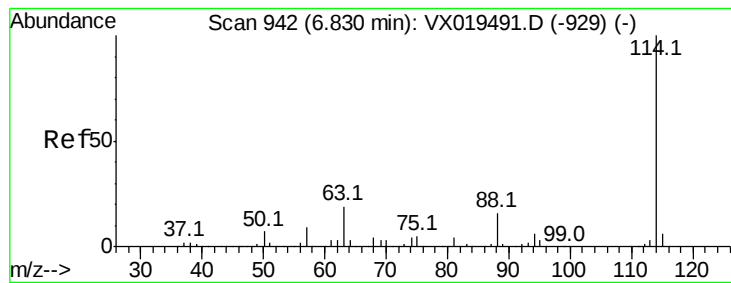

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21

Instrument :

MSVOA_X

ClientSampleId :

PAV-B47-113020-12-12.75


Tot Ion:114 Resp: 497208

Ion Ratio Lower Upper

114 100

63 21.6 0.0 38.8




88 16.3 0.0 31.6



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

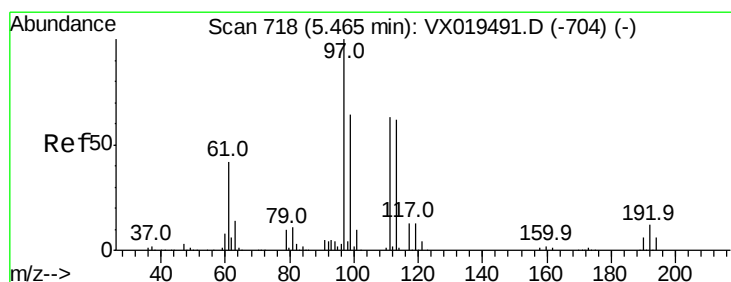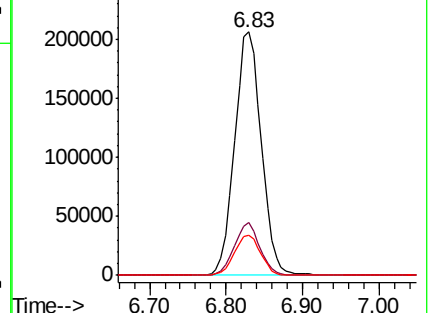

#35

Dibromofluoromethane

Concen: 48.109 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21


Tgt Ion:113 Resp: 150147

Ion Ratio Lower Upper

113 100

111 102.0 81.5 122.3



192 19.6 16.2 24.2




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

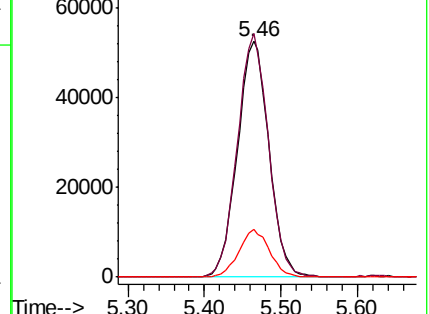



#36

1,1-Dichloropropene

Concen: 4.724 ug/l

RT: 5.62 min Scan# 744

Delta R.T. -0.14 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21

Instrument :

MSVOA_X

ClientSampleId :

PAV-B47-113020-12-12.75


Tot Ion: 75 Resp: 22022

Ion Ratio Lower Upper

75 100

110 9.2 18.1 54.3#




77 0.0 24.2 36.4#

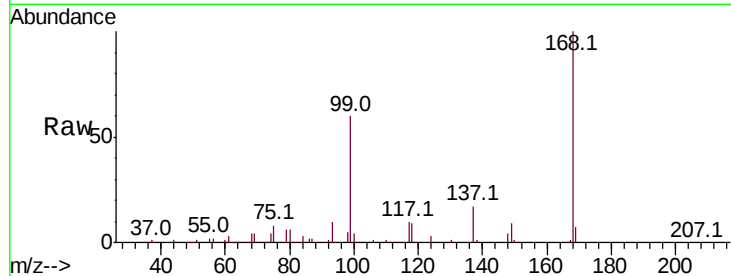

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): VX0

Ion 76.90 (76.60 to 77.60): VX0

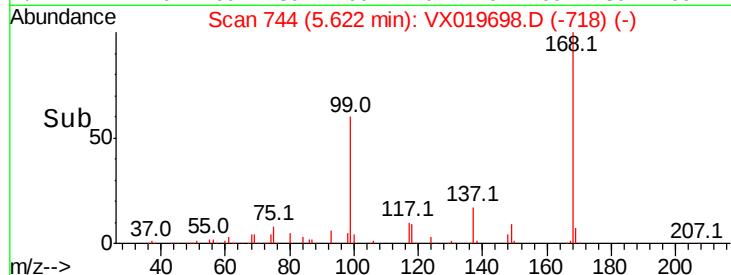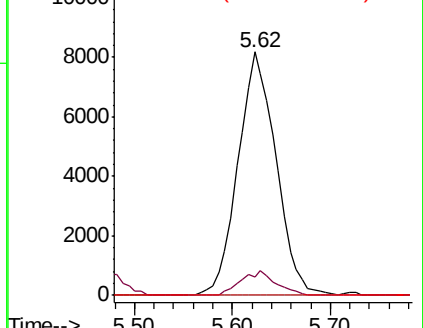

#37

Ethyl Acetate

Concen: 3.142 ug/l

RT: 4.64 min Scan# 583

Delta R.T. -0.15 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21


Tgt Ion: 43 Resp: 13749

Ion Ratio Lower Upper

43 100

61 0.0 12.7 19.1#



70 0.0 10.2 15.2#




Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 70.00 (69.70 to 70.70): VX0

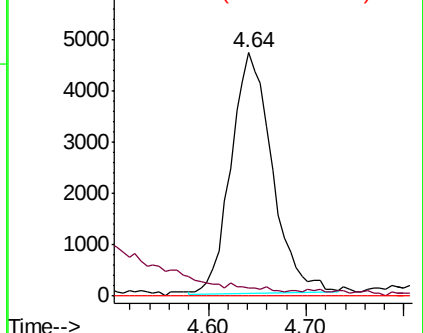



#38

Carbon Tetrachloride

Concen: 6.404 ug/l

RT: 5.62 min Scan# 744

Delta R.T. -0.13 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21

Instrument :

MSVOA_X

ClientSampleId :

PAV-B47-113020-12-12.75


Tot Ion:117 Resp: 28893

Ion Ratio Lower Upper

117 100

119 4.1 75.9 113.9#




121 0.0 24.0 36.0#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

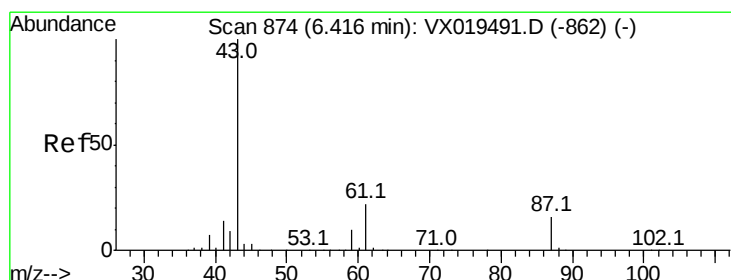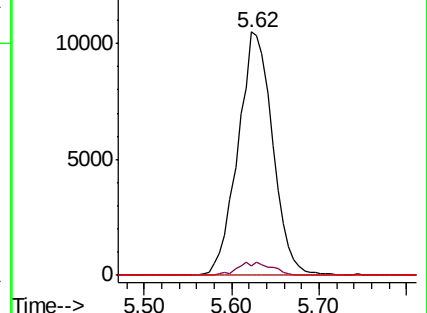

#43

Isopropyl Acetate

Concen: 4.289 ug/l

RT: 6.41 min Scan# 873

Delta R.T. -0.01 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21


Tgt Ion: 43 Resp: 31552

Ion Ratio Lower Upper

43 100

61 22.2 18.2 27.2



87 15.1 12.6 18.8




Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0



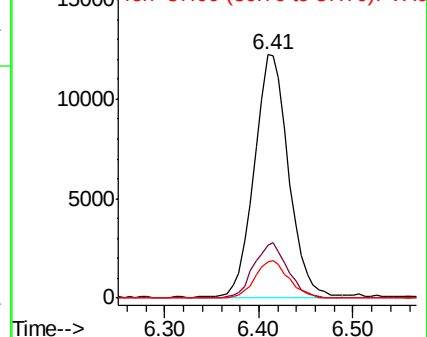





#48
Methvl methacrylate
Concen: 2.097 ug/l
RT: 7.65 min Scan# 1076
Delta R.T. -0.10 min
Lab File: VX019698.D
Acq: 01 Dec 2020 16:21




Instrument :
MSVOA_X
ClientSampleId :
PAV-B47-113020-12-12.75


Tot Ion: 41 Resp: 7225
Ion Ratio Lower Upper
41 100
69 0.0 77.0 115.6#
39 0.0 45.6 68.4#

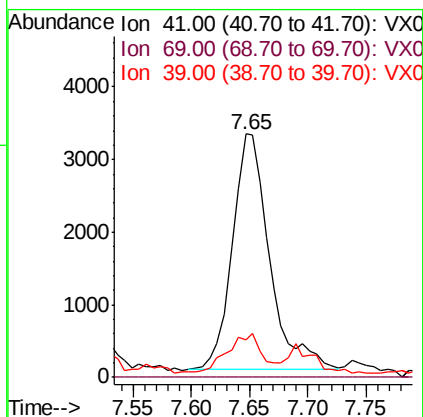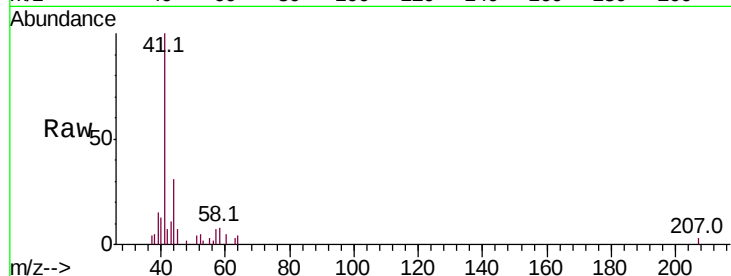

#49
1,4-Dioxane
Concen: 3.068 ug/l
RT: 7.85 min Scan# 1110
Delta R.T. 0.13 min
Lab File: VX019698.D
Acq: 01 Dec 2020 16:21

Tgt Ion: 88 Resp: 240
Ion Ratio Lower Upper
88 100
43 536960.0 23.8 35.6#
58 2768.3 54.2 81.2#



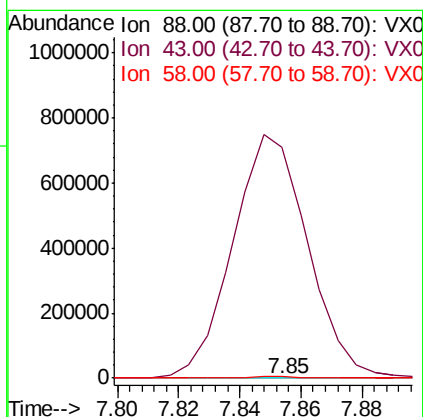





#50
Toluene-d8
Concen: 49.019 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX019698.D
Acq: 01 Dec 2020 16:21




Instrument :
MSVOA_X
ClientSampleId :
PAV-B47-113020-12-12.75


Tot Ion: 98 Resp: 594489
Ion Ratio Lower Upper
98 100
100 66.6 52.4 78.6

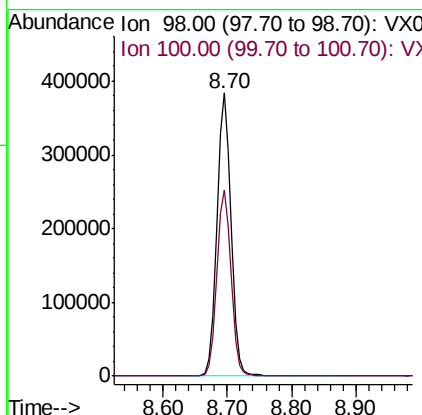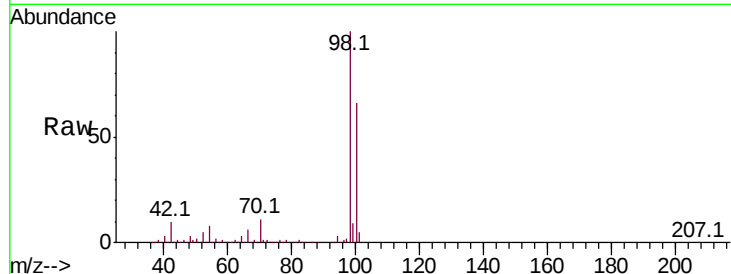

#51
4-Methyl-2-Pentanone
Concen: 18.723 ug/l
RT: 8.59 min Scan# 1231
Delta R.T. -0.03 min
Lab File: VX019698.D
Acq: 01 Dec 2020 16:21

Tgt Ion: 43 Resp: 80314
Ion Ratio Lower Upper
43 100
58 9.2 35.1 52.7#

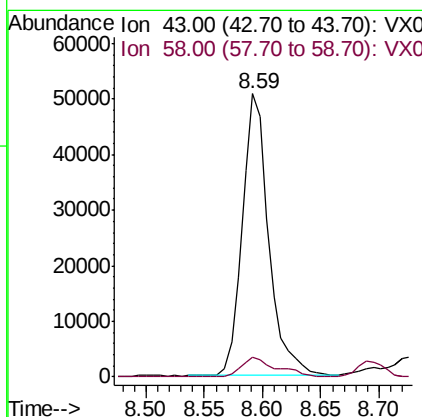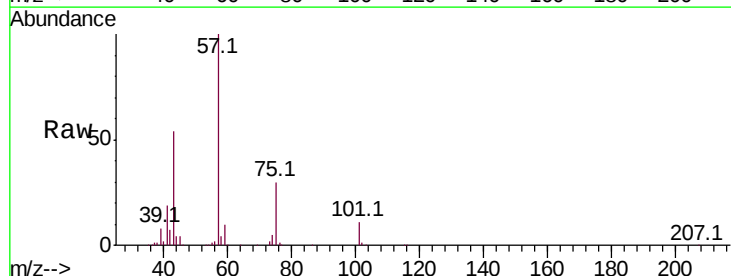



#54

cis-1,3-Dichloropropene

Concen: 7.776 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. 0.18 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21

Instrument :

MSVOA_X

ClientSampleId :

PAV-B47-113020-12-12.75


Tot Ion: 75 Resp: 43640

Ion Ratio Lower Upper

75 100

77 0.5 25.8 38.6#




39 26.2 34.6 51.8#

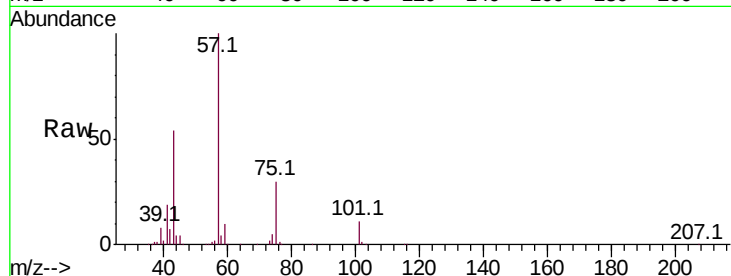

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 76.90 (76.60 to 77.60): VX0

Ion 39.00 (38.70 to 39.70): VX0

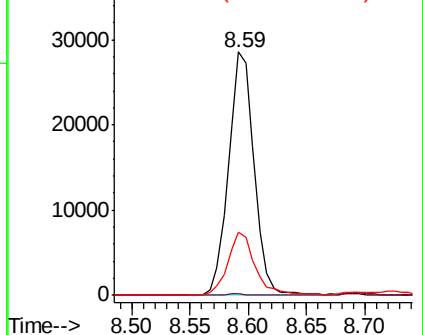

#57

1,3-Dichloropropane

Concen: 2.891 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.17 min

Lab File: VX019698.D


Acq: 01 Dec 2020 16:21

Tgt Ion: 76 Resp: 17268

Ion Ratio Lower Upper



76 100


78 0.6 25.7 38.5#



Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

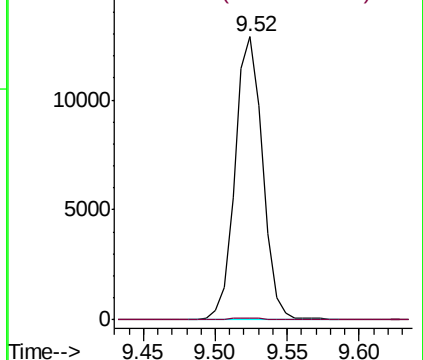



#59

2-Hexanone

Concen: 63.902 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.05 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21

Instrument :

MSVOA_X

ClientSampleId :





PAV-B47-113020-12-12.75

Tot Ion: 43 Resp: 207893

Ion Ratio Lower Upper

43 100

58 21.3 30.6 91.6#

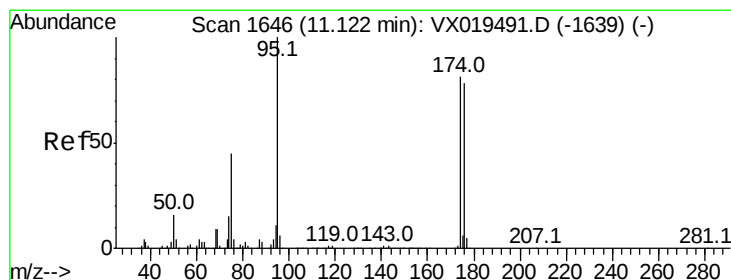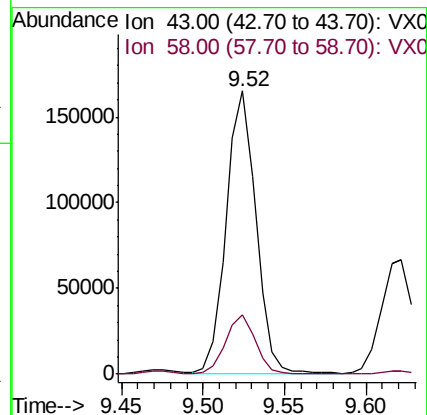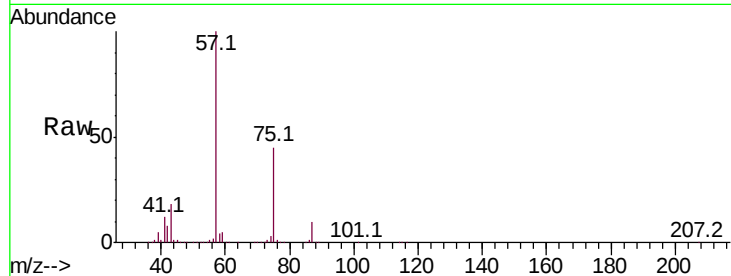

#62

4-Bromofluorobenzene

Concen: 45.594 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21




Tgt Ion: 95 Resp: 198944


Ion Ratio Lower Upper

95 100

174 77.3 0.0 156.2

176 73.4 0.0 151.4


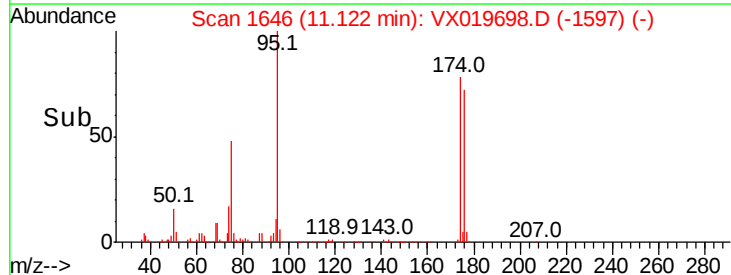
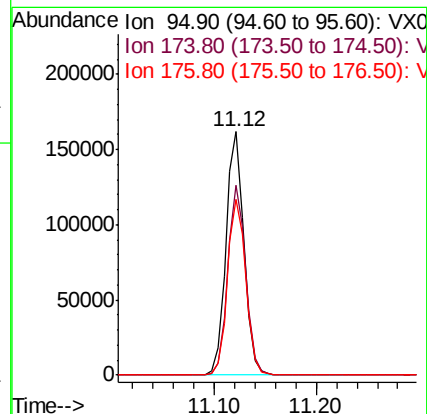





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX019698.D
Acq: 01 Dec 2020 16:21




Instrument :
MSVOA_X
ClientSampleId :
PAV-B47-113020-12-12.75


Tot Ion:117 Resp: 438577
Ion Ratio Lower Upper
117 100
82 54.9 43.0 64.4
119 31.1 25.6 38.4

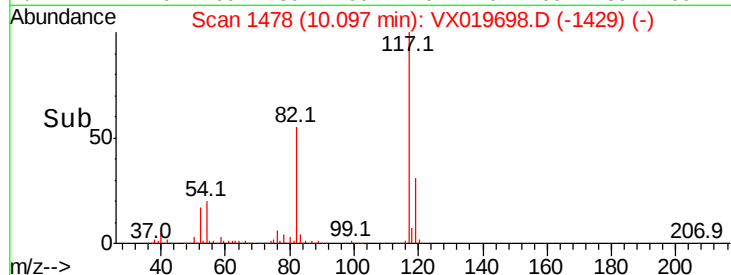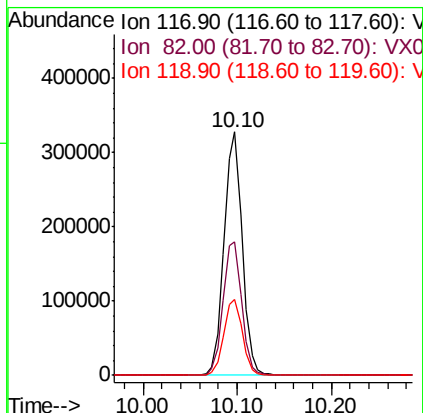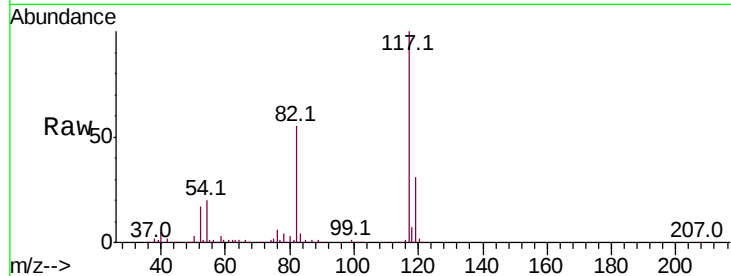

#70
Styrene
Concen: 1.664 ug/l
RT: 10.69 min Scan# 1575
Delta R.T. -0.01 min
Lab File: VX019698.D
Acq: 01 Dec 2020 16:21

Tgt Ion:104 Resp: 196
Ion Ratio Lower Upper
104 100
78 37.8 39.5 59.3#
103 42.3 43.6 65.4#

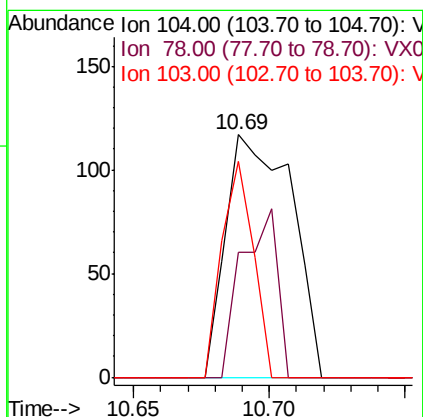



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21

Instrument :

MSVOA_X

ClientSampleId :

PAV-B47-113020-12-12.75


Tot Ion:152 Resp: 174386

Ion Ratio Lower Upper

152 100

115 61.4 41.8 125.4




150 161.3 0.0 348.2

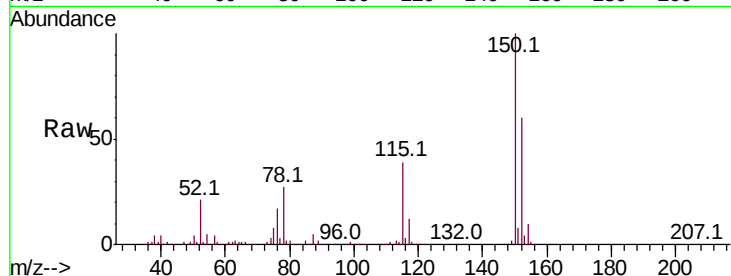

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

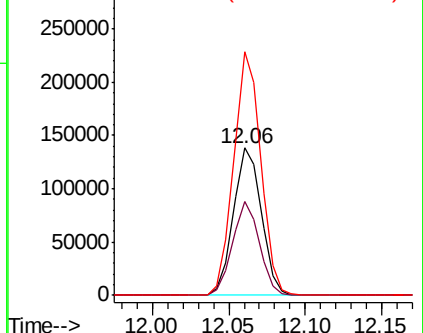

#76

1,2,3-Trichloropropane

Concen: 25.484 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX019698.D


Acq: 01 Dec 2020 16:21

Tgt Ion: 75 Resp: 96984

Ion Ratio Lower Upper



75 100


77 1.2 20.0 60.0#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

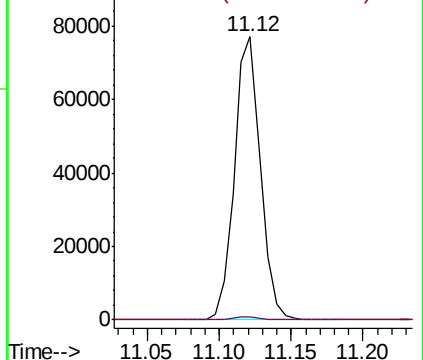



#81

trans-1,4-Dichloro-2-butene

Concen: 67.236 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.07 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21

Instrument :

MSVOA_X

ClientSampleId :

PAV-B47-113020-12-12.75


Tot Ion: 75 Resp: 96984

Ion Ratio Lower Upper




75 100

53 0.0 73.9 110.9#

89 0.0 37.3 55.9#

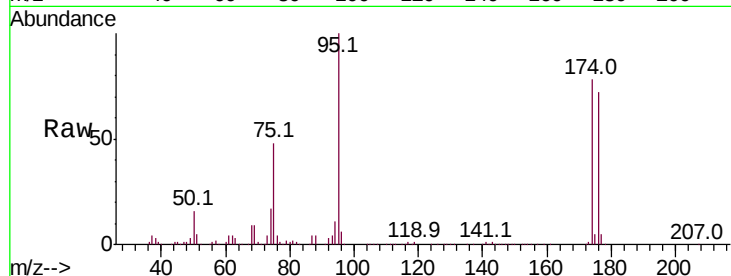

Abundance Ion 74.90 (74.60 to 75.60): VX0
Ion 53.00 (52.70 to 53.70): VX0
Ion 88.90 (88.60 to 89.60): VX0

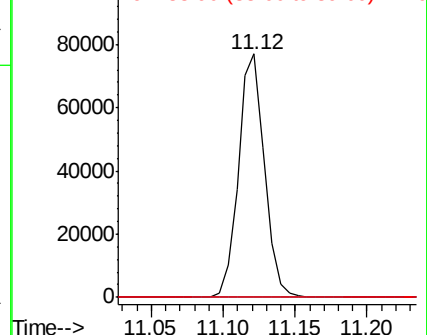

#95

Naphthalene

Concen: 3.046 ug/l

RT: 13.82 min Scan# 2088

Delta R.T. 0.00 min

Lab File: VX019698.D

Acq: 01 Dec 2020 16:21


Tgt Ion:128 Resp: 11670

Ion Ratio Lower Upper

128 100

127 12.2 10.3 15.5

129 10.2 8.7 13.1



Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

