

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120121\
 Data File : VX025411.D
 Acq On : 01 Dec 2021 14:25
 Operator : JC/MD
 Sample : M4866-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 16952

Quant Time: Dec 02 08:28:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 17 15:36:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	120247	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	201309	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	178945	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	84533	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	67793	53.486	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 106.980%			
35) Dibromofluoromethane	5.391	113	61461	49.759	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 99.520%			
50) Toluene-d8	8.653	98	230204	49.570	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 99.140%			
62) 4-Bromofluorobenzene	11.079	95	82606	47.018	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 94.040%			
Target Compounds						
					Qvalue	
3) Chloromethane	1.252	50	15052	11.663	ug/l #	42
6) Chloroethane	1.892	64	525	0.537	ug/l #	79
11) Tert butyl alcohol	2.959	59	4965	7.151	ug/l	94
13) Acrolein	1.977	56	21	0.362	ug/l #	1
16) Acetone	2.380	43	4879	6.928	ug/l	94
17) Carbon Disulfide	2.520	76	3111	0.992	ug/l #	93
25) 2-Butanone	4.574	43	883	0.867	ug/l #	83
31) Cyclohexane	5.556	56	2180	1.113	ug/l #	7
36) 1,1-Dichloropropene	5.556	75	8145	4.637	ug/l #	50
37) Ethyl Acetate	4.574	43	883	0.442	ug/l #	68
38) Carbon Tetrachloride	5.556	117	11039	5.706	ug/l #	18
48) Methyl methacrylate	7.684	41	1054	0.675	ug/l #	31
51) 4-Methyl-2-Pentanone	8.580	43	1948	0.934	ug/l	96
52) Toluene	8.720	92	3295	0.949	ug/l	96
55) 1,1,2-Trichloroethane	9.019	97	555	0.402	ug/l #	15
59) 2-Hexanone	9.439	43	1131	0.688	ug/l	81
68) m/p-Xylenes	10.305	106	1221	0.474	ug/l	97
69) o-Xylene	10.646	106	709	0.281	ug/l	92
74) N-amyl acetate	10.890	43	2927	1.123	ug/l #	43
76) 1,2,3-Trichloropropane	11.366	75	1503	0.868	ug/l	90
78) n-propylbenzene	11.366	91	52040	7.695	ug/l #	56
79) 2-Chlorotoluene	11.366	91	52040	12.640	ug/l	97
80) 1,3,5-Trimethylbenzene	11.451	105	1571	0.310	ug/l	86
81) trans-1,4-Dichloro-2-b...	11.079	75	39446	57.405	ug/l #	9
82) 4-Chlorotoluene	11.457	91	34788	7.402	ug/l	88
84) 1,2,4-Trimethylbenzene	11.750	105	7926	1.584	ug/l	99
89) n-Butylbenzene	12.323	91	1058	0.233	ug/l #	20
90) Hexachloroethane	12.530	117	304	0.307	ug/l #	11
92) 1,2-Dibromo-3-Chloropr...	13.061	75	118	0.290	ug/l #	1
95) Naphthalene	13.780	128	12186	1.775	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120121\
Data File : VX025411.D
Acq On : 01 Dec 2021 14:25
Operator : JC/MD
Sample : M4866-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
16952

Quant Time: Dec 02 08:28:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 17 15:36:16 2021
Response via : Initial Calibration




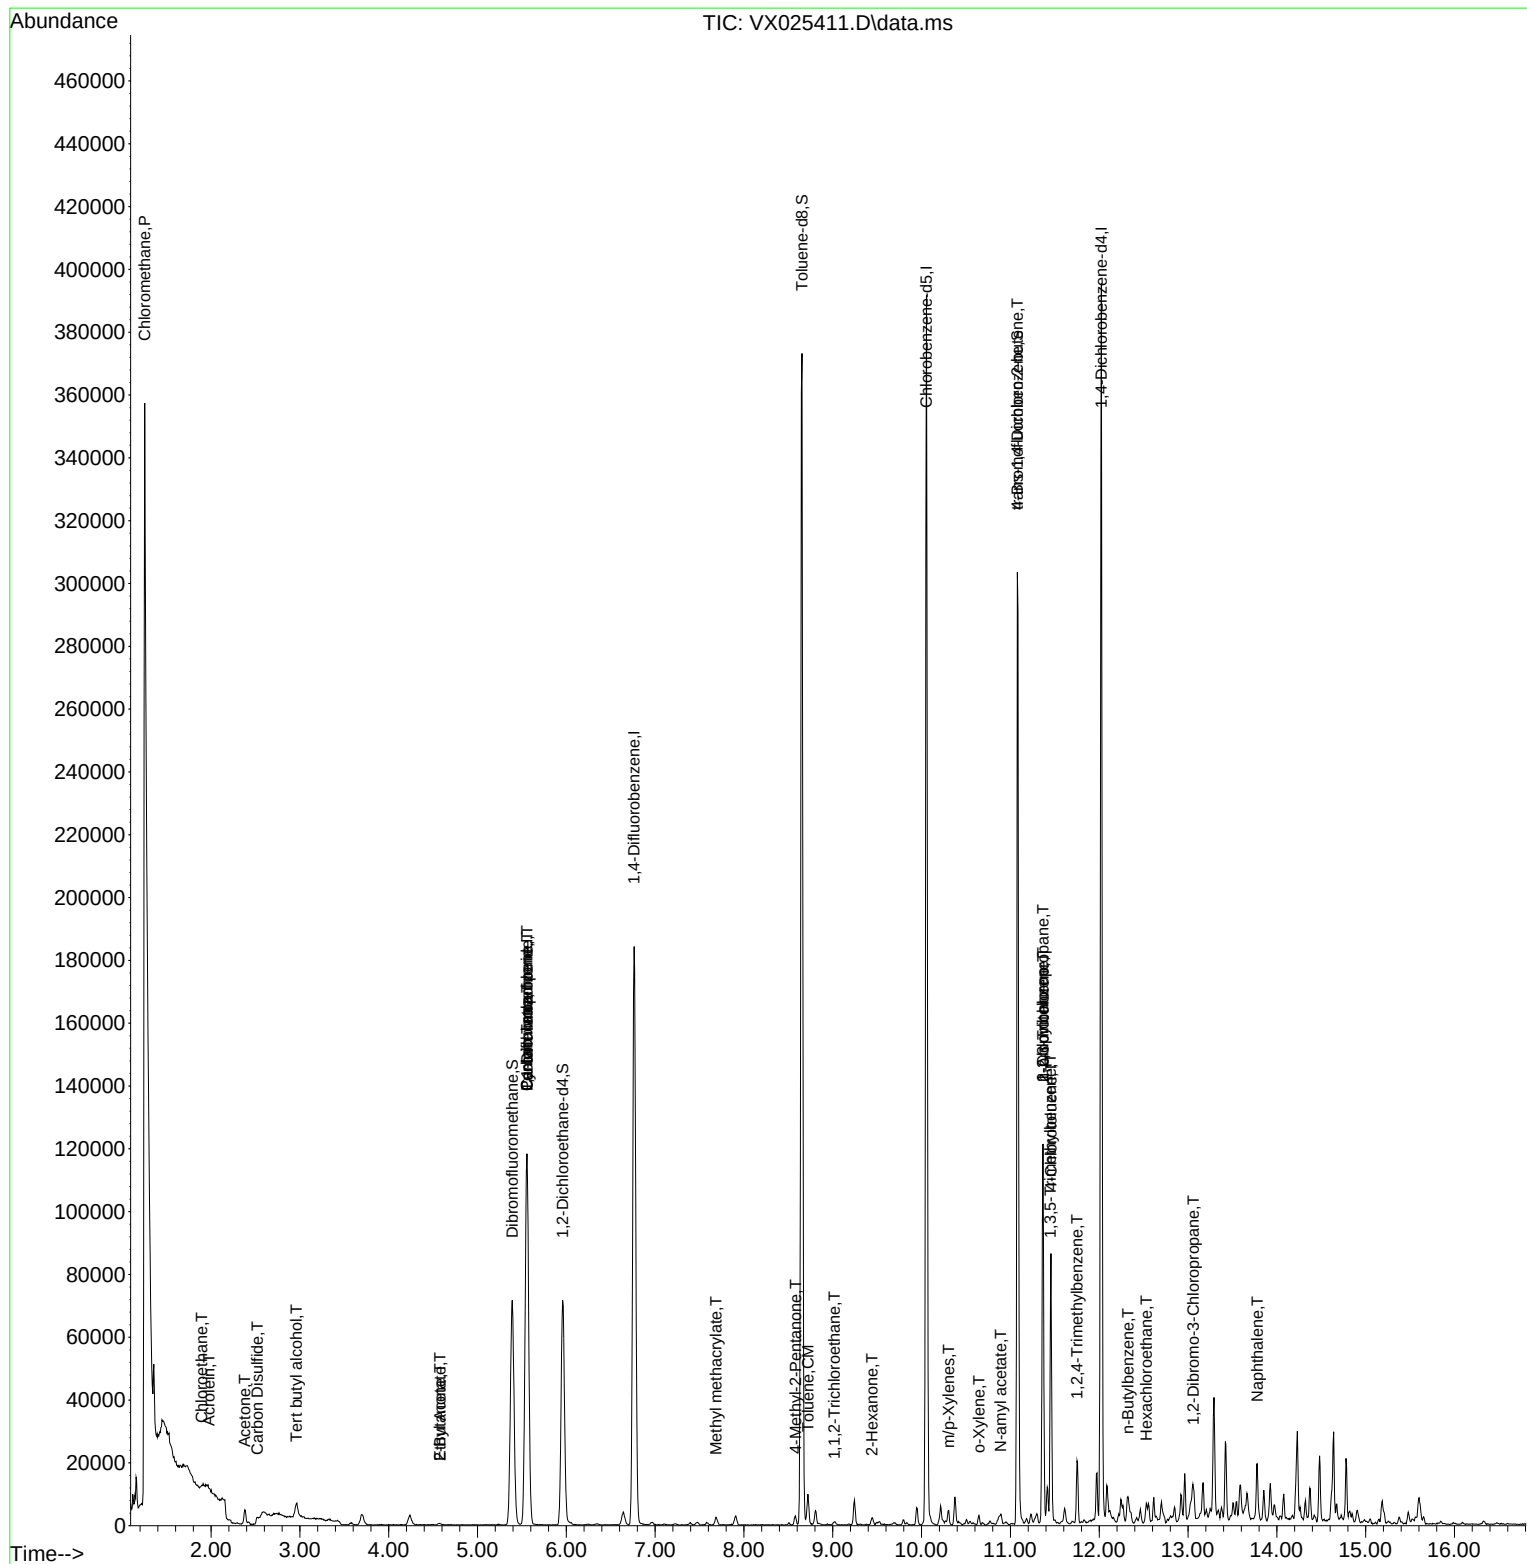


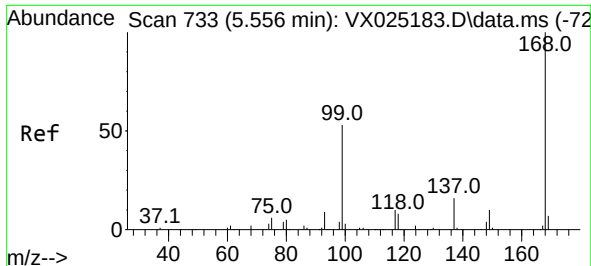

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25




Instrument :
MSVOA_X
ClientSampleId :
16952

Tgt Ion:168 Resp: 120247
Ion Ratio Lower Upper
168 100
99 55.1 46.4 69.6

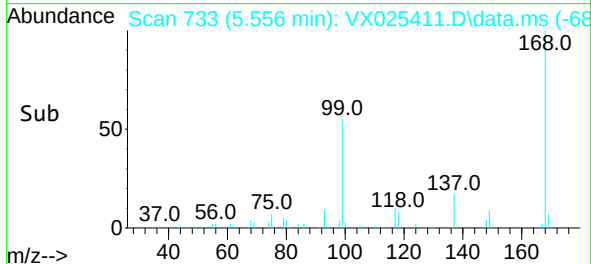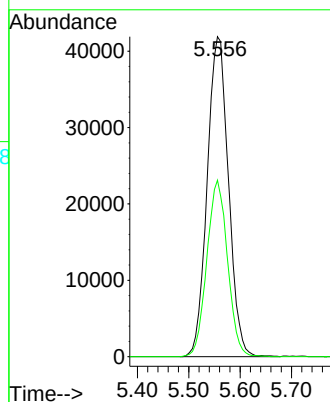


#3
Chloromethane
Concen: 11.663 ug/l
RT: 1.252 min Scan# 27
Delta R.T. -0.036 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25

Tgt Ion: 50 Resp: 15052
Ion Ratio Lower Upper
50 100
52 0.0 25.9 38.9#

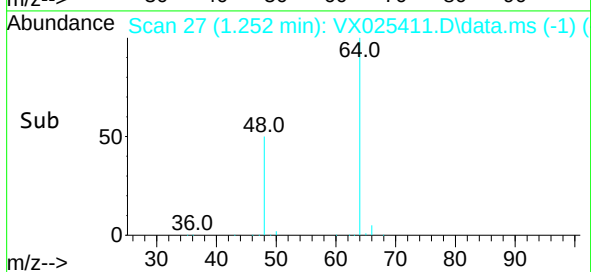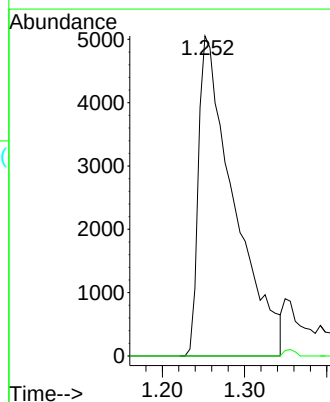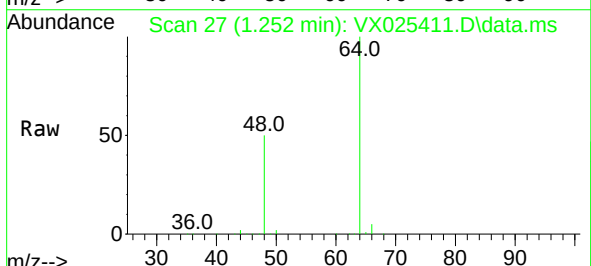

Abundance Scan 97 (1.679 min): VX025183.D\data.ms (-88)

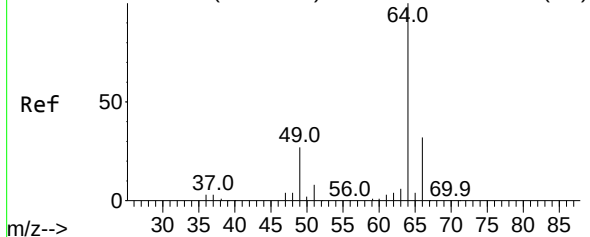

#6

Chloroethane

Concen: 0.537 ug/l

RT: 1.892 min Scan# 11

Delta R.T. 0.213 min

Lab File: VX025411.D

Acq: 01 Dec 2021 14:25

Instrument :

MSVOA_X

ClientSampleId :

16952



Tgt Ion: 64 Resp: 525

Ion Ratio Lower Upper


64 100

66 20.4 25.6 38.4#


Abundance Scan 132 (1.892 min): VX025411.D\data.ms

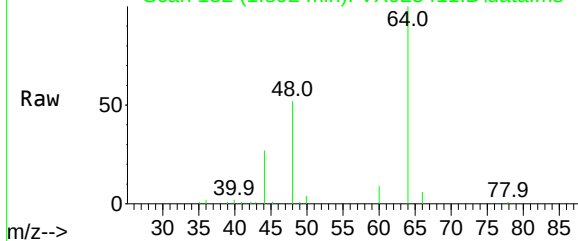

Abundance Scan 132 (1.892 min): VX025411.D\data.ms (-48)

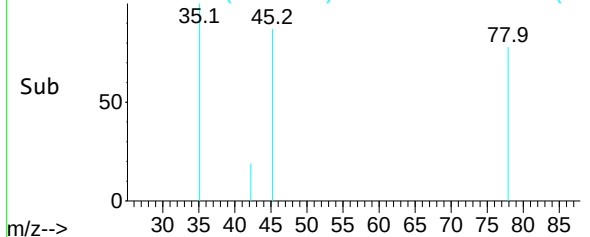

Abundance Scan 308 (2.965 min): VX025183.D\data.ms (-29)

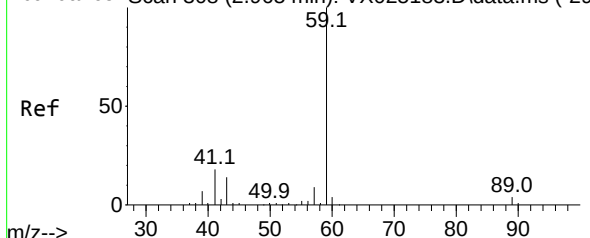

#11

Tert butyl alcohol

Concen: 7.151 ug/l

RT: 2.959 min Scan# 307

Delta R.T. -0.006 min

Lab File: VX025411.D

Acq: 01 Dec 2021 14:25



Tgt Ion: 59 Resp: 4965

Ion Ratio Lower Upper


59 100


57 8.5 8.5 12.7

Abundance Scan 307 (2.959 min): VX025411.D\data.ms

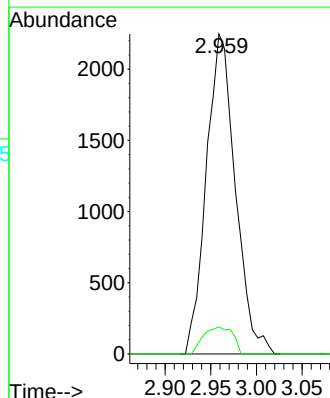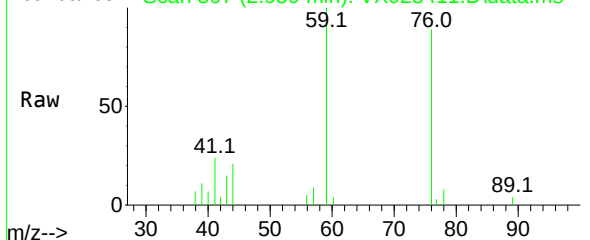

Abundance Scan 307 (2.959 min): VX025411.D\data.ms (-25)

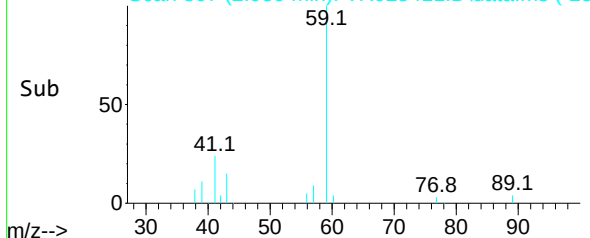

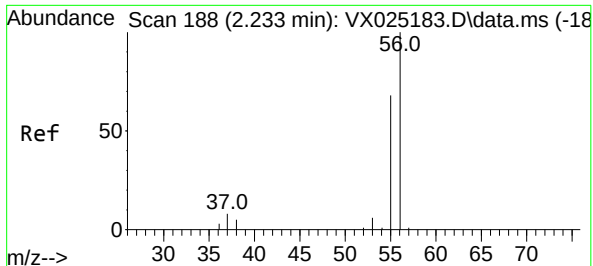

#13

Acrolein

Concen: 0.362 ug/l

RT: 1.977 min Scan# 146

Delta R.T. -0.256 min

Lab File: VX025411.D

Acq: 01 Dec 2021 14:25

Instrument :

MSVOA_X

ClientSampleId :





16952

Tgt Ion: 56 Resp: 21

Ion Ratio Lower Upper

56 100

55 947.6 58.6 87.8#

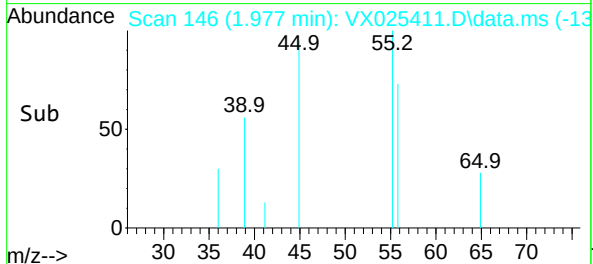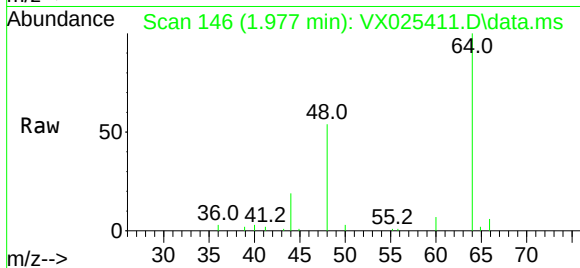

#16

Acetone

Concen: 6.928 ug/l

RT: 2.380 min Scan# 212

Delta R.T. -0.000 min

Lab File: VX025411.D




Acq: 01 Dec 2021 14:25


Tgt Ion: 43 Resp: 4879

Ion Ratio Lower Upper

43 100

58 33.0 24.0 36.0


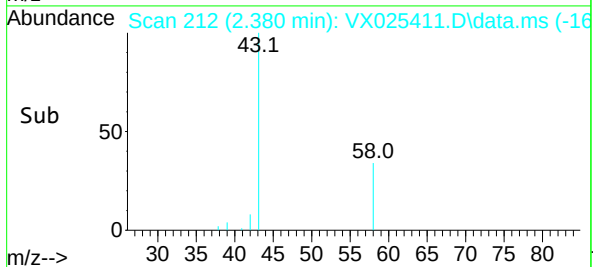

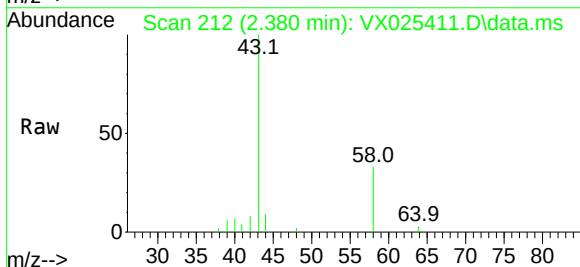




#17
Carbon Disulfide
Concen: 0.992 ug/l
RT: 2.520 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25




Instrument :
MSVOA_X
ClientSampleId :
16952


Tgt Ion: 76 Resp: 3111
Ion Ratio Lower Upper
76 100
78 6.0 6.9 10.3#

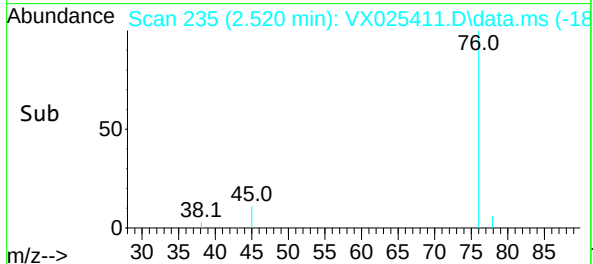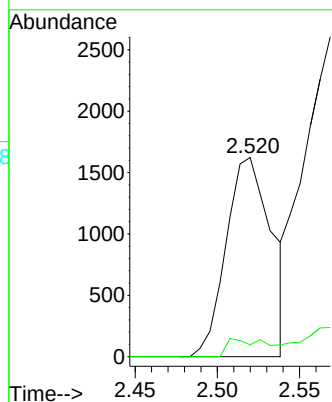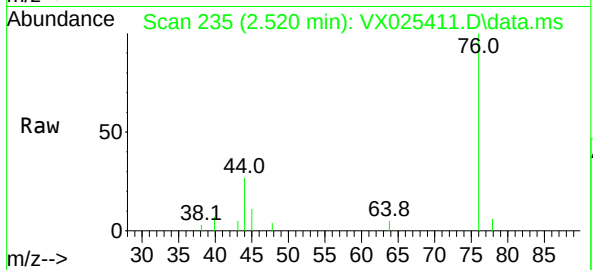

#25
2-Butanone
Concen: 0.867 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.018 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25

Tgt Ion: 43 Resp: 883
Ion Ratio Lower Upper
43 100
72 17.9 21.2 31.8#


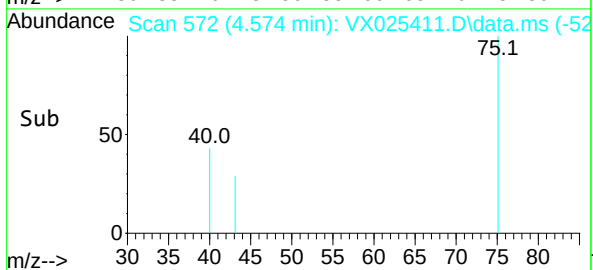
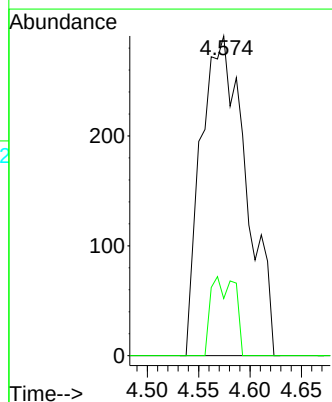
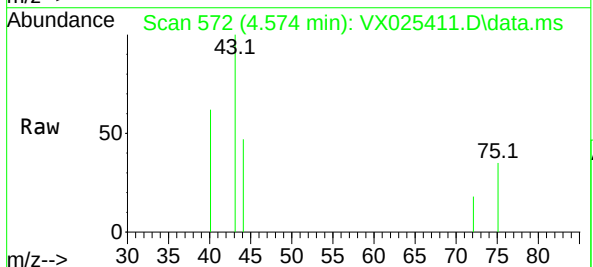


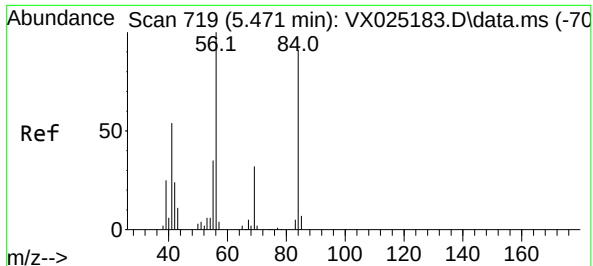

#31
Cyclohexane
Concen: 1.113 ug/l
RT: 5.556 min Scan# 719
Delta R.T. 0.085 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25




Instrument :
MSVOA_X
ClientSampleId :
16952


Tgt Ion: 56 Resp: 2180
Ion Ratio Lower Upper
56 100
69 172.1 24.2 36.2#
84 123.0 71.5 107.3#

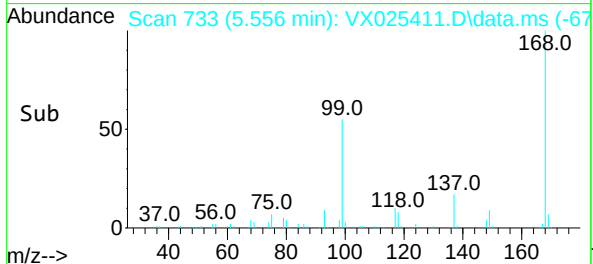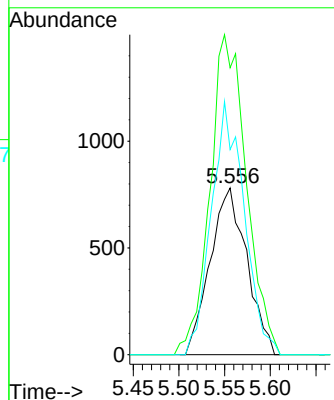

#33
1,2-Dichloroethane-d4
Concen: 53.486 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25

Tgt Ion: 65 Resp: 67793
Ion Ratio Lower Upper
65 100
67 51.7 0.0 101.0


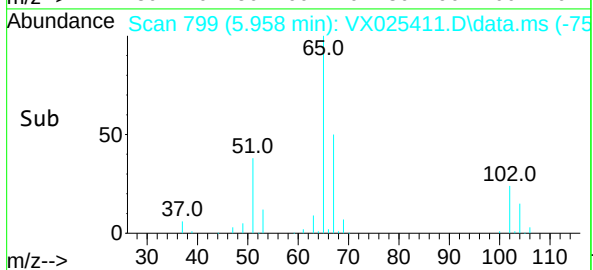
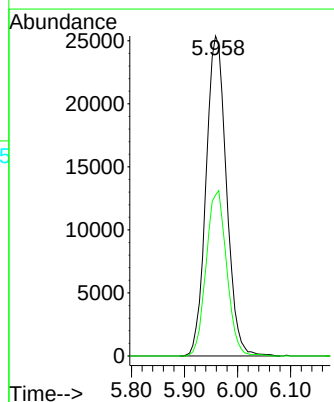
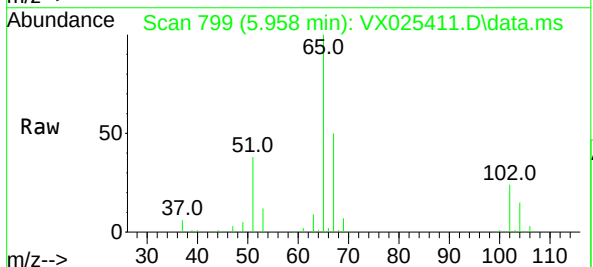


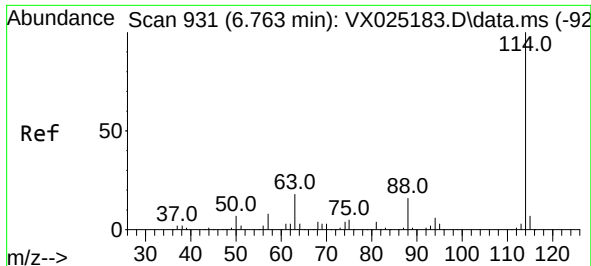

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25




Instrument :
MSVOA_X
ClientSampleId :
16952


Tgt Ion:114 Resp: 201309
Ion Ratio Lower Upper
114 100
63 18.1 0.0 41.0
88 14.7 0.0 34.8

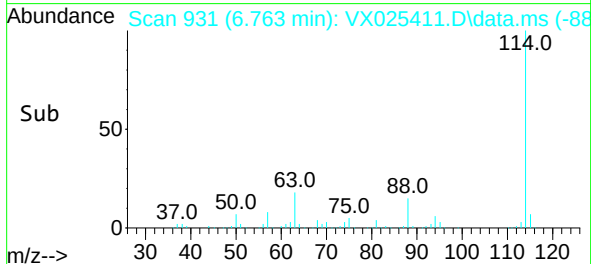

#35
Dibromofluoromethane
Concen: 49.759 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25

Tgt Ion:113 Resp: 61461
Ion Ratio Lower Upper
113 100
111 102.3 82.1 123.1
192 21.2 15.6 23.4

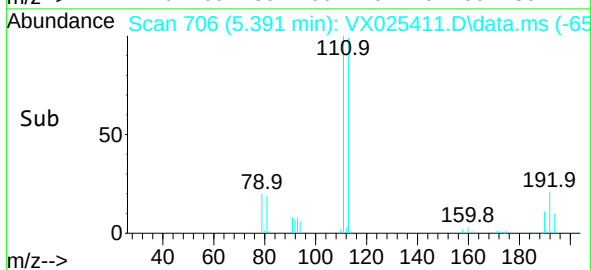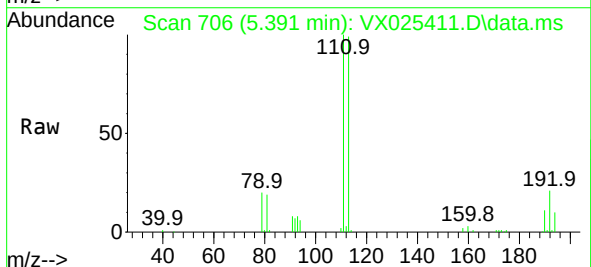

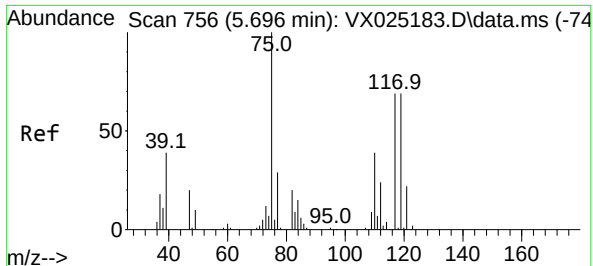

#36

1,1-Dichloropropene

Concen: 4.637 ug/l

RT: 5.556 min Scan# 71

Delta R.T. -0.140 min

Lab File: VX025411.D

Acq: 01 Dec 2021 14:25

Instrument :

MSVOA_X

ClientSampleId :

16952





Tgt Ion: 75 Resp: 8145

Ion Ratio Lower Upper

75 100

110 9.3 18.1 54.3#

77 0.0 24.4 36.6#

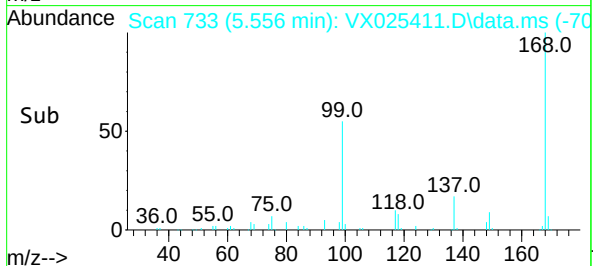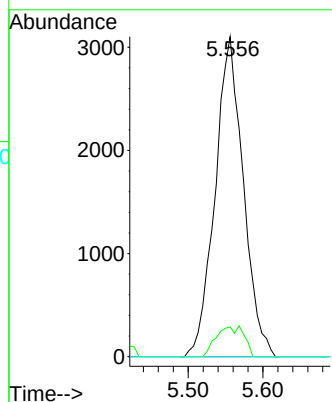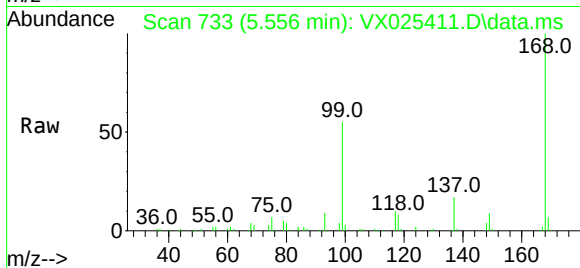

#37

Ethyl Acetate

Concen: 0.442 ug/l

RT: 4.574 min Scan# 572

Delta R.T. -0.141 min

Lab File: VX025411.D

Acq: 01 Dec 2021 14:25




Tgt Ion: 43 Resp: 883


Ion Ratio Lower Upper

43 100

61 0.0 11.4 17.0#


70 0.0 8.6 12.8#

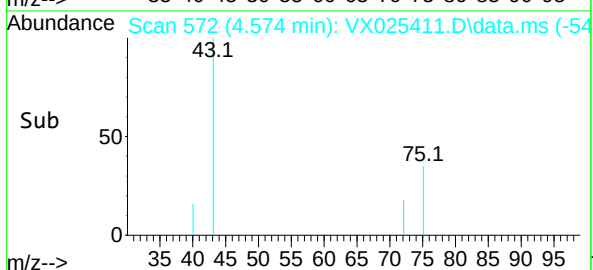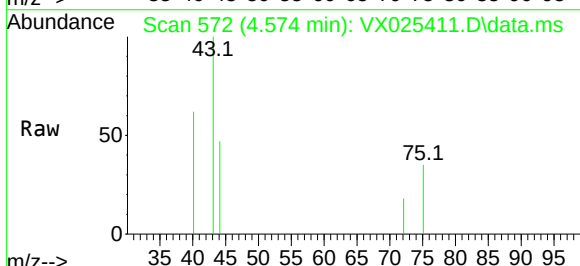



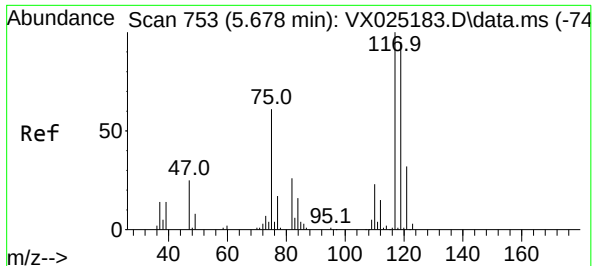


#38
Carbon Tetrachloride
Concen: 5.706 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25

Instrument :
MSVOA_X
ClientSampleId :
16952







Tgt Ion:117 Resp: 11039
Ion Ratio Lower Upper
117 100
119 6.9 75.6 113.4#
121 0.0 23.7 35.5#

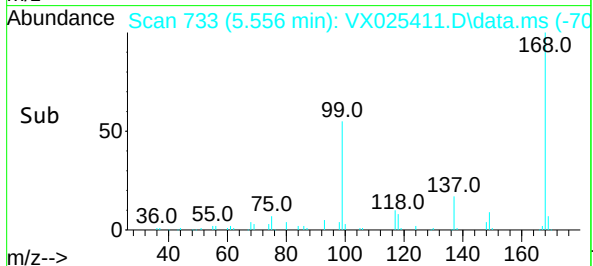

#48
Methyl methacrylate
Concen: 0.675 ug/l
RT: 7.684 min Scan# 1082
Delta R.T. -0.012 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25

Tgt Ion: 41 Resp: 1054
Ion Ratio Lower Upper
41 100
69 0.0 64.5 96.7#
39 28.9 46.9 70.3#


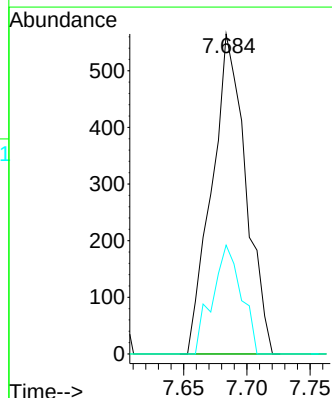

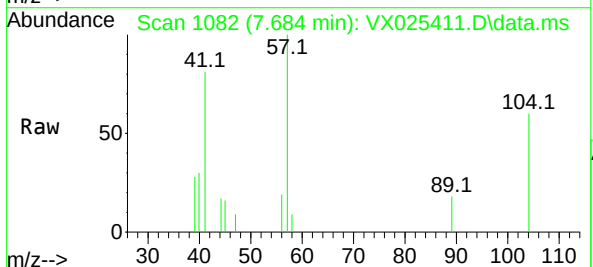


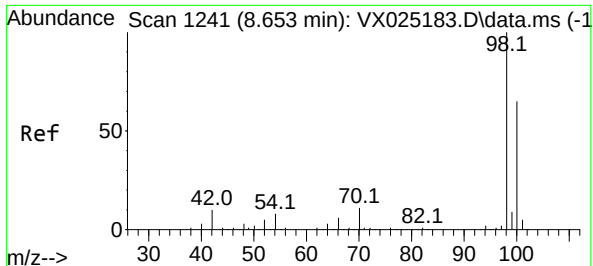

#50
Toluene-d8
Concen: 49.570 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25




Instrument :
MSVOA_X
ClientSampleId :
16952


Tgt Ion: 98 Resp: 230204
Ion Ratio Lower Upper
98 100
100 66.5 51.4 77.0

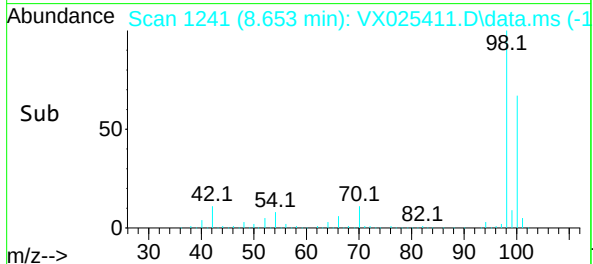

#51
4-Methyl-2-Pentanone
Concen: 0.934 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. 0.006 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25

Tgt Ion: 43 Resp: 1948
Ion Ratio Lower Upper
43 100
58 36.0 30.9 46.3


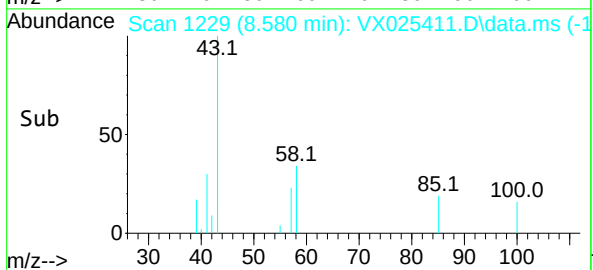

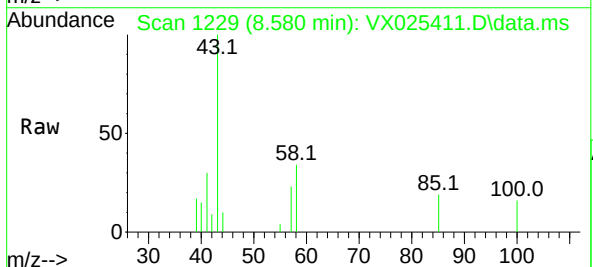




#52
Toluene
Concen: 0.949 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25




Instrument :
MSVOA_X
ClientSampleId :
16952


Tgt Ion: 92 Resp: 3295
Ion Ratio Lower Upper
92 100
91 167.1 138.6 208.0

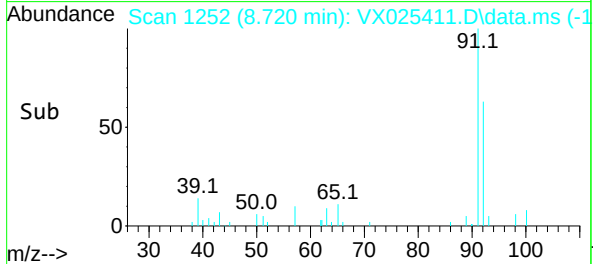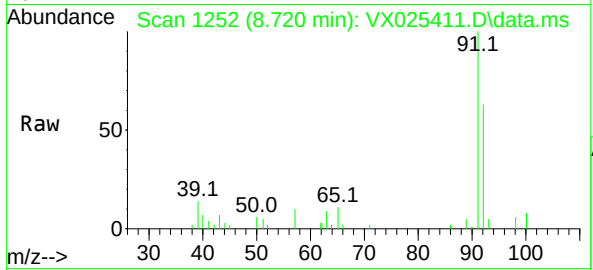

#55
1,1,2-Trichloroethane
Concen: 0.402 ug/l
RT: 9.019 min Scan# 1301
Delta R.T. -0.134 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25

Tgt Ion: 97 Resp: 555
Ion Ratio Lower Upper
97 100
83 0.0 69.2 103.8#
85 0.0 43.3 64.9#
99 0.0 49.1 73.7#

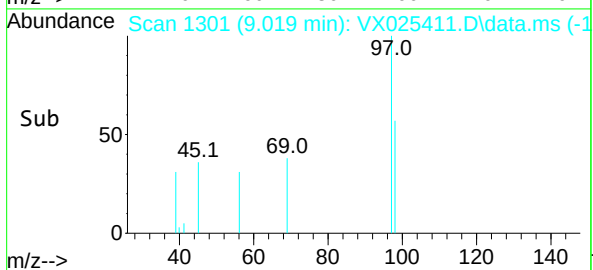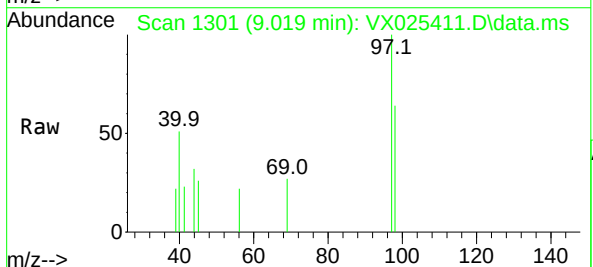

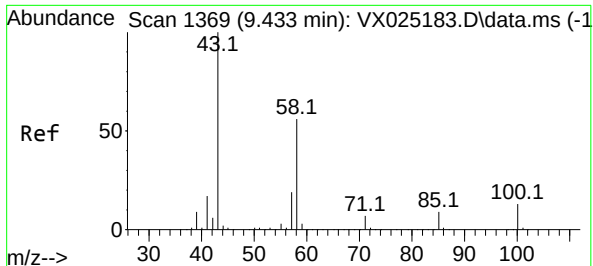

#59

2-Hexanone

Concen: 0.688 ug/l

RT: 9.439 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX025411.D

Acq: 01 Dec 2021 14:25

Instrument :

MSVOA_X

ClientSampleId :





16952

Tgt Ion: 43 Resp: 1131

Ion Ratio Lower Upper

43 100

58 39.9 26.6 79.7

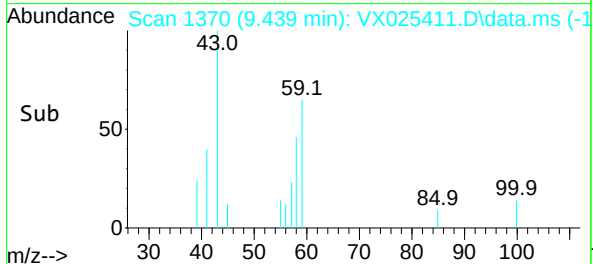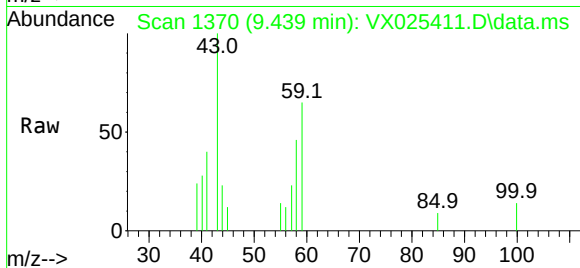

#62

4-Bromofluorobenzene

Concen: 47.018 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX025411.D

Acq: 01 Dec 2021 14:25




Tgt Ion: 95 Resp: 82606


Ion Ratio Lower Upper

95 100

174 83.8 0.0 158.0

176 82.2 0.0 153.6


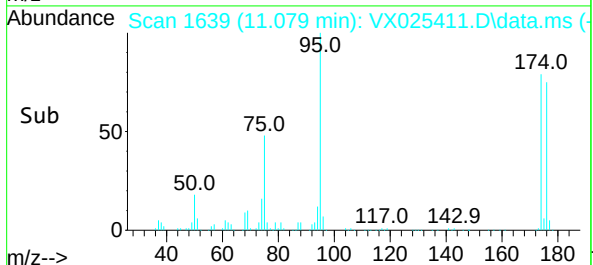
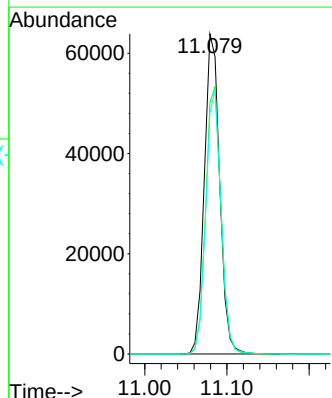
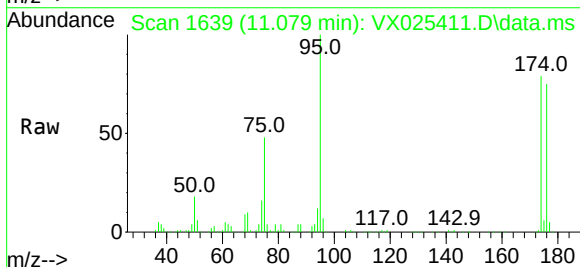




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25




Instrument :
MSVOA_X
ClientSampleId :
16952


Tgt Ion:117 Resp: 178945
Ion Ratio Lower Upper
117 100
82 53.1 44.6 67.0
119 32.5 24.8 37.2

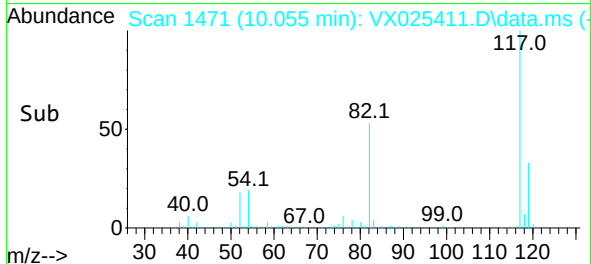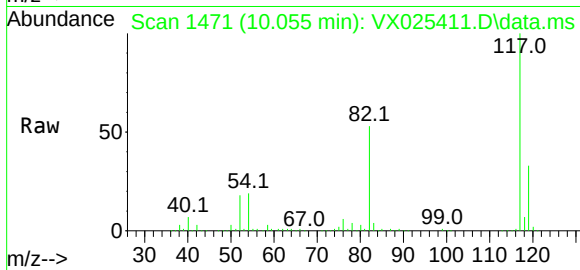

#68
m/p-Xylenes
Concen: 0.474 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25

Tgt Ion:106 Resp: 1221
Ion Ratio Lower Upper
106 100
91 200.1 163.4 245.0


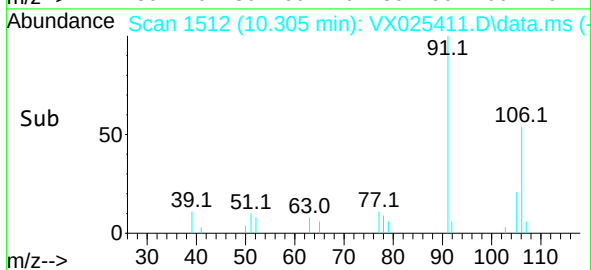
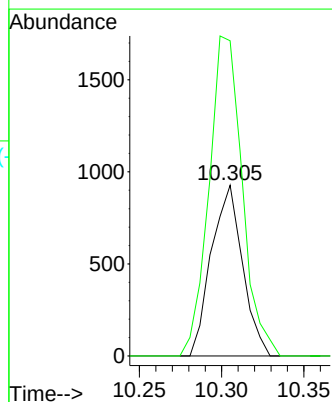
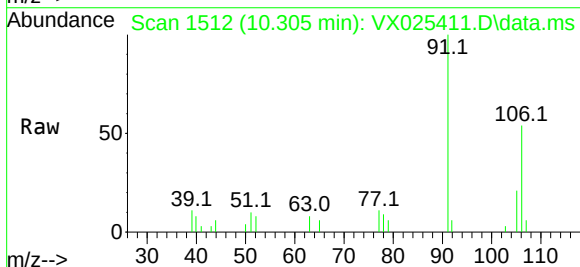


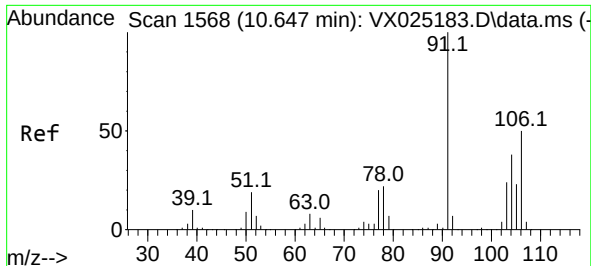

#69
o-Xylene
Concen: 0.281 ug/l
RT: 10.646 min Scan# 11
Delta R.T. -0.001 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25




Instrument :
MSVOA_X
ClientSampleId :
16952


Tgt Ion:106 Resp: 709
Ion Ratio Lower Upper
106 100
91 206.1 109.5 328.4

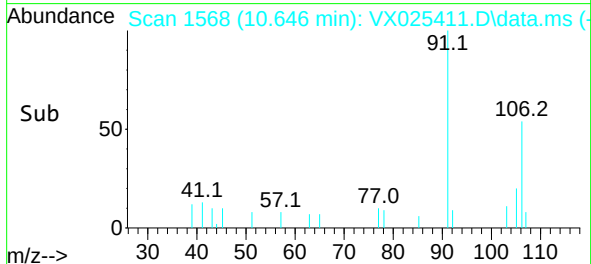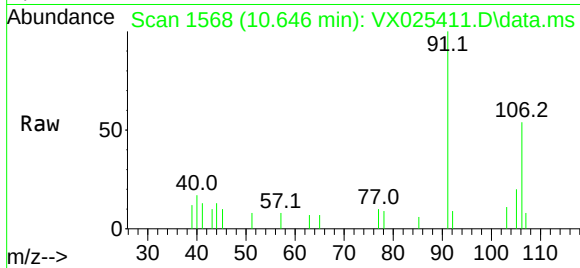

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25

Tgt Ion:152 Resp: 84533
Ion Ratio Lower Upper
152 100
115 57.3 43.3 129.8
150 157.2 0.0 351.2


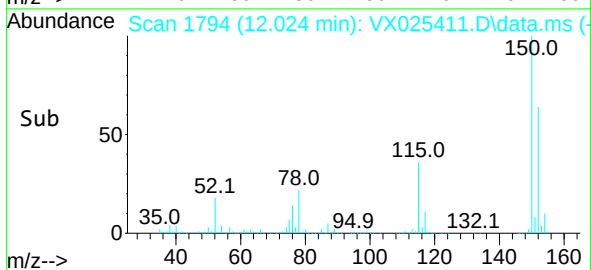

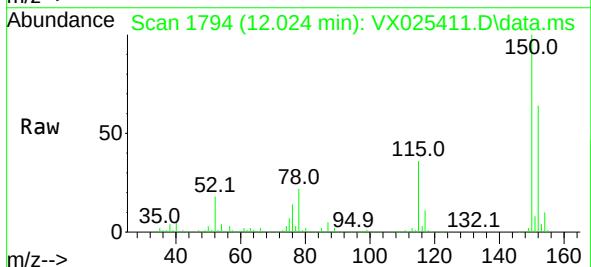




#74
N-amy1 acetate
Concen: 1.123 ug/l
RT: 10.890 min Scan# 1608
Delta R.T. 0.048 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25




Instrument :
MSVOA_X
ClientSampleId :
16952


Tgt Ion: 43	Resp: 2927
Ion Ratio	Lower Upper
43	100
70	0.0 33.7 50.5#
55	0.0 19.7 29.5#
61	0.0 19.0 28.4#

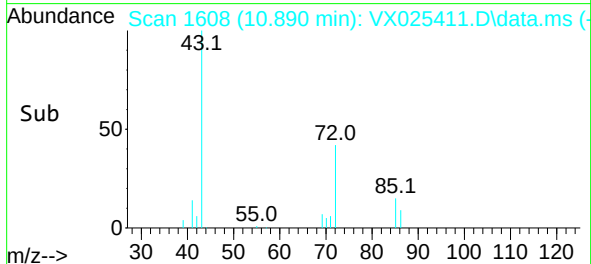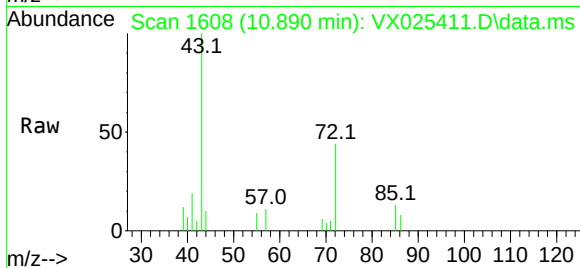

#76
1,2,3-Trichloropropane
Concen: 0.868 ug/l
RT: 11.366 min Scan# 1686
Delta R.T. 0.122 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25

Tgt Ion: 75	Resp: 1503
Ion Ratio	Lower Upper
75	100
77	33.7 20.0 59.9


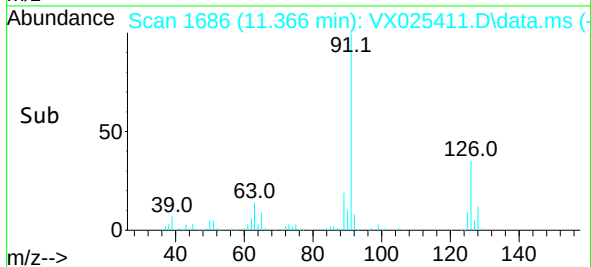

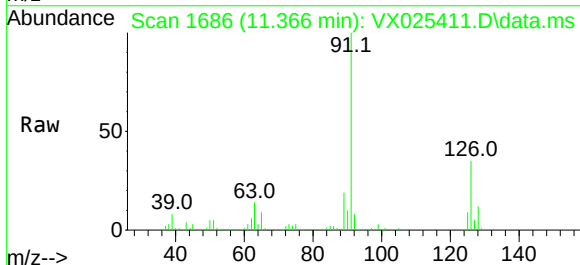


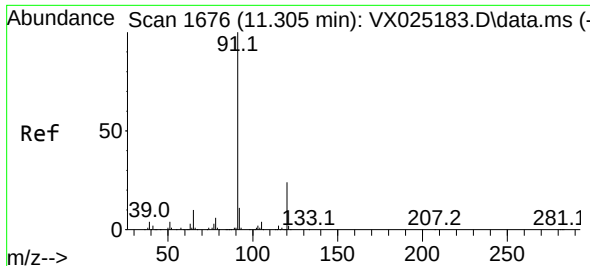

#78
n-propylbenzene
Concen: 7.695 ug/l
RT: 11.366 min Scan# 1686
Delta R.T. 0.061 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25




Instrument :
MSVOA_X
ClientSampleId :
16952


Tgt Ion: 91 Resp: 52040
Ion Ratio Lower Upper
91 100
120 1.7 11.7 35.0#

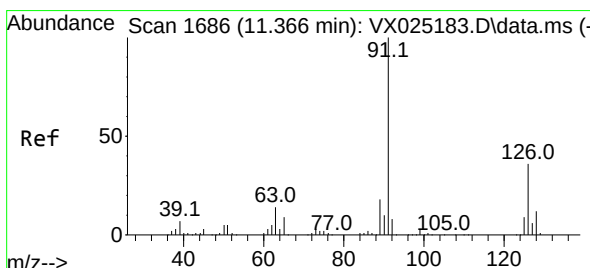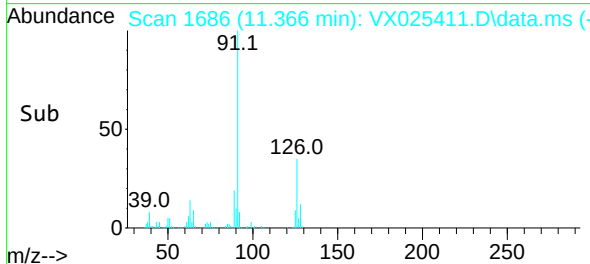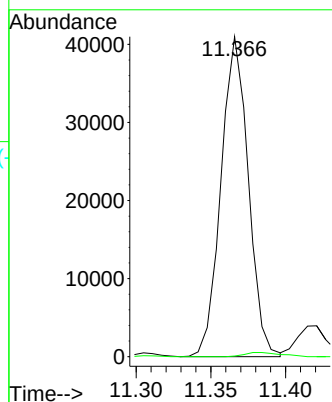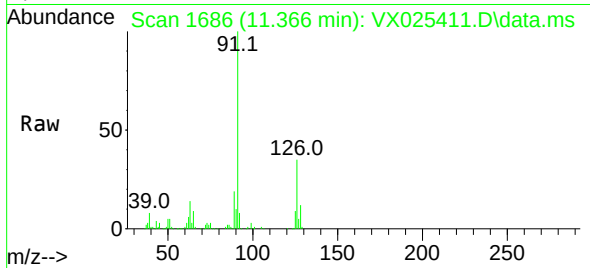

#79
2-Chlorotoluene
Concen: 12.640 ug/l
RT: 11.366 min Scan# 1686
Delta R.T. -0.000 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25

Tgt Ion: 91 Resp: 52040
Ion Ratio Lower Upper
91 100
126 35.5 17.0 50.9

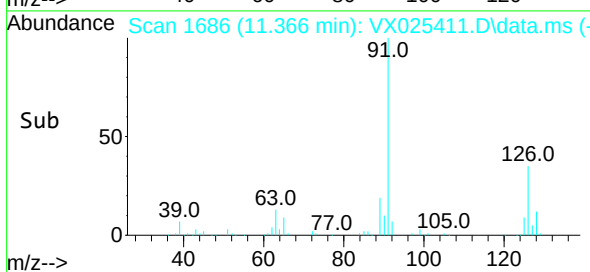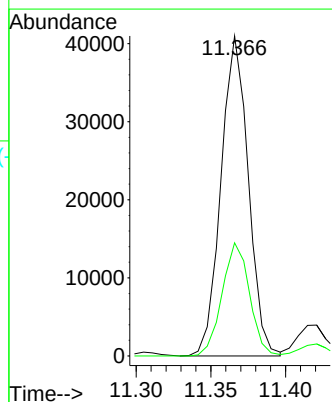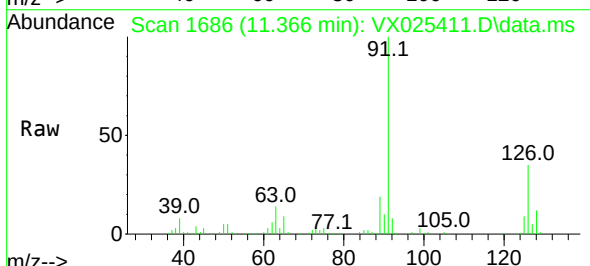



#80

1,3,5-Trimethylbenzene

Concen: 0.310 ug/l

RT: 11.451 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX025411.D

Acq: 01 Dec 2021 14:25

Instrument :

MSVOA_X

ClientSampleId :





16952

Tgt Ion:105 Resp: 1571

Ion Ratio Lower Upper

105 100

120 57.4 23.8 71.5

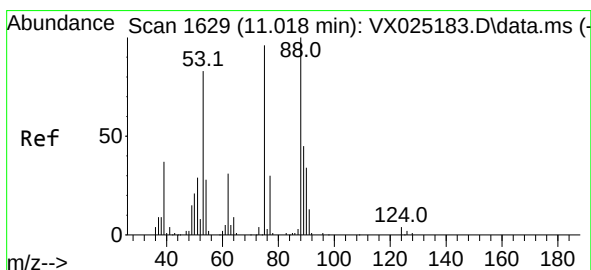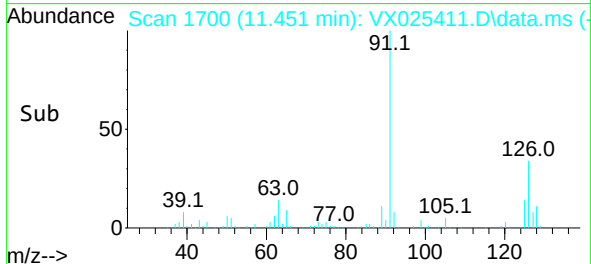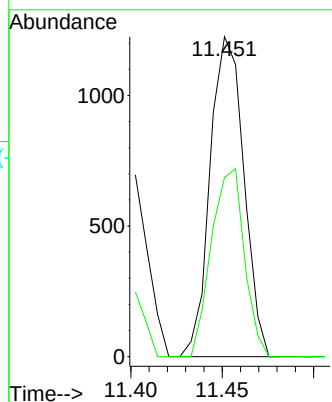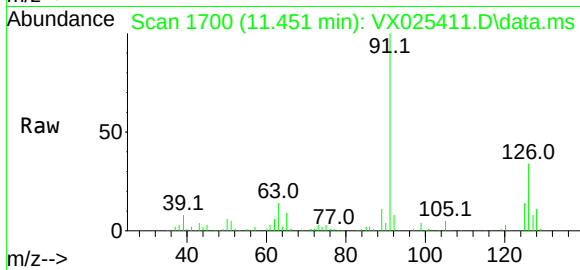

#81

trans-1,4-Dichloro-2-butene

Concen: 57.405 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX025411.D

Acq: 01 Dec 2021 14:25




Tgt Ion: 75 Resp: 39446


Ion Ratio Lower Upper

75 100

53 0.0 81.9 122.9#

89 0.0 38.2 57.2#

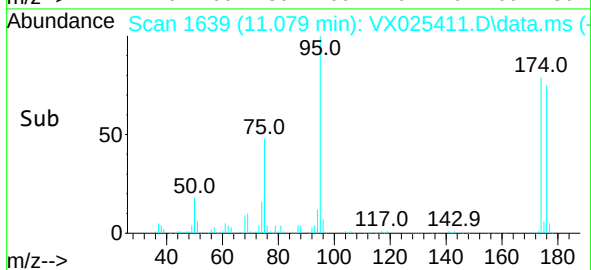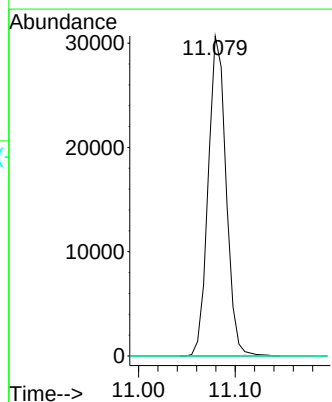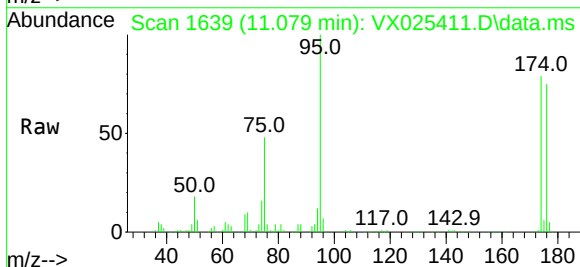



#82

4-Chlorotoluene

Concen: 7.402 ug/l

RT: 11.457 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX025411.D

Acq: 01 Dec 2021 14:25

Instrument :

MSVOA_X

ClientSampleId :





16952

Tgt Ion: 91 Resp: 34788

Ion Ratio Lower Upper

91 100

126 36.1 14.9 44.5

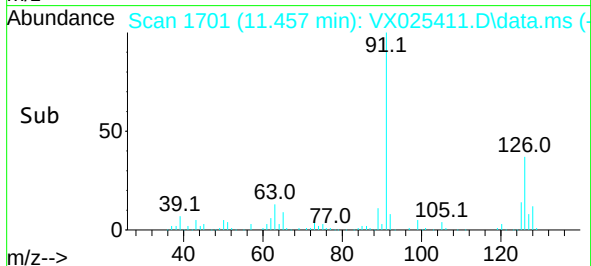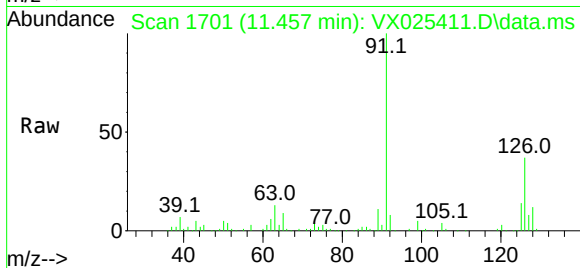

#84

1,2,4-Trimethylbenzene

Concen: 1.584 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.006 min

Lab File: VX025411.D




Acq: 01 Dec 2021 14:25


Tgt Ion: 105 Resp: 7926

Ion Ratio Lower Upper

105 100

120 43.7 22.1 66.3

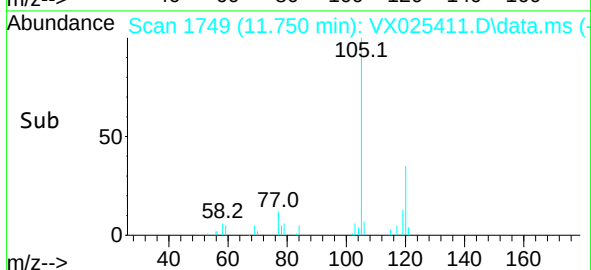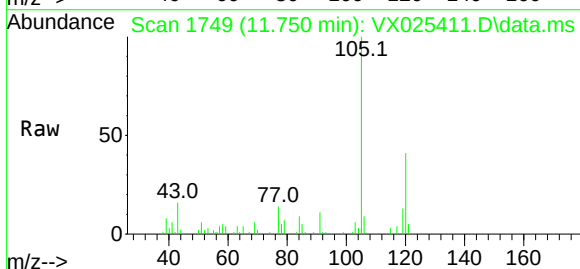

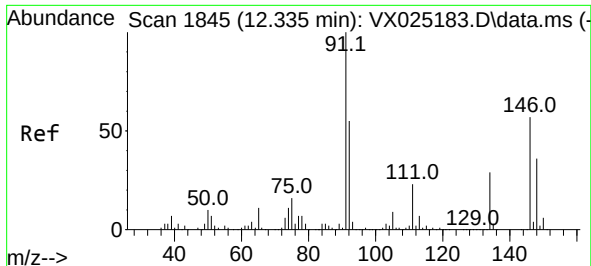

#89

n-Butylbenzene

Concen: 0.233 ug/l

RT: 12.323 min Scan# 11

Delta R.T. -0.012 min

Lab File: VX025411.D

Acq: 01 Dec 2021 14:25

Instrument :

MSVOA_X

ClientSampleId :

16952





Tgt Ion: 91 Resp: 1058

Ion Ratio Lower Upper

91 100

92 29.9 26.3 78.8

134 115.7 13.0 38.9#

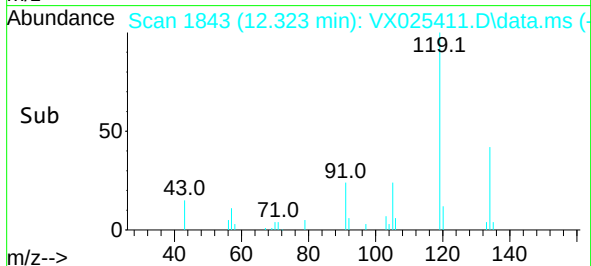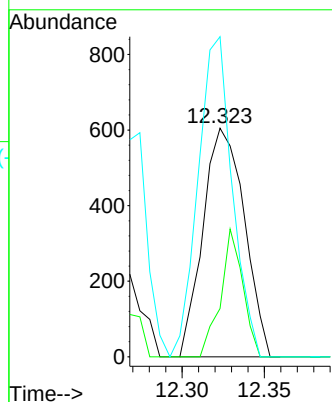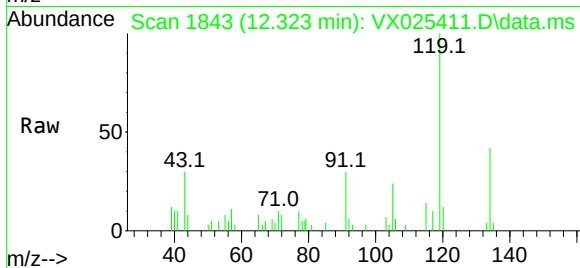

#90

Hexachloroethane

Concen: 0.307 ug/l

RT: 12.530 min Scan# 1877

Delta R.T. -0.013 min

Lab File: VX025411.D




Acq: 01 Dec 2021 14:25


Tgt Ion: 117 Resp: 304

Ion Ratio Lower Upper

117 100

201 0.0 38.9 116.6#


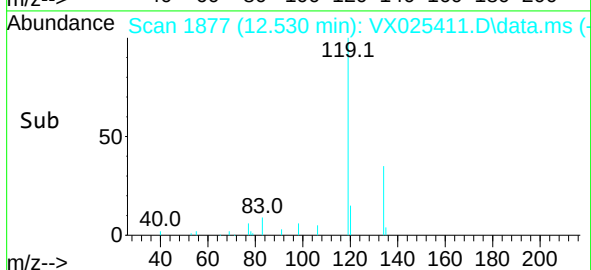

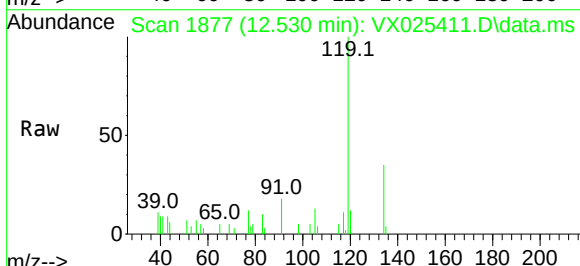


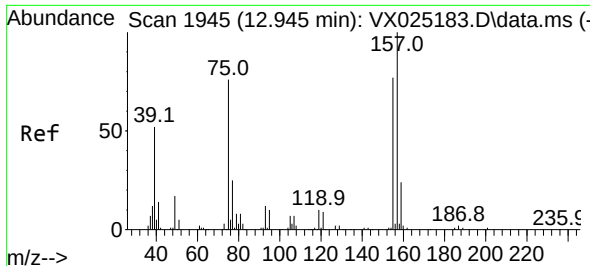

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.290 ug/l
RT: 13.061 min Scan# 1945
Delta R.T. 0.116 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25

Instrument :
MSVOA_X
ClientSampleId :
16952

Tgt Ion: 75 Resp: 118
Ion Ratio Lower Upper
75 100
155 0.0 43.1 129.3#
157 0.0 53.6 160.9#

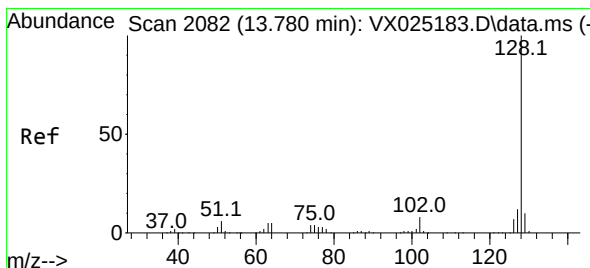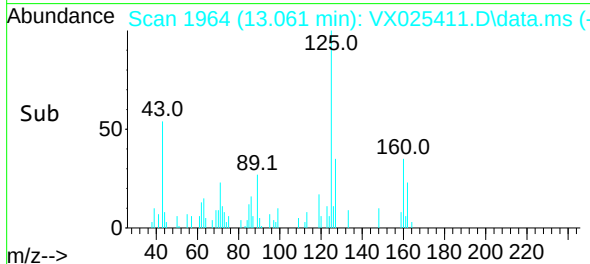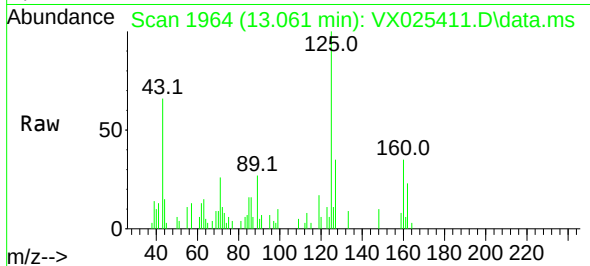

#95
Naphthalene
Concen: 1.775 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX025411.D
Acq: 01 Dec 2021 14:25

Tgt Ion:128 Resp: 12186
Ion Ratio Lower Upper
128 100
127 13.4 10.3 15.5
129 11.2 8.8 13.2

