

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
 Data File : VX033157.D
 Acq On : 01 Dec 2022 12:50
 Operator : JC/MD
 Sample : N5815-27
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB-2022-11-29

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Title : SW846 8260

Signal : TIC: VX033157.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.325	32	39	42	rBV2	3336	8751	1.40%	0.227%
2	1.374	44	47	51	rVB	6946	7591	1.21%	0.197%
3	1.752	104	109	118	rVB	16425	22407	3.58%	0.581%
4	1.959	136	143	153	rBV	7642	11342	1.81%	0.294%
5	2.941	297	304	314	rVB	12203	27573	4.41%	0.715%
6	4.306	518	528	539	rVB4	4131	11986	1.92%	0.311%
7	4.568	561	571	573	rBV2	3263	6646	1.06%	0.172%
8	5.385	693	705	718	rBV	70429	210131	33.61%	5.453%
9	5.550	722	732	753	rVB	157785	452671	72.40%	11.746%
10	5.958	789	799	812	rBV2	74260	200286	32.03%	5.197%
11	6.763	920	931	949	rBV	236060	558950	89.39%	14.504%
12	8.647	1233	1240	1254	rBV	359858	551343	88.18%	14.307%
13	10.055	1465	1471	1488	rBV	462813	625274	100.00%	16.225%
14	10.195	1490	1494	1502	rVB	16995	22740	3.64%	0.590%
15	10.305	1507	1512	1520	rVB	16044	22447	3.59%	0.582%
16	11.079	1634	1639	1653	rBV	302791	379302	60.66%	9.843%
17	11.305	1671	1676	1683	rBV2	10299	14569	2.33%	0.378%
18	11.402	1685	1692	1697	rBV	9928	13950	2.23%	0.362%
19	11.750	1745	1749	1756	rVB	19867	25474	4.07%	0.661%
20	12.024	1788	1794	1801	rBV	454681	583770	93.36%	15.148%
21	12.085	1801	1804	1815	rVB	5272	7047	1.13%	0.183%
22	12.244	1826	1830	1838	rVB3	5740	8537	1.37%	0.222%
23	12.317	1838	1842	1852	rBV3	5876	10575	1.69%	0.274%
24	12.616	1885	1891	1894	rBV2	7581	8897	1.42%	0.231%
25	13.292	1998	2002	2011	rVB5	4436	6504	1.04%	0.169%
26	13.774	2076	2081	2086	rBV	9078	12982	2.08%	0.337%
27	13.823	2086	2089	2100	rVB2	5107	8333	1.33%	0.216%
28	14.640	2217	2223	2228	rBV	16709	22745	3.64%	0.590%
29	14.780	2241	2246	2251	rVB	8700	10852	1.74%	0.282%




Sum of corrected areas: 3853675

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
Data File : VX033157.D
Acq On : 01 Dec 2022 12:50
Operator : JC/MD
Sample : N5815-27
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2022-11-29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

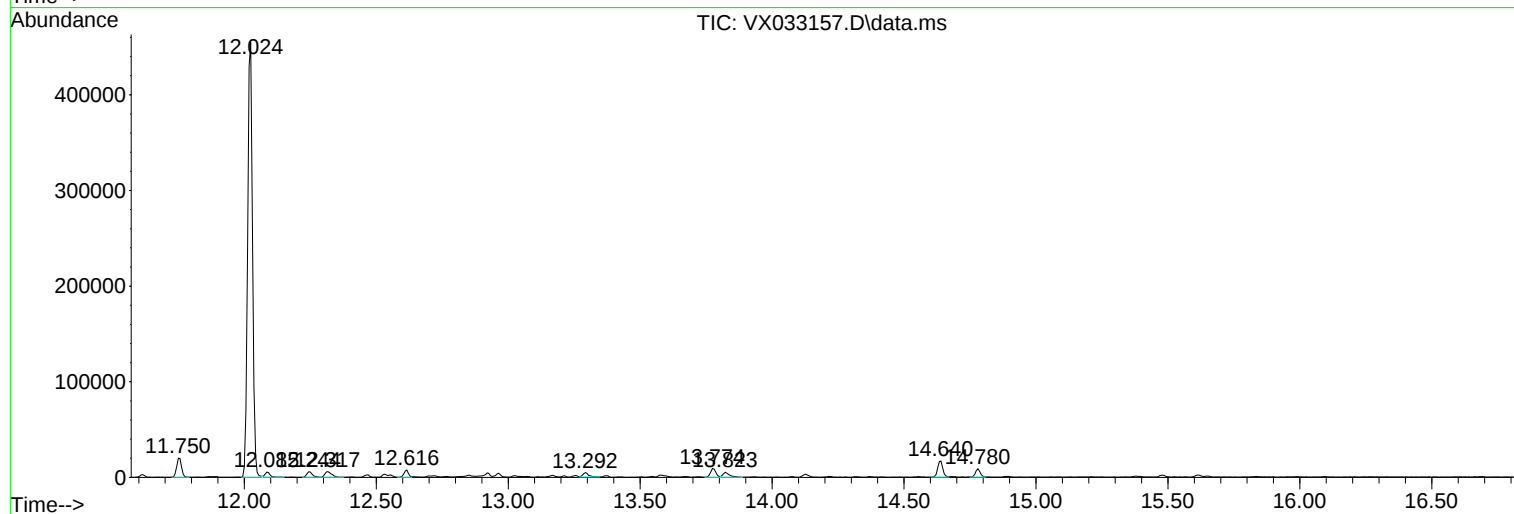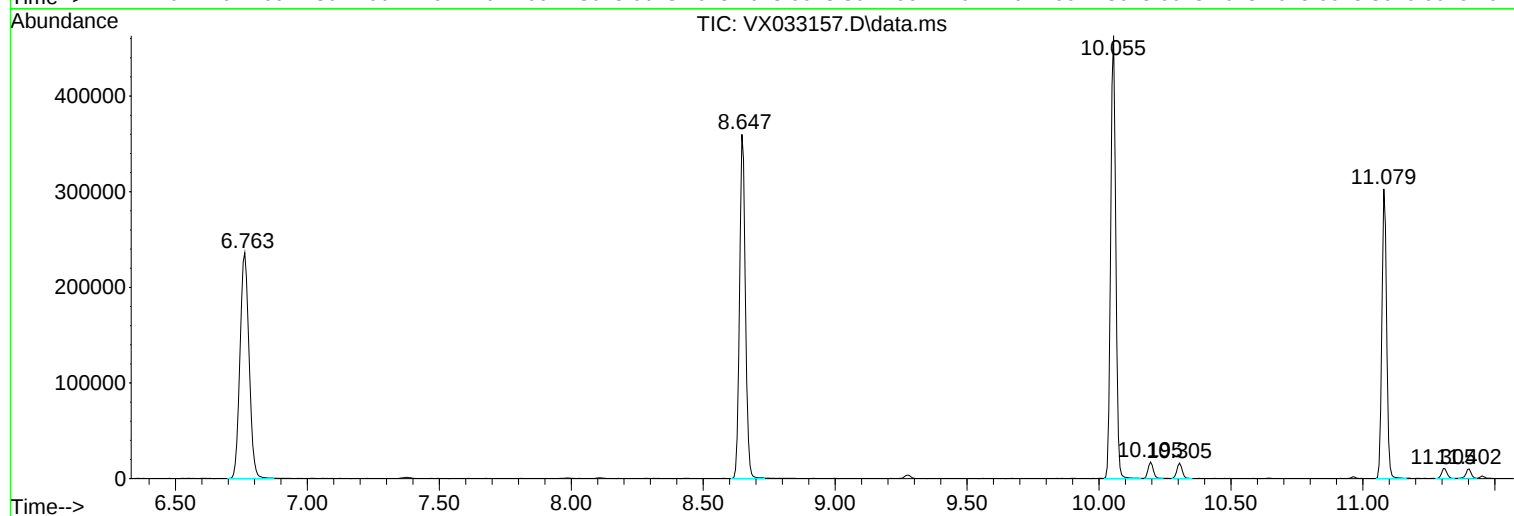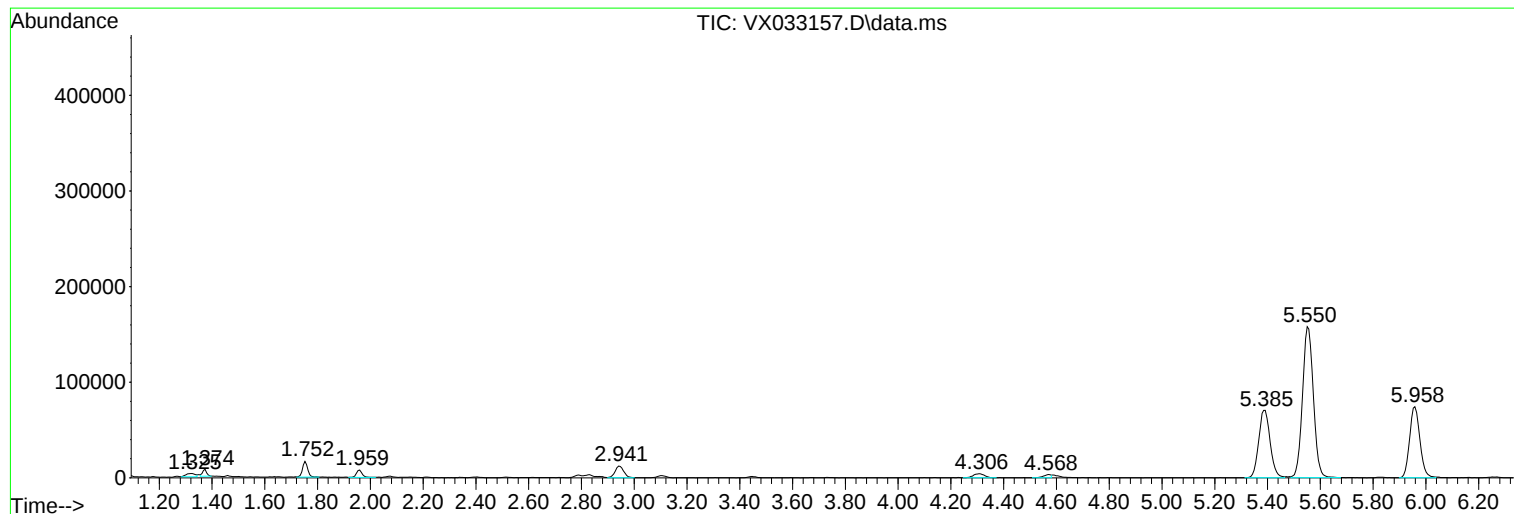

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
Data File : VX033157.D
Acq On : 01 Dec 2022 12:50
Operator : JC/MD
Sample : N5815-27
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2022-11-29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
Data File : VX033157.D
Acq On : 01 Dec 2022 12:50
Operator : JC/MD
Sample : N5815-27
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2022-11-29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc