

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
 Data File : VX033158.D
 Acq On : 01 Dec 2022 13:13
 Operator : JC/MD
 Sample : N5815-28
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-2022-11-29

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M

Title : SW846 8260

Signal : TIC: VX033158.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.295	30	34	44	rBV	6353	17843	3.10%	0.539%
2	1.752	105	109	114	rVB2	6043	8226	1.43%	0.249%
3	5.385	695	705	718	rBV	65567	192701	33.44%	5.821%
4	5.556	721	733	746	rVV	142780	409367	71.04%	12.367%
5	5.958	786	799	812	rBV2	70136	188328	32.68%	5.689%
6	6.763	921	931	947	rBV	210089	507356	88.04%	15.327%
7	8.647	1234	1240	1253	rBV	325778	502917	87.27%	15.193%
8	10.055	1465	1471	1485	rBV	422870	576289	100.00%	17.410%
9	10.195	1489	1494	1499	rVV	5826	7069	1.23%	0.214%
10	10.305	1506	1512	1518	rBV	5547	8202	1.42%	0.248%
11	11.079	1634	1639	1652	rBV	272002	351033	60.91%	10.605%
12	11.756	1745	1750	1755	rBV	5684	7153	1.24%	0.216%
13	12.024	1788	1794	1802	rBV	420595	533704	92.61%	16.123%




Sum of corrected areas: 3310188

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
Data File : VX033158.D
Acq On : 01 Dec 2022 13:13
Operator : JC/MD
Sample : N5815-28
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-2022-11-29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

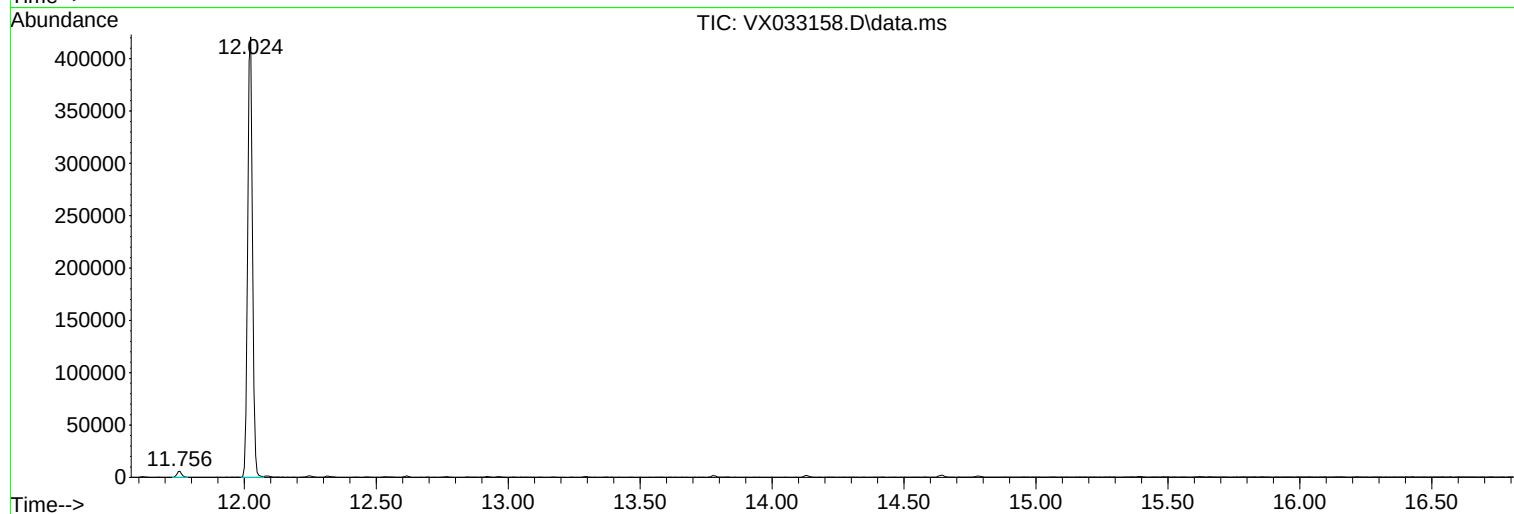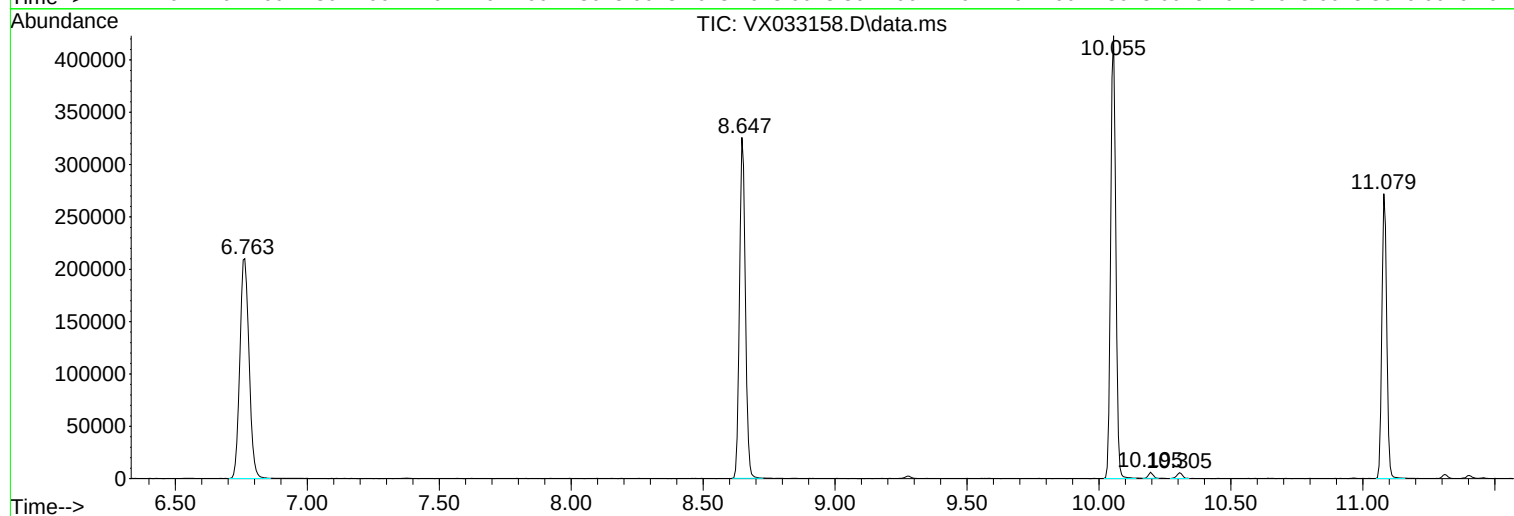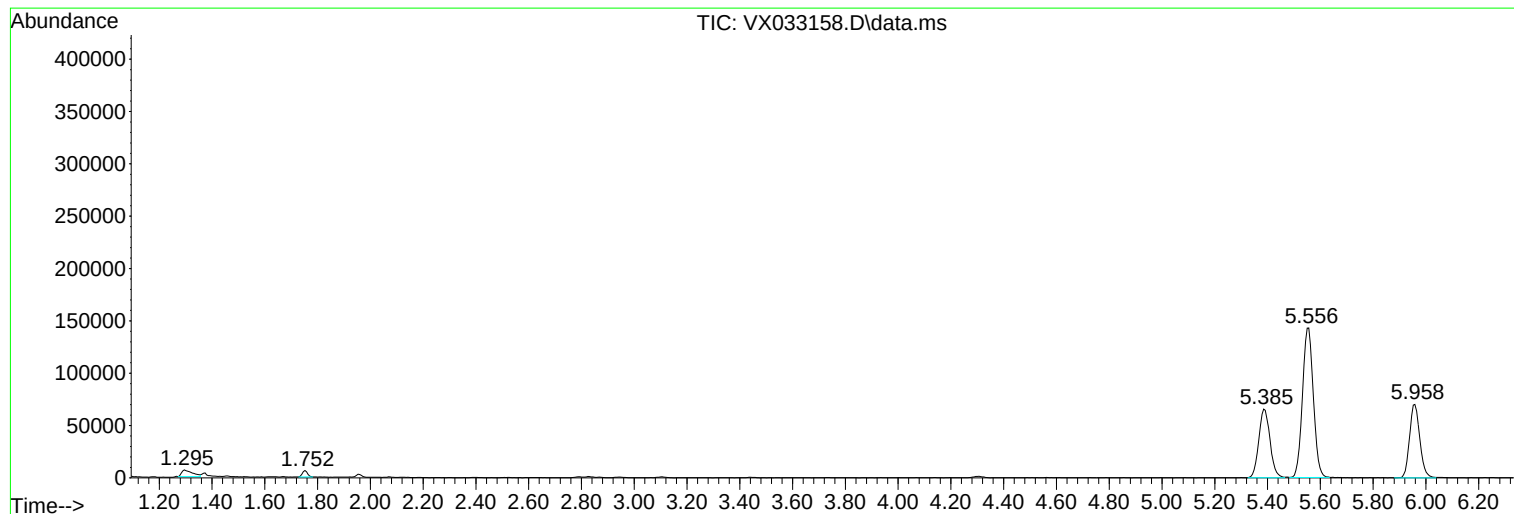

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
Data File : VX033158.D
Acq On : 01 Dec 2022 13:13
Operator : JC/MD
Sample : N5815-28
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-2022-11-29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
Data File : VX033158.D
Acq On : 01 Dec 2022 13:13
Operator : JC/MD
Sample : N5815-28
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-2022-11-29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc