

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
 Data File : VX033159.D
 Acq On : 01 Dec 2022 13:36
 Operator : JC/MD
 Sample : N5828-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-02-11302022

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M

Title : SW846 8260

Signal : TIC: VX033159.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.288	27	33	44	rBV2	9085	28625	5.10%	0.868%
2	1.752	104	109	116	rVB3	4465	6526	1.16%	0.198%
3	2.617	237	251	253	rBV	3163	10263	1.83%	0.311%
4	2.941	295	304	319	rBV	16593	39428	7.02%	1.196%
5	4.580	560	573	581	rBV	4471	15352	2.73%	0.466%
6	5.385	692	705	721	rBV2	65604	192932	34.35%	5.853%
7	5.556	721	733	750	rVB	140648	396733	70.64%	12.036%
8	5.958	787	799	811	rBV	69635	185020	32.94%	5.613%
9	6.763	921	931	945	rBV	204347	490139	87.27%	14.870%
10	8.647	1234	1240	1252	rBV	313701	493595	87.89%	14.975%
11	10.055	1465	1471	1478	rBV	417500	561625	100.00%	17.038%
12	11.079	1634	1639	1655	rVB	270004	349186	62.17%	10.593%
13	12.024	1788	1794	1802	rBV	421277	526805	93.80%	15.982%




Sum of corrected areas: 3296229

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
Data File : VX033159.D
Acq On : 01 Dec 2022 13:36
Operator : JC/MD
Sample : N5828-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-02-11302022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

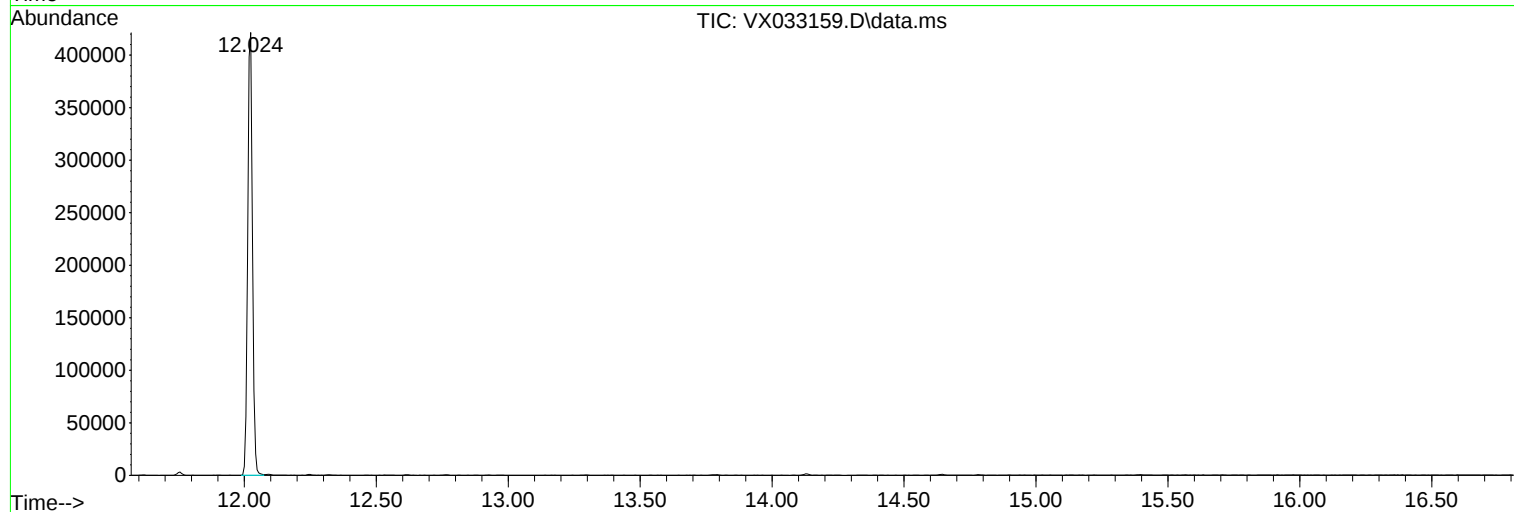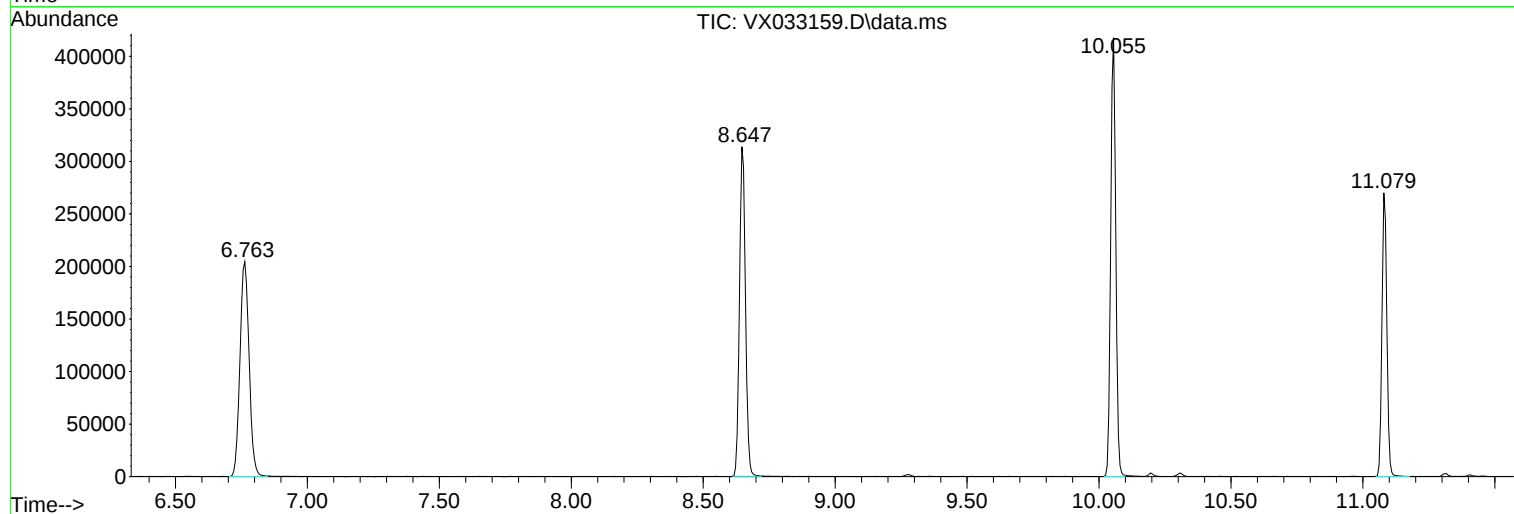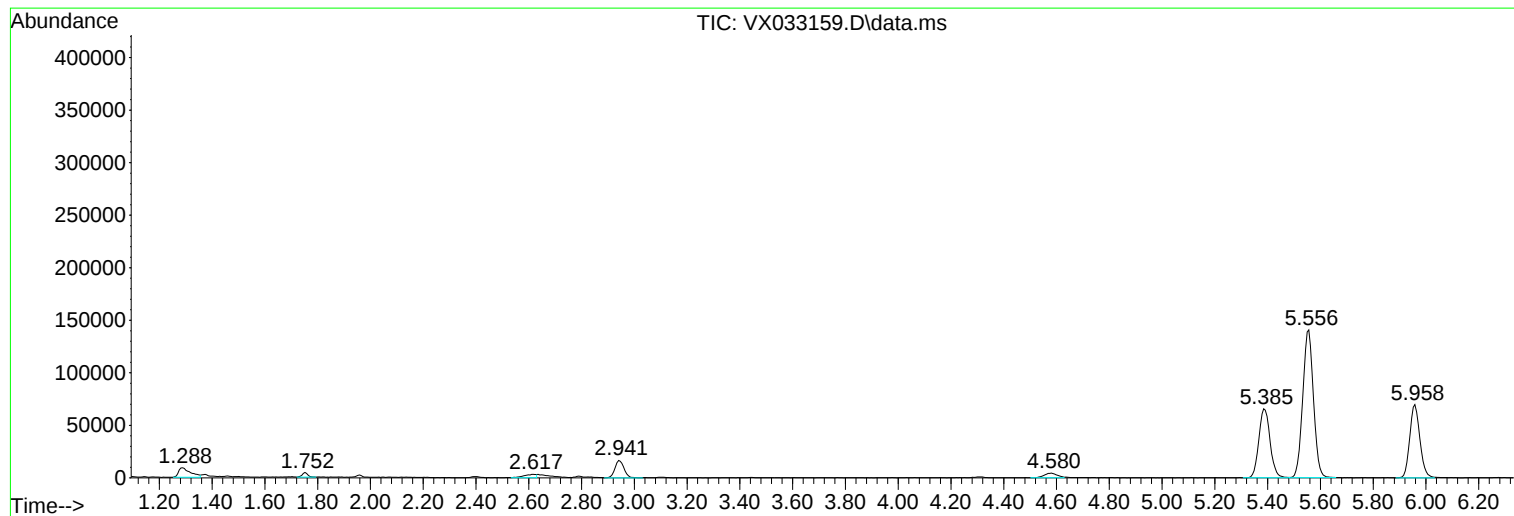

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
Data File : VX033159.D
Acq On : 01 Dec 2022 13:36
Operator : JC/MD
Sample : N5828-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-02-11302022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
Data File : VX033159.D
Acq On : 01 Dec 2022 13:36
Operator : JC/MD
Sample : N5828-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-02-11302022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc