

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
 Data File : VX033162.D
 Acq On : 01 Dec 2022 14:46
 Operator : JC/MD
 Sample : N5828-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RW9-PT-IN-02-11302022

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M

Title : SW846 8260

Signal : TIC: VX033162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	30	36	44	rBV	4747	14030	2.62%	0.457%
2	2.941	297	304	313	rVB	6238	14483	2.70%	0.472%
3	4.587	562	574	585	rBV2	1641	6030	1.12%	0.196%
4	5.385	694	705	720	rBV	62949	182564	34.05%	5.948%
5	5.556	722	733	746	rVB	132263	375228	69.98%	12.226%
6	5.958	789	799	816	rBV	66216	177334	33.07%	5.778%
7	6.763	920	931	945	rBV	196332	469931	87.65%	15.312%
8	8.647	1233	1240	1251	rBV	298150	471039	87.85%	15.348%
9	10.055	1465	1471	1486	rBV	399592	536164	100.00%	17.470%
10	11.079	1634	1639	1651	rBV	257259	328797	61.32%	10.713%
11	12.024	1788	1794	1802	rBV	391281	493490	92.04%	16.079%




Sum of corrected areas: 3069090

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
Data File : VX033162.D
Acq On : 01 Dec 2022 14:46
Operator : JC/MD
Sample : N5828-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RW9-PT-IN-02-11302022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

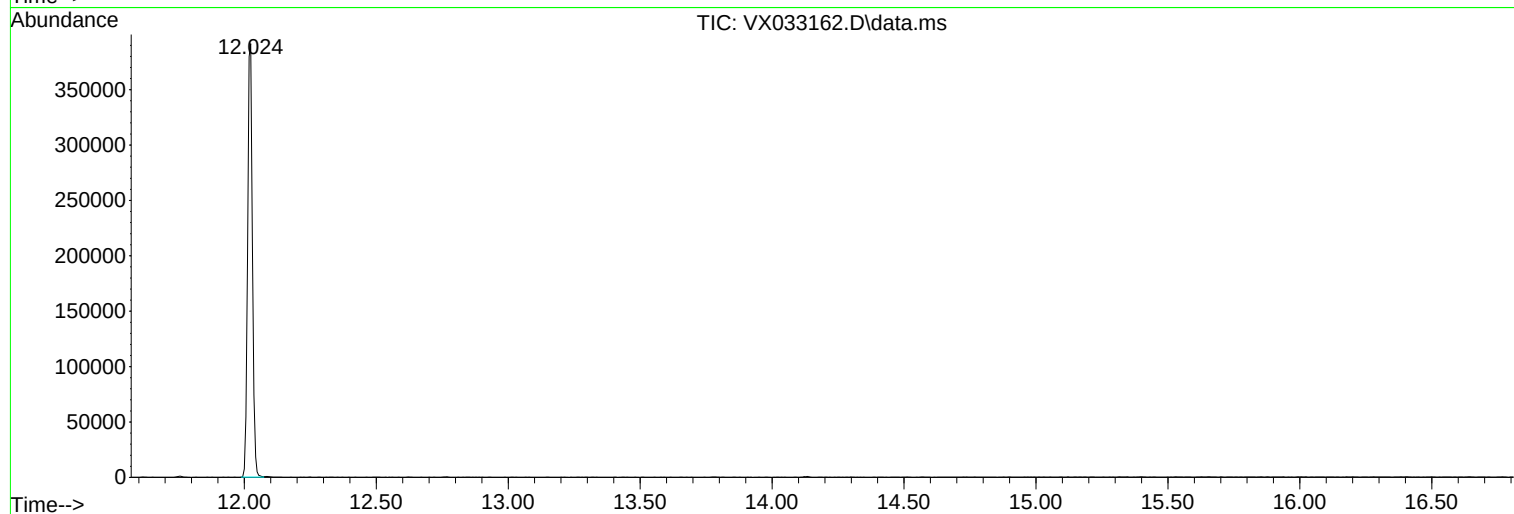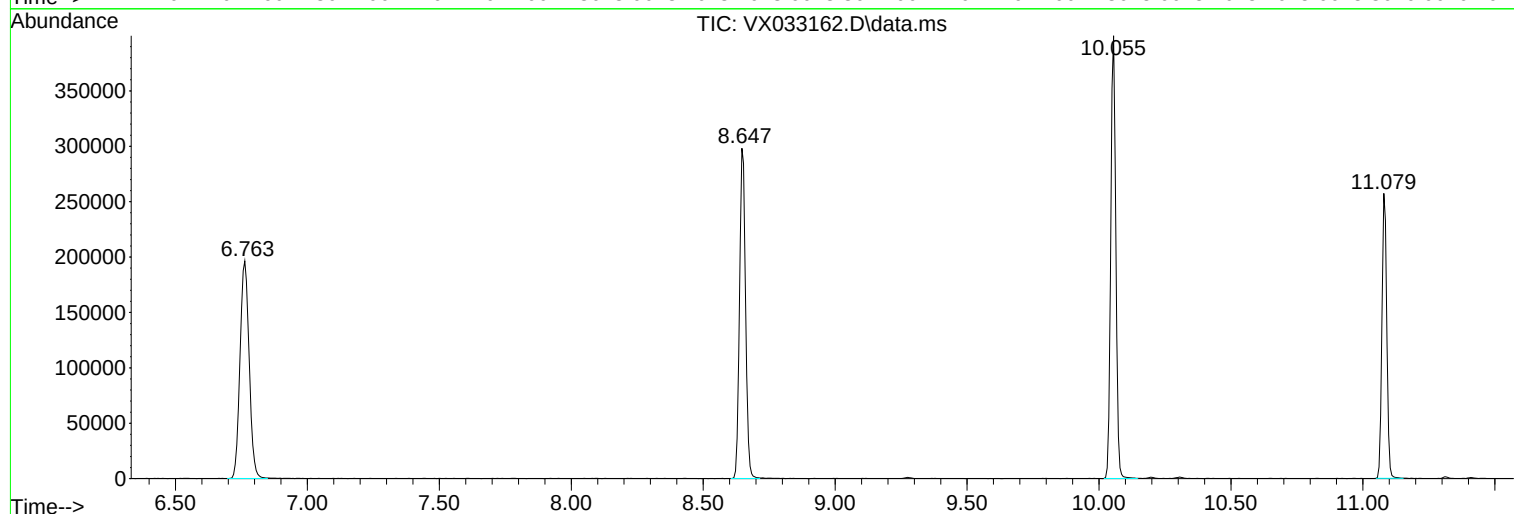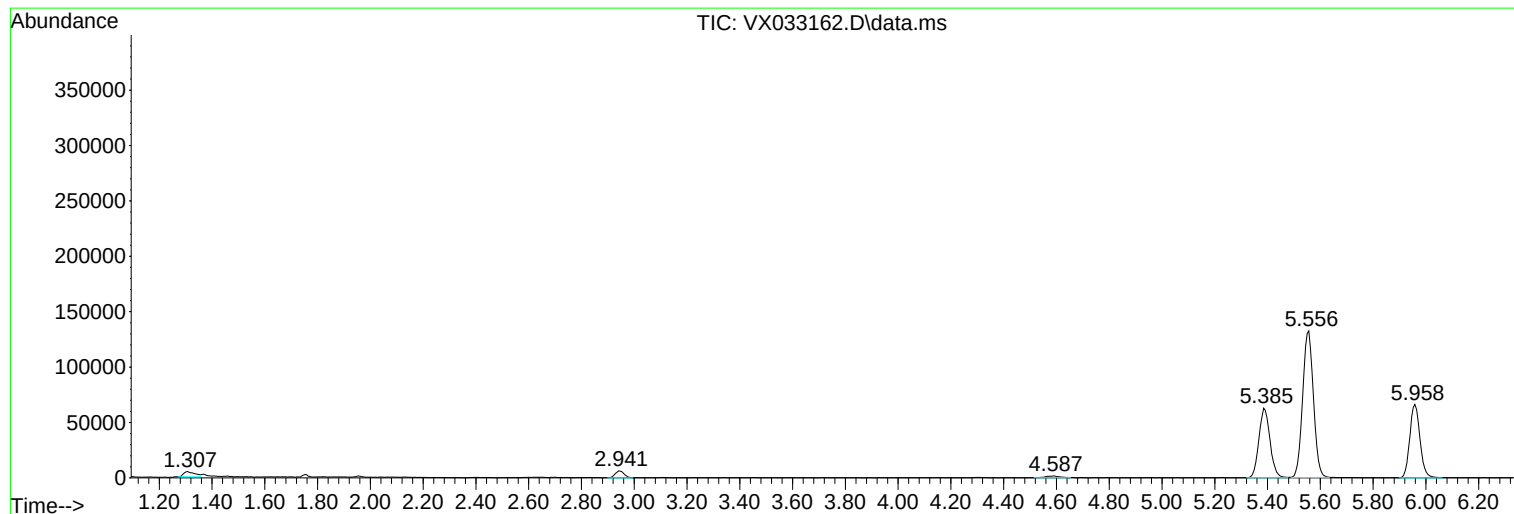

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
Data File : VX033162.D
Acq On : 01 Dec 2022 14:46
Operator : JC/MD
Sample : N5828-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RW9-PT-IN-02-11302022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
Data File : VX033162.D
Acq On : 01 Dec 2022 14:46
Operator : JC/MD
Sample : N5828-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RW9-PT-IN-02-11302022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------