

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
 Data File : VX033168.D
 Acq On : 01 Dec 2022 17:04
 Operator : JC/MD
 Sample : N5821-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 22-MW-6S

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M

Title : SW846 8260

Signal : TIC: VX033168.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	58	rVB	919537	1030354	56.10%	17.406%
2	4.489	546	558	581	rBV	681346	1836585	100.00%	31.026%
3	5.385	693	705	722	rBV2	61568	177764	9.68%	3.003%
4	5.550	722	732	746	rVV	131709	371099	20.21%	6.269%
5	5.958	787	799	816	rBV	66443	174284	9.49%	2.944%
6	6.763	921	931	944	rBV	194412	465676	25.36%	7.867%
7	7.129	981	991	1001	rBV2	27758	62101	3.38%	1.049%
8	8.647	1234	1240	1248	rBV	286687	452792	24.65%	7.649%
9	10.055	1465	1471	1484	rBV	402791	535487	29.16%	9.046%
10	11.079	1634	1639	1651	rBV	254770	320116	17.43%	5.408%
11	12.024	1788	1794	1801	rBV	391002	493330	26.86%	8.334%




Sum of corrected areas: 5919588

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
Data File : VX033168.D
Acq On : 01 Dec 2022 17:04
Operator : JC/MD
Sample : N5821-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
22-MW-6S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

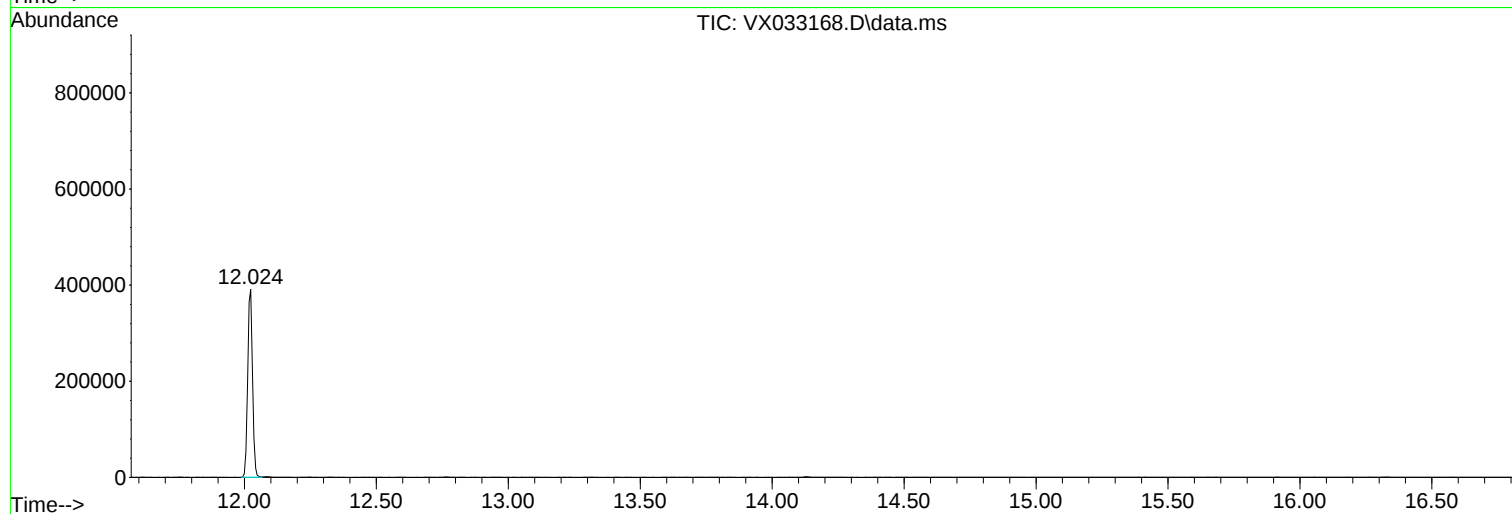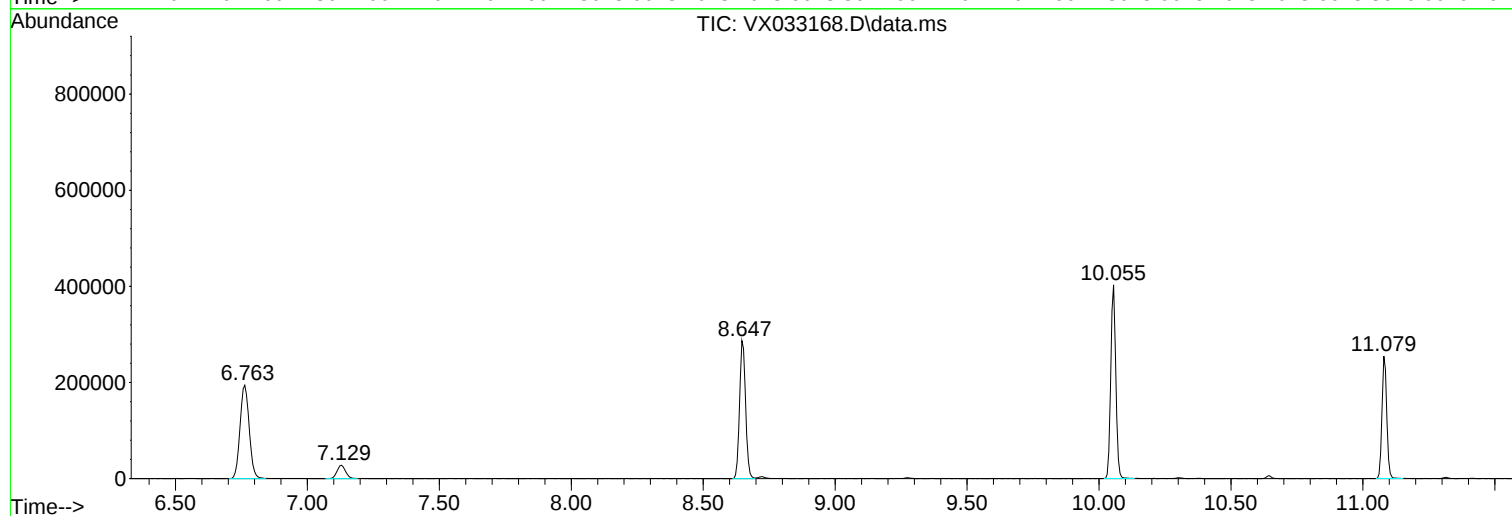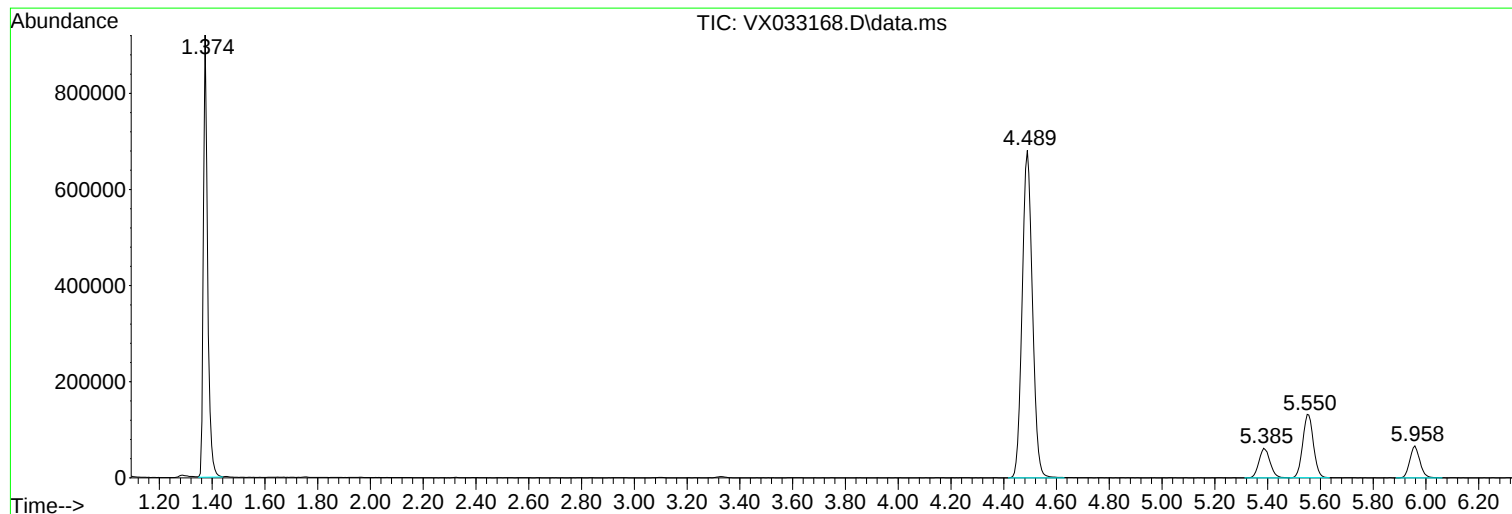

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
Data File : VX033168.D
Acq On : 01 Dec 2022 17:04
Operator : JC/MD
Sample : N5821-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
22-MW-6S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120122\
Data File : VX033168.D
Acq On : 01 Dec 2022 17:04
Operator : JC/MD
Sample : N5821-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
22-MW-6S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------