

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025418.D
Acq On : 02 Dec 2021 10:57
Operator : JC/MD
Sample : VX1202WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1202WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M

Title : SW846 8260

Signal : TIC: VX025418.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	31	rBV	13570	20547	3.50%	0.661%
2	1.563	68	78	81	rBV6	3436	7549	1.29%	0.243%
3	2.947	296	305	316	rBV2	3799	8860	1.51%	0.285%
4	5.391	694	706	721	rBV	69109	200478	34.20%	6.452%
5	5.556	721	733	748	rVB2	114324	323387	55.16%	10.408%
6	5.958	786	799	813	rBV	71003	190062	32.42%	6.117%
7	6.763	920	931	955	rBV	183517	432269	73.73%	13.913%
8	8.653	1234	1241	1251	rBV	374366	586259	100.00%	18.869%
9	10.055	1465	1471	1493	rBV	381589	503374	85.86%	16.201%
10	11.085	1634	1640	1652	rVB	284057	378269	64.52%	12.175%
11	12.024	1789	1794	1807	rVB	364878	455956	77.77%	14.675%




Sum of corrected areas: 3107010

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025418.D
Acq On : 02 Dec 2021 10:57
Operator : JC/MD
Sample : VX1202WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1202WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

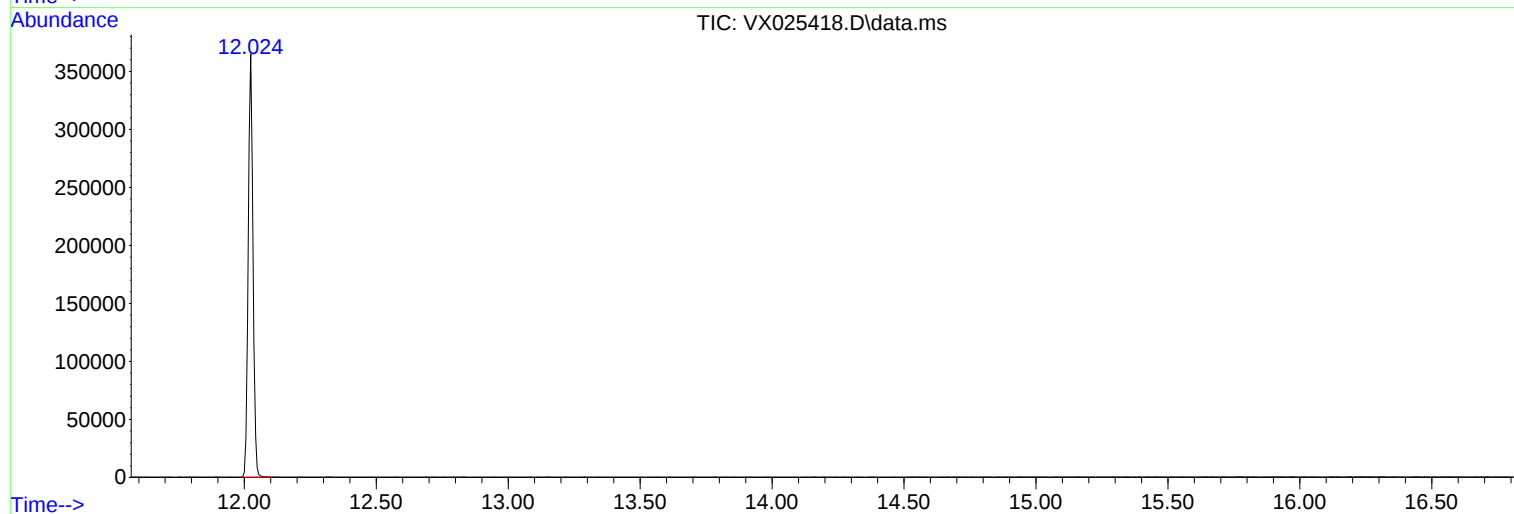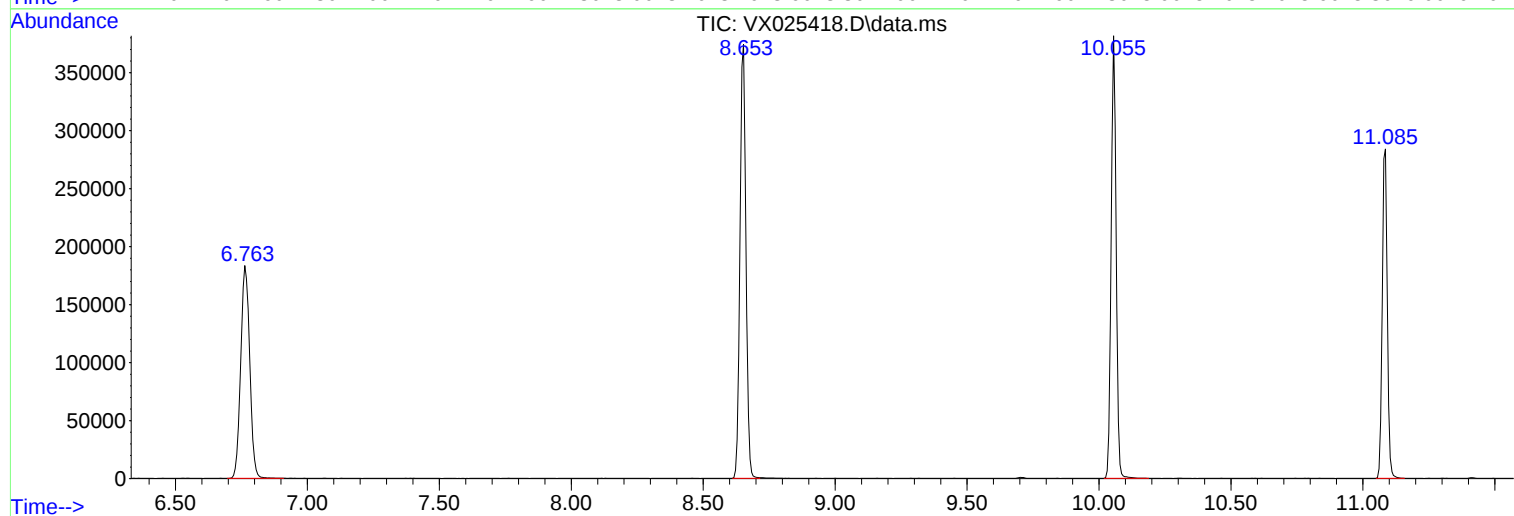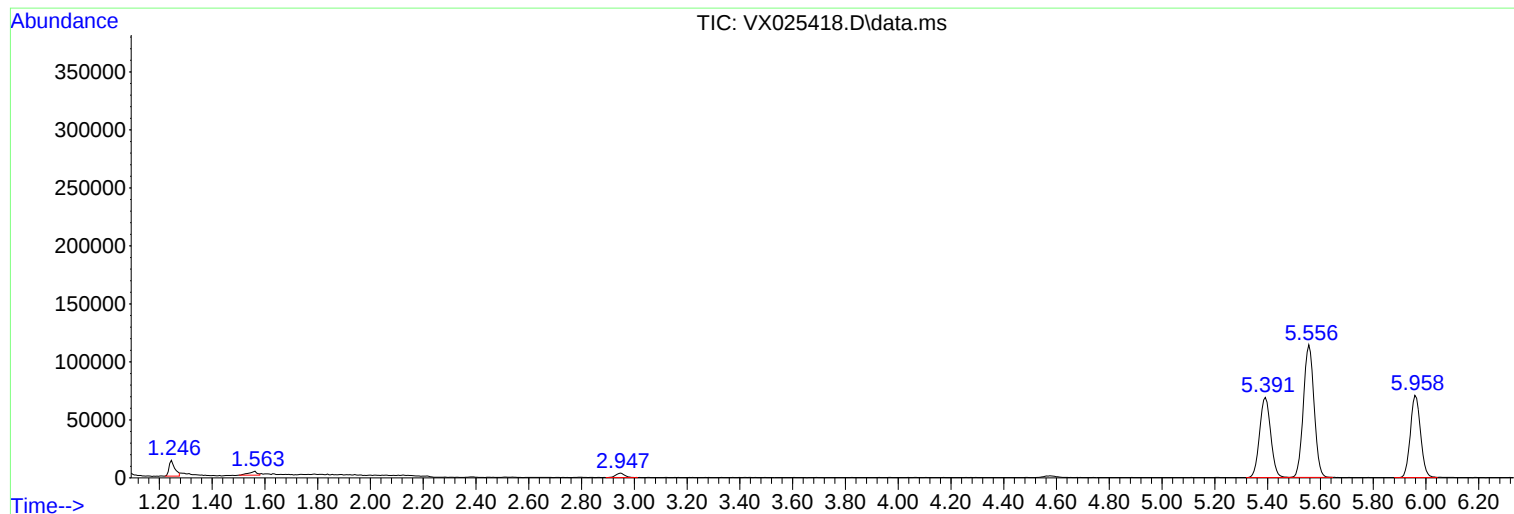

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025418.D
Acq On : 02 Dec 2021 10:57
Operator : JC/MD
Sample : VX1202WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1202WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025418.D
Acq On : 02 Dec 2021 10:57
Operator : JC/MD
Sample : VX1202WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1202WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc