

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
 Data File : VX025440.D
 Acq On : 02 Dec 2021 19:51
 Operator : JC/MD
 Sample : M4917-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-26

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
 Title : SW846 8260

Signal : TIC: VX025440.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	45	rBV	284710	589416	100.00%	16.116%
2	1.746	105	108	120	rVB3	4693	8951	1.52%	0.245%
3	2.380	207	212	222	rVB	3805	6365	1.08%	0.174%
4	2.544	230	239	246	rBV	6462	13036	2.21%	0.356%
5	2.965	300	308	319	rBV	16418	33866	5.75%	0.926%
6	3.117	325	333	344	rVB	10654	25401	4.31%	0.695%
7	3.770	431	440	447	rBV5	2438	6618	1.12%	0.181%
8	5.391	694	706	719	rBV	66632	189743	32.19%	5.188%
9	5.556	722	733	757	rVB	106970	302676	51.35%	8.276%
10	5.958	789	799	810	rBV	68110	179452	30.45%	4.907%
11	6.239	837	845	858	rBV2	11874	33187	5.63%	0.907%
12	6.763	920	931	944	rBV	169633	404627	68.65%	11.063%
13	8.427	1197	1204	1211	rBV	4716	7971	1.35%	0.218%
14	8.653	1234	1241	1248	rBV	353732	549832	93.28%	15.033%
15	8.720	1248	1252	1260	rVB	4230	7279	1.23%	0.199%
16	10.055	1465	1471	1489	rVB	351912	466372	79.12%	12.751%
17	10.195	1490	1494	1501	rVB	10794	14034	2.38%	0.384%
18	10.305	1507	1512	1518	rBV	19431	26268	4.46%	0.718%
19	10.646	1562	1568	1573	rBV	6567	9065	1.54%	0.248%
20	11.085	1634	1640	1655	rVB	275329	348534	59.13%	9.530%
21	11.750	1745	1749	1755	rBV	10967	13797	2.34%	0.377%
22	12.024	1789	1794	1801	rBV	333118	410101	69.58%	11.213%
23	13.780	2077	2082	2089	rVB	8286	10824	1.84%	0.296%




Sum of corrected areas: 3657415

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025440.D
Acq On : 02 Dec 2021 19:51
Operator : JC/MD
Sample : M4917-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

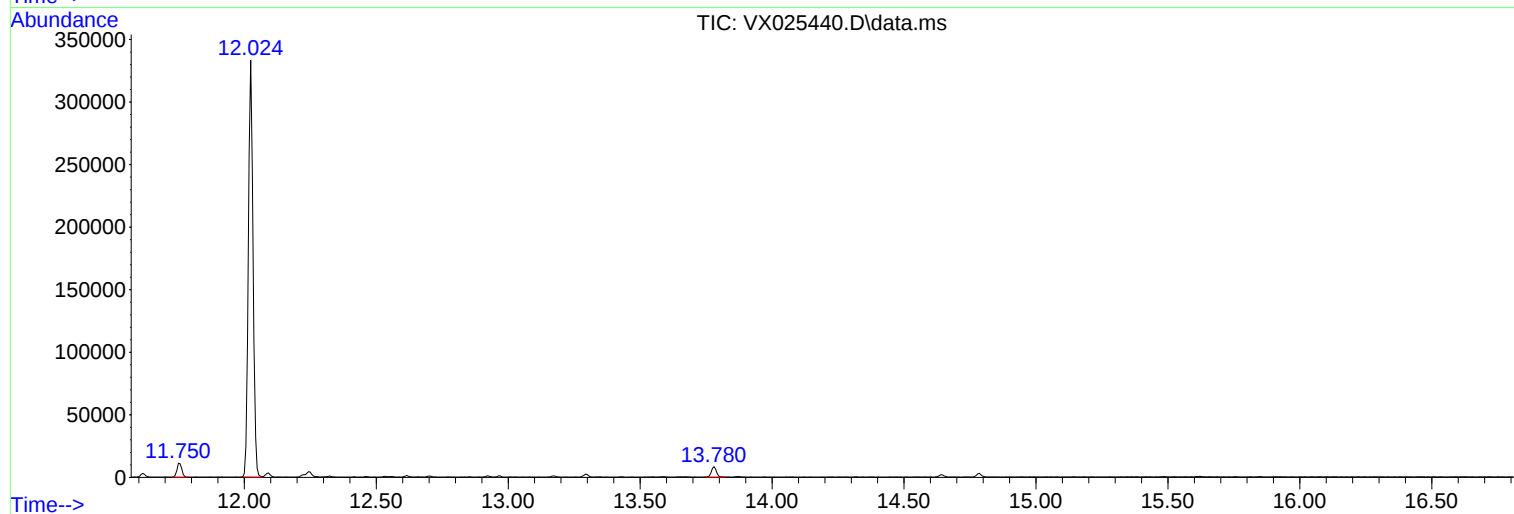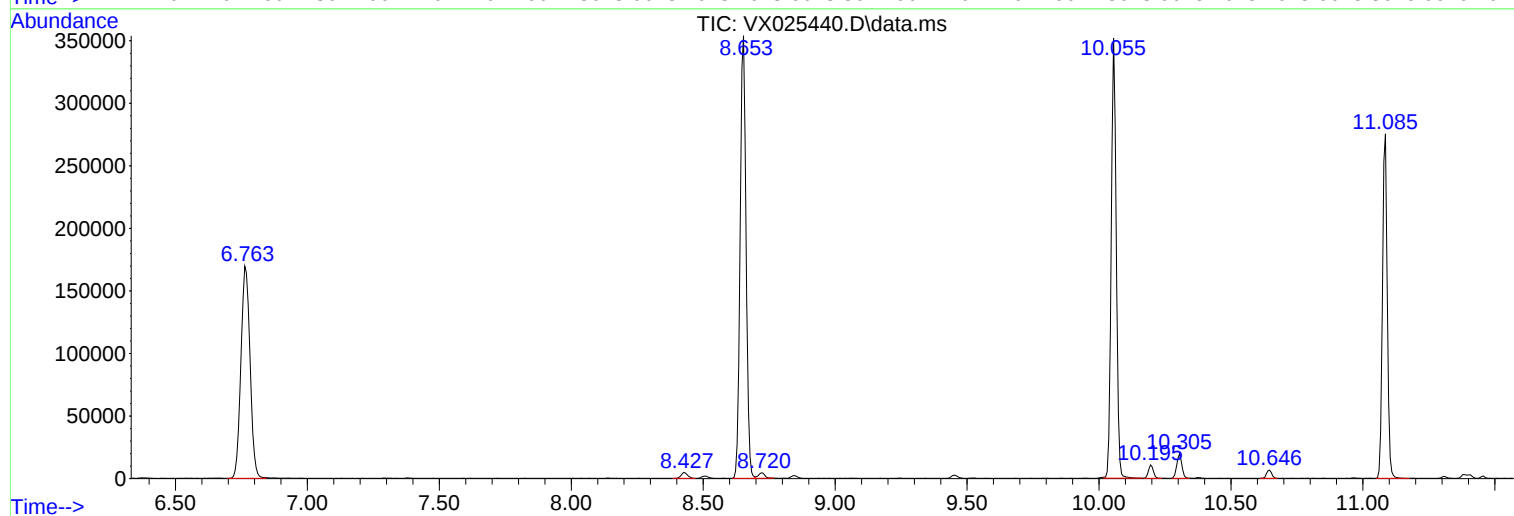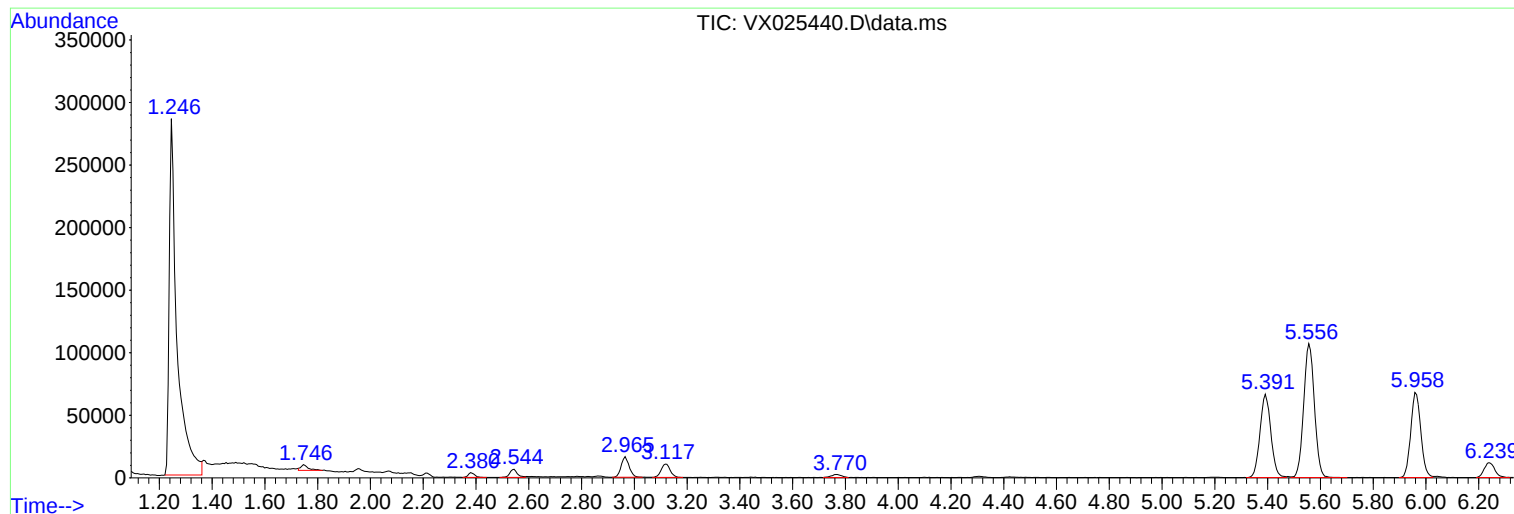

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025440.D
Acq On : 02 Dec 2021 19:51
Operator : JC/MD
Sample : M4917-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025440.D
Acq On : 02 Dec 2021 19:51
Operator : JC/MD
Sample : M4917-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------