

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
 Data File : VX025446.D
 Acq On : 02 Dec 2021 22:59
 Operator : JC/MD
 Sample : VX1202WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1202WBL02

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M

Title : SW846 8260

Signal : TIC: VX025446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	21	26	44	rBV	27824	51939	9.80%	1.828%
2	2.947	298	305	315	rBV2	4372	9842	1.86%	0.346%
3	5.391	694	706	722	rBV	62383	181437	34.24%	6.384%
4	5.556	722	733	750	rVB	101837	288238	54.40%	10.142%
5	5.964	788	800	811	rBV2	65549	171840	32.43%	6.046%
6	6.763	921	931	949	rBV	163856	387700	73.17%	13.642%
7	8.653	1234	1241	1250	rBV	337987	529894	100.00%	18.645%
8	10.055	1465	1471	1489	rVB	340576	459040	86.63%	16.152%
9	11.085	1634	1640	1650	rBV	258535	343874	64.89%	12.100%
10	12.024	1789	1794	1803	rBV	332719	418218	78.92%	14.716%




Sum of corrected areas: 2842022

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025446.D
Acq On : 02 Dec 2021 22:59
Operator : JC/MD
Sample : VX1202WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1202WBL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

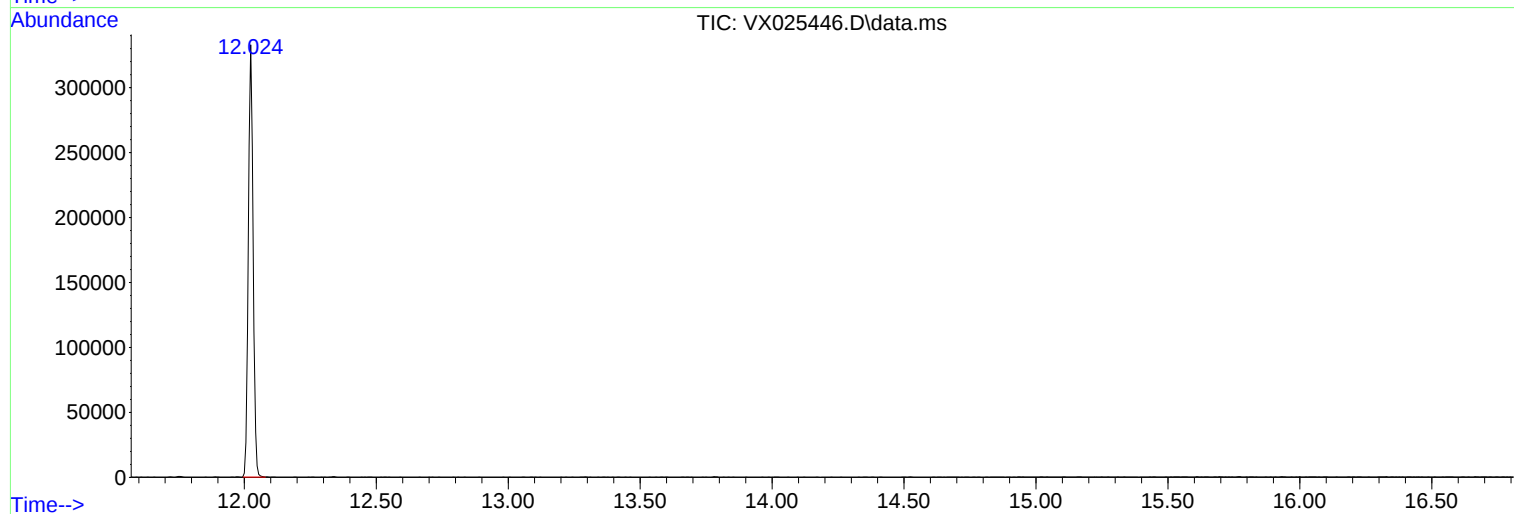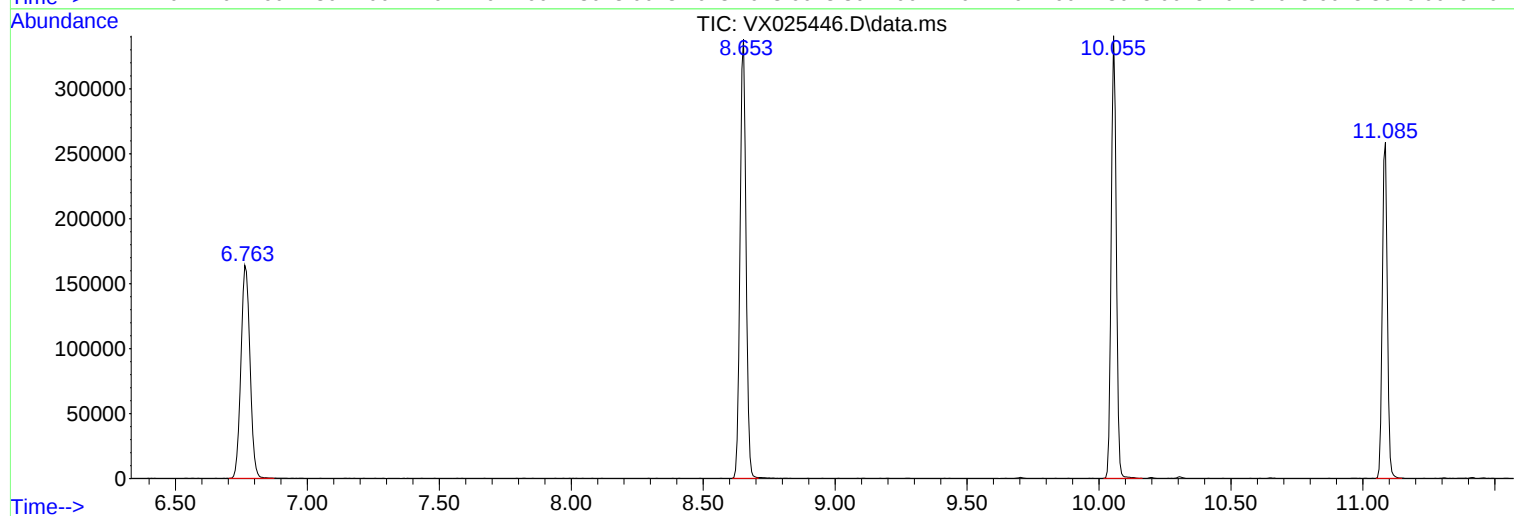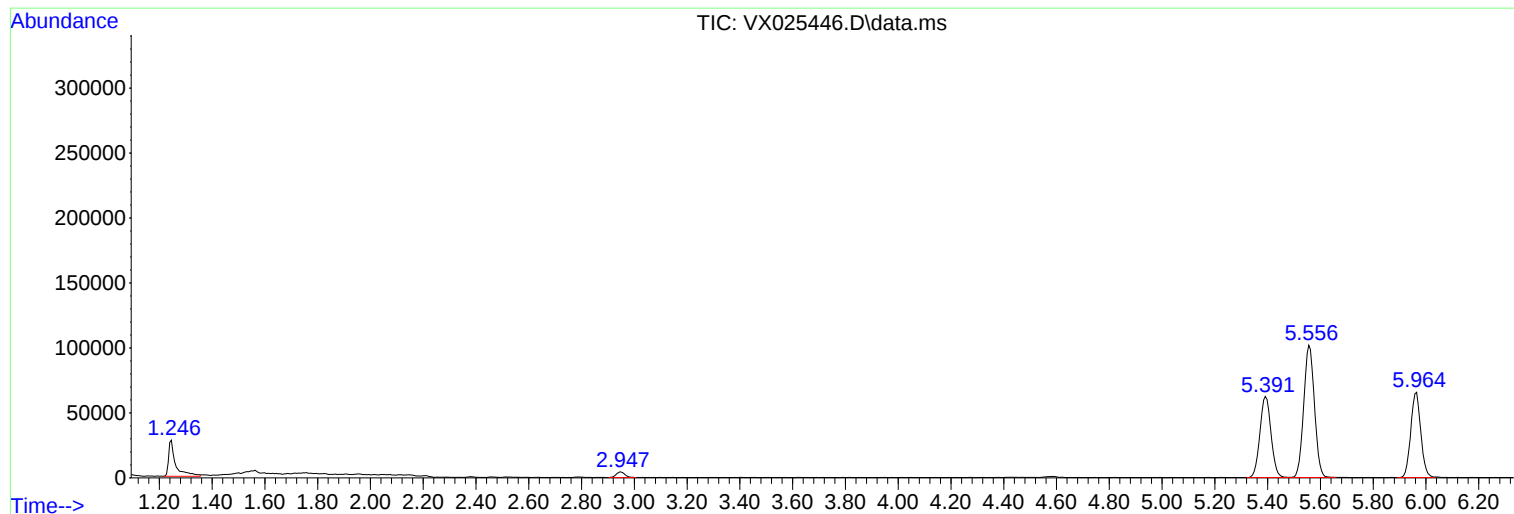

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025446.D
Acq On : 02 Dec 2021 22:59
Operator : JC/MD
Sample : VX1202WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1202WBL02










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.246	9.01 ug/l	51939	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	90
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

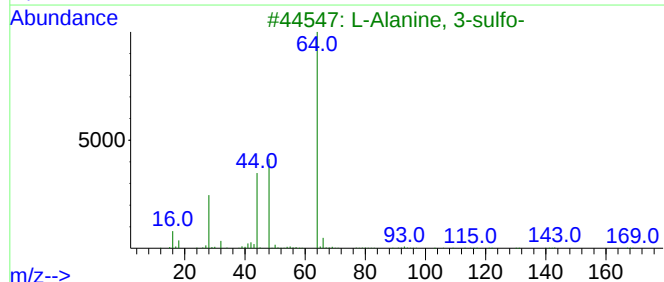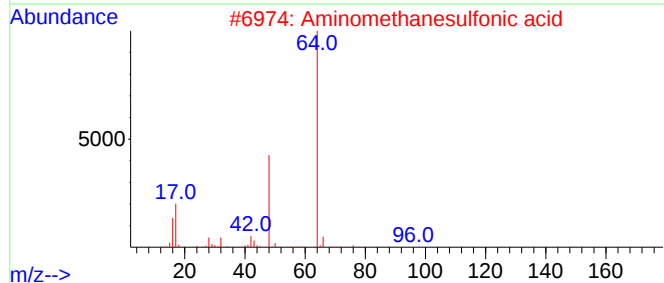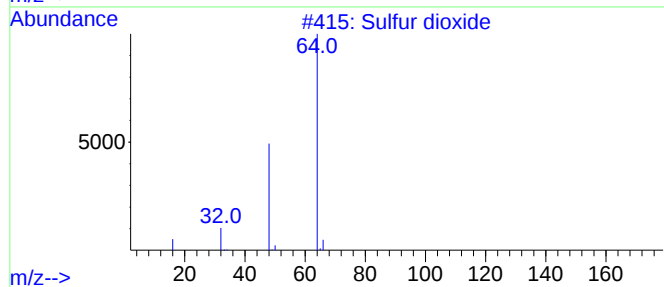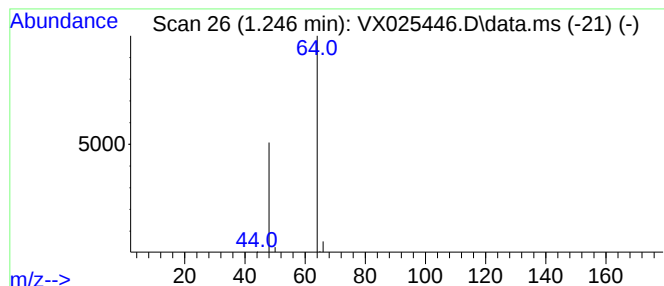

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025446.D
Acq On : 02 Dec 2021 22:59
Operator : JC/MD
Sample : VX1202WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1202WBL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.246	9.0	ug/l	51939	1	5.556	288238	50.0