

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025457.D
Acq On : 03 Dec 2021 03:17
Operator : JC/MD
Sample : M4918-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-37

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M

Title : SW846 8260

Signal : TIC: VX025457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	3	6	10	rBV	8495	13603	1.74%	0.378%
2	1.252	22	27	48	rBV	374535	783727	100.00%	21.766%
3	3.117	325	333	343	rVB	27168	62938	8.03%	1.748%
4	5.391	694	706	722	rBV	64327	184886	23.59%	5.135%
5	5.556	722	733	748	rVB	99993	283718	36.20%	7.880%
6	5.958	788	799	811	rBV	68250	179084	22.85%	4.974%
7	6.763	918	931	948	rBV	159869	384117	49.01%	10.668%
8	8.653	1234	1241	1256	rBV	328860	521991	66.60%	14.497%
9	10.055	1465	1471	1491	rVB	336033	447139	57.05%	12.418%
10	11.085	1634	1640	1652	rVB	255169	337038	43.00%	9.360%
11	12.024	1789	1794	1802	rBV	328725	402410	51.35%	11.176%




Sum of corrected areas: 3600651

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025457.D
Acq On : 03 Dec 2021 03:17
Operator : JC/MD
Sample : M4918-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

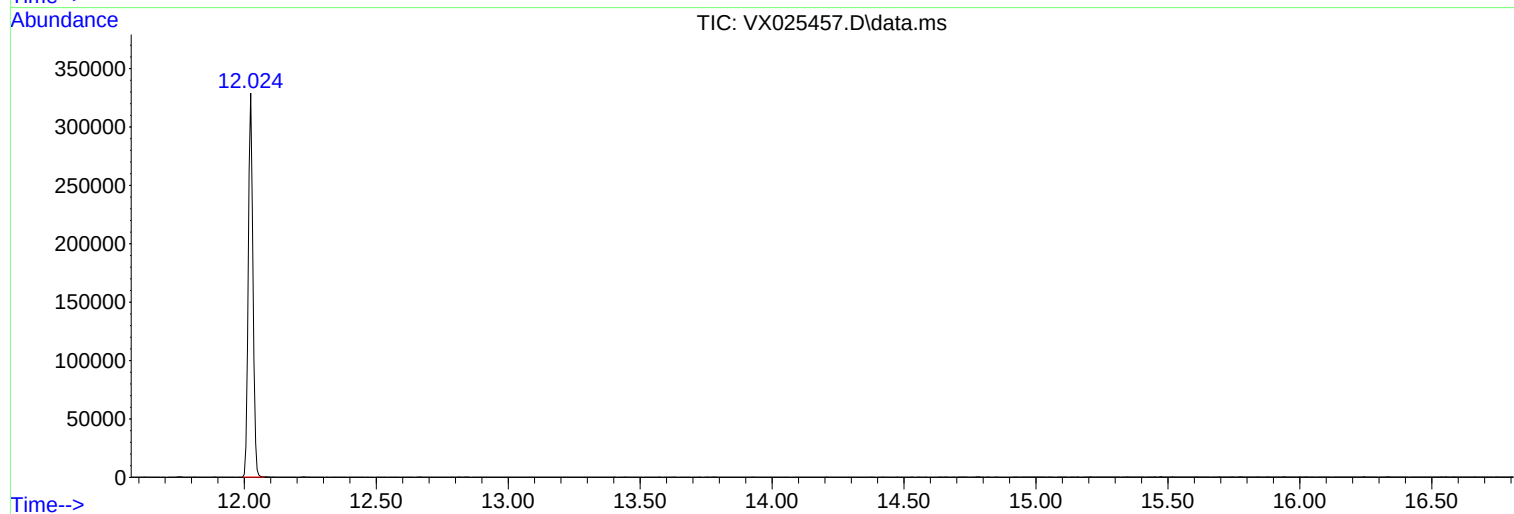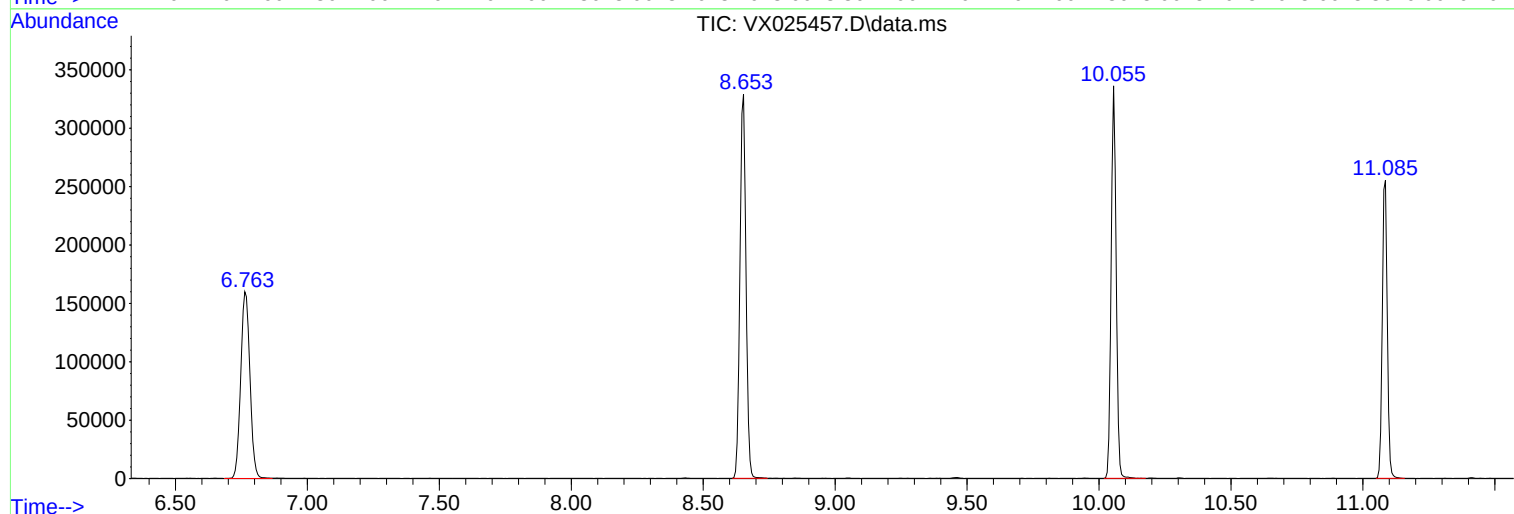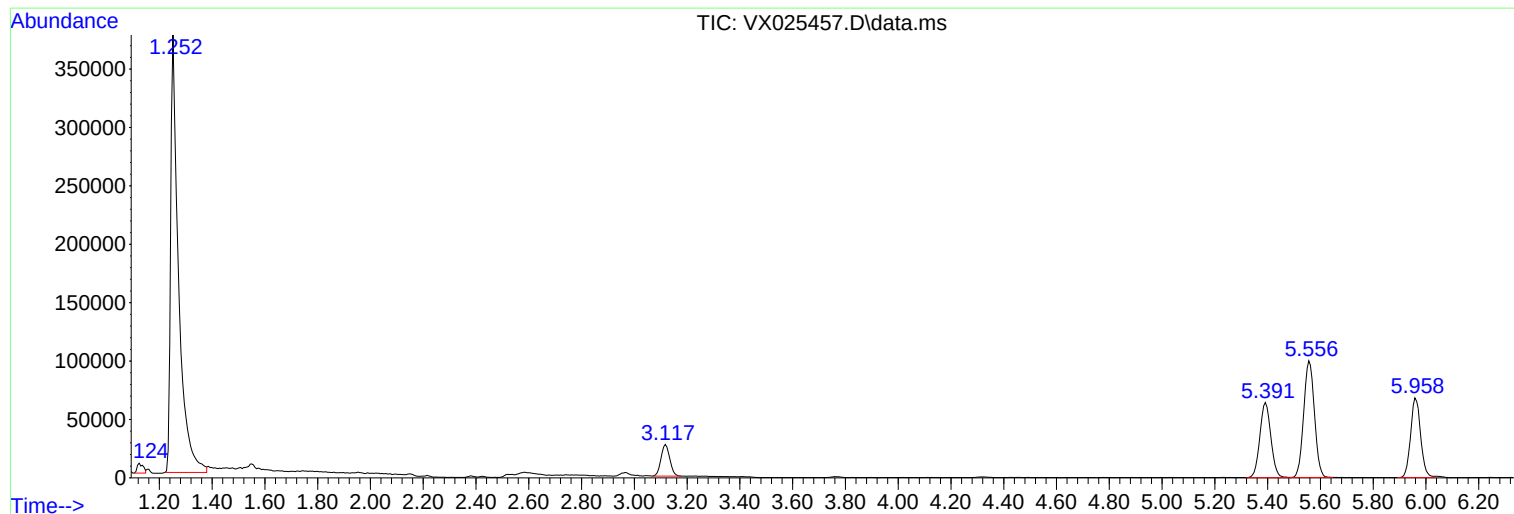

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025457.D
Acq On : 03 Dec 2021 03:17
Operator : JC/MD
Sample : M4918-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-37










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.252	138.12 ug/l	783727	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	83
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

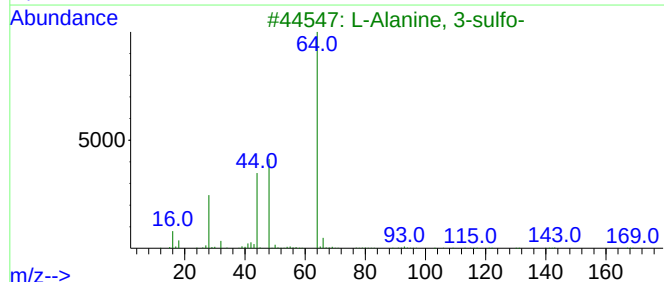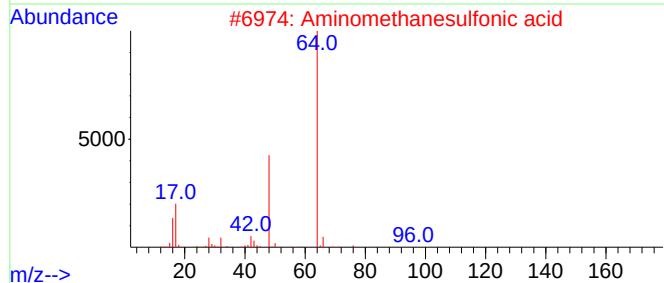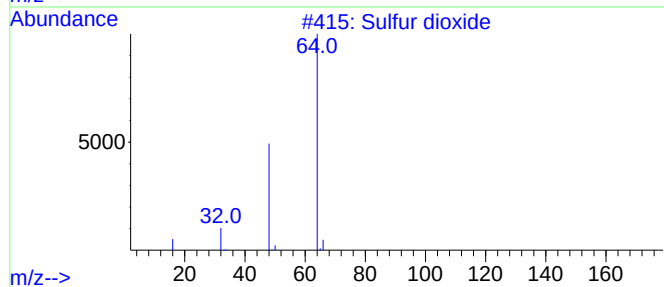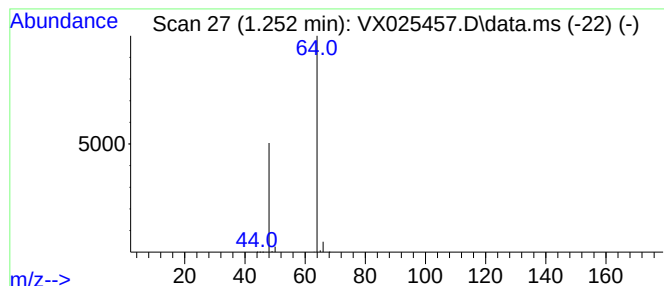

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025457.D
Acq On : 03 Dec 2021 03:17
Operator : JC/MD
Sample : M4918-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.252	138.1	ug/l	783727	1	5.556	283718	50.0