

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025466.D
Acq On : 03 Dec 2021 06:47
Operator : JC/MD
Sample : M4918-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-45A

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M

Title : SW846 8260

Signal : TIC: VX025466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.245	22	26	33	rBV	36672	55584	9.86%	1.842%
2	5.391	694	706	720	rBV3	66452	193092	34.27%	6.398%
3	5.556	722	733	747	rVB	107378	304022	53.95%	10.074%
4	5.958	789	799	812	rBV	69558	184203	32.69%	6.103%
5	6.763	921	931	947	rBV	172618	410989	72.93%	13.618%
6	8.653	1234	1241	1249	rBV	355469	563512	100.00%	18.672%
7	10.055	1465	1471	1489	rVB	366460	487820	86.57%	16.164%
8	10.305	1507	1512	1521	rVB	5583	7827	1.39%	0.259%
9	11.085	1634	1640	1652	rBV	275604	368941	65.47%	12.225%
10	12.024	1789	1794	1802	rBV	363142	442042	78.44%	14.647%




Sum of corrected areas: 3018032

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025466.D
Acq On : 03 Dec 2021 06:47
Operator : JC/MD
Sample : M4918-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-45A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

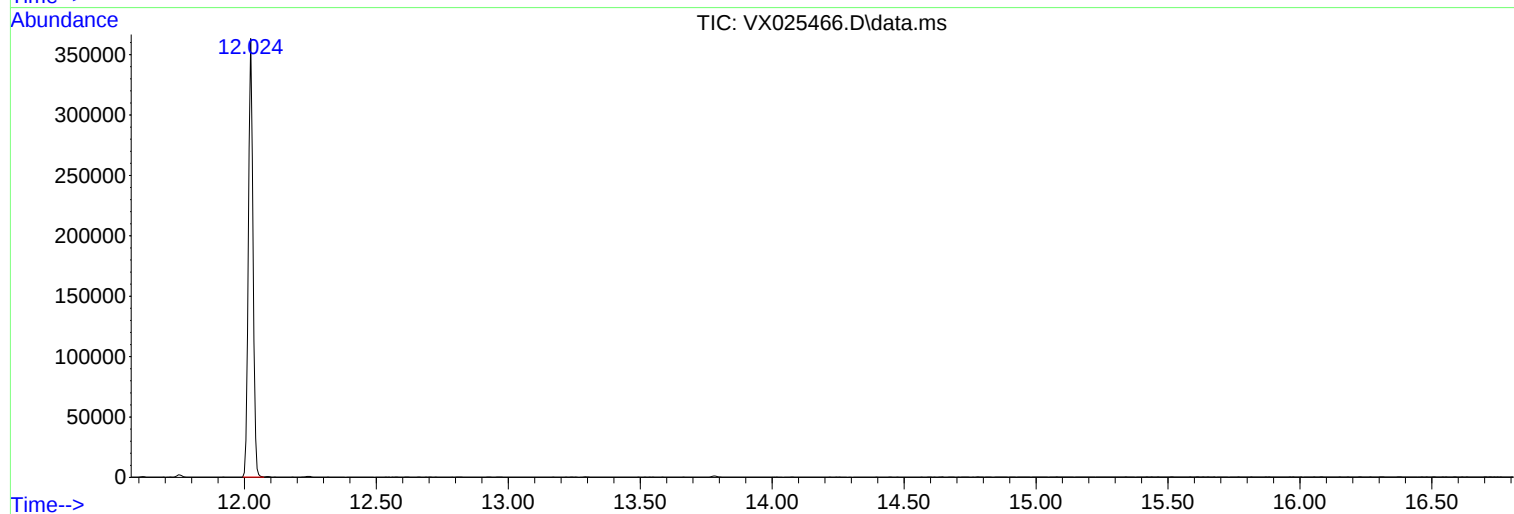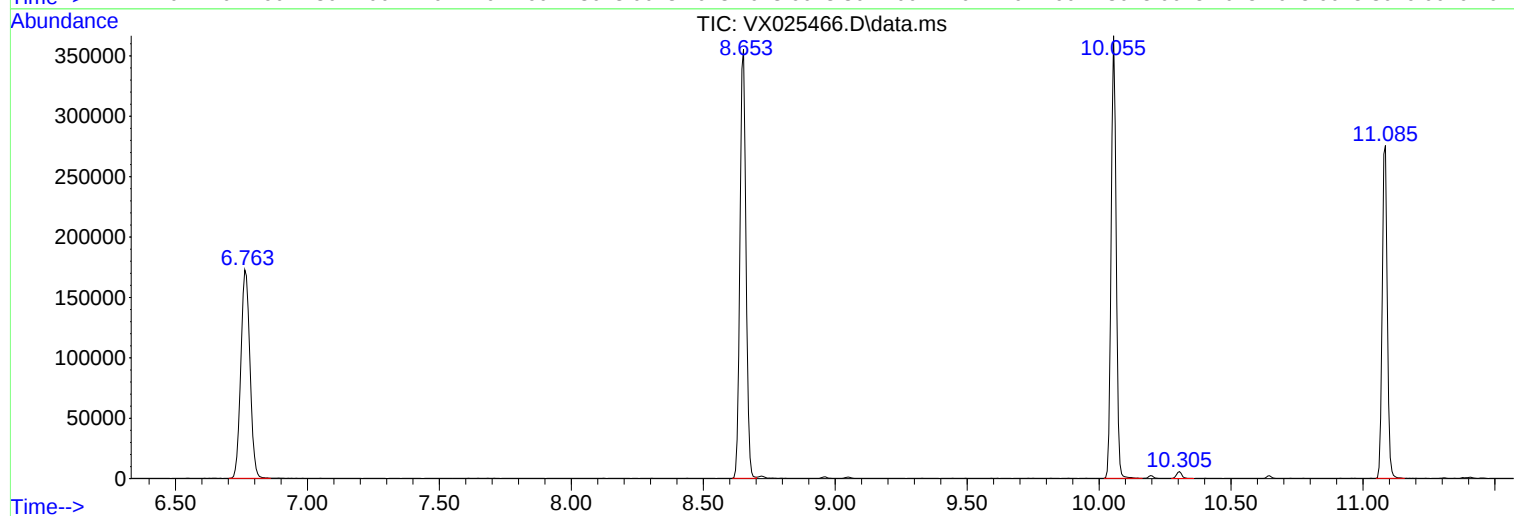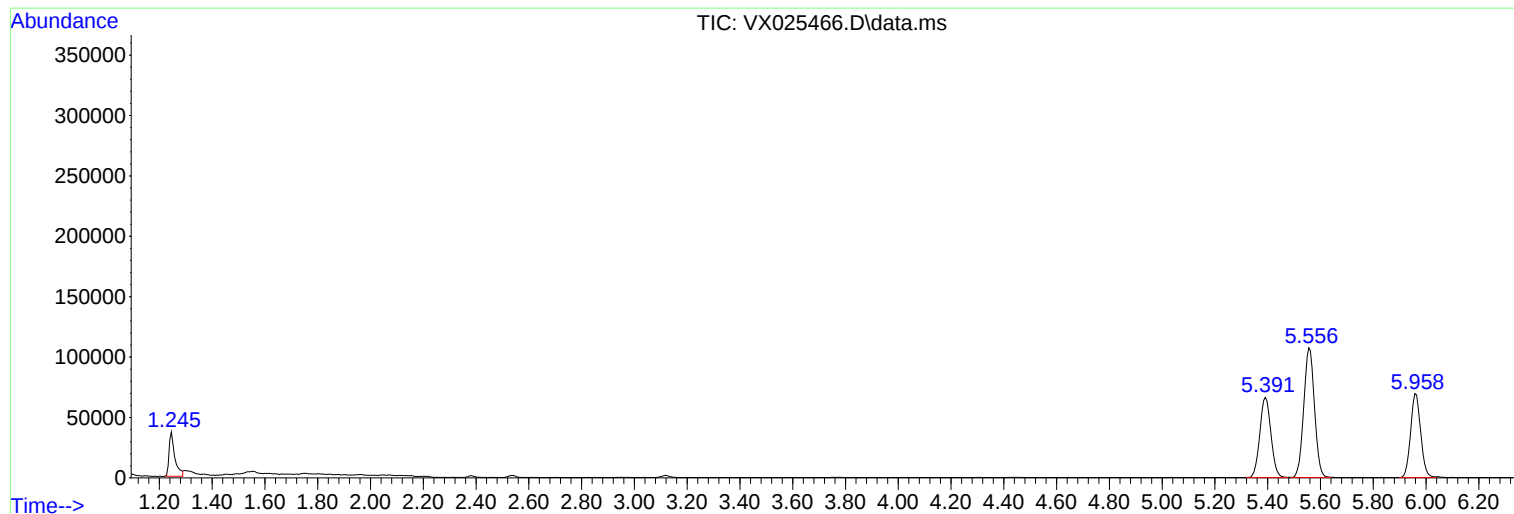

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025466.D
Acq On : 03 Dec 2021 06:47
Operator : JC/MD
Sample : M4918-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-45A










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.245	9.14 ug/l	55584	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	83
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

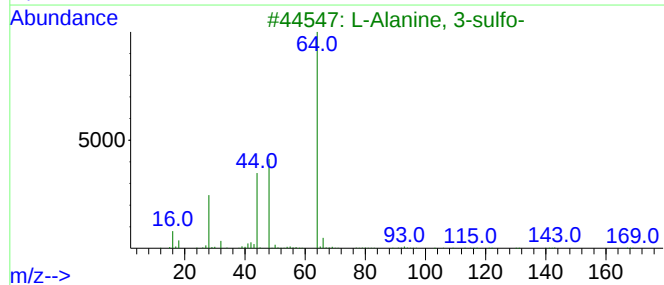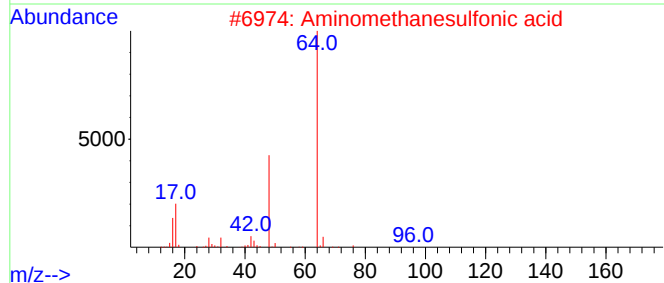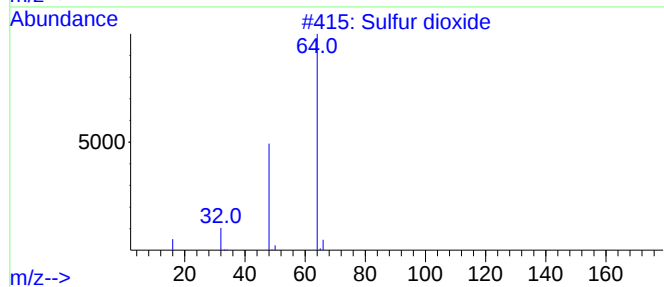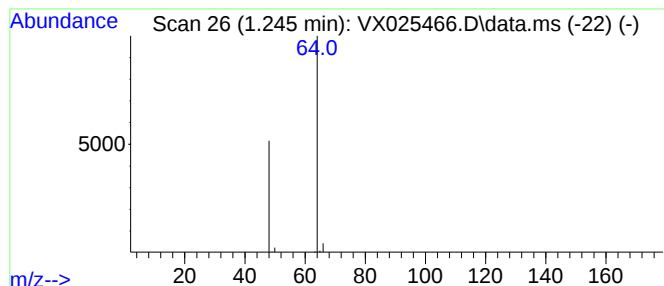

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120221\
Data File : VX025466.D
Acq On : 03 Dec 2021 06:47
Operator : JC/MD
Sample : M4918-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-45A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.245	9.1	ug/l	55584	1	5.556	304022	50.0