

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX120222\  
 Data File : VX033189.D  
 Acq On : 02 Dec 2022 16:34  
 Operator : JC/MD  
 Sample : N5858-01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 COMP-SAMPLE-TANK-26-27-28-30

Quant Time: Dec 03 04:34:08 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X112222W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Nov 22 13:58:46 2022  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon  | Response | Conc     | Units | Dev(Min) |
|-----------------------------|--------|-------|----------|----------|-------|----------|
| -----                       |        |       |          |          |       |          |
| Internal Standards          |        |       |          |          |       |          |
| 1) Pentafluorobenzene       | 5.550  | 168   | 114956   | 50.000   | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene     | 6.763  | 114   | 187063   | 50.000   | ug/l  | 0.00     |
| 63) Chlorobenzene-d5        | 10.055 | 117   | 167291   | 50.000   | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4  | 12.024 | 152   | 76225    | 50.000   | ug/l  | 0.00     |
| System Monitoring Compounds |        |       |          |          |       |          |
| 33) 1,2-Dichloroethane-d4   | 5.958  | 65    | 61754    | 55.308   | ug/l  | 0.00     |
| Spiked Amount               | 50.000 | Range | 78 - 117 | Recovery | =     | 110.620% |
| 35) Dibromofluoromethane    | 5.385  | 113   | 49220    | 46.672   | ug/l  | 0.00     |
| Spiked Amount               | 50.000 | Range | 75 - 124 | Recovery | =     | 93.340%  |
| 50) Toluene-d8              | 8.647  | 98    | 161290   | 50.868   | ug/l  | 0.00     |
| Spiked Amount               | 50.000 | Range | 92 - 112 | Recovery | =     | 101.740% |
| 62) 4-Bromofluorobenzene    | 11.079 | 95    | 60588    | 43.736   | ug/l  | 0.00     |
| Spiked Amount               | 50.000 | Range | 83 - 123 | Recovery | =     | 87.480%  |


Target Compounds Qvalue

-----  
 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX120222\  
Data File : VX033189.D  
Acq On : 02 Dec 2022 16:34  
Operator : JC/MD  
Sample : N5858-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
COMP-SAMPLE-TANK-26-27-28-30

Quant Time: Dec 03 04:34:08 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X112222W.M  
Quant Title : SW846 8260  
QLast Update : Tue Nov 22 13:58:46 2022  
Response via : Initial Calibration




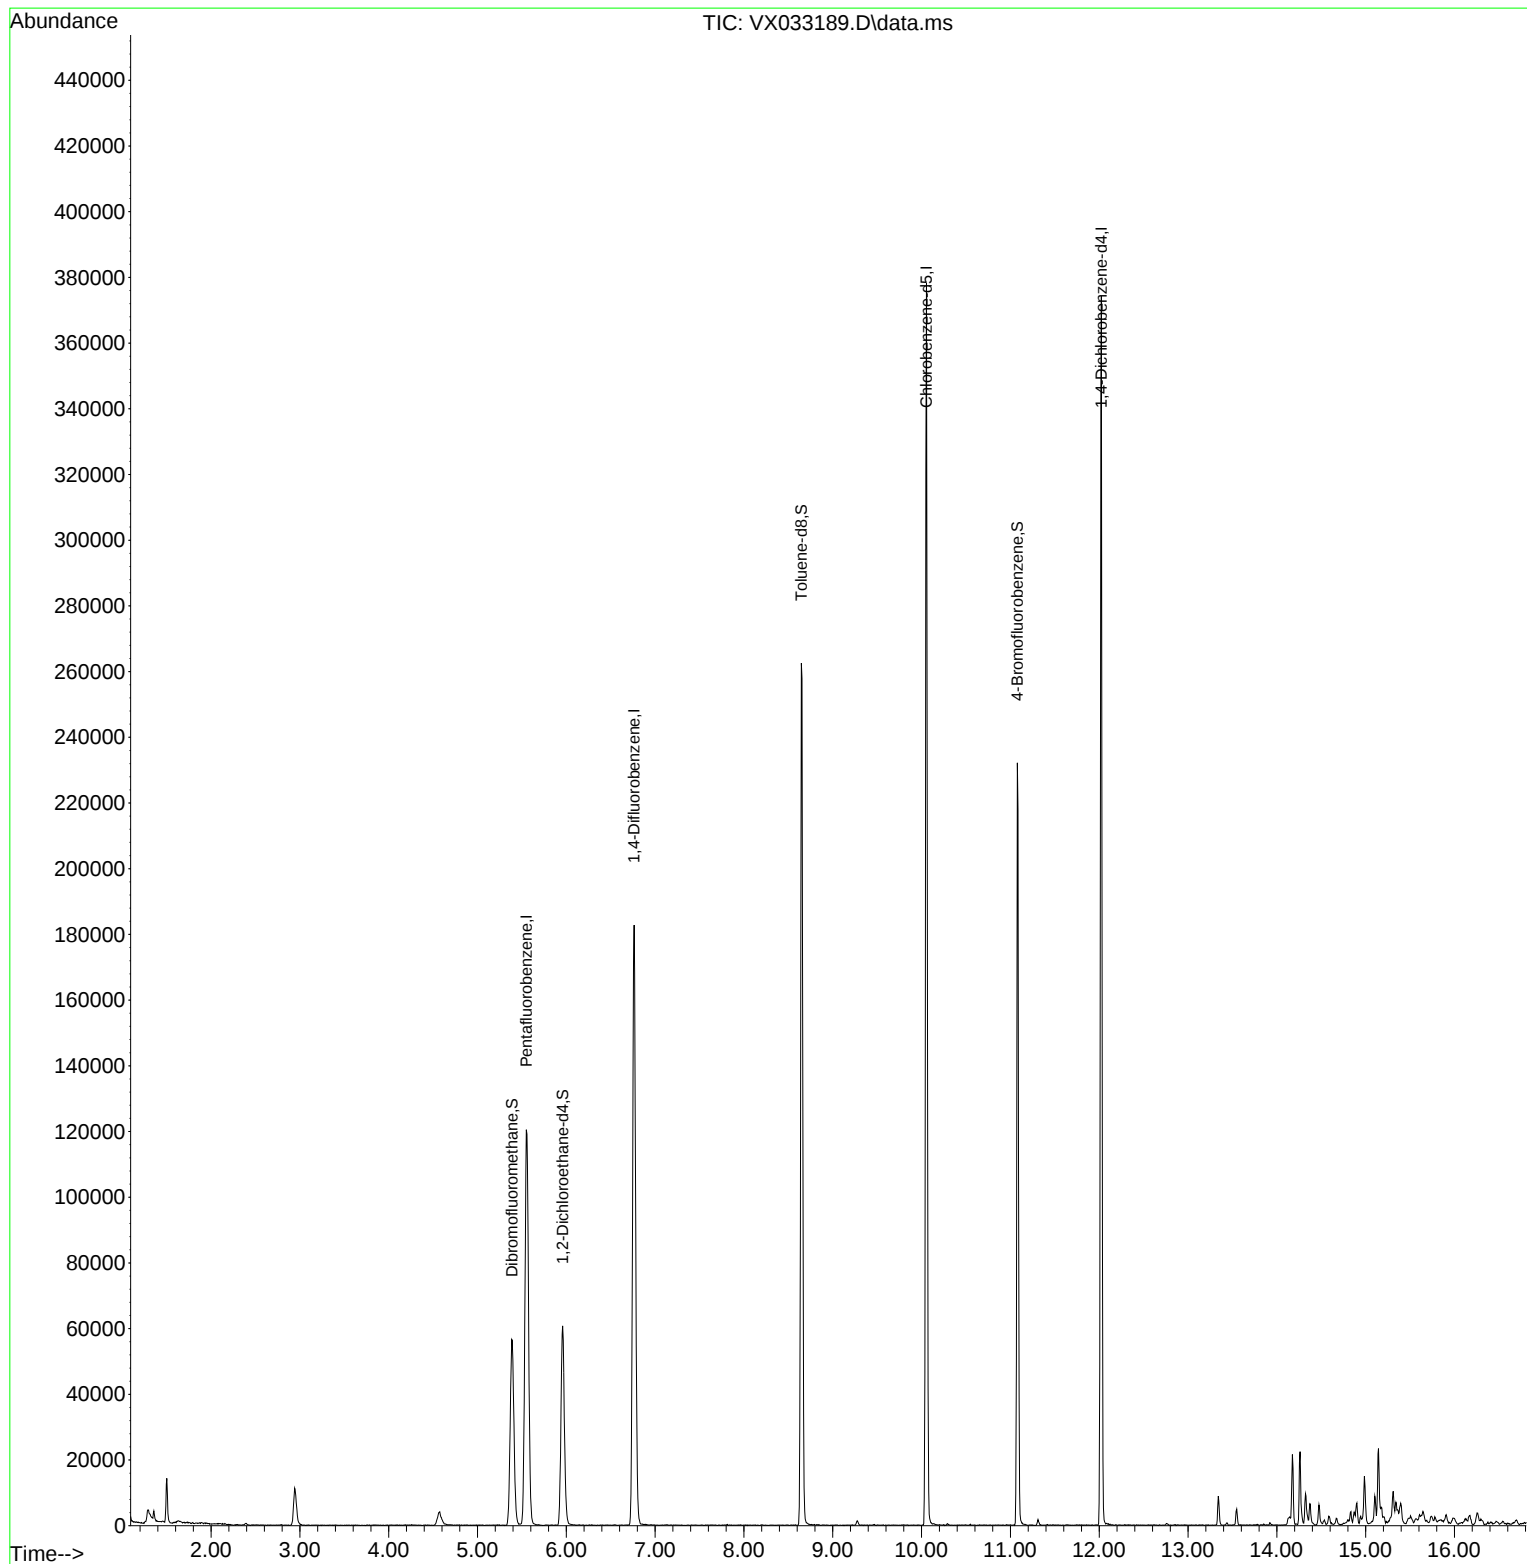




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 713  
Delta R.T. -0.006 min  
Lab File: VX033189.D  
Acq: 02 Dec 2022 16:34




Instrument :  
MSVOA\_X  
ClientSampleId :  
COMP-SAMPLE-TANK-26-27-28-30

Tgt Ion:168 Resp: 114956  
Ion Ratio Lower Upper  
168 100  
99 59.9 46.1 69.1

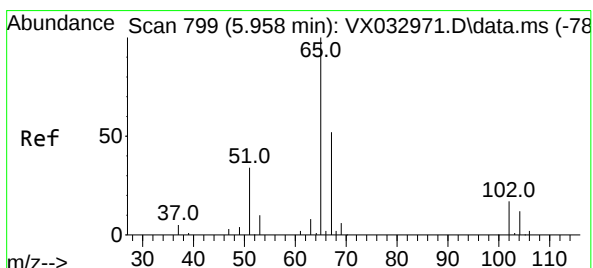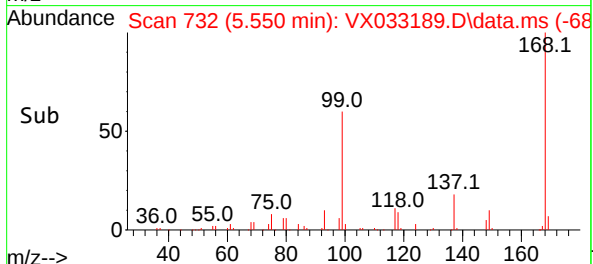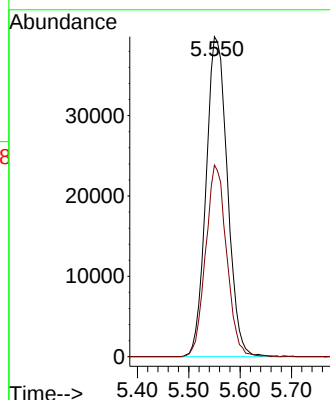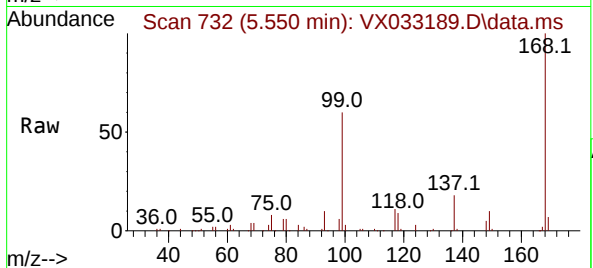

#33  
1,2-Dichloroethane-d4  
Concen: 55.308 ug/l  
RT: 5.958 min Scan# 799  
Delta R.T. 0.000 min  
Lab File: VX033189.D  
Acq: 02 Dec 2022 16:34

Tgt Ion: 65 Resp: 61754  
Ion Ratio Lower Upper  
65 100  
67 50.0 0.0 101.8

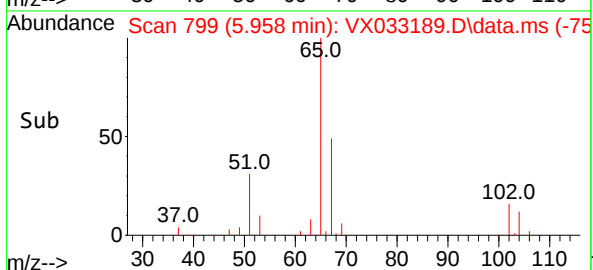
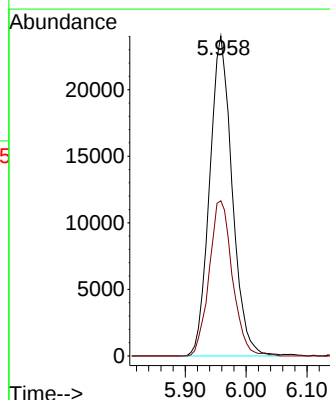
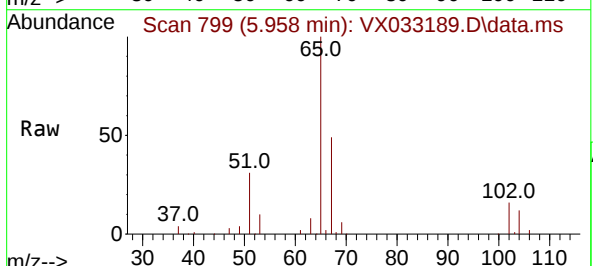




#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.763 min Scan# 911  
Delta R.T. 0.000 min  
Lab File: VX033189.D  
Acq: 02 Dec 2022 16:34




Instrument :  
MSVOA\_X  
ClientSampleId :  
COMP-SAMPLE-TANK-26-27-28-30


Tgt Ion:114 Resp: 187063  
Ion Ratio Lower Upper  
114 100  
63 20.6 0.0 41.6  
88 15.6 0.0 33.4

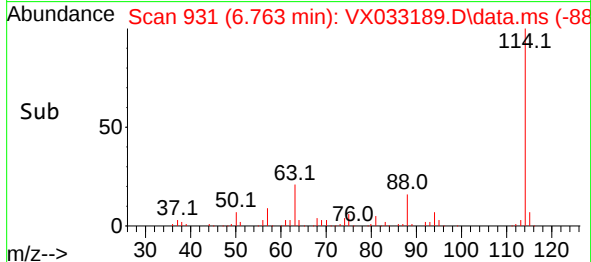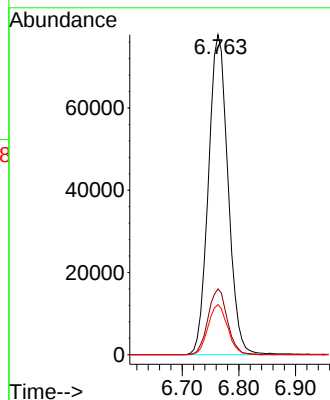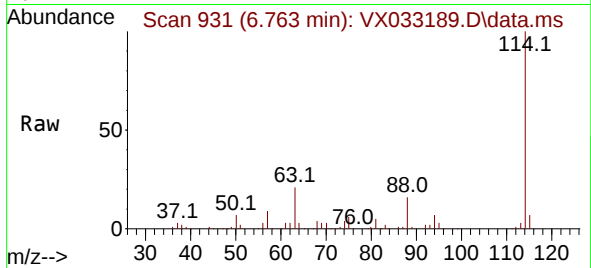

#35  
Dibromofluoromethane  
Concen: 46.672 ug/l  
RT: 5.385 min Scan# 705  
Delta R.T. 0.000 min  
Lab File: VX033189.D  
Acq: 02 Dec 2022 16:34

Tgt Ion:113 Resp: 49220  
Ion Ratio Lower Upper  
113 100  
111 102.3 82.4 123.6  
192 18.6 15.4 23.2


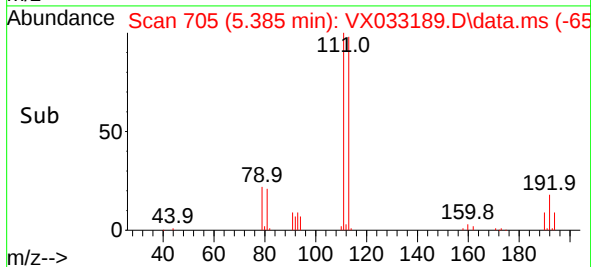
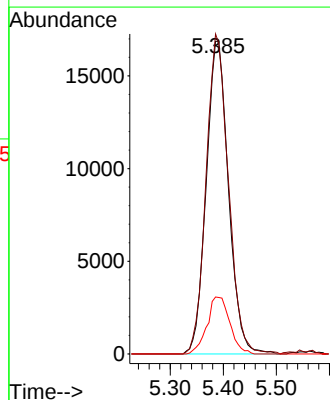
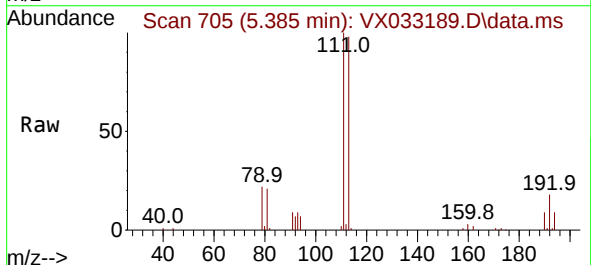


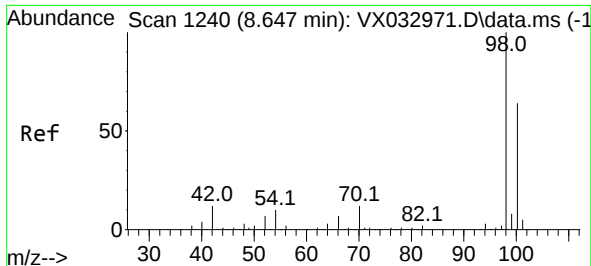

#50  
Toluene-d8  
Concen: 50.868 ug/l  
RT: 8.647 min Scan# 11  
Delta R.T. -0.006 min  
Lab File: VX033189.D  
Acq: 02 Dec 2022 16:34




Instrument :  
MSVOA\_X  
ClientSampleId :  
COMP-SAMPLE-TANK-26-27-28-30


Tgt Ion: 98 Resp: 161290  
Ion Ratio Lower Upper  
98 100  
100 63.5 50.9 76.3

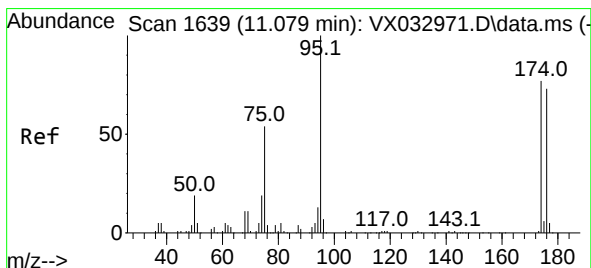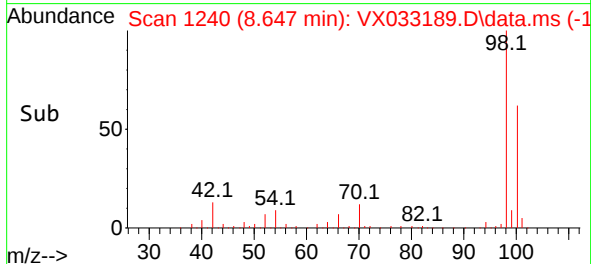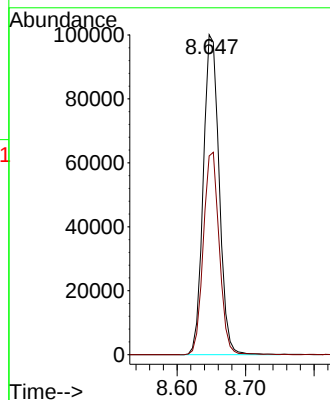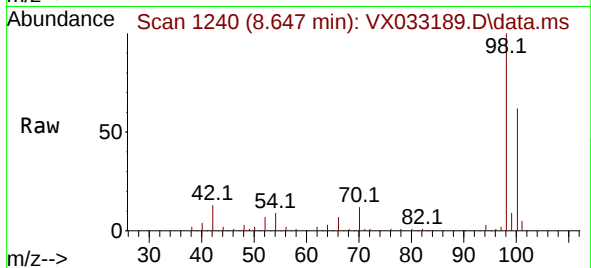

#62  
4-Bromofluorobenzene  
Concen: 43.736 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. 0.000 min  
Lab File: VX033189.D  
Acq: 02 Dec 2022 16:34

Tgt Ion: 95 Resp: 60588  
Ion Ratio Lower Upper  
95 100  
174 80.5 0.0 164.0  
176 77.2 0.0 154.4


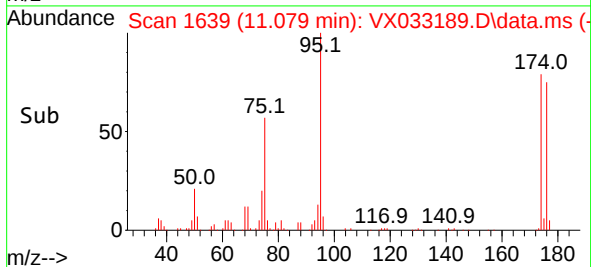
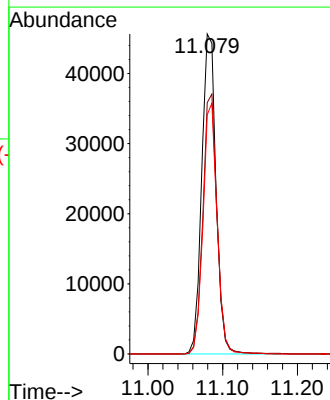
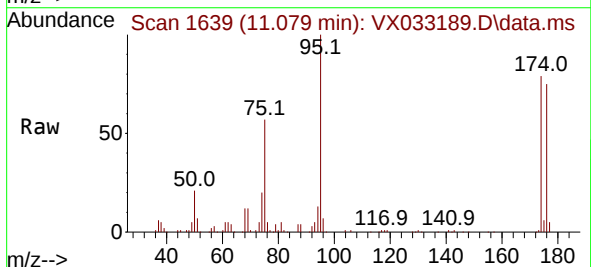


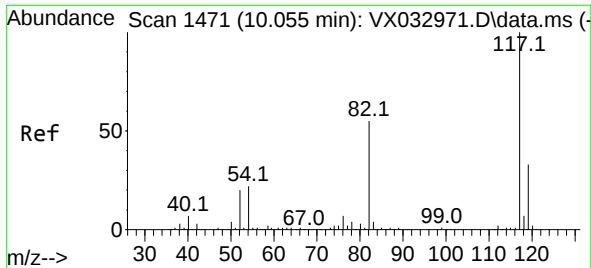

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. 0.000 min  
Lab File: VX033189.D  
Acq: 02 Dec 2022 16:34

Instrument :  
MSVOA\_X  
ClientSampleId :  
COMP-SAMPLE-TANK-26-27-28-30

Tgt Ion:117 Resp: 167291  
Ion Ratio Lower Upper  
117 100  
82 55.3 44.3 66.5  
119 31.6 25.7 38.5

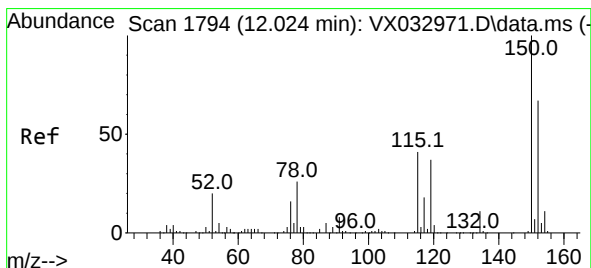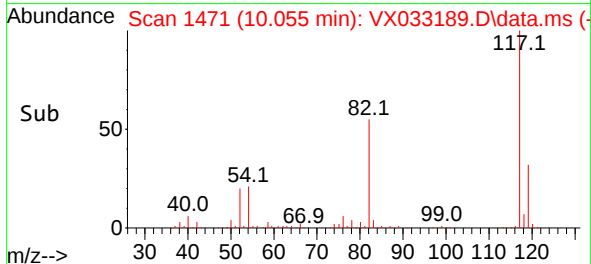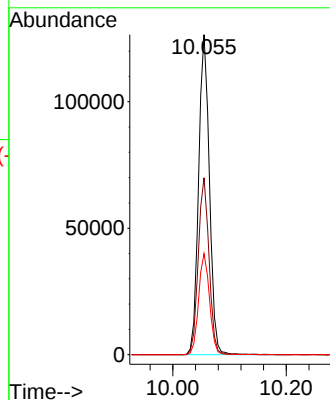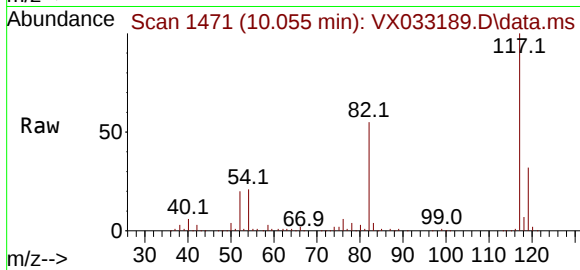

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.024 min Scan# 1794  
Delta R.T. 0.000 min  
Lab File: VX033189.D  
Acq: 02 Dec 2022 16:34

Tgt Ion:152 Resp: 76225  
Ion Ratio Lower Upper  
152 100  
115 60.2 44.0 132.0  
150 158.2 0.0 351.8

