

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120222\
 Data File : VX033188.D
 Acq On : 02 Dec 2022 16:11
 Operator : JC/MD
 Sample : N5857-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-SAMPLE-TANK-10-11-12-31-33

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Title : SW846 8260

Signal : TIC: VX033188.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.288	30	33	42	rBV2	2756	6931	1.37%	0.242%
2	5.385	692	705	722	rBV2	56352	165534	32.69%	5.774%
3	5.556	722	733	752	rVB	119963	342655	67.67%	11.953%
4	5.958	789	799	812	rBV	60588	160523	31.70%	5.600%
5	6.763	920	931	945	rBV	184430	430237	84.96%	15.008%
6	8.647	1234	1240	1251	rBV	266995	429285	84.77%	14.975%
7	10.055	1465	1471	1483	rBV	375699	506387	100.00%	17.664%
8	11.079	1634	1639	1656	rBV	236956	303345	59.90%	10.582%
9	12.024	1788	1794	1804	rBV	376368	471505	93.11%	16.448%
10	14.176	2144	2147	2152	rVB2	6309	8245	1.63%	0.288%
11	14.262	2157	2161	2167	rBV2	6986	9614	1.90%	0.335%
12	14.323	2167	2171	2176	rBV4	4040	5596	1.11%	0.195%
13	14.987	2275	2280	2286	rVB2	6431	10062	1.99%	0.351%
14	15.146	2302	2306	2309	rBV	9064	11540	2.28%	0.403%
15	15.395	2344	2347	2352	rVB3	3499	5261	1.04%	0.184%




Sum of corrected areas: 2866720

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120222\
Data File : VX033188.D
Acq On : 02 Dec 2022 16:11
Operator : JC/MD
Sample : N5857-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-SAMPLE-TANK-10-11-12-31-33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

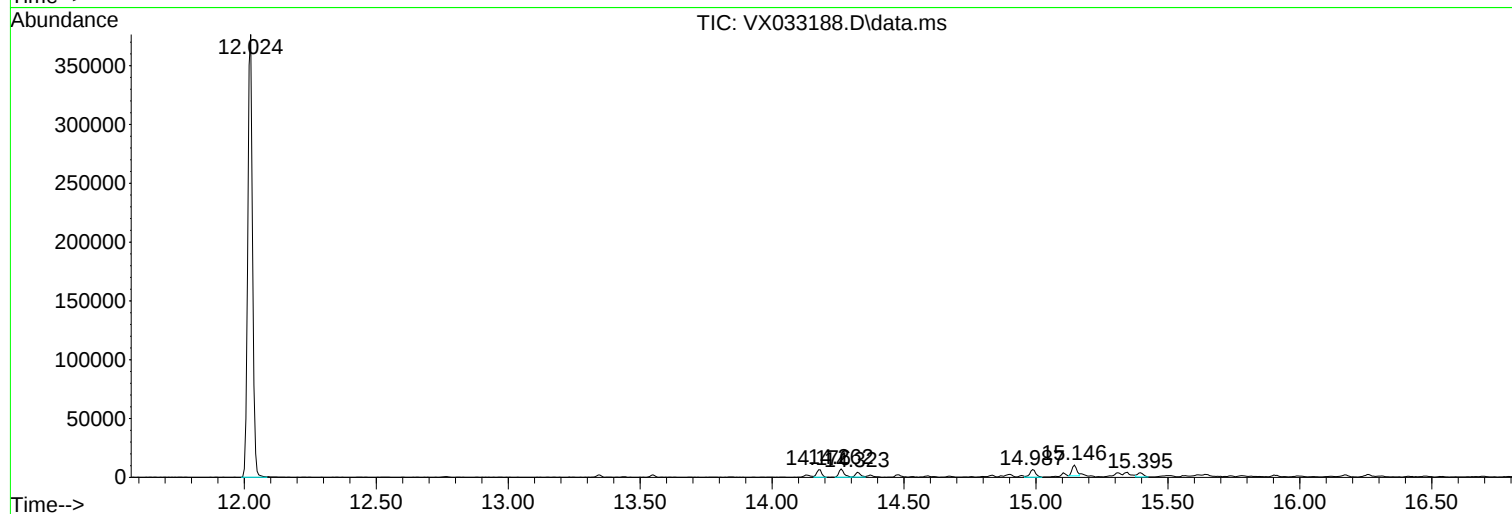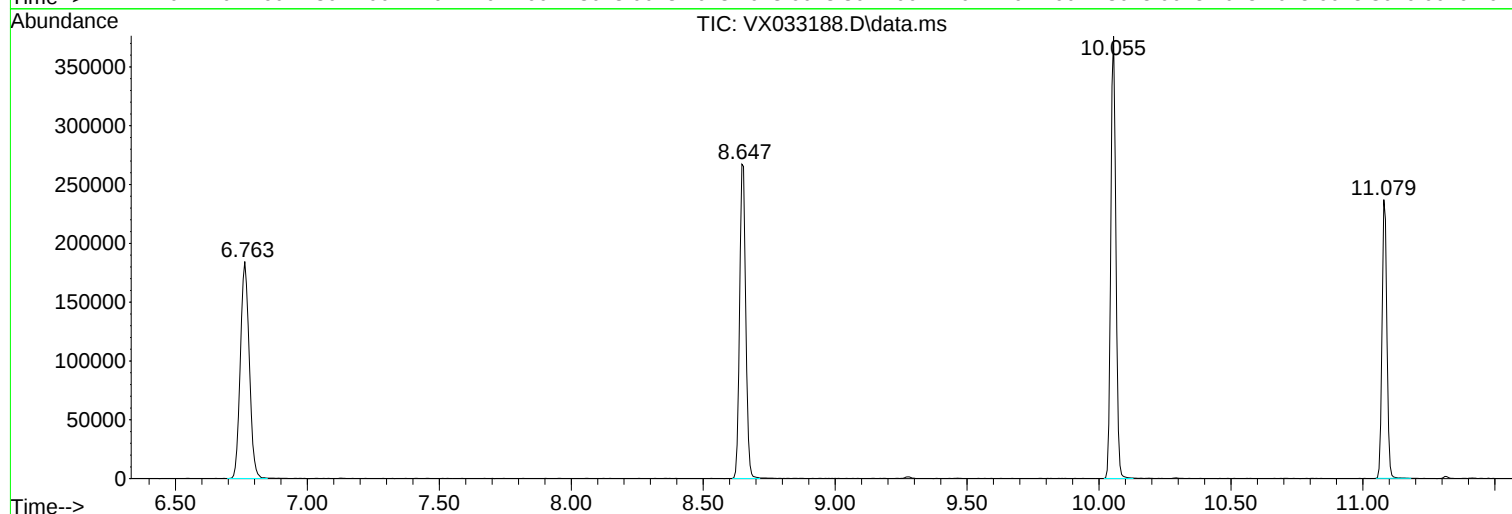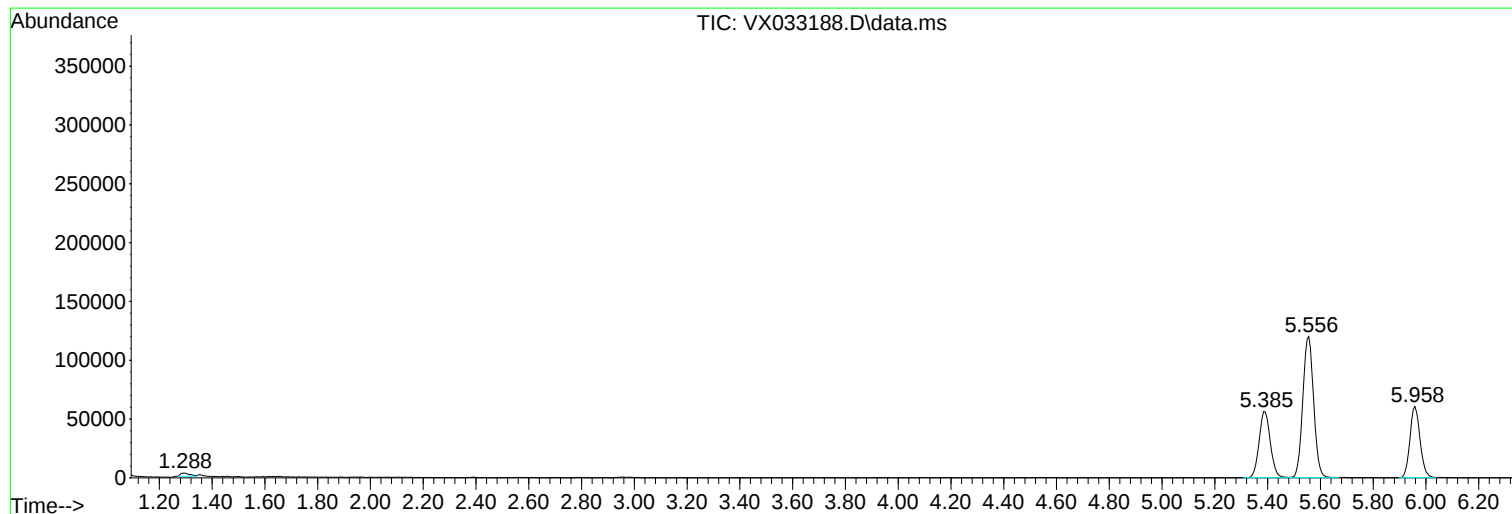

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120222\
Data File : VX033188.D
Acq On : 02 Dec 2022 16:11
Operator : JC/MD
Sample : N5857-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-SAMPLE-TANK-10-11-12-31-33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120222\
Data File : VX033188.D
Acq On : 02 Dec 2022 16:11
Operator : JC/MD
Sample : N5857-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-SAMPLE-TANK-10-11-12-31-33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------