

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120222\
 Data File : VX033189.D
 Acq On : 02 Dec 2022 16:34
 Operator : JC/MD
 Sample : N5858-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-SAMPLE-TANK-26-27-28-30

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Title : SW846 8260

Signal : TIC: VX033189.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.288	26	33	42	rBV3	4112	12696	2.51%	0.411%
2	1.502	64	68	78	rVB	13672	16942	3.35%	0.548%
3	2.941	294	304	319	rBV	11340	27010	5.34%	0.874%
4	4.574	561	572	582	rBV2	4125	13711	2.71%	0.443%
5	5.385	695	705	718	rBV	56594	164858	32.61%	5.332%
6	5.550	722	732	750	rVB	120348	343039	67.85%	11.095%
7	5.958	789	799	820	rBV2	60660	161188	31.88%	5.213%
8	6.763	921	931	945	rBV	182635	432562	85.56%	13.990%
9	8.647	1234	1240	1256	rBV	262368	424600	83.98%	13.733%
10	10.055	1465	1471	1482	rBV	377974	505579	100.00%	16.352%
11	11.079	1634	1639	1650	rBV	232130	303062	59.94%	9.802%
12	12.024	1788	1794	1802	rBV	374149	470299	93.02%	15.211%
13	13.341	2006	2010	2019	rVB	8866	10665	2.11%	0.345%
14	13.548	2038	2044	2049	rVB	4868	6065	1.20%	0.196%
15	14.176	2143	2147	2152	rVV	21397	26278	5.20%	0.850%
16	14.262	2156	2161	2168	rVV	22225	29227	5.78%	0.945%
17	14.323	2168	2171	2176	rVV3	9341	14134	2.80%	0.457%
18	14.371	2176	2179	2189	rVB2	6528	9750	1.93%	0.315%
19	14.475	2191	2196	2202	rBV	6134	8584	1.70%	0.278%
20	14.902	2263	2266	2270	rVB3	6250	8040	1.59%	0.260%
21	14.987	2275	2280	2288	rVB2	14458	20588	4.07%	0.666%
22	15.103	2295	2299	2302	rBV2	7707	9667	1.91%	0.313%
23	15.146	2302	2306	2310	rBV	20494	26575	5.26%	0.860%
24	15.310	2322	2333	2336	rBV2	9619	17322	3.43%	0.560%
25	15.396	2343	2347	2357	rVB4	6161	11608	2.30%	0.375%
26	15.987	2438	2444	2454	rVB6	1887	5267	1.04%	0.170%
27	16.176	2471	2475	2481	rVB5	2767	5062	1.00%	0.164%
28	16.255	2481	2488	2493	rBV2	3534	7511	1.49%	0.243%




Sum of corrected areas: 3091889

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120222\
Data File : VX033189.D
Acq On : 02 Dec 2022 16:34
Operator : JC/MD
Sample : N5858-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-SAMPLE-TANK-26-27-28-30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

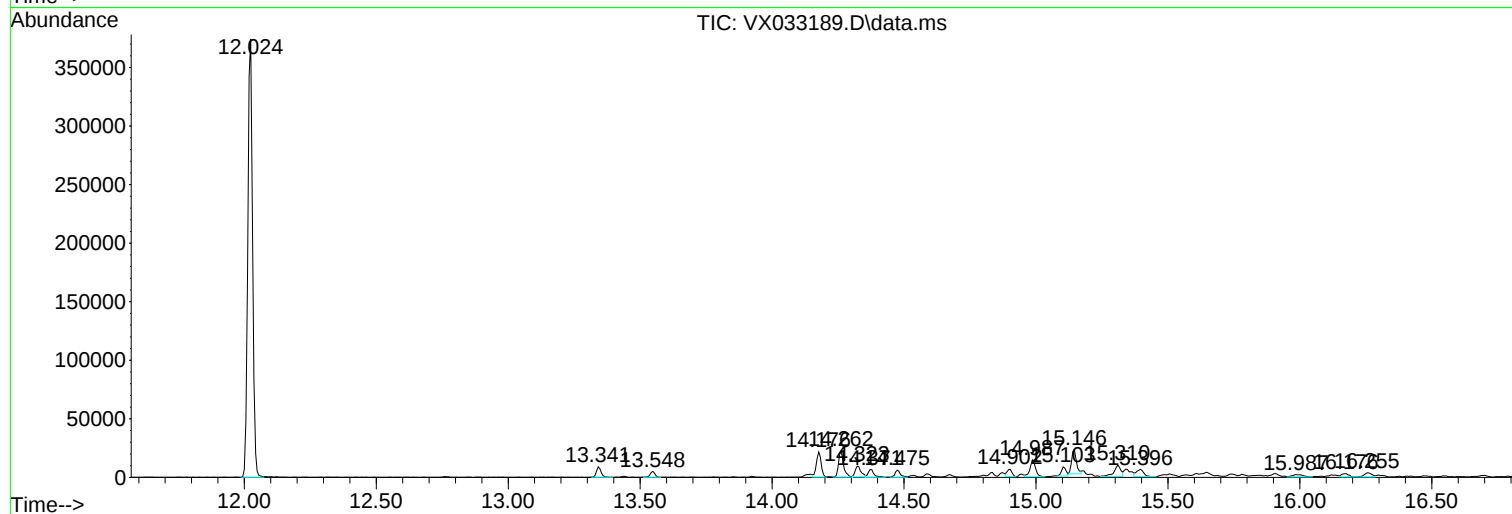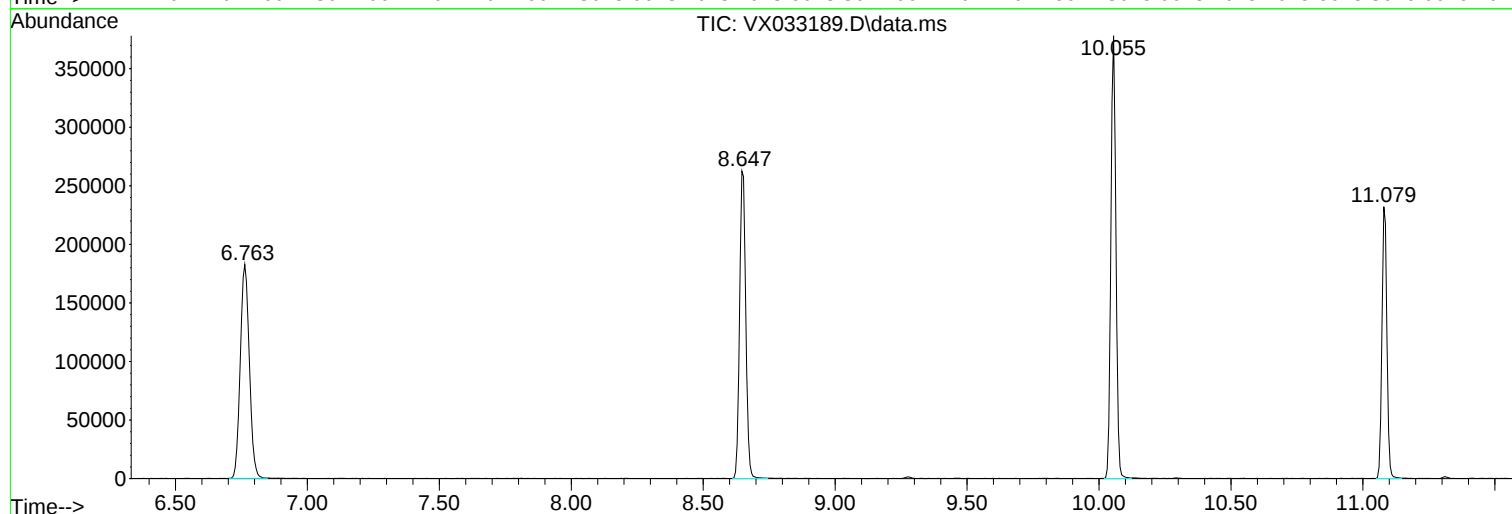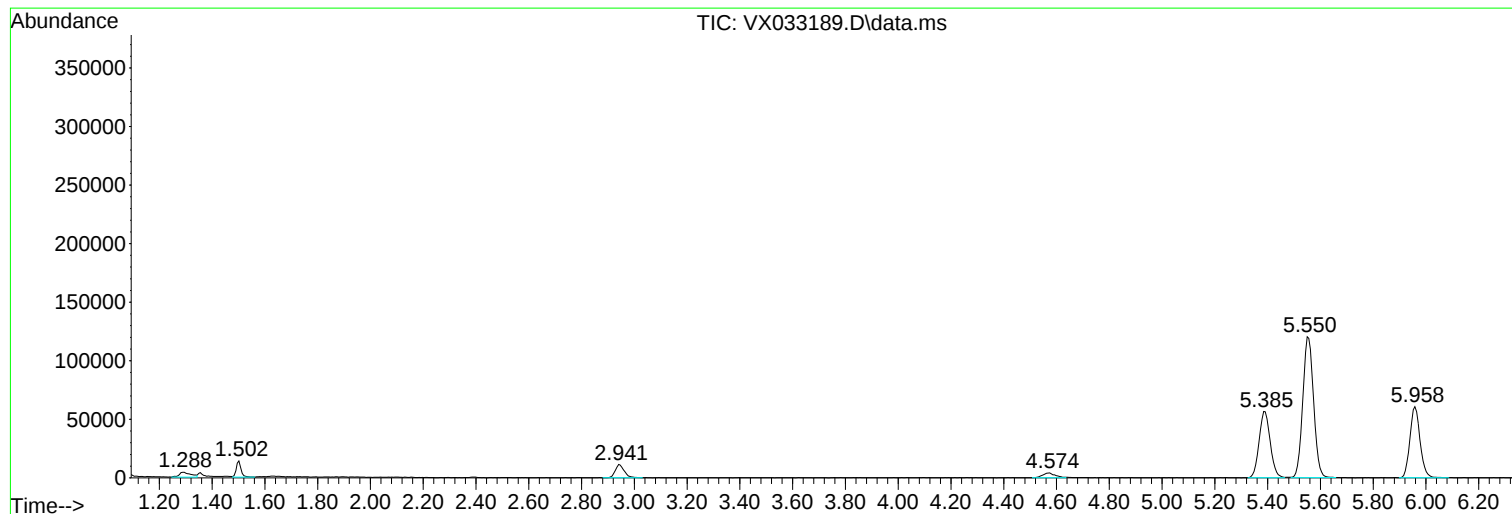

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120222\
Data File : VX033189.D
Acq On : 02 Dec 2022 16:34
Operator : JC/MD
Sample : N5858-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-SAMPLE-TANK-26-27-28-30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120222\
Data File : VX033189.D
Acq On : 02 Dec 2022 16:34
Operator : JC/MD
Sample : N5858-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-SAMPLE-TANK-26-27-28-30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc