

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120222\
 Data File : VX033191.D
 Acq On : 02 Dec 2022 17:21
 Operator : JC/MD
 Sample : N5847-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 B-40-GW-01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Title : SW846 8260

Signal : TIC: VX033191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	14	rVB2	5607	6582	1.31%	0.234%
2	1.355	42	44	54	rVB3	4654	6697	1.33%	0.238%
3	2.386	206	213	223	rBV	4510	9603	1.91%	0.342%
4	5.385	694	705	721	rBV	55686	163445	32.52%	5.816%
5	5.556	722	733	749	rVB	118881	335713	66.80%	11.945%
6	5.958	787	799	818	rBV	60494	162019	32.24%	5.765%
7	6.763	921	931	947	rBV	181812	433330	86.22%	15.419%
8	8.653	1234	1241	1250	rBV	264717	424135	84.39%	15.092%
9	10.055	1465	1471	1482	rBV	376524	502564	100.00%	17.882%
10	11.079	1634	1639	1649	rBV	231912	297129	59.12%	10.572%
11	12.024	1788	1794	1802	rBV	363086	462828	92.09%	16.468%
12	12.219	1822	1826	1835	rVB3	3592	6355	1.26%	0.226%




Sum of corrected areas: 2810400

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120222\
Data File : VX033191.D
Acq On : 02 Dec 2022 17:21
Operator : JC/MD
Sample : N5847-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
B-40-GW-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

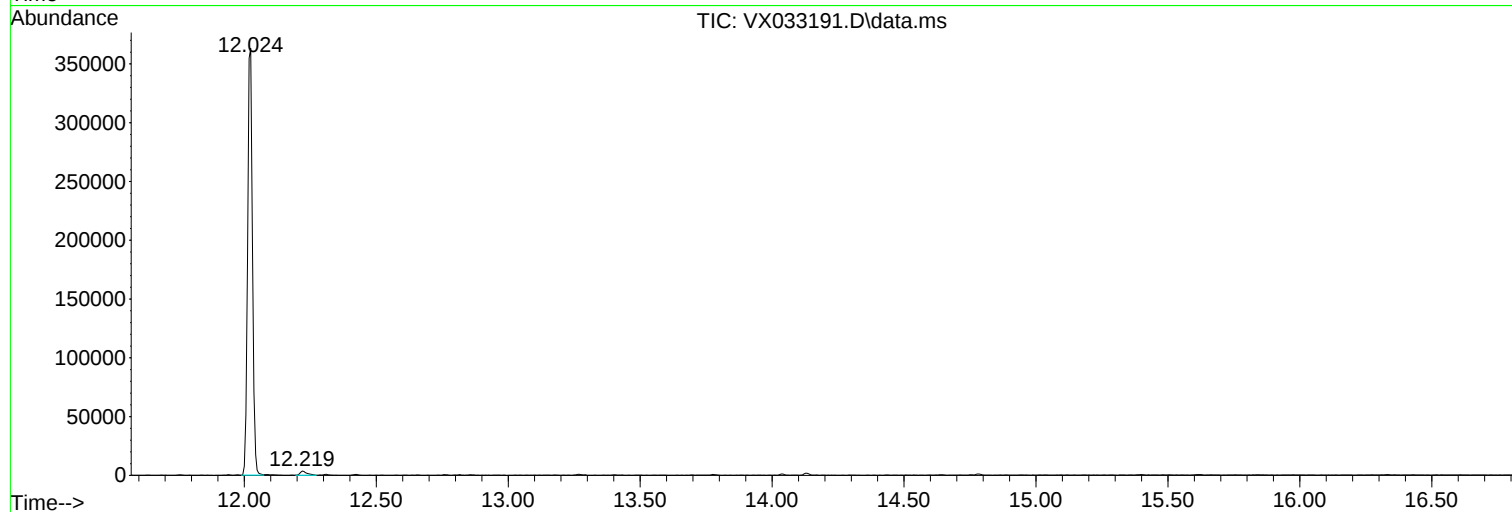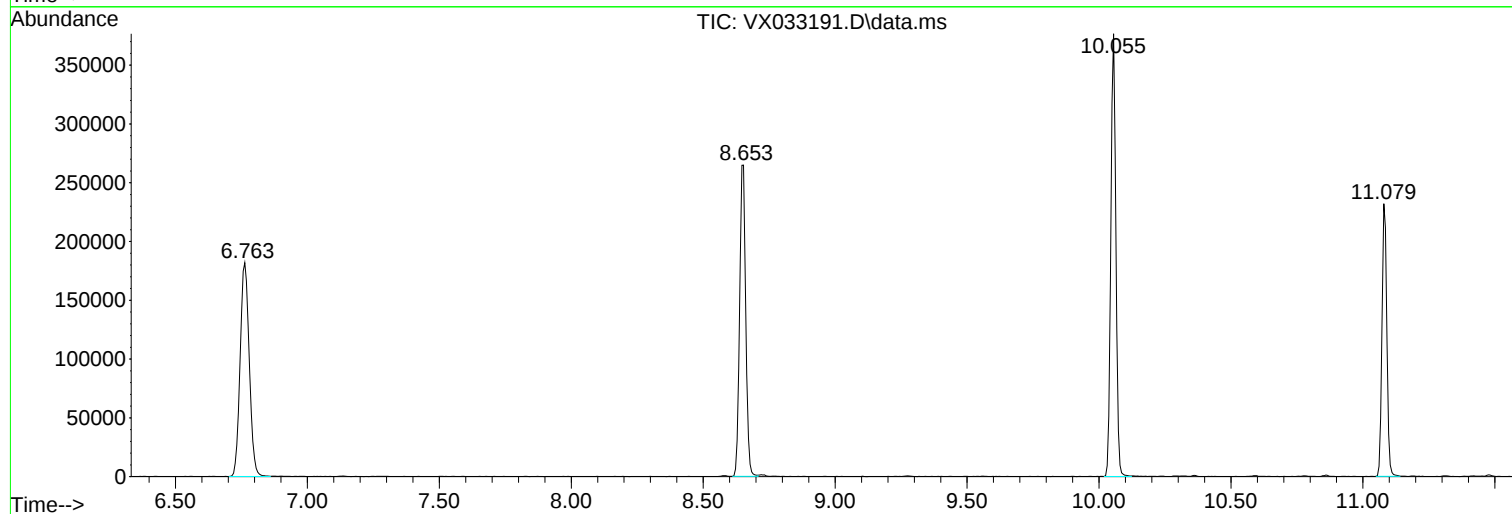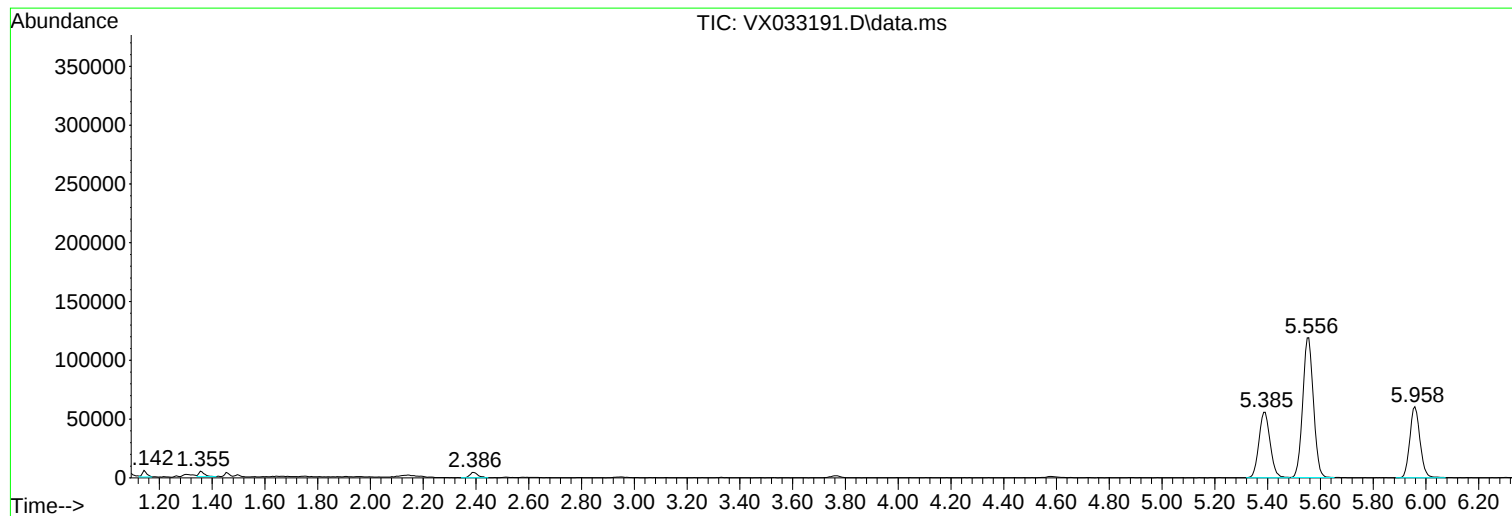

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120222\
Data File : VX033191.D
Acq On : 02 Dec 2022 17:21
Operator : JC/MD
Sample : N5847-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
B-40-GW-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120222\
Data File : VX033191.D
Acq On : 02 Dec 2022 17:21
Operator : JC/MD
Sample : N5847-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
B-40-GW-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------