

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX120318\
 Data File : VX006244.D
 Acq On : 03 Dec 2018 11:11
 Operator : JC/MD
 Sample : VX1203MBL01
 Misc : 5.00g/10mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1203MBL01

Quant Time: Dec 04 05:09:28 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 30 03:55:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	972879	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	1439313	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	1314427	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	655326	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	470528	47.38	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.76%	
35) Dibromofluoromethane	5.50	113	460546	49.42	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.84%	
50) Toluene-d8	8.71	98	1681865	49.62	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.24%	
62) 4-Bromofluorobenzene	11.13	95	625812	48.99	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.98%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX120318\
Data File : VX006244.D
Acq On : 03 Dec 2018 11:11
Operator : JC/MD
Sample : VX1203MBL01
Misc : 5.00g/10mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1203MBL01

Quant Time: Dec 04 05:09:28 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 30 03:55:33 2018
Response via : Initial Calibration

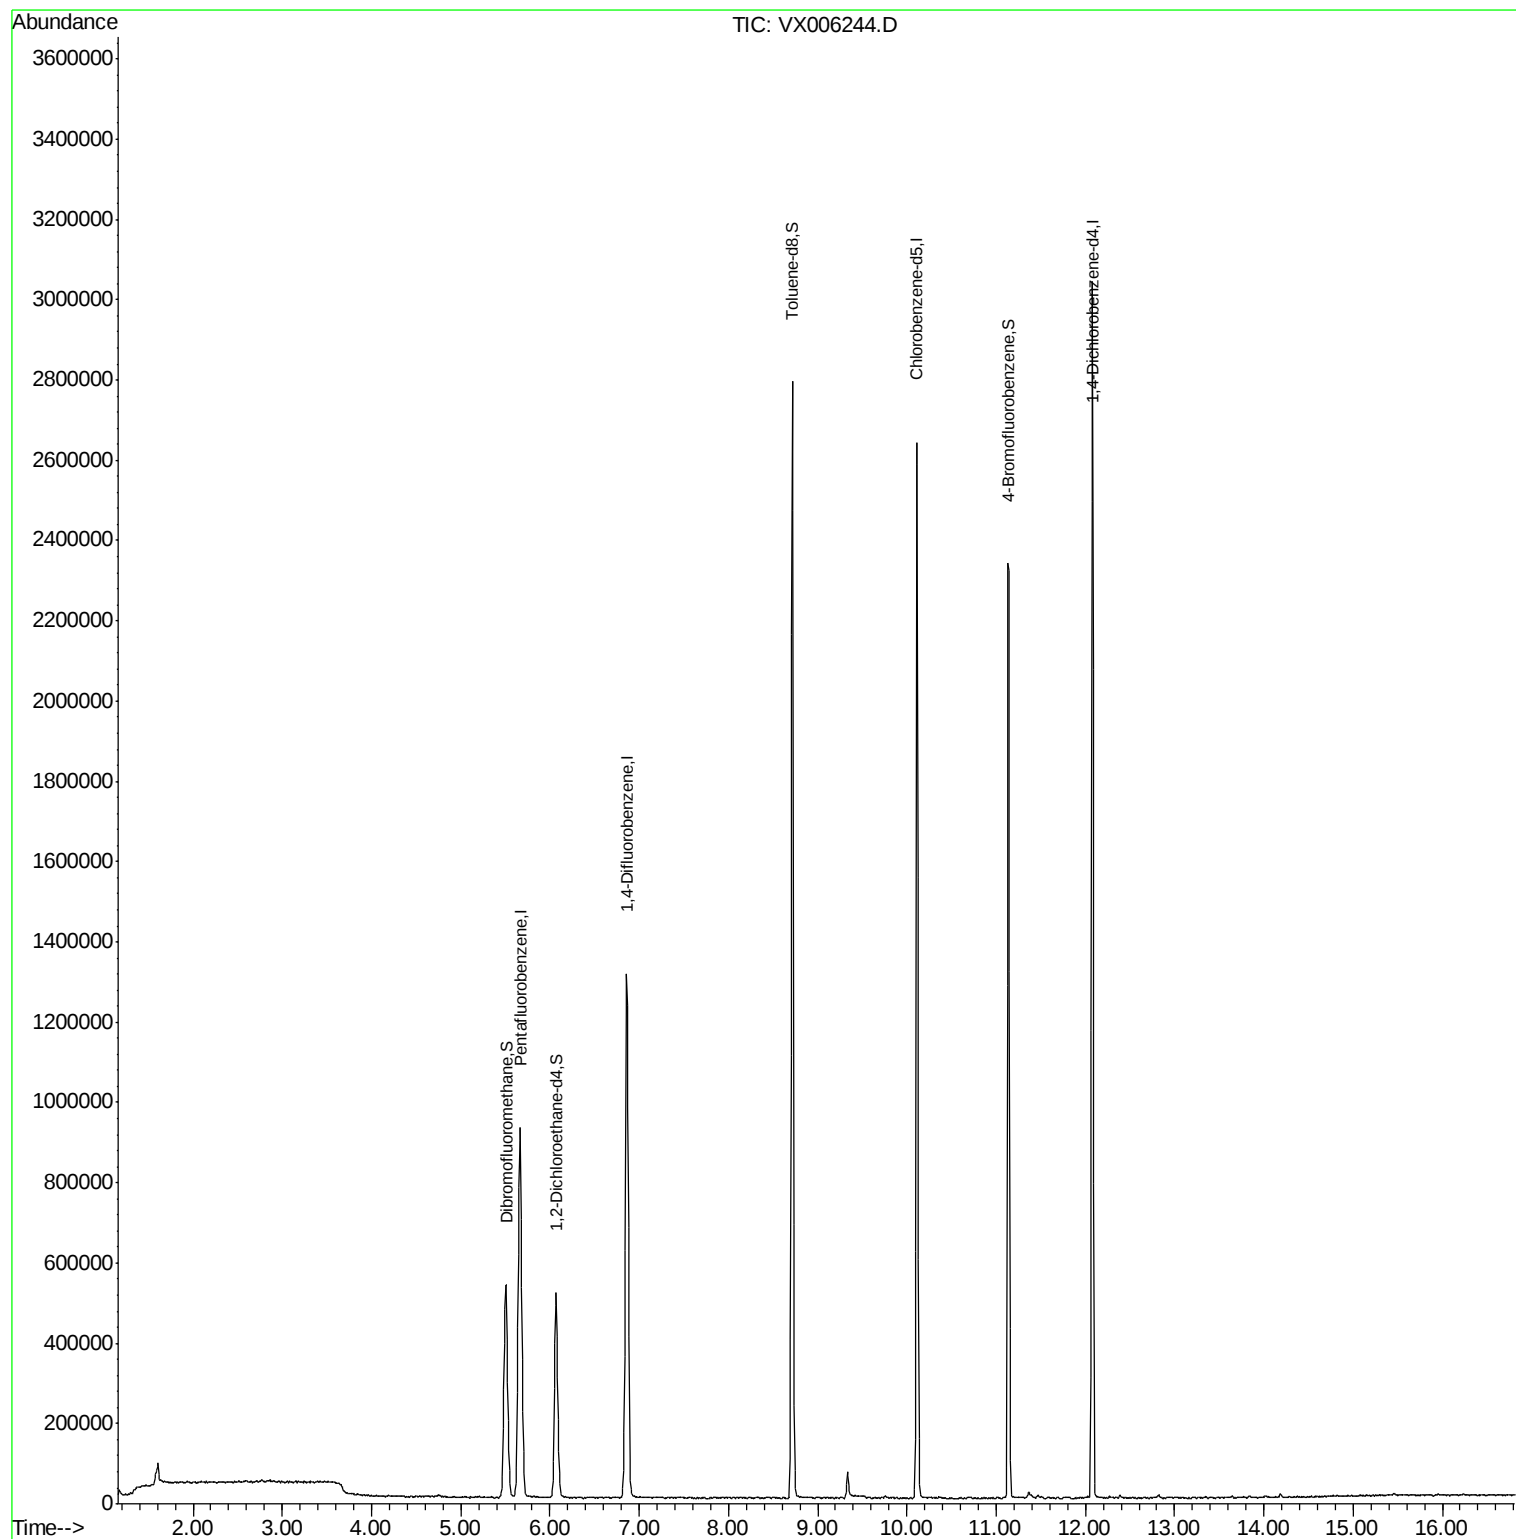



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX006244.D

Acq: 03 Dec 2018 11:11

Instrument :

MSVOA_X

ClientSampleId :


VX1203MBL01

Tgt Ion:168 Resp: 972879

Ion Ratio Lower Upper

168 100

99 49.8 37.8 56.8

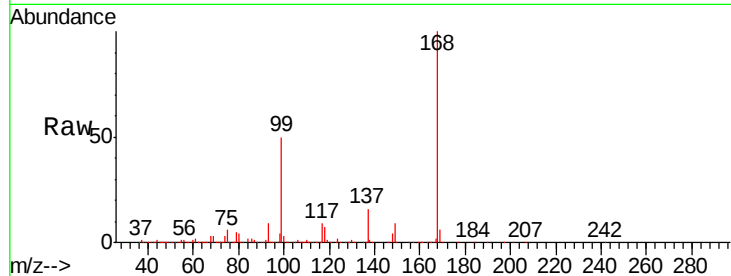

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

400000

300000



200000

100000

0

5.50 5.60 5.70 5.80

Time-->

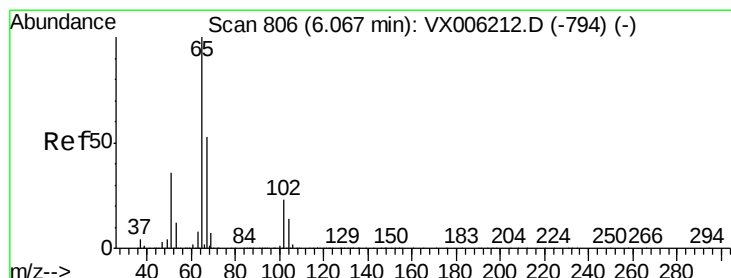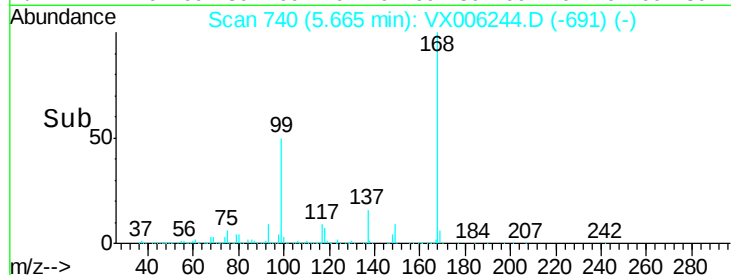

#33

1,2-Dichloroethane-d4

Concen: 47.377 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.00 min

Lab File: VX006244.D


Acq: 03 Dec 2018 11:11

Tgt Ion: 65 Resp: 470528

Ion Ratio Lower Upper

65 100

67 53.9 0.0 107.2

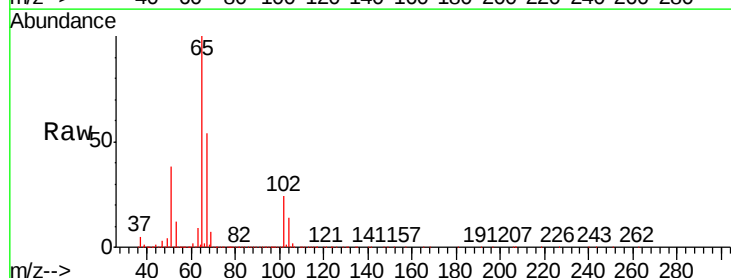

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

200000

150000


100000


50000

0

5.90 6.00 6.10 6.20

Time-->

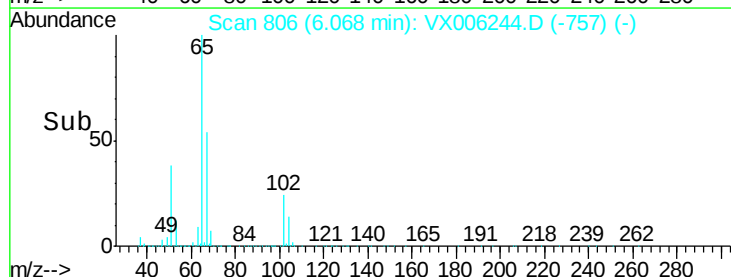

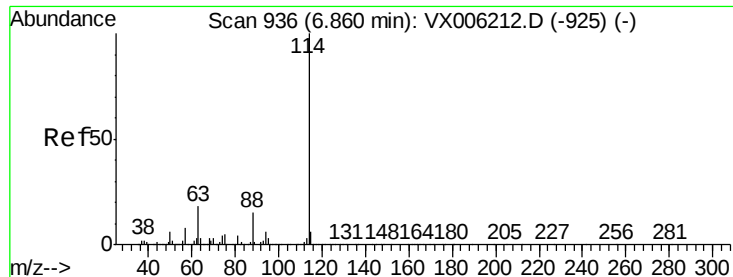

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX006244.D

Acq: 03 Dec 2018 11:11

Instrument :

MSVOA_X

ClientSampleId :

VX1203MBL01


Tgt Ion:114 Resp: 1439313

Ion Ratio Lower Upper

114 100

63 17.9 0.0 36.6




88 15.3 0.0 29.0

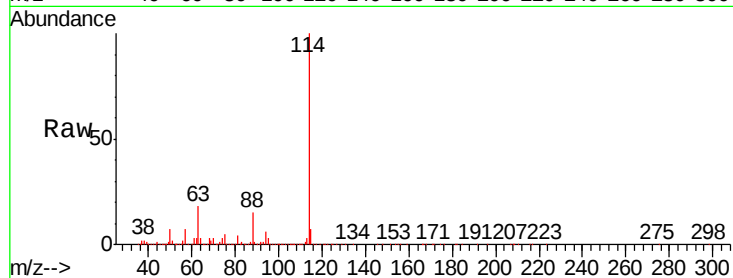

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

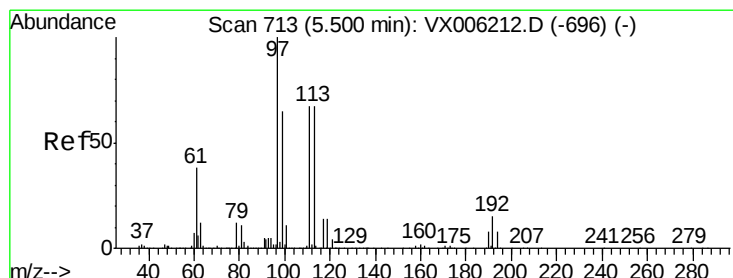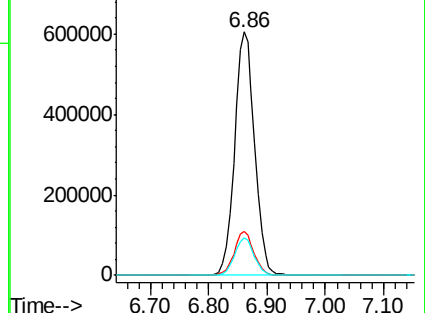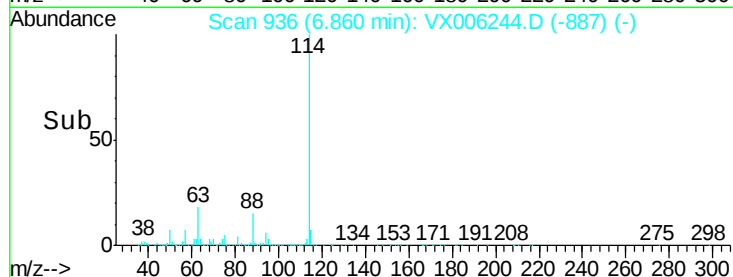

#35

Dibromofluoromethane

Concen: 49.420 ug/l

RT: 5.50 min Scan# 713

Delta R.T. 0.00 min

Lab File: VX006244.D

Acq: 03 Dec 2018 11:11


Tgt Ion:113 Resp: 460546

Ion Ratio Lower Upper

113 100

111 101.6 81.1 121.7



192 22.6 18.2 27.2

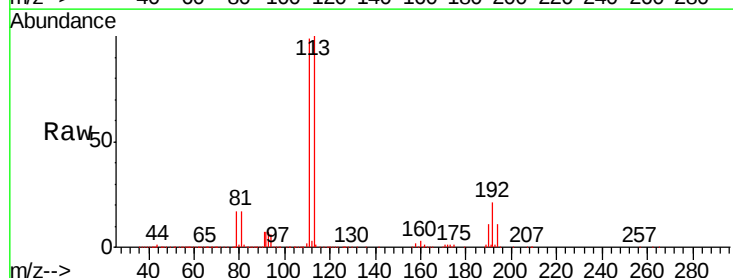

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



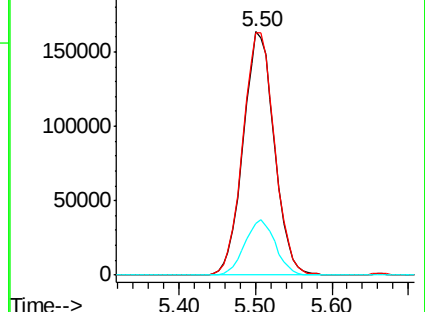
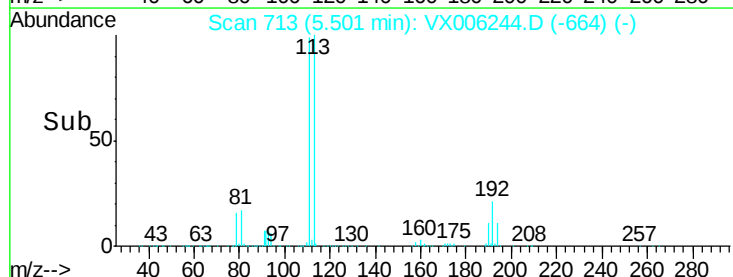




#50
Toluene-d8
Concen: 49.617 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. 0.00 min
Lab File: VX006244.D
Acq: 03 Dec 2018 11:11




Instrument :
MSVOA_X
ClientSampleId :
VX1203MBL01


Tgt Ion: 98 Resp: 1681865
Ion Ratio Lower Upper
98 100
100 64.6 52.2 78.2

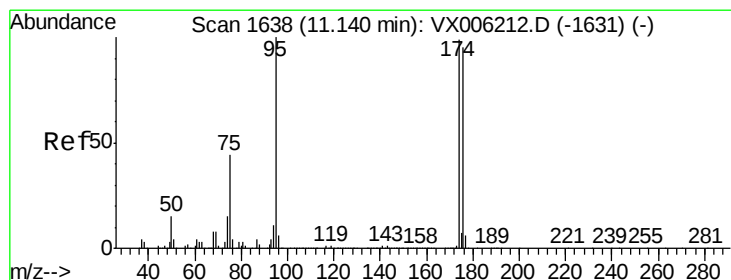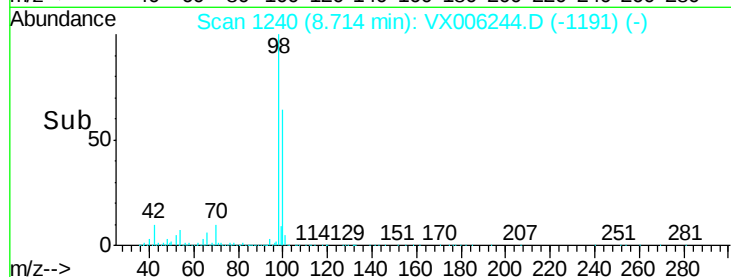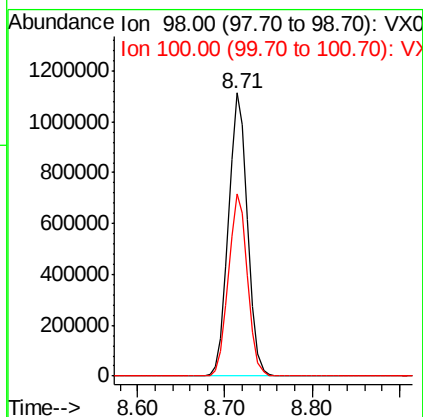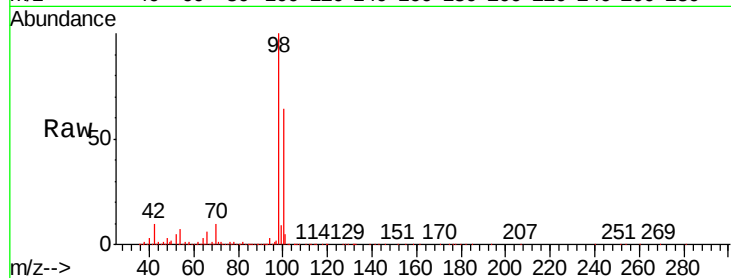

#62
4-Bromofluorobenzene
Concen: 48.993 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.01 min
Lab File: VX006244.D
Acq: 03 Dec 2018 11:11

Tgt Ion: 95 Resp: 625812
Ion Ratio Lower Upper
95 100
174 91.8 0.0 187.0
176 89.6 0.0 181.8

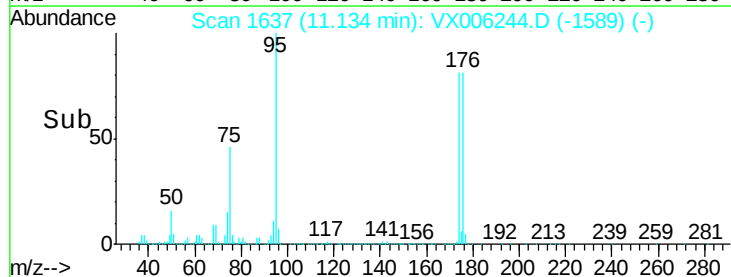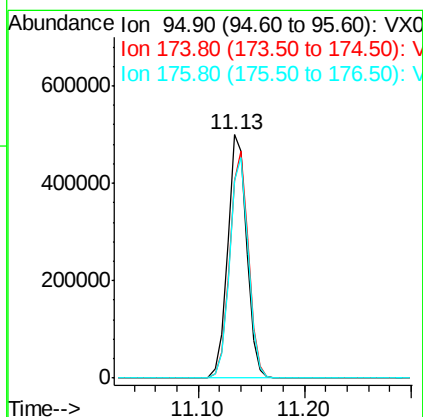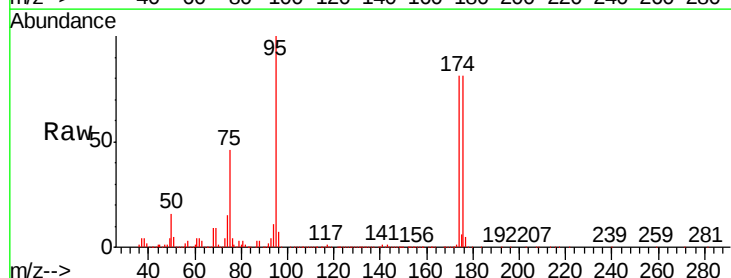

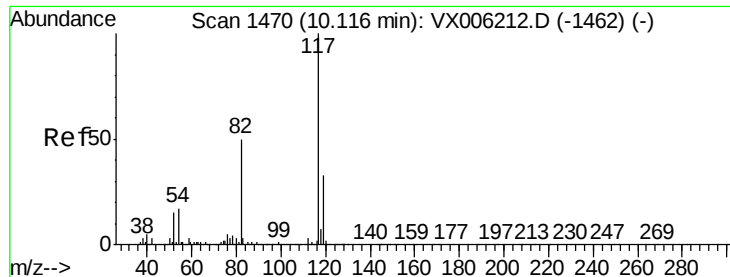

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.12 min Scan# 1470

Delta R.T. 0.00 min

Lab File: VX006244.D

Acq: 03 Dec 2018 11:11

Instrument :

MSVOA_X

ClientSampleId :

VX1203MBL01


Tgt Ion:117 Resp: 1314427

Ion Ratio Lower Upper

117 100

82 49.8 39.6 59.4




119 32.5 26.3 39.5

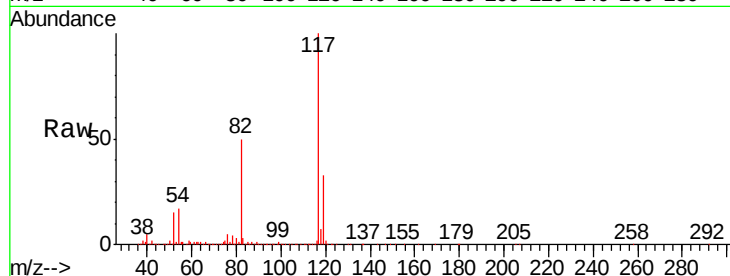

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

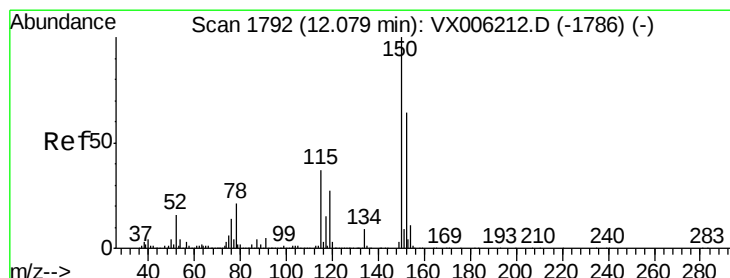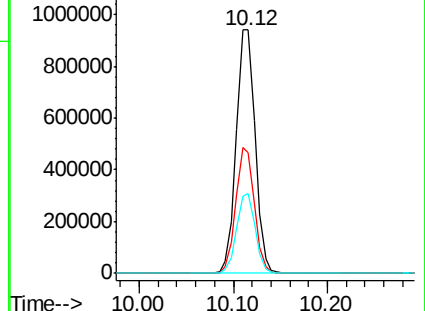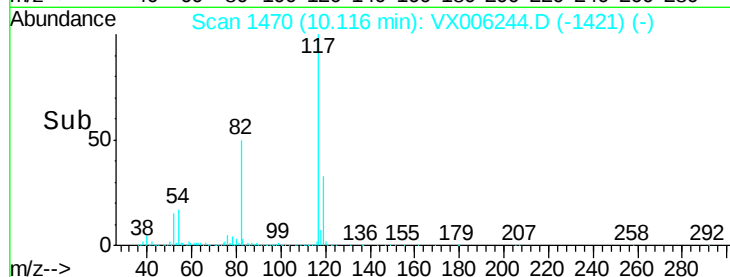

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX006244.D

Acq: 03 Dec 2018 11:11


Tgt Ion:152 Resp: 655326

Ion Ratio Lower Upper

152 100

115 55.4 39.0 116.9

150 157.0 0.0 345.8

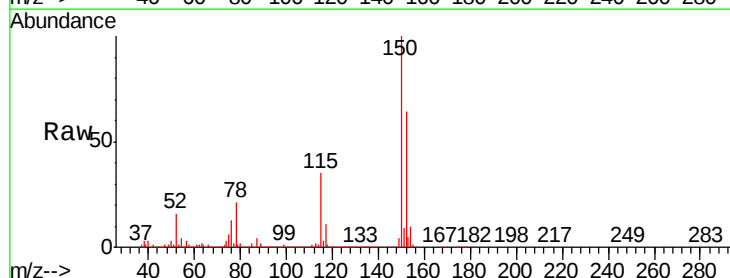

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

