


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX120318\  
Data File : VX006241.D  
Acq On : 03 Dec 2018 09:40  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X112918W.M  
Title : SW846 8260  
Last Update : Fri Nov 30 03:55:33 2018

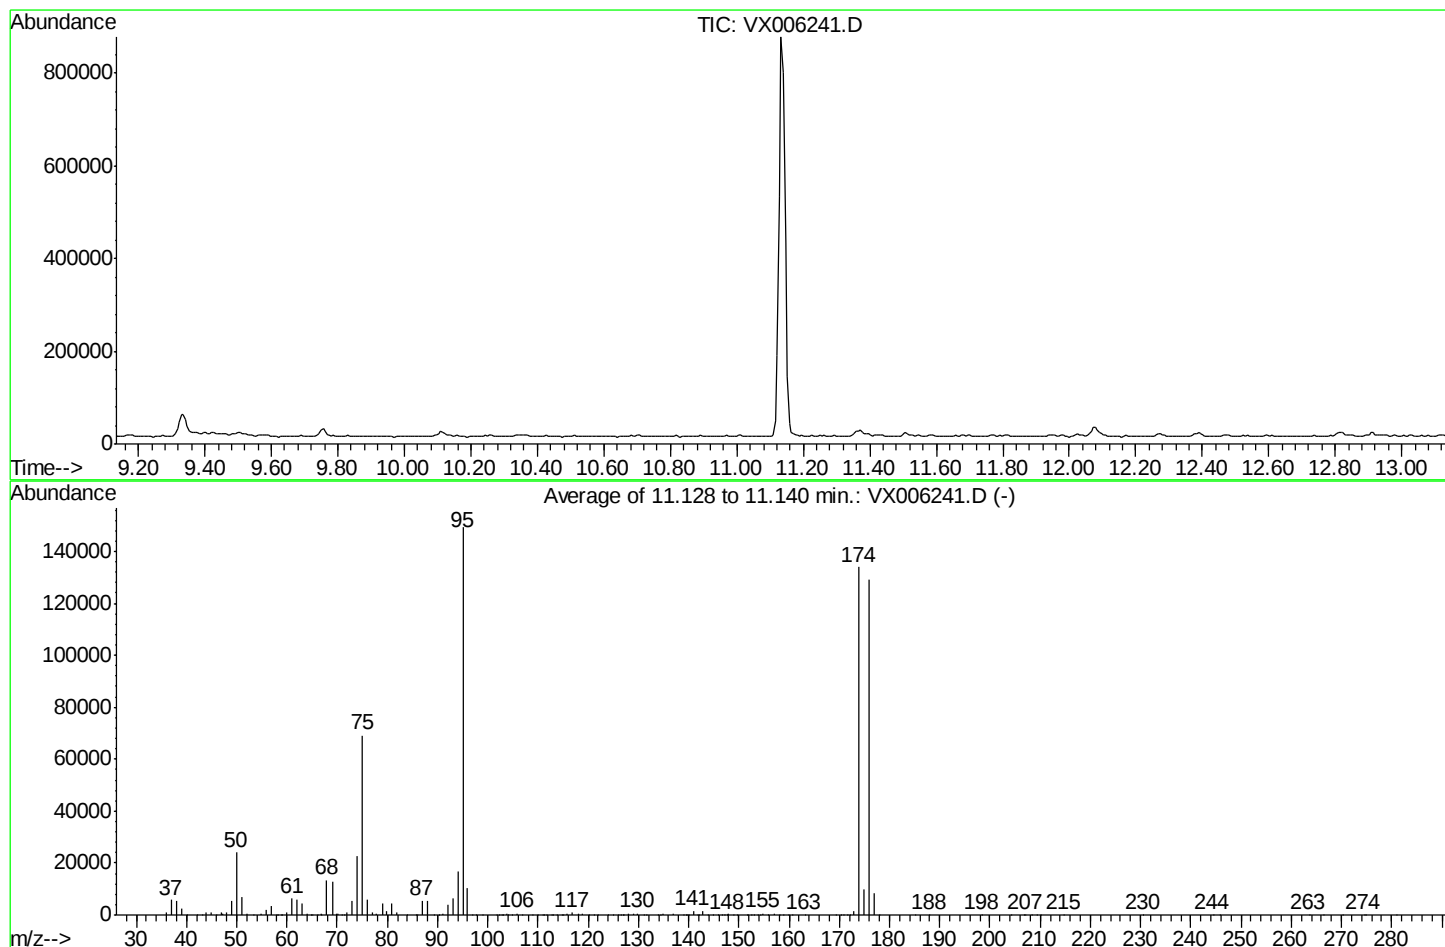

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1628

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.1      | 24086   | PASS             |
| 75          | 95           | 30           | 60           | 46.3      | 69162   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 149283  | PASS             |
| 96          | 95           | 5            | 9            | 6.9       | 10354   | PASS             |
| 173         | 174          | 0.00         | 2            | 1.1       | 1513    | PASS             |
| 174         | 95           | 50           | 100          | 89.7      | 133965  | PASS             |
| 175         | 174          | 5            | 9            | 7.4       | 9879    | PASS             |
| 176         | 174          | 95           | 101          | 96.3      | 129021  | PASS             |
| 177         | 176          | 5            | 9            | 6.4       | 8276    | PASS             |