


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX120319\
Data File : VX013715.D
Acq On : 03 Dec 2019 10:24
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
Title : SW846 8260
Last Update : Tue Nov 26 15:53:00 2019

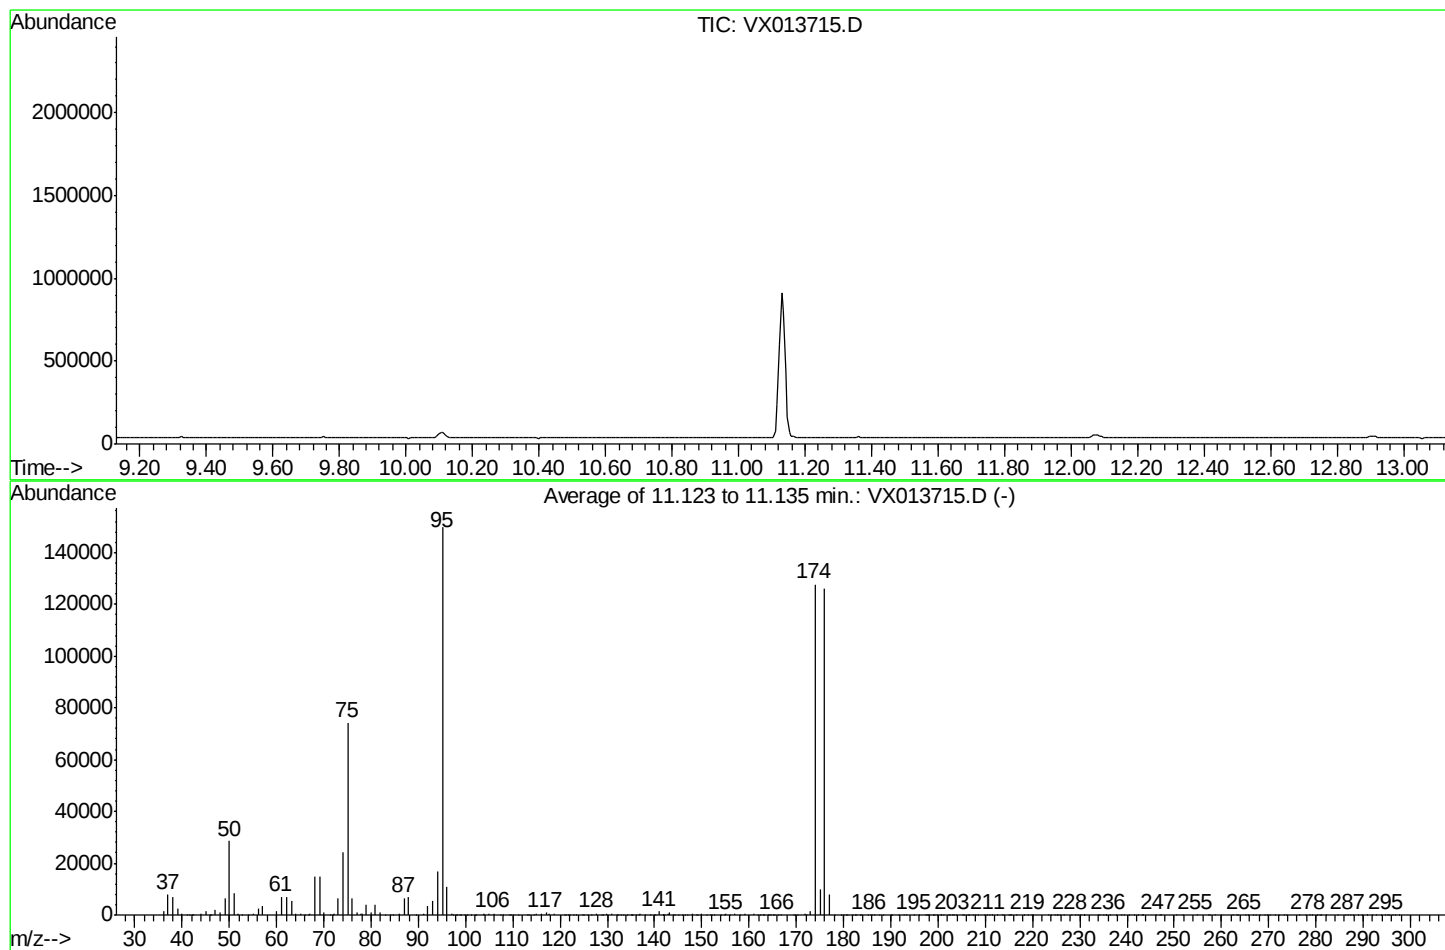

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	28627	PASS
75	95	30	60	49.6	74237	PASS
95	95	100	100	100.0	149733	PASS
96	95	5	9	7.2	10829	PASS
173	174	0.00	2	1.3	1636	PASS
174	95	50	100	85.2	127585	PASS
175	174	5	9	7.9	10119	PASS
176	174	95	101	98.9	126213	PASS
177	176	5	9	6.2	7778	PASS