

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120321\
 Data File : VX025483.D
 Acq On : 03 Dec 2021 15:32
 Operator : JC/MD
 Sample : M4918-05DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP120221DL

Quant Time: Dec 04 06:50:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 17 15:36:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	105699	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	179175	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	162329	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	73446	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	62588	56.176	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 112.360%			
35) Dibromofluoromethane	5.391	113	55227	50.236	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 100.480%			
50) Toluene-d8	8.653	98	208188	50.367	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 100.740%			
62) 4-Bromofluorobenzene	11.085	95	73819	47.207	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 94.420%			
Target Compounds						Qvalue
5) Bromomethane	1.624	94	148	0.276	ug/l #	49
6) Chloroethane	1.593	64	3521	4.097	ug/l #	43
11) Tert butyl alcohol	2.953	59	2289	Below Cal	#	78
13) Acrolein	2.221	56	198	3.879	ug/l #	1
16) Acetone	2.380	43	496	0.801	ug/l	93
18) Methyl Acetate	2.782	43	872	0.441	ug/l #	52
19) Methyl tert-butyl Ether	3.123	73	1671	0.490	ug/l #	46
20) Methylene Chloride	2.794	84	285	0.245	ug/l #	69
25) 2-Butanone	4.294	43	180	0.201	ug/l #	48
31) Cyclohexane	5.483	56	1079	0.627	ug/l #	86
36) 1,1-Dichloropropene	5.550	75	7274	4.653	ug/l #	49
38) Carbon Tetrachloride	5.556	117	9841	5.716	ug/l #	16
39) Methylcyclohexane	7.379	83	903	0.450	ug/l #	80
40) Benzene	6.044	78	51414	10.857	ug/l	98
42) 1,2-Dichloroethane	6.044	62	364	0.236	ug/l #	77
52) Toluene	8.720	92	86277	27.906	ug/l	97
53) t-1,3-Dichloropropene	8.720	75	951	0.515	ug/l #	1
67) Ethyl Benzene	10.195	91	128629	22.501	ug/l	98
68) m/p-Xylenes	10.305	106	142644	61.091	ug/l	94
69) o-Xylene	10.647	106	85100	37.238	ug/l	93
70) Styrene	10.647	104	4531	1.200	ug/l #	1
73) Isopropylbenzene	10.964	105	5139	0.982	ug/l	100
76) 1,2,3-Trichloropropane	11.085	75	35541	23.631	ug/l #	37
78) n-propylbenzene	11.305	91	15322	2.608	ug/l	99
79) 2-Chlorotoluene	11.378	91	7945	2.221	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.451	105	20745	4.715	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.085	75	35541	59.530	ug/l #	9
82) 4-Chlorotoluene	11.457	91	2183	0.535	ug/l #	45
83) tert-Butylbenzene	11.756	119	10661	2.384	ug/l #	61
84) 1,2,4-Trimethylbenzene	11.756	105	87662	20.158	ug/l	96
85) sec-Butylbenzene	11.756	105	87662	16.126	ug/l #	56
89) n-Butylbenzene	12.317	91	1327	0.337	ug/l #	17
90) Hexachloroethane	12.646	117	1022	1.187	ug/l #	11
95) Naphthalene	13.780	128	38570	7.464	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120321\
Data File : VX025483.D
Acq On : 03 Dec 2021 15:32
Operator : JC/MD
Sample : M4918-05DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL

Quant Time: Dec 04 06:50:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 17 15:36:16 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120321\
Data File : VX025483.D
Acq On : 03 Dec 2021 15:32
Operator : JC/MD
Sample : M4918-05DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL

Quant Time: Dec 04 06:50:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 17 15:36:16 2021
Response via : Initial Calibration




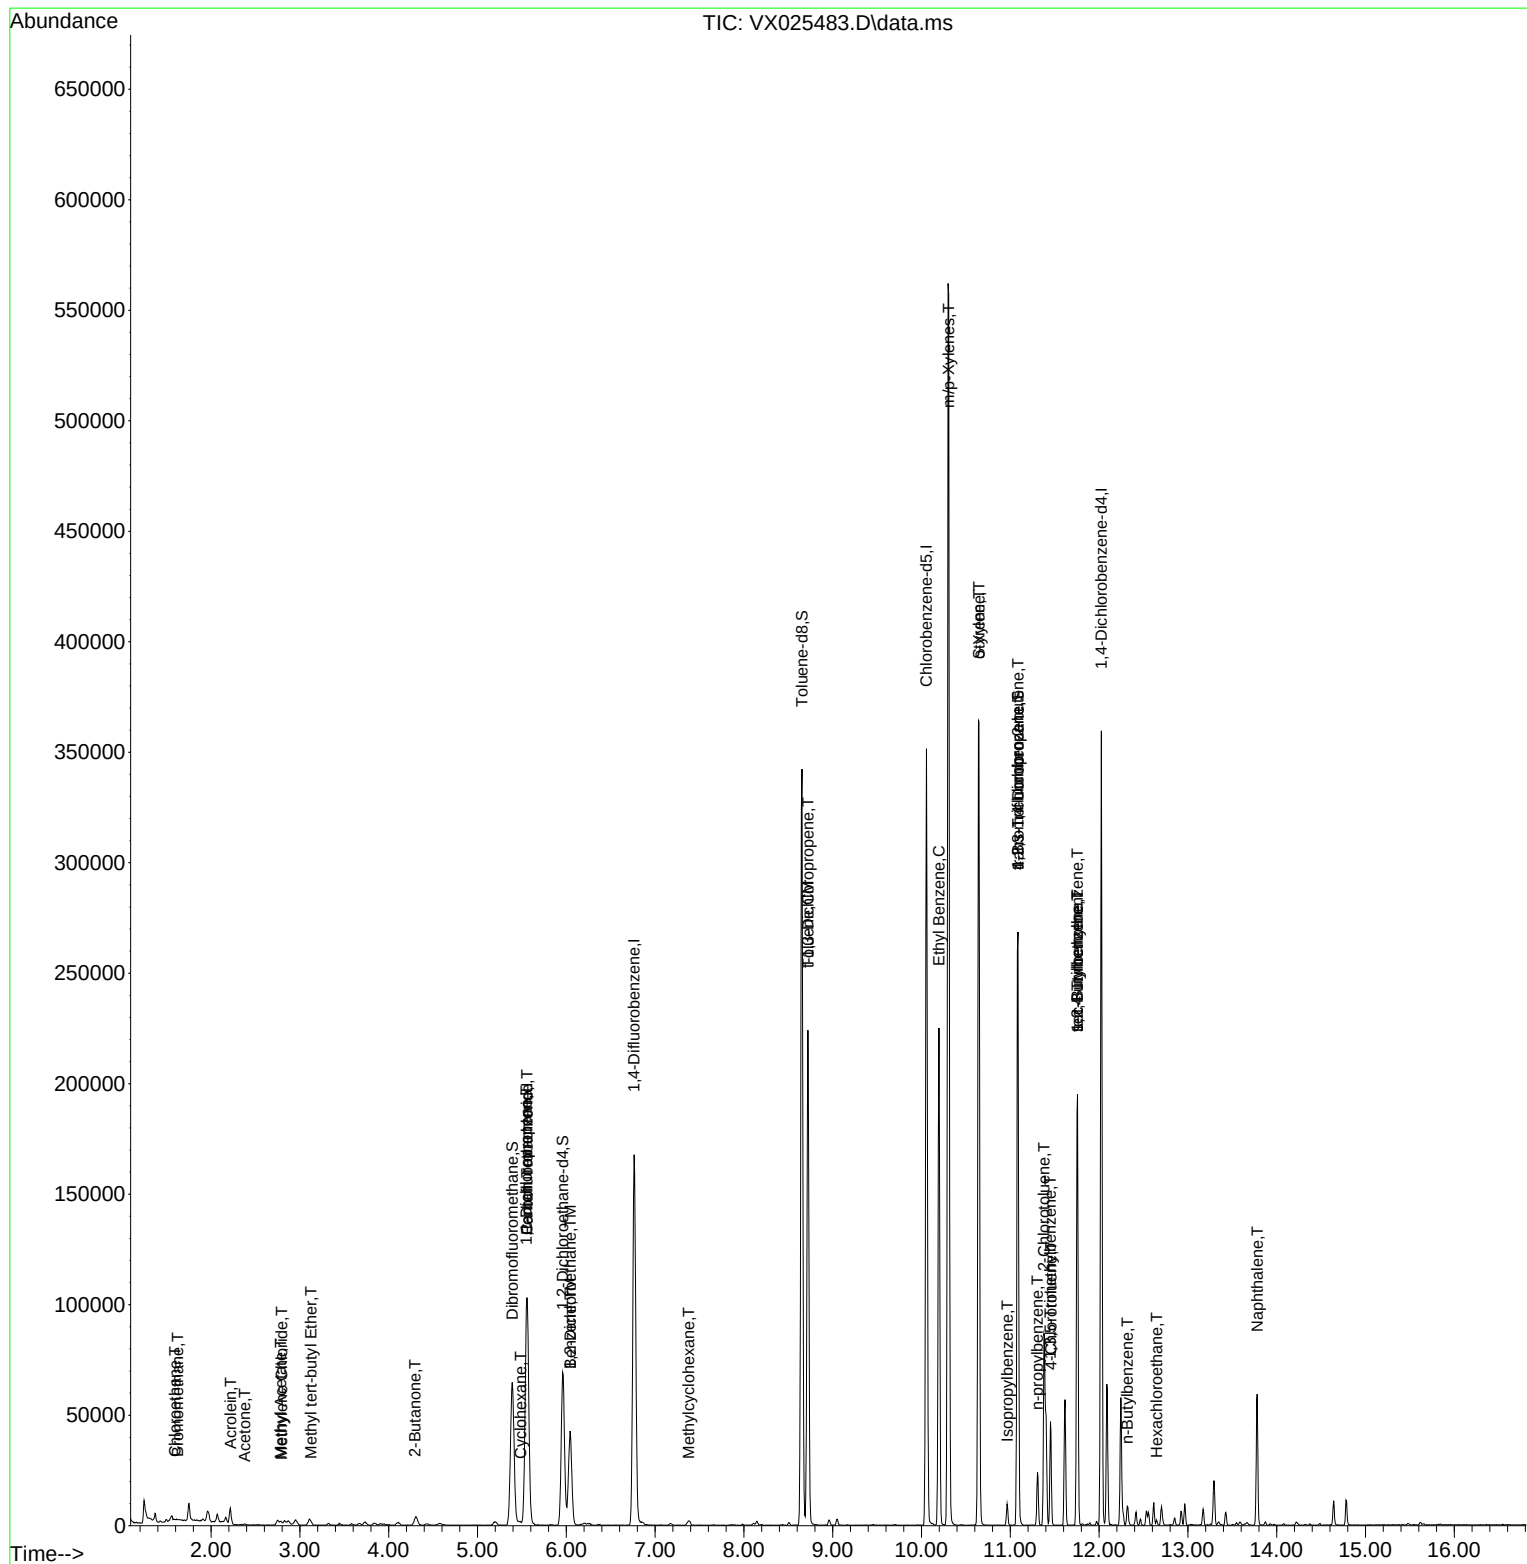




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32




Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL


Tgt Ion:168 Resp: 105699
Ion Ratio Lower Upper
168 100
99 52.1 46.4 69.6

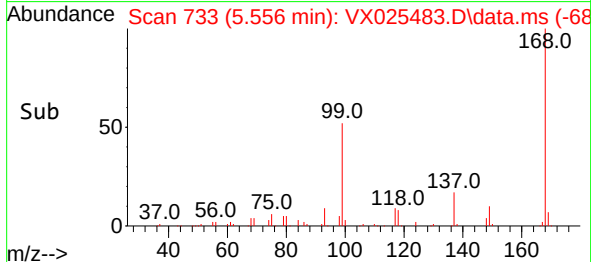

#5
Bromomethane
Concen: 0.276 ug/l
RT: 1.624 min Scan# 88
Delta R.T. 0.025 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Tgt Ion: 94 Resp: 148
Ion Ratio Lower Upper
94 100
96 44.3 74.8 112.2#




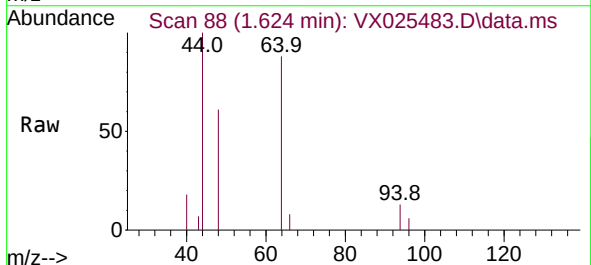


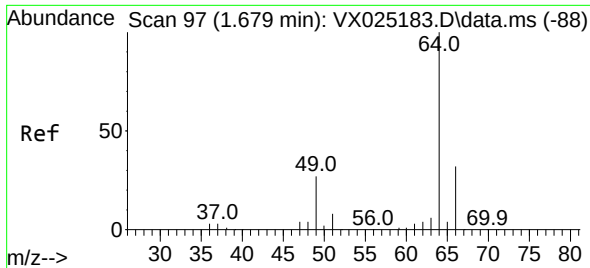

#6
Chloroethane
Concen: 4.097 ug/l
RT: 1.593 min Scan# 81
Delta R.T. -0.086 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32




Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL


Tgt Ion: 64 Resp: 3521
Ion Ratio Lower Upper
64 100
66 0.0 25.6 38.4#

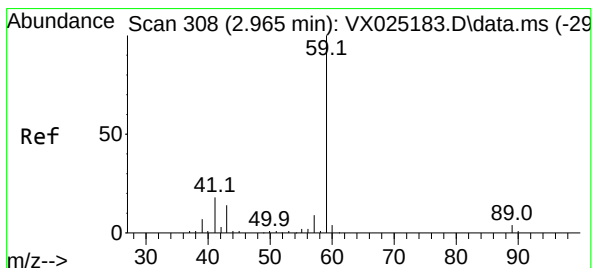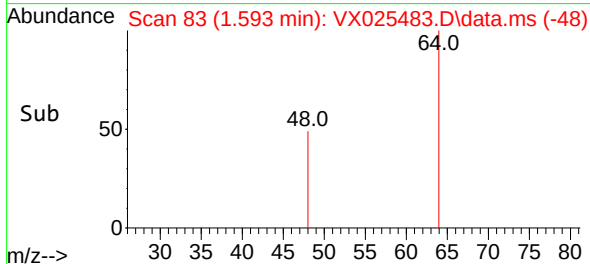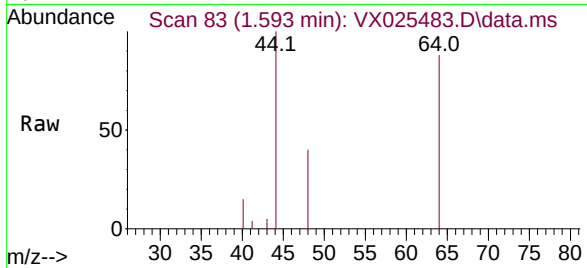

#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.953 min Scan# 306
Delta R.T. -0.012 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Tgt Ion: 59 Resp: 2289
Ion Ratio Lower Upper
59 100
57 2.2 8.5 12.7#


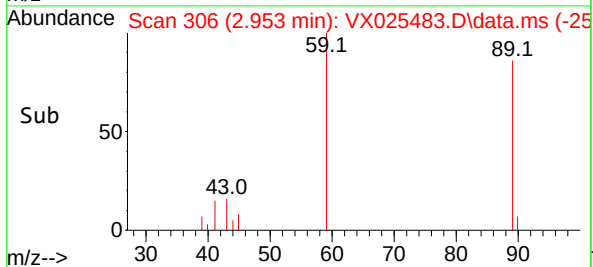

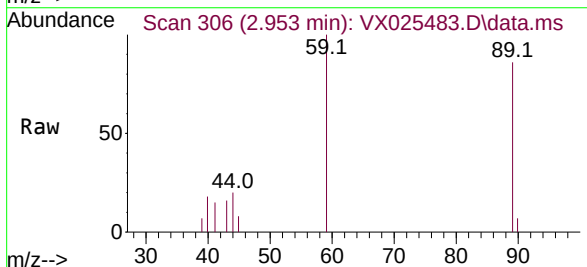


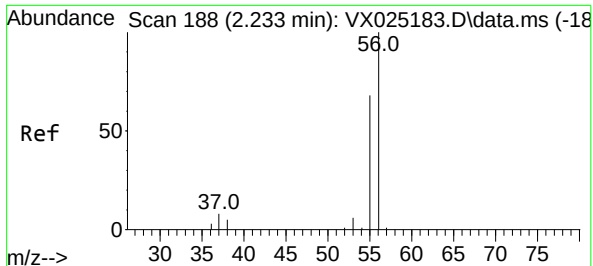

#13
Acrolein
Concen: 3.879 ug/l
RT: 2.221 min Scan# 188
Delta R.T. -0.012 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32




Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL


Tgt Ion: 56 Resp: 198
Ion Ratio Lower Upper
56 100
55 1723.2 58.6 87.8#

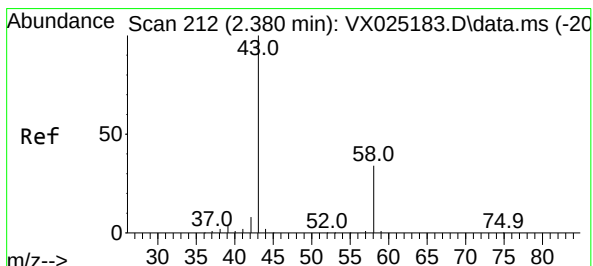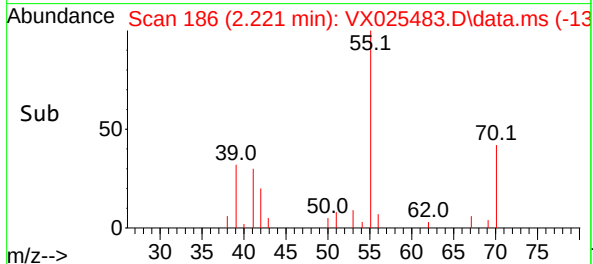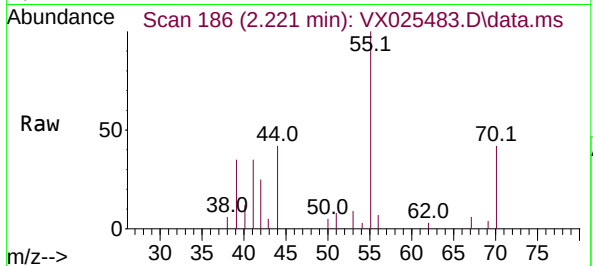

#16
Acetone
Concen: 0.801 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Tgt Ion: 43 Resp: 496
Ion Ratio Lower Upper
43 100
58 26.1 24.0 36.0

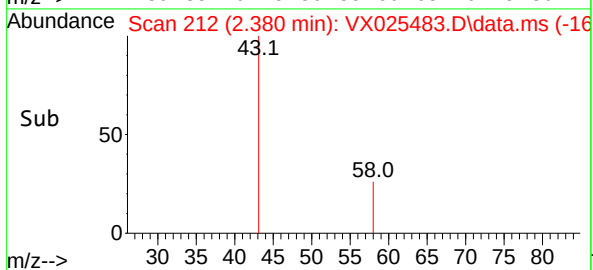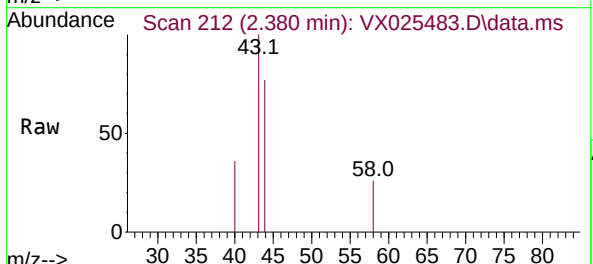



#18

Methyl Acetate

Concen: 0.441 ug/l

RT: 2.782 min Scan# 21

Delta R.T. 0.079 min

Lab File: VX025483.D

Acq: 03 Dec 2021 15:32

Instrument :

MSVOA_X

ClientSampleId :





DUP120221DL

Tgt Ion: 43 Resp: 872

Ion Ratio Lower Upper

43 100

74 0.0 19.0 28.6#

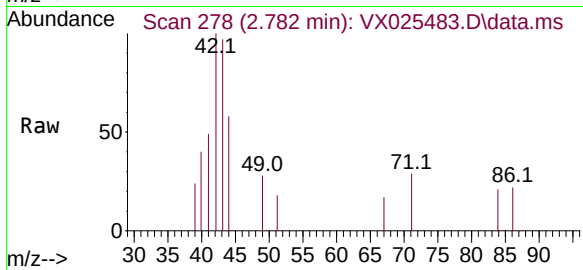

#19

Methyl tert-butyl Ether

Concen: 0.490 ug/l

RT: 3.123 min Scan# 334

Delta R.T. 0.006 min

Lab File: VX025483.D




Acq: 03 Dec 2021 15:32


Tgt Ion: 73 Resp: 1671

Ion Ratio Lower Upper

73 100

57 47.4 17.5 26.3#




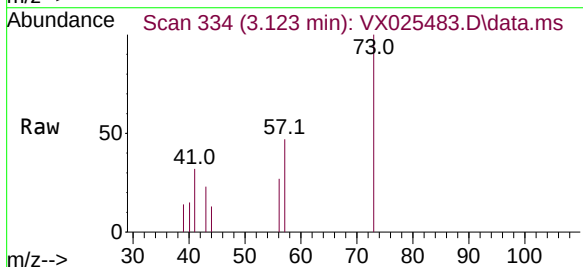




#20
Methylene Chloride
Concen: 0.245 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32




Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL


Tgt Ion:	84	Resp:	285
Ion	Ratio	Lower	Upper
84	100		
49	71.8	98.2	147.2#
51	28.7	30.2	45.4#
86	54.5	52.2	78.2

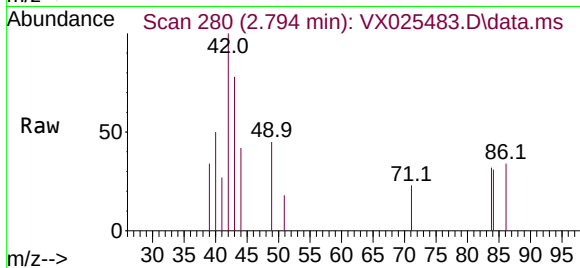

#25
2-Butanone
Concen: 0.201 ug/l
RT: 4.294 min Scan# 526
Delta R.T. -0.262 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Tgt Ion:	43	Resp:	180
Ion	Ratio	Lower	Upper
43	100		
72	0.0	21.2	31.8#




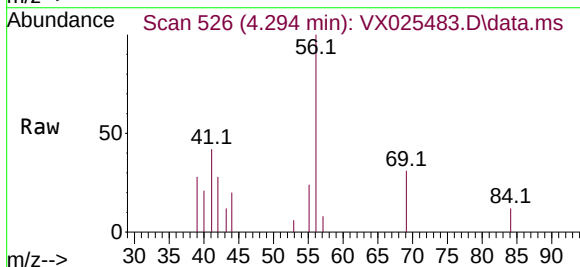


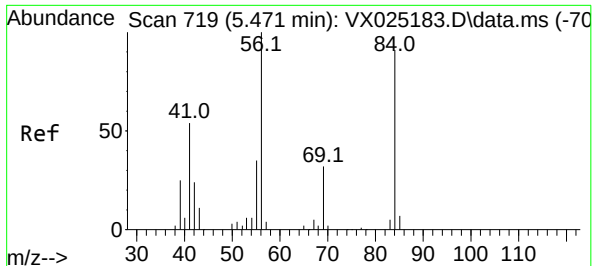

#31
Cyclohexane
Concen: 0.627 ug/l
RT: 5.483 min Scan# 719
Delta R.T. 0.012 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32




Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL


Tgt Ion: 56 Resp: 1079
Ion Ratio Lower Upper
56 100
69 22.9 24.2 36.2#
84 75.9 71.5 107.3

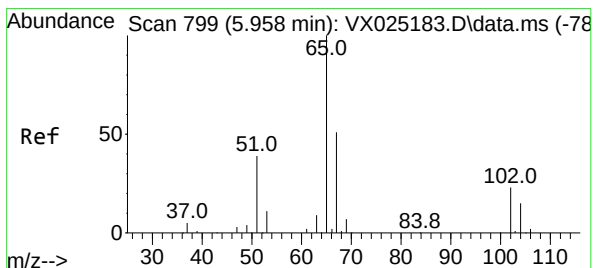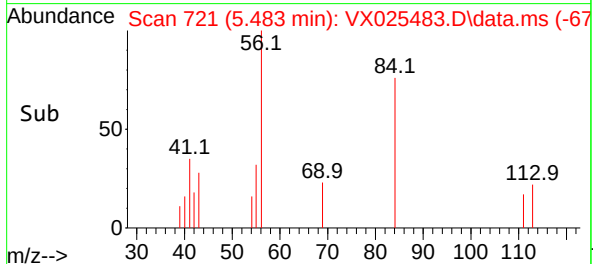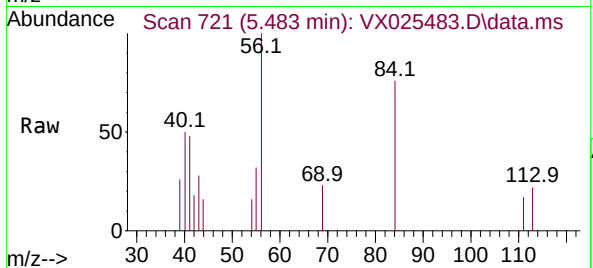

#33
1,2-Dichloroethane-d4
Concen: 56.176 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Tgt Ion: 65 Resp: 62588
Ion Ratio Lower Upper
65 100
67 52.3 0.0 101.0


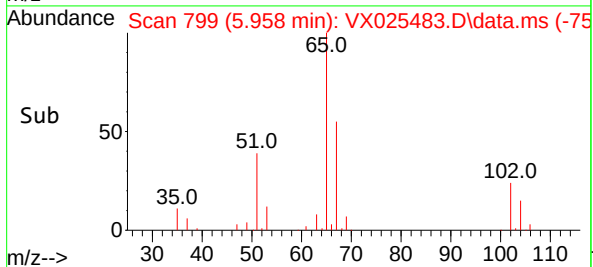

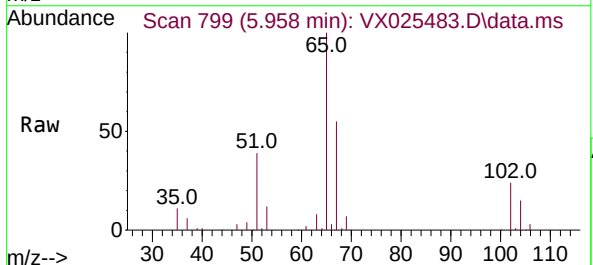


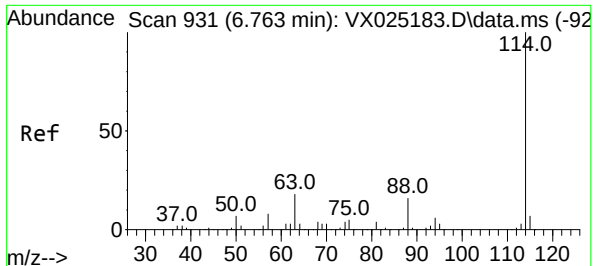

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32




Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL


Tgt Ion:114 Resp: 179175
Ion Ratio Lower Upper
114 100
63 19.5 0.0 41.0
88 15.3 0.0 34.8

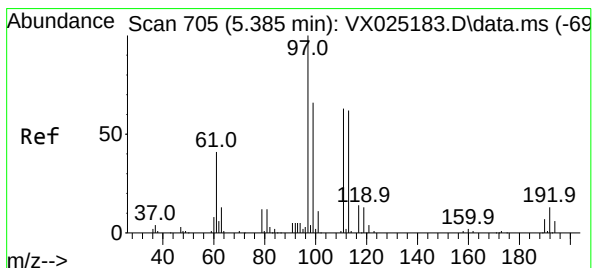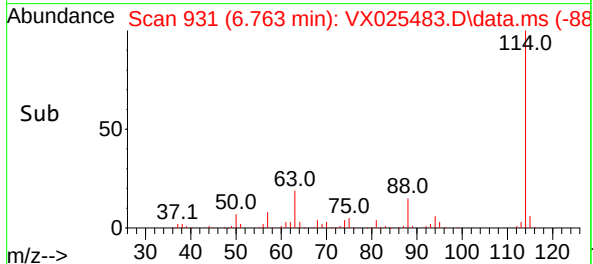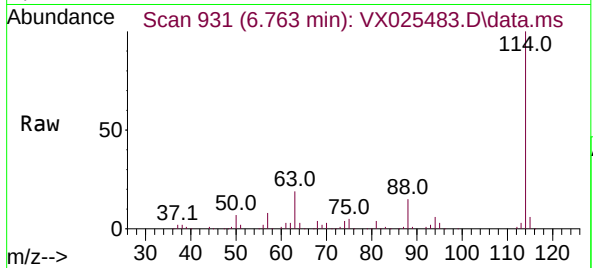

#35
Dibromofluoromethane
Concen: 50.236 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Tgt Ion:113 Resp: 55227
Ion Ratio Lower Upper
113 100
111 102.7 82.1 123.1
192 20.7 15.6 23.4


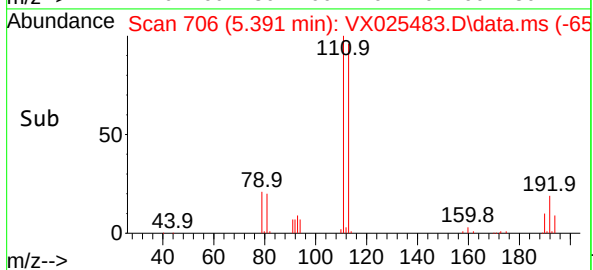

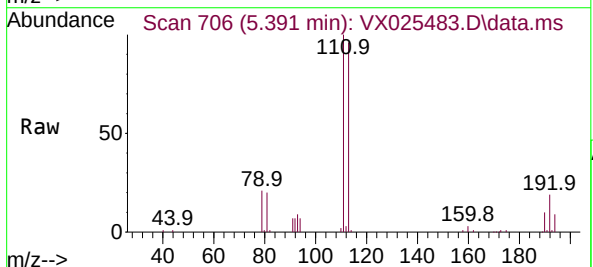




#36
1,1-Dichloropropene
Concen: 4.653 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.146 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32




Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL


Tgt Ion: 75 Resp: 7274
Ion Ratio Lower Upper
75 100
110 8.5 18.1 54.3#
77 0.0 24.4 36.6#



#38
Carbon Tetrachloride
Concen: 5.716 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.122 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Tgt Ion: 117 Resp: 9841
Ion Ratio Lower Upper
117 100
119 4.6 75.6 113.4#
121 0.0 23.7 35.5#

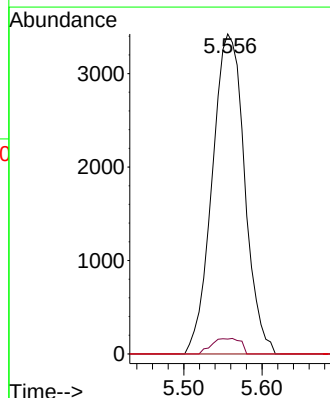

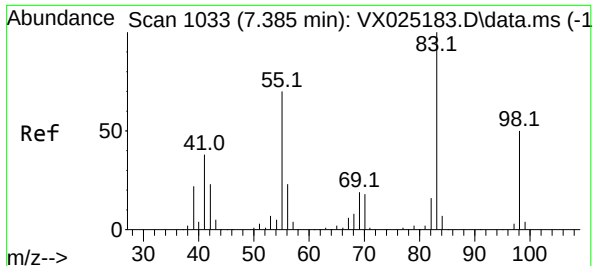

#39

Methylcyclohexane

Concen: 0.450 ug/l

RT: 7.379 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX025483.D

Acq: 03 Dec 2021 15:32

Instrument :

MSVOA_X

ClientSampleId :

DUP120221DL





Tgt Ion: 83 Resp: 903

Ion Ratio Lower Upper

83 100

55 53.2 60.8 91.2#

98 53.0 37.0 55.4

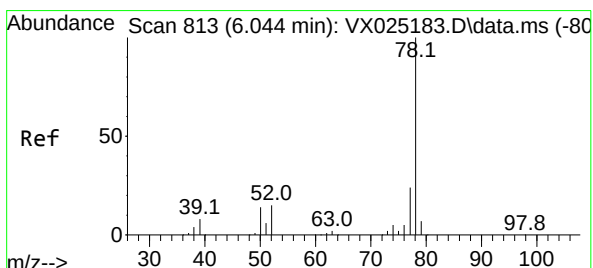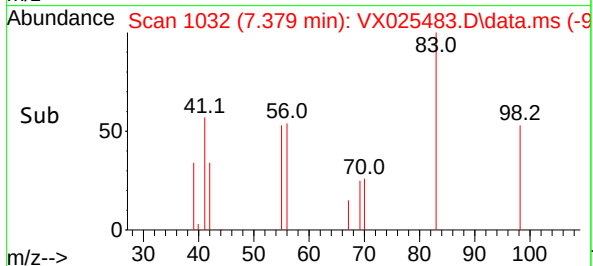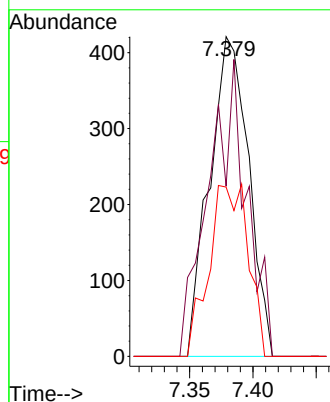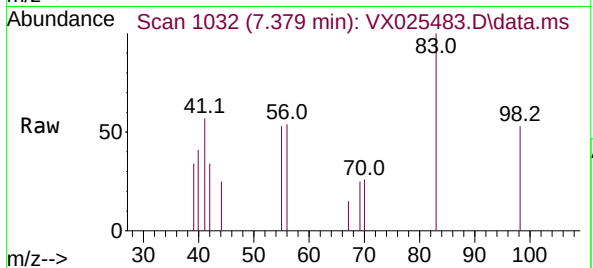

#40

Benzene

Concen: 10.857 ug/l

RT: 6.044 min Scan# 813

Delta R.T. -0.000 min

Lab File: VX025483.D




Acq: 03 Dec 2021 15:32


Tgt Ion: 78 Resp: 51414

Ion Ratio Lower Upper

78 100

77 24.0 18.3 27.5

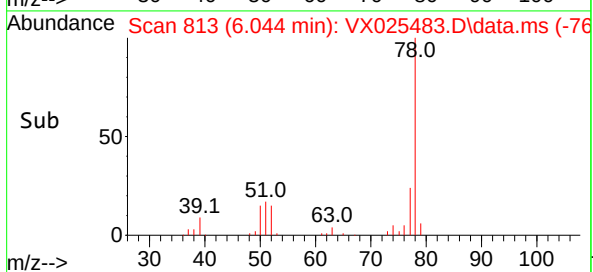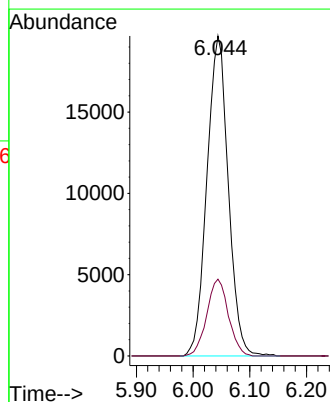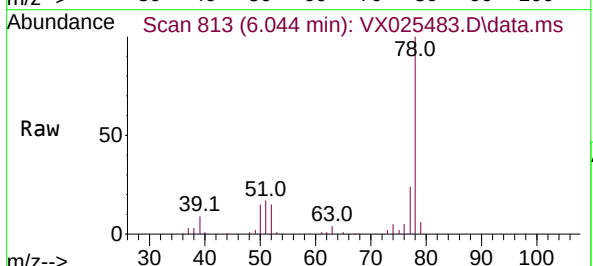



#42

1,2-Dichloroethane

Concen: 0.236 ug/l

RT: 6.044 min Scan# 81

Delta R.T. -0.042 min

Lab File: VX025483.D

Acq: 03 Dec 2021 15:32

Instrument :

MSVOA_X

ClientSampleId :





DUP120221DL

Tgt Ion: 62 Resp: 364

Ion Ratio Lower Upper

62 100

98 0.0 0.0 16.0

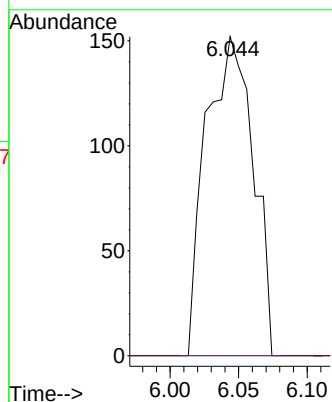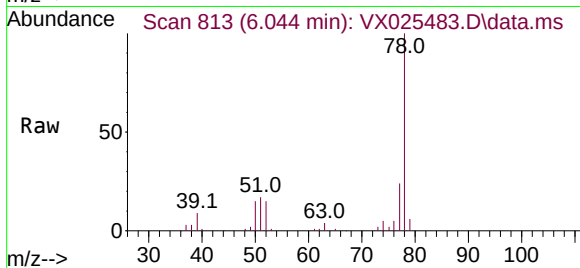

#50

Toluene-d8

Concen: 50.367 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX025483.D




Acq: 03 Dec 2021 15:32


Tgt Ion: 98 Resp: 208188

Ion Ratio Lower Upper

98 100

100 65.8 51.4 77.0

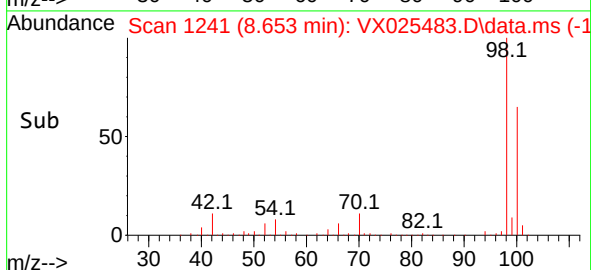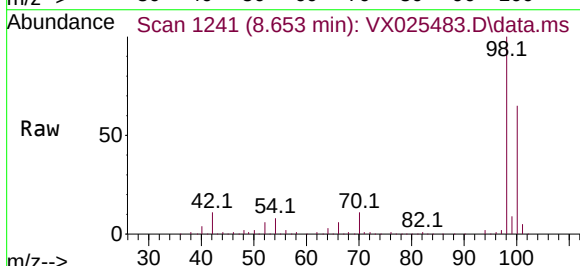



#52

Toluene

Concen: 27.906 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. 0.000 min

Lab File: VX025483.D

Acq: 03 Dec 2021 15:32

Instrument :

MSVOA_X

ClientSampleId :





DUP120221DL

Tgt Ion: 92 Resp: 86277

Ion Ratio Lower Upper

92 100

91 169.8 138.6 208.0



#53

t-1,3-Dichloropropene

Concen: 0.515 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.262 min

Lab File: VX025483.D




Acq: 03 Dec 2021 15:32


Tgt Ion: 75 Resp: 951

Ion Ratio Lower Upper

75 100

77 166.2 25.6 38.4#

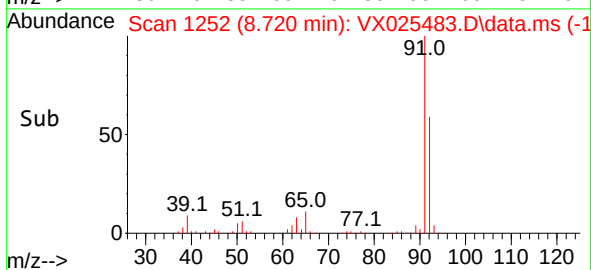



#62

4-Bromofluorobenzene

Concen: 47.207 ug/l

RT: 11.085 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX025483.D

Acq: 03 Dec 2021 15:32

Instrument :

MSVOA_X

ClientSampleId :

DUP120221DL





Tgt Ion: 95 Resp: 73819

Ion Ratio Lower Upper

95 100

174 84.0 0.0 158.0

176 80.6 0.0 153.6

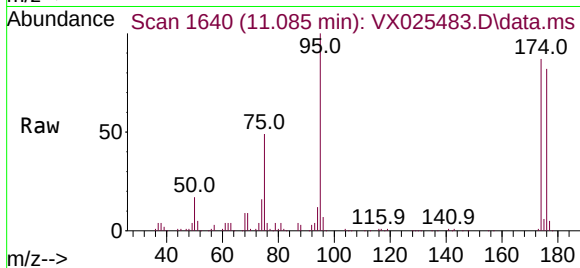

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX025483.D

Acq: 03 Dec 2021 15:32




Tgt Ion: 117 Resp: 162329


Ion Ratio Lower Upper

117 100

82 52.0 44.6 67.0

119 32.3 24.8 37.2




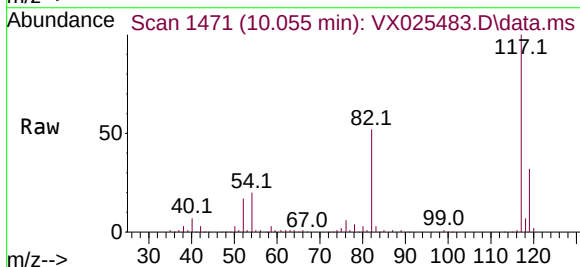




#67
Ethyl Benzene
Concen: 22.501 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32




Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL


Tgt Ion: 91 Resp: 128629
Ion Ratio Lower Upper
91 100
106 32.0 24.7 37.1



#68
m/p-Xylenes
Concen: 61.091 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Tgt Ion:106 Resp: 142644
Ion Ratio Lower Upper
106 100
91 195.7 163.4 245.0


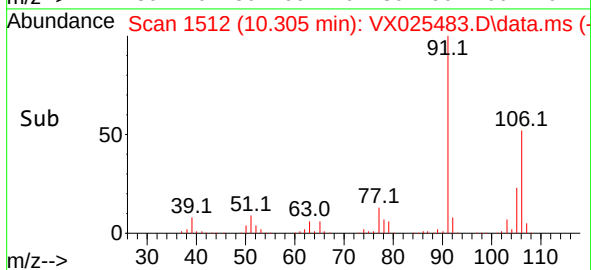






#69
o-Xylene
Concen: 37.238 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. -0.000 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32




Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL


Tgt Ion:106 Resp: 85100
Ion Ratio Lower Upper
106 100
91 208.1 109.5 328.4



#70
Styrene
Concen: 1.200 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. -0.012 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Tgt Ion:104 Resp: 4531
Ion Ratio Lower Upper
104 100
78 269.9 41.3 61.9#
103 246.5 43.5 65.3#



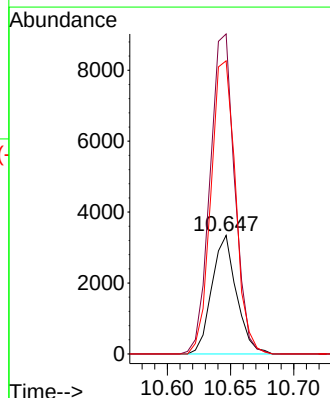





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32




Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL


Tgt Ion:152 Resp: 73446
Ion Ratio Lower Upper
152 100
115 58.4 43.3 129.8
150 158.5 0.0 351.2

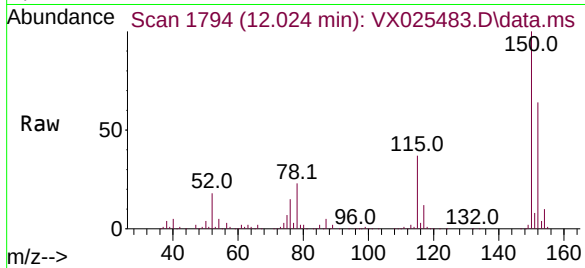

#73
Isopropylbenzene
Concen: 0.982 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. -0.000 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Tgt Ion:105 Resp: 5139
Ion Ratio Lower Upper
105 100
120 26.7 13.3 39.8


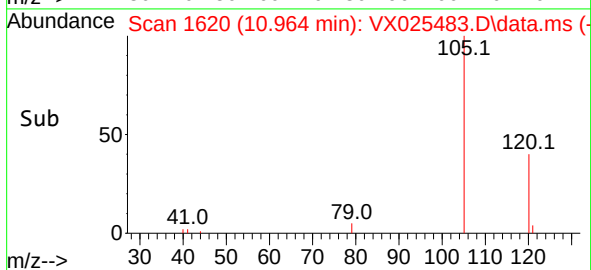

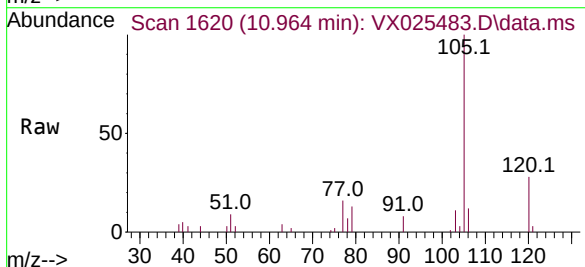




#76
1,2,3-Trichloropropane
Concen: 23.631 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32




Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL


Tgt Ion: 75 Resp: 35541
Ion Ratio Lower Upper
75 100
77 1.1 20.0 59.9#

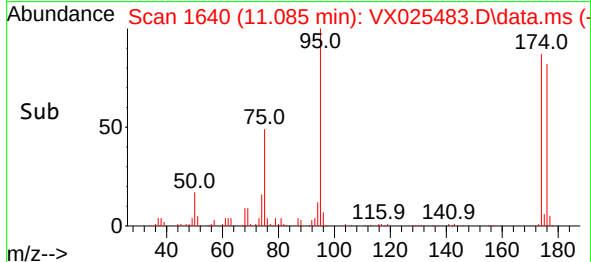

#78
n-propylbenzene
Concen: 2.608 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Tgt Ion: 91 Resp: 15322
Ion Ratio Lower Upper
91 100
120 23.7 11.7 35.0




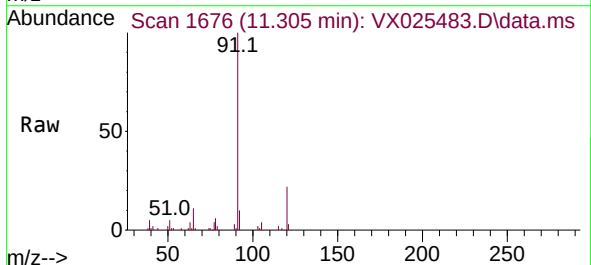




#79
2-Chlorotoluene
Concen: 2.221 ug/l
RT: 11.378 min Scan# 1
Delta R.T. 0.012 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32




Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL


Tgt Ion: 91 Resp: 7945
Ion Ratio Lower Upper
91 100
126 0.0 17.0 50.9#

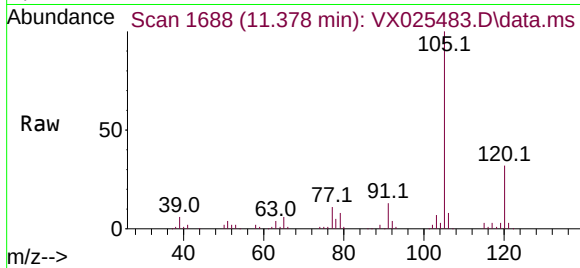

#80
1,3,5-Trimethylbenzene
Concen: 4.715 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Tgt Ion: 105 Resp: 20745
Ion Ratio Lower Upper
105 100
120 48.0 23.8 71.5


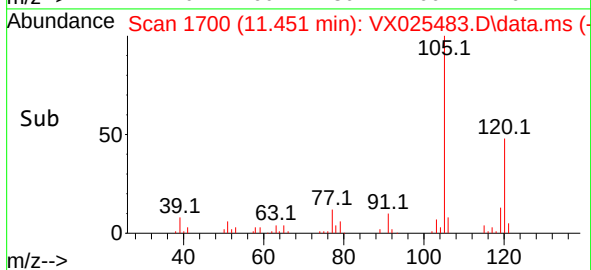

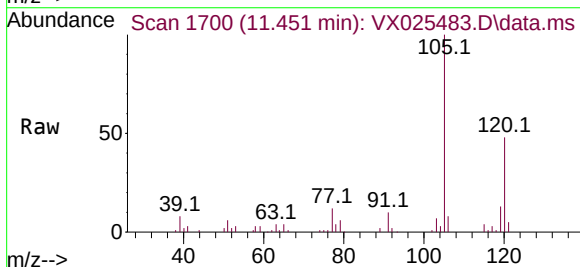




#81
trans-1,4-Dichloro-2-butene
Concen: 59.530 ug/l
RT: 11.085 min Scan# 1
Delta R.T. 0.067 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32




Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL


Tgt Ion: 75 Resp: 35541
Ion Ratio Lower Upper
75 100
53 0.0 81.9 122.9#
89 0.0 38.2 57.2#

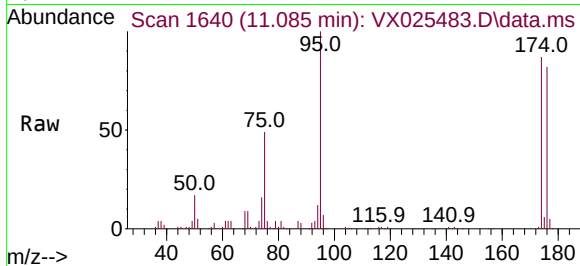

#82
4-Chlorotoluene
Concen: 0.535 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Tgt Ion: 91 Resp: 2183
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#




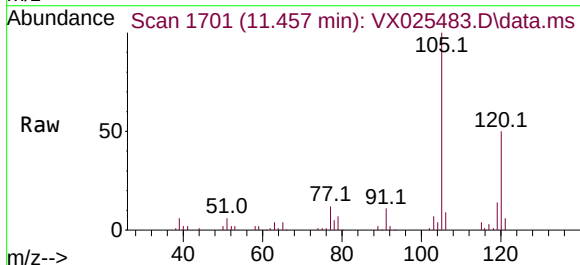




#83
tert-Butylbenzene
Concen: 2.384 ug/l
RT: 11.756 min Scan# 11
Delta R.T. 0.036 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32




Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL


Tgt Ion:119 Resp: 10661
Ion Ratio Lower Upper
119 100
91 88.2 30.3 90.9
134 0.0 11.4 34.1#

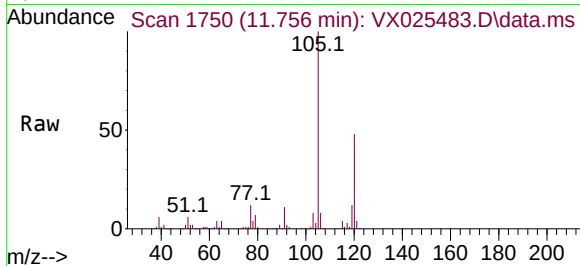

#84
1,2,4-Trimethylbenzene
Concen: 20.158 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Tgt Ion:105 Resp: 87662
Ion Ratio Lower Upper
105 100
120 47.0 22.1 66.3




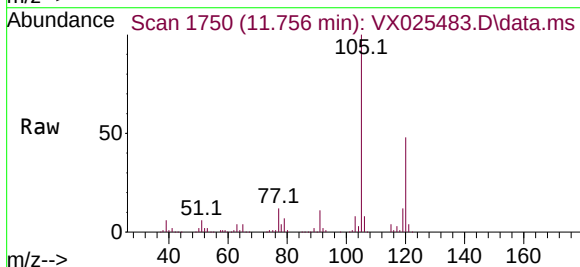




#85
 sec-Butylbenzene
 Concen: 16.126 ug/l
 RT: 11.756 min Scan# 11
 Delta R.T. -0.134 min
 Lab File: VX025483.D
 Acq: 03 Dec 2021 15:32




Instrument :
 MSVOA_X
 ClientSampleId :
 DUP120221DL


Tgt Ion:105 Resp: 87662
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.2 30.4#

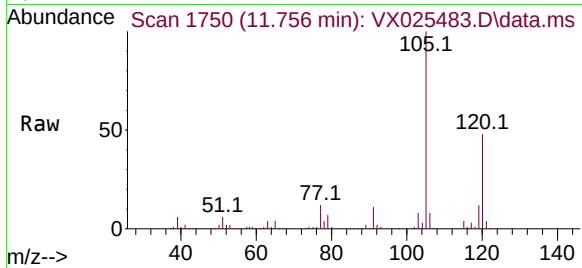

#89
 n-Butylbenzene
 Concen: 0.337 ug/l
 RT: 12.317 min Scan# 1842
 Delta R.T. -0.018 min
 Lab File: VX025483.D
 Acq: 03 Dec 2021 15:32

Tgt Ion: 91 Resp: 1327
 Ion Ratio Lower Upper
 91 100
 92 24.8 26.3 78.8#
 134 113.3 13.0 38.9#




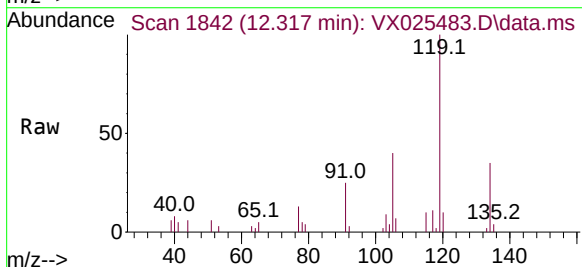




#90
Hexachloroethane
Concen: 1.187 ug/l
RT: 12.646 min Scan# 1896
Delta R.T. 0.103 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Instrument :
MSVOA_X
ClientSampleId :
DUP120221DL

Tgt Ion:117 Resp: 1022
Ion Ratio Lower Upper
117 100
201 0.0 38.9 116.6#

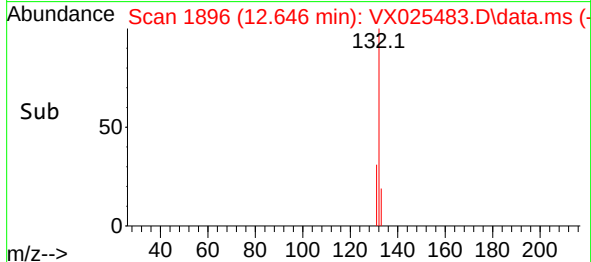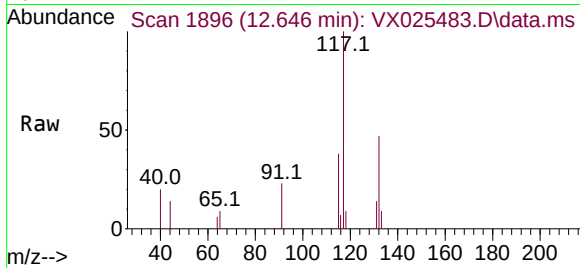

#95
Naphthalene
Concen: 7.464 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX025483.D
Acq: 03 Dec 2021 15:32

Tgt Ion:128 Resp: 38570
Ion Ratio Lower Upper
128 100
127 12.6 10.3 15.5
129 10.7 8.8 13.2

