

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120321\
 Data File : VX025484.D
 Acq On : 03 Dec 2021 15:56
 Operator : JC/MD
 Sample : M4917-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 04 06:51:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 17 15:36:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	102231	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	172290	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	151583	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	68096	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	60782	56.406	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 112.820%	
35) Dibromofluoromethane	5.391	113	53206	50.331	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.660%	
50) Toluene-d8	8.653	98	197536	49.699	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 99.400%	
62) 4-Bromofluorobenzene	11.079	95	69252	46.056	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 92.120%	


Target Compounds			Qvalue			
3) Chloromethane	1.294	50	676	0.616	ug/l #	42
5) Bromomethane	1.618	94	114	0.220	ug/l	88
6) Chloroethane	1.672	64	271	0.326	ug/l #	43
11) Tert butyl alcohol	2.959	59	586	Below Cal	#	72
14) Allyl chloride	2.776	41	618	0.360	ug/l #	67
16) Acetone	2.380	43	675	1.127	ug/l #	85
18) Methyl Acetate	2.776	43	1457	0.762	ug/l #	52
19) Methyl tert-butyl Ether	3.117	73	9472	2.869	ug/l #	83
31) Cyclohexane	5.556	56	2076	1.247	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	6821	4.538	ug/l #	50
38) Carbon Tetrachloride	5.562	117	9834	5.940	ug/l #	15
39) Methylcyclohexane	7.184	83	673	0.349	ug/l	93
40) Benzene	6.044	78	1616	0.355	ug/l #	90
52) Toluene	8.726	92	642	0.216	ug/l	95
55) 1,1,2-Trichloroethane	9.110	97	2440	2.065	ug/l #	19
56) Ethyl methacrylate	9.110	69	736	0.384	ug/l #	18
67) Ethyl Benzene	10.195	91	1221	0.229	ug/l	98
68) m/p-Xylenes	10.305	106	1250	0.573	ug/l	94
69) o-Xylene	10.640	106	568	0.266	ug/l	99
73) Isopropylbenzene	10.963	105	1645	0.339	ug/l	97
76) 1,2,3-Trichloropropane	11.079	75	33158	23.778	ug/l #	38
78) n-propylbenzene	11.305	91	7558	1.387	ug/l	98
79) 2-Chlorotoluene	11.305	91	7558	2.279	ug/l #	41
81) trans-1,4-Dichloro-2-b...	11.079	75	33158	59.902	ug/l #	9
82) 4-Chlorotoluene	11.305	91	7558	1.996	ug/l #	45
83) tert-Butylbenzene	11.975	119	1284	0.310	ug/l	69
84) 1,2,4-Trimethylbenzene	11.756	105	1679	0.416	ug/l	94
85) sec-Butylbenzene	11.890	105	11446	2.271	ug/l	93
86) p-Isopropyltoluene	11.975	119	1284	0.297	ug/l #	67
89) n-Butylbenzene	12.335	91	21005	5.755	ug/l #	66
90) Hexachloroethane	12.616	117	2858	3.581	ug/l #	11
92) 1,2-Dibromo-3-Chloropr...	12.963	75	196	0.598	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120321\
Data File : VX025484.D
Acq On : 03 Dec 2021 15:56
Operator : JC/MD
Sample : M4917-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Dec 04 06:51:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 17 15:36:16 2021
Response via : Initial Calibration

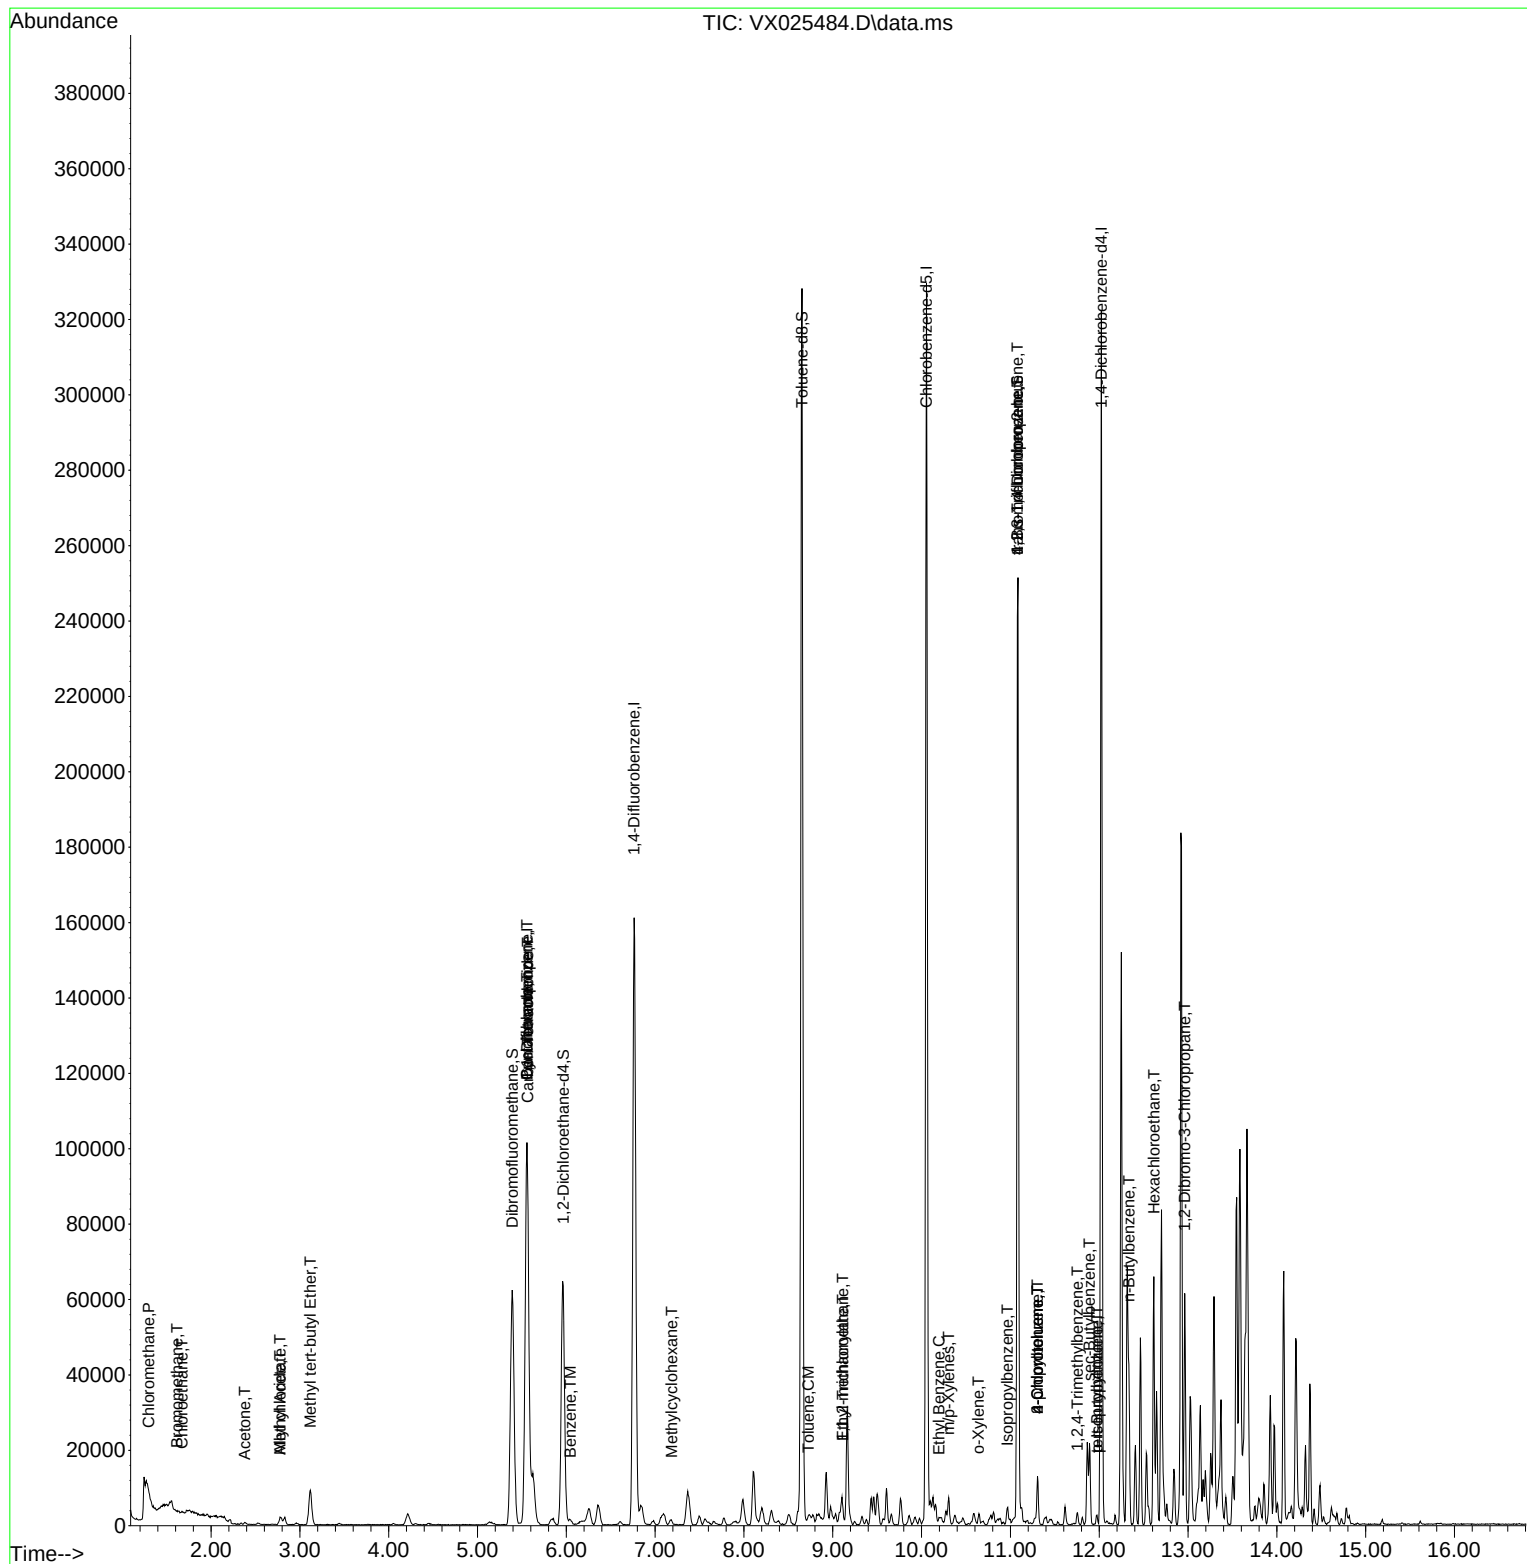






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:168 Resp: 102231
Ion Ratio Lower Upper
168 100
99 51.8 46.4 69.6



#3
Chloromethane
Concen: 0.616 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.006 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Tgt Ion: 50 Resp: 676
Ion Ratio Lower Upper
50 100
52 0.0 25.9 38.9#


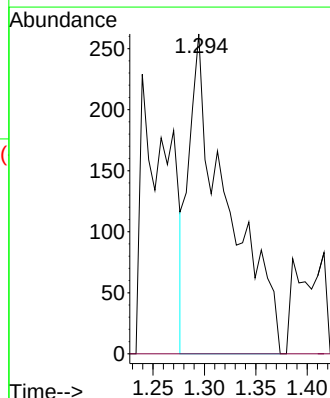
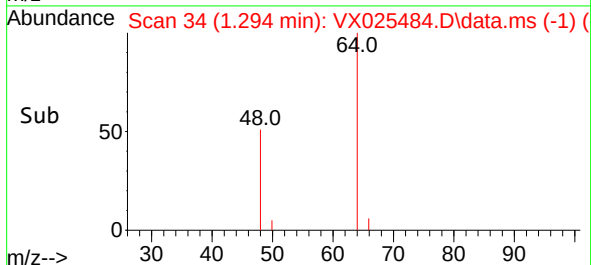



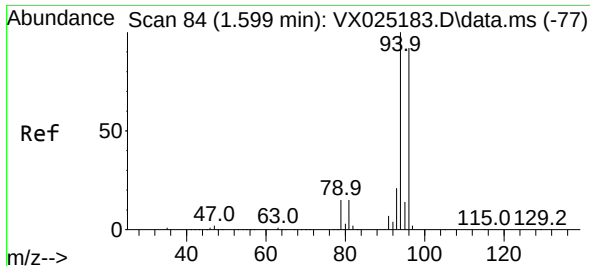

#5
Bromomethane
Concen: 0.220 ug/l
RT: 1.618 min Scan# 81
Delta R.T. 0.019 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 94 Resp: 114
Ion Ratio Lower Upper
94 100
96 105.5 74.8 112.2

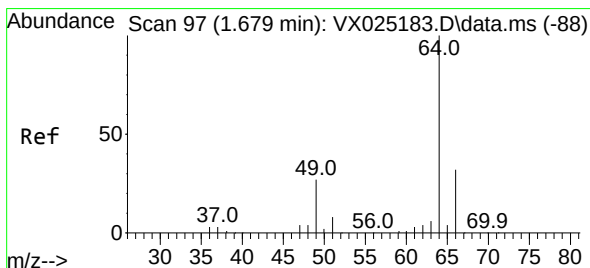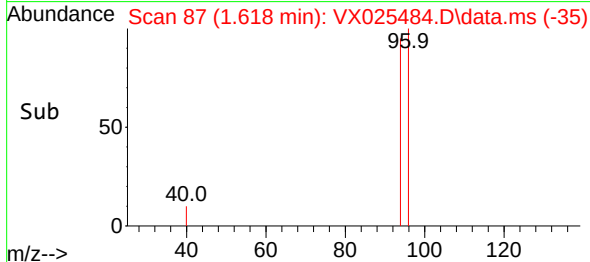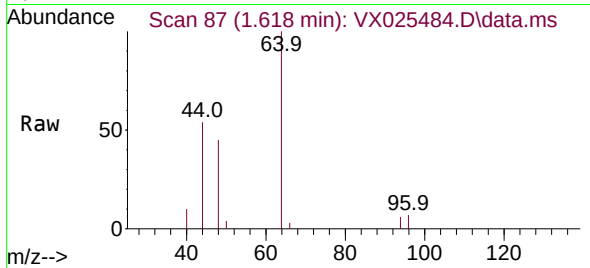

#6
Chloroethane
Concen: 0.326 ug/l
RT: 1.672 min Scan# 96
Delta R.T. -0.007 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Tgt Ion: 64 Resp: 271
Ion Ratio Lower Upper
64 100
66 0.0 25.6 38.4#


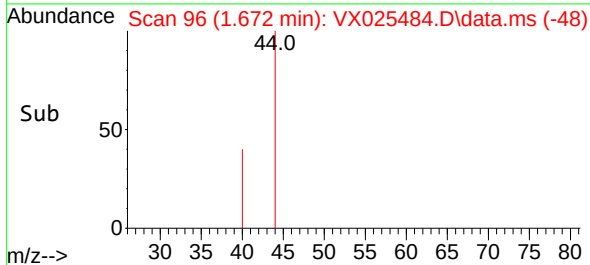

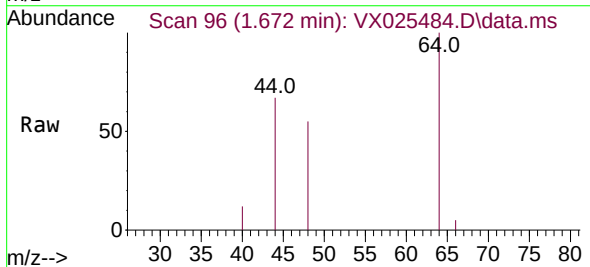


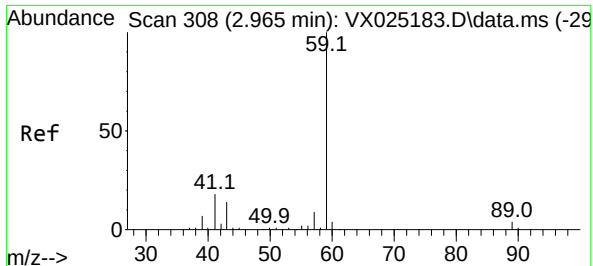

#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.959 min Scan# 308
Delta R.T. -0.006 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 59 Resp: 586
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#

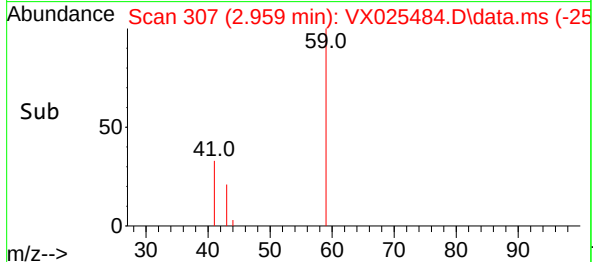

#14
Allyl chloride
Concen: 0.360 ug/l
RT: 2.776 min Scan# 277
Delta R.T. 0.116 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56


Tgt Ion: 41 Resp: 618
Ion Ratio Lower Upper
41 100
39 51.1 54.6 82.0#
76 0.0 25.3 37.9#

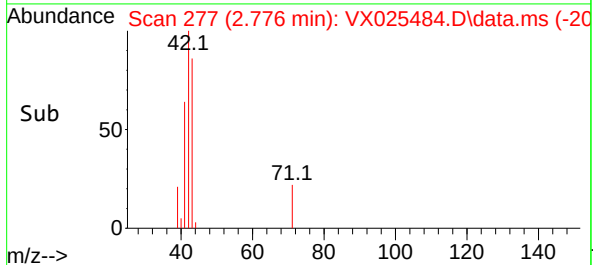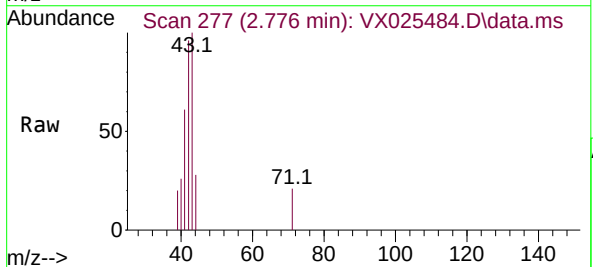



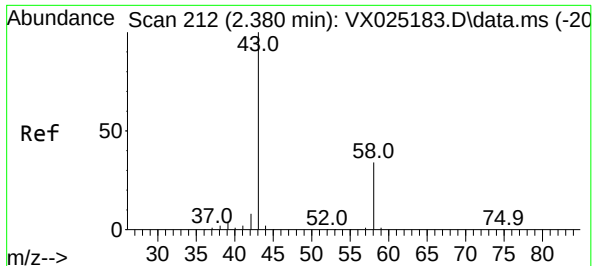


#16
Acetone
Concen: 1.127 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 43 Resp: 675
Ion Ratio Lower Upper
43 100
58 38.3 24.0 36.0#

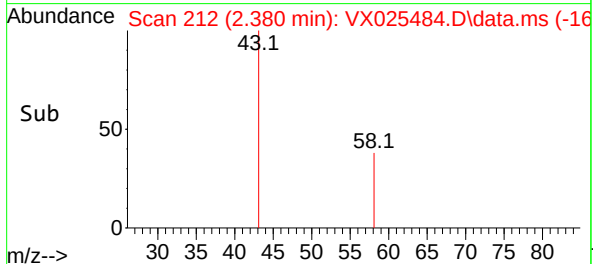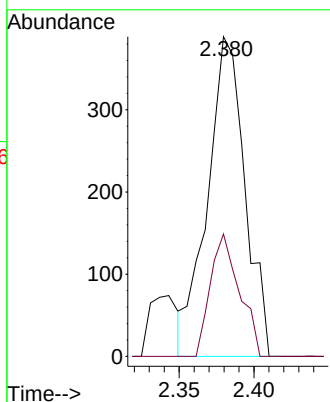

#18
Methyl Acetate
Concen: 0.762 ug/l
RT: 2.776 min Scan# 277
Delta R.T. 0.073 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Tgt Ion: 43 Resp: 1457
Ion Ratio Lower Upper
43 100
74 0.0 19.0 28.6#


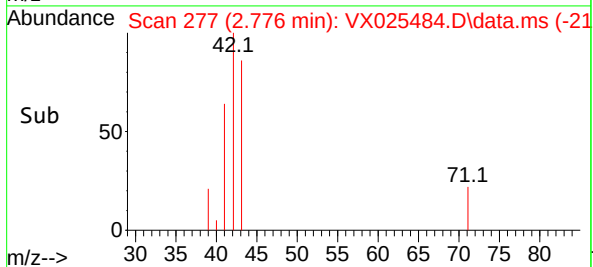

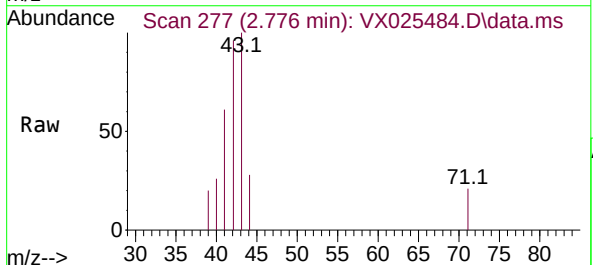




#19
Methyl tert-butyl Ether
Concen: 2.869 ug/l
RT: 3.117 min Scan# 31
Delta R.T. 0.000 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 73 Resp: 9472
Ion Ratio Lower Upper
73 100
57 30.2 17.5 26.3#

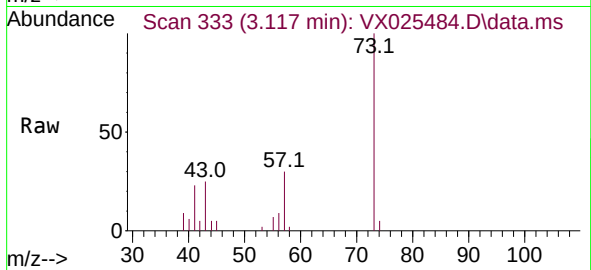

#31
Cyclohexane
Concen: 1.247 ug/l
RT: 5.556 min Scan# 733
Delta R.T. 0.085 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Tgt Ion: 56 Resp: 2076
Ion Ratio Lower Upper
56 100
69 176.8 24.2 36.2#
84 144.2 71.5 107.3#





#33

1,2-Dichloroethane-d4

Concen: 56.406 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.006 min

Lab File: VX025484.D

Acq: 03 Dec 2021 15:56

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 60782

Ion Ratio Lower Upper

65 100

67 51.4 0.0 101.0

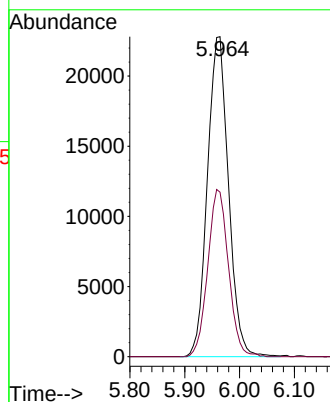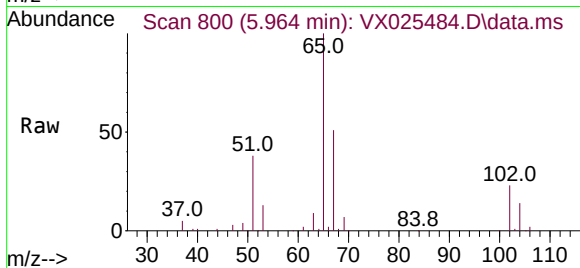

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX025484.D

Acq: 03 Dec 2021 15:56




Tgt Ion: 114 Resp: 172290


Ion Ratio Lower Upper

114 100

63 18.3 0.0 41.0

88 14.9 0.0 34.8

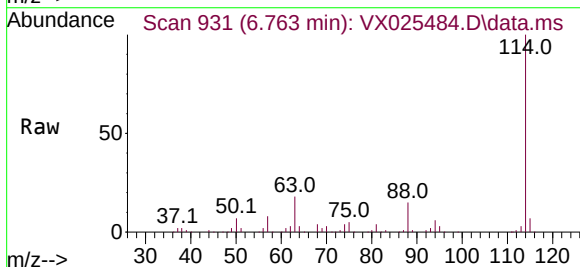

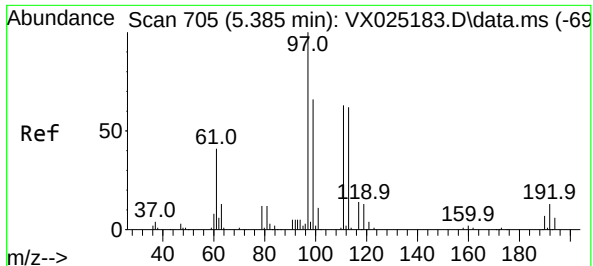

#35

Dibromofluoromethane

Concen: 50.331 ug/l

RT: 5.391 min Scan# 705

Delta R.T. 0.006 min


Lab File: VX025484.D

Acq: 03 Dec 2021 15:56

Instrument :

MSVOA_X

ClientSampleId :

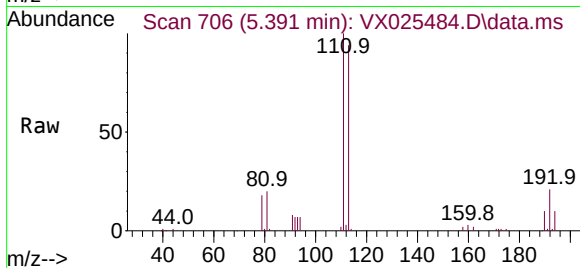




Tgt Ion:113 Resp: 53206

Ion Ratio Lower Upper

113 100

111 102.4 82.1 123.1

192 21.2 15.6 23.4

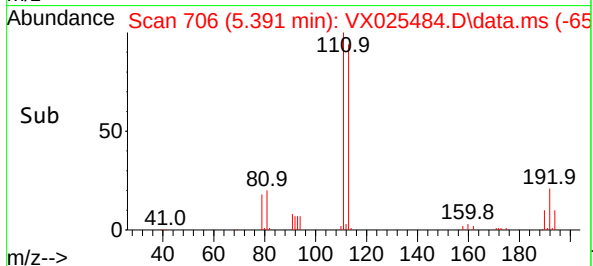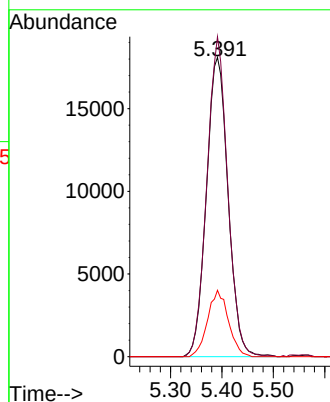

#36

1,1-Dichloropropene

Concen: 4.538 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min

Lab File: VX025484.D

Acq: 03 Dec 2021 15:56




Tgt Ion: 75 Resp: 6821


Ion Ratio Lower Upper

75 100

110 9.2 18.1 54.3#


77 0.0 24.4 36.6#

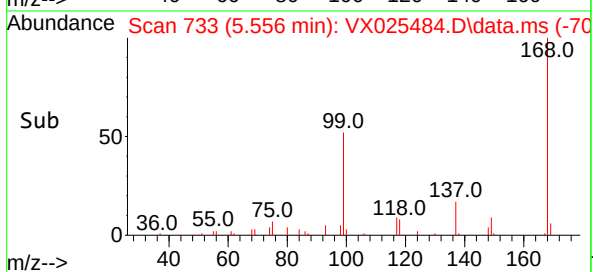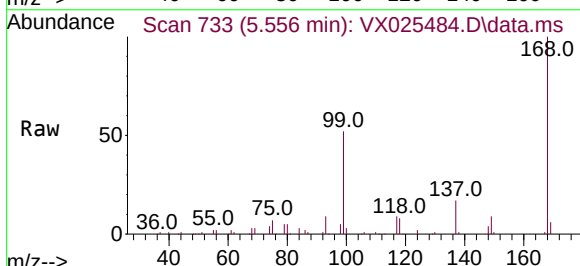






#38
Carbon Tetrachloride
Concen: 5.940 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.116 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 9834
Ion Ratio Lower Upper
117 100
119 3.5 75.6 113.4#
121 0.0 23.7 35.5#



#39
Methylcyclohexane
Concen: 0.349 ug/l
RT: 7.184 min Scan# 1000
Delta R.T. -0.201 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Tgt Ion: 83 Resp: 673
Ion Ratio Lower Upper
83 100
55 84.4 60.8 91.2
98 46.9 37.0 55.4




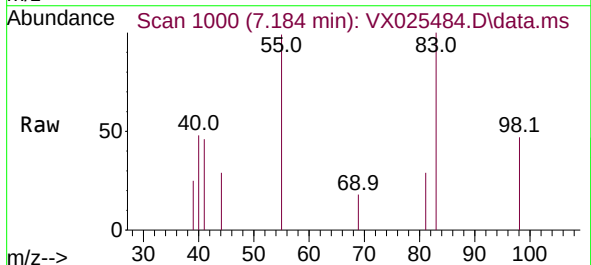




#40
Benzene
Concen: 0.355 ug/l
RT: 6.044 min Scan# 813
Delta R.T. -0.000 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 78 Resp: 1616
Ion Ratio Lower Upper
78 100
77 18.1 18.3 27.5#

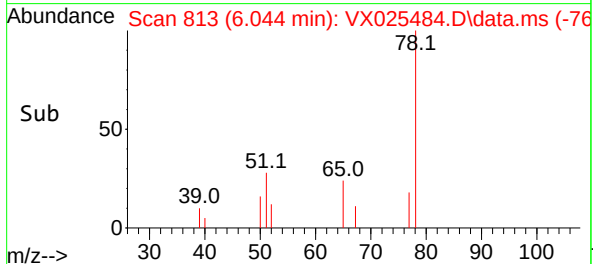

#50
Toluene-d8
Concen: 49.699 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Tgt Ion: 98 Resp: 197536
Ion Ratio Lower Upper
98 100
100 66.7 51.4 77.0


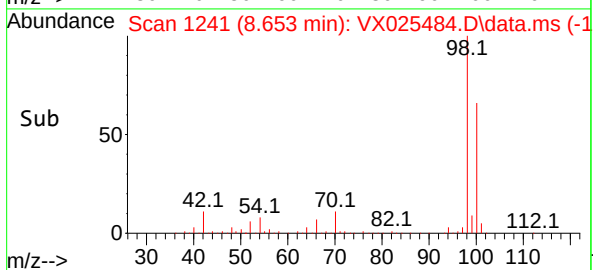

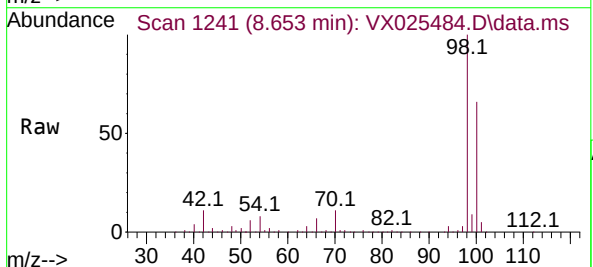




#52
Toluene
Concen: 0.216 ug/l
RT: 8.726 min Scan# 1316
Delta R.T. 0.006 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 92 Resp: 642
Ion Ratio Lower Upper
92 100
91 180.2 138.6 208.0

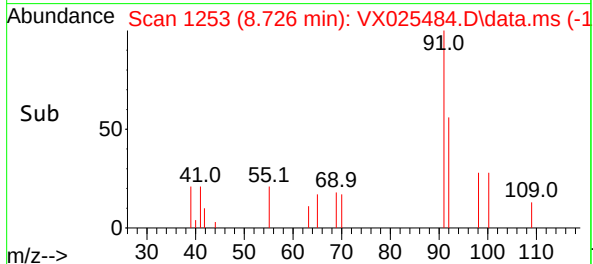

#55
1,1,2-Trichloroethane
Concen: 2.065 ug/l
RT: 9.110 min Scan# 1316
Delta R.T. -0.043 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Tgt Ion: 97 Resp: 2440
Ion Ratio Lower Upper
97 100
83 8.3 69.2 103.8#
85 0.0 43.3 64.9#
99 0.0 49.1 73.7#


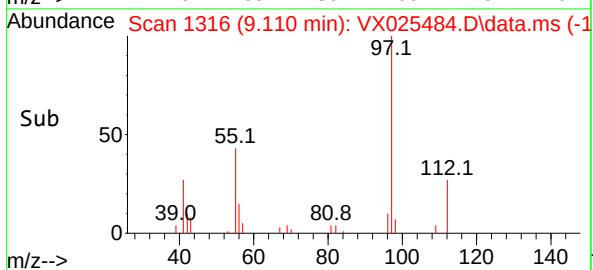

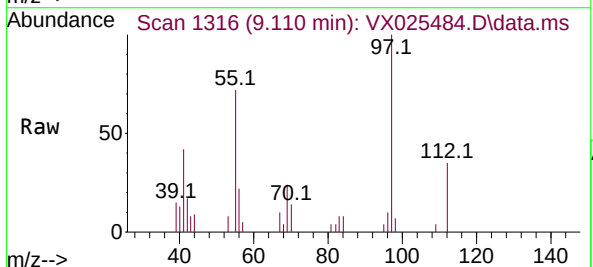




#56
Ethyl methacrylate
Concen: 0.384 ug/l
RT: 9.110 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 69 Resp: 736
Ion Ratio Lower Upper
69 100
41 123.0 55.3 82.9#
39 105.4 30.2 45.4#



#62
4-Bromofluorobenzene
Concen: 46.056 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Tgt Ion: 95 Resp: 69252
Ion Ratio Lower Upper
95 100
174 82.8 0.0 158.0
176 80.7 0.0 153.6









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 151583
Ion Ratio Lower Upper
117 100
82 53.7 44.6 67.0
119 32.4 24.8 37.2

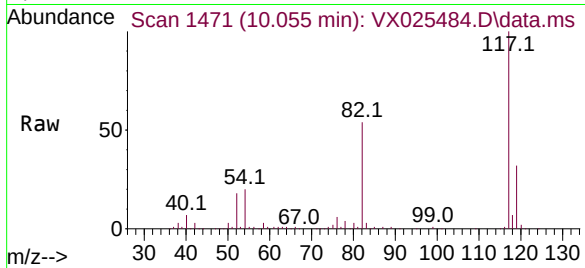

#67
Ethyl Benzene
Concen: 0.229 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Tgt Ion: 91 Resp: 1221
Ion Ratio Lower Upper
91 100
106 29.6 24.7 37.1



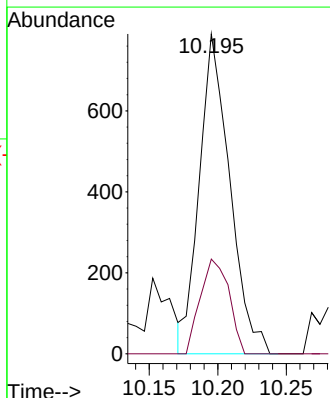
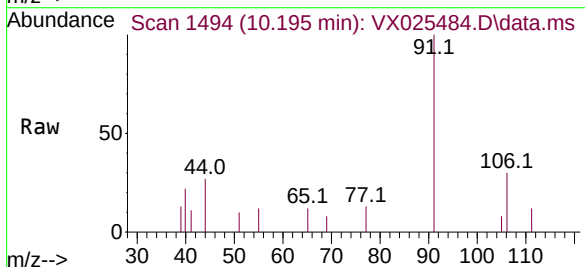




#68
m/p-Xylenes
Concen: 0.573 ug/l
RT: 10.305 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 1250
Ion Ratio Lower Upper
106 100
91 212.8 163.4 245.0

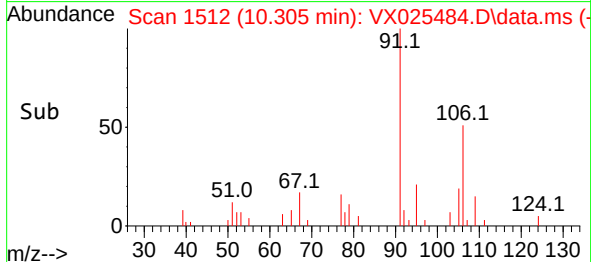

#69
o-Xylene
Concen: 0.266 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.007 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Tgt Ion:106 Resp: 568
Ion Ratio Lower Upper
106 100
91 220.4 109.5 328.4




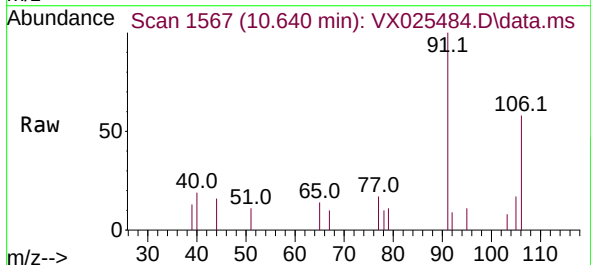




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:152 Resp: 68096
Ion Ratio Lower Upper
152 100
115 57.5 43.3 129.8
150 155.7 0.0 351.2

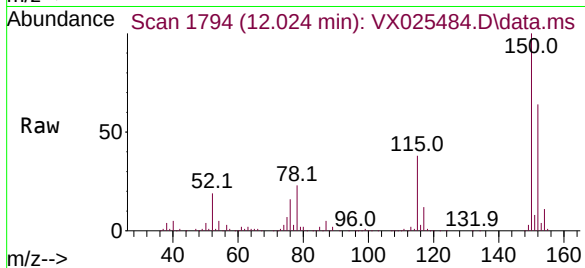

#73
Isopropylbenzene
Concen: 0.339 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.001 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Tgt Ion:105 Resp: 1645
Ion Ratio Lower Upper
105 100
120 24.9 13.3 39.8

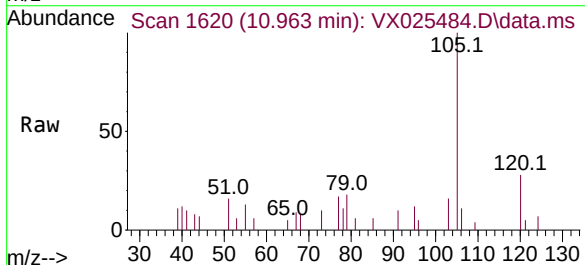



#76

1,2,3-Trichloropropane

Concen: 23.778 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.165 min

Lab File: VX025484.D

Acq: 03 Dec 2021 15:56

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 33158

Ion Ratio Lower Upper

75 100

77 1.3 20.0 59.9#

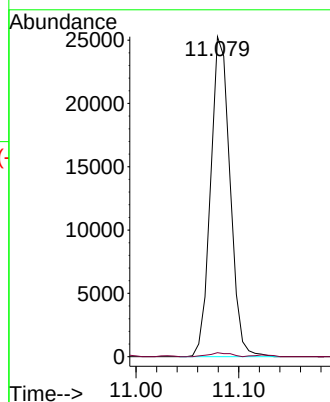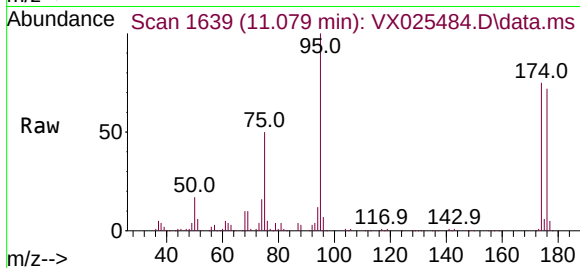

#78

n-propylbenzene

Concen: 1.387 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX025484.D




Acq: 03 Dec 2021 15:56


Tgt Ion: 91 Resp: 7558

Ion Ratio Lower Upper

91 100

120 24.5 11.7 35.0


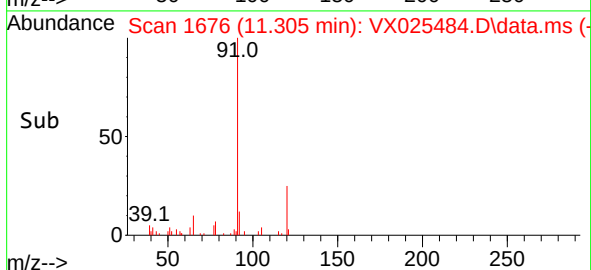

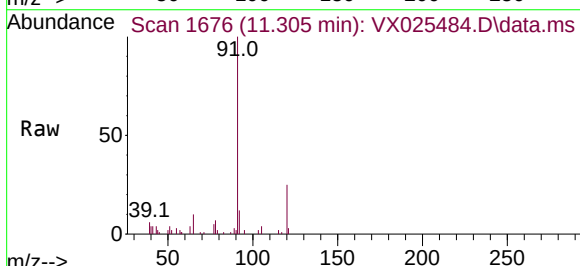




#79
2-Chlorotoluene
Concen: 2.279 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.061 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 7558
Ion Ratio Lower Upper
91 100
126 0.0 17.0 50.9#

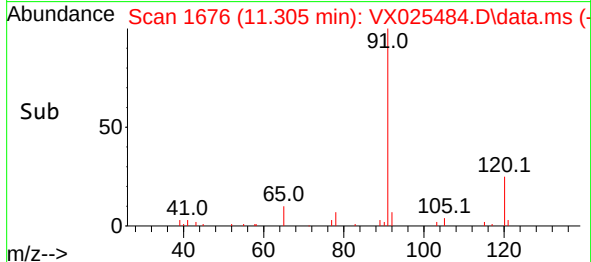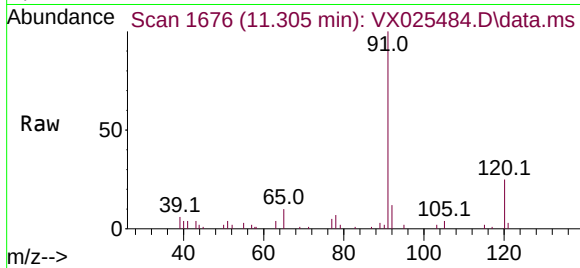

#81
trans-1,4-Dichloro-2-butene
Concen: 59.902 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Tgt Ion: 75 Resp: 33158
Ion Ratio Lower Upper
75 100
53 0.1 81.9 122.9#
89 0.0 38.2 57.2#




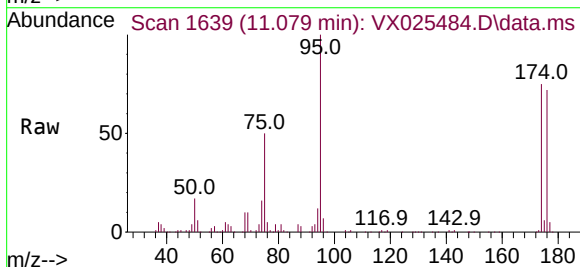




#82
4-Chlorotoluene
Concen: 1.996 ug/l
RT: 11.305 min Scan# 1786
Delta R.T. -0.152 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 7558
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

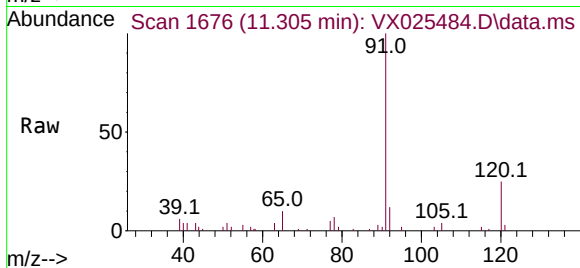

#83
tert-Butylbenzene
Concen: 0.310 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. 0.255 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Tgt Ion: 119 Resp: 1284
Ion Ratio Lower Upper
119 100
91 31.2 30.3 90.9
134 28.4 11.4 34.1

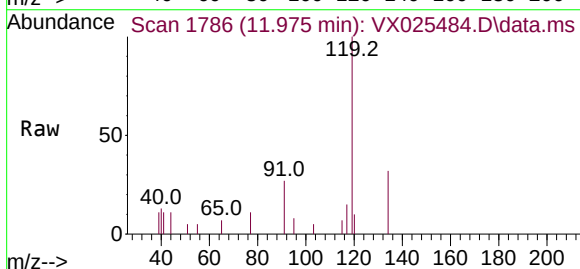



#84

1,2,4-Trimethylbenzene

Concen: 0.416 ug/l

RT: 11.756 min Scan# 1750

Delta R.T. -0.000 min

Lab File: VX025484.D

Acq: 03 Dec 2021 15:56

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 1679

Ion Ratio Lower Upper

105 100

120 47.8 22.1 66.3

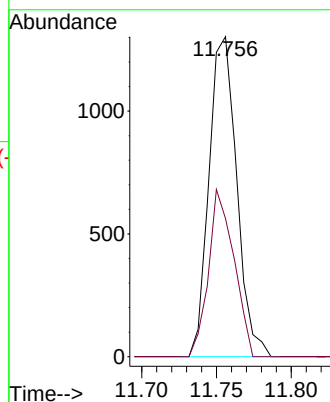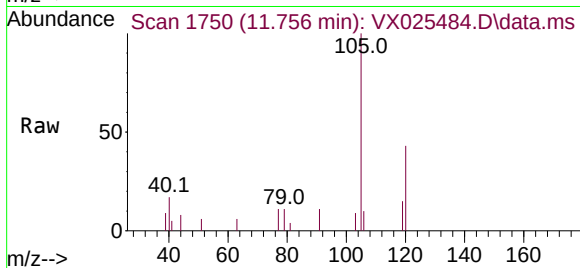

#85

sec-Butylbenzene

Concen: 2.271 ug/l

RT: 11.890 min Scan# 1772

Delta R.T. 0.000 min

Lab File: VX025484.D




Acq: 03 Dec 2021 15:56


Tgt Ion:105 Resp: 11446

Ion Ratio Lower Upper

105 100

134 16.9 10.2 30.4


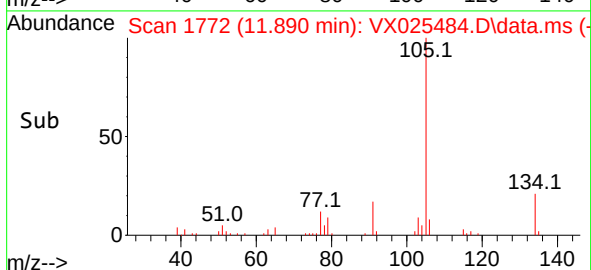

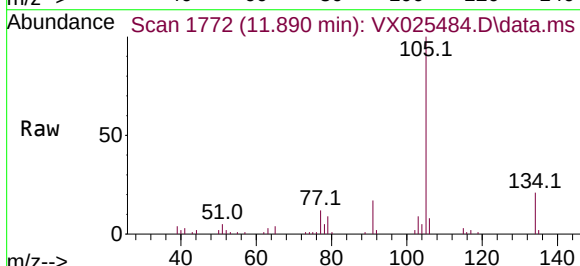




#86
p-Isopropyltoluene
Concen: 0.297 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. -0.037 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:119 Resp: 1284
Ion Ratio Lower Upper
119 100
134 0.0 13.2 39.5#
91 31.2 12.4 37.0

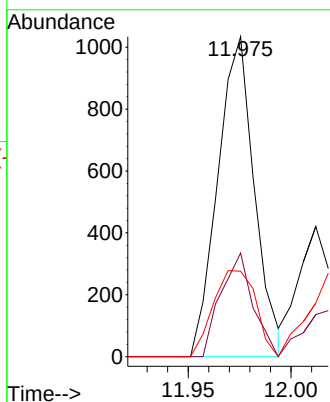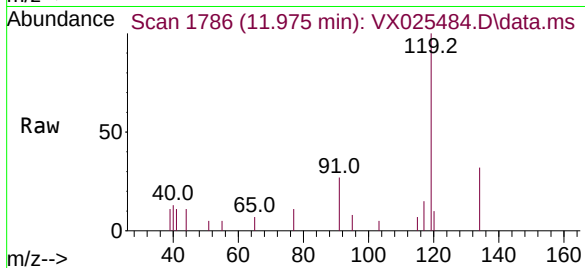

#89
n-Butylbenzene
Concen: 5.755 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Tgt Ion: 91 Resp: 21005
Ion Ratio Lower Upper
91 100
92 43.7 26.3 78.8
134 64.8 13.0 38.9#




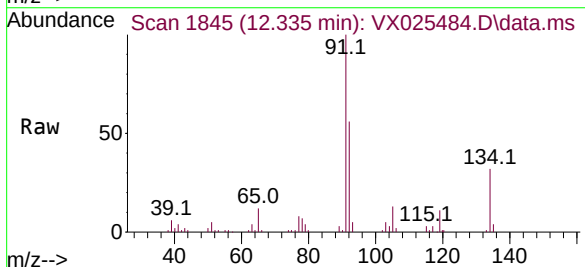




#90
Hexachloroethane
Concen: 3.581 ug/l
RT: 12.616 min Scan# 1879
Delta R.T. 0.073 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:117 Resp: 2858
Ion Ratio Lower Upper
117 100
201 0.0 38.9 116.6#

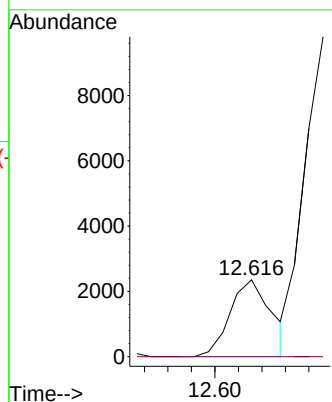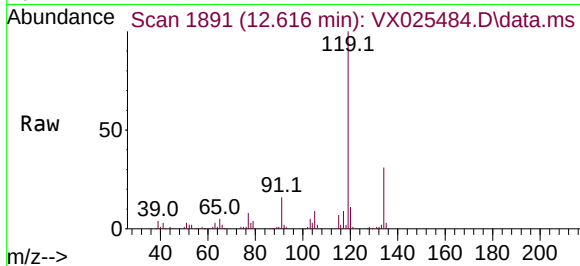

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.598 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. 0.018 min
Lab File: VX025484.D
Acq: 03 Dec 2021 15:56

Tgt Ion: 75 Resp: 196
Ion Ratio Lower Upper
75 100
155 0.0 43.1 129.3#
157 0.0 53.6 160.9#

