

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120321\
 Data File : VX025486.D
 Acq On : 03 Dec 2021 16:42
 Operator : JC/MD
 Sample : M4918-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-40

Quant Time: Dec 04 06:51:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 17 15:36:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	102394	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	174173	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	157508	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	70421	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	61123	56.632	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 113.260%			
35) Dibromofluoromethane	5.391	113	53723	50.271	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 100.540%			
50) Toluene-d8	8.653	98	199895	49.749	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 99.500%			
62) 4-Bromofluorobenzene	11.085	95	70387	46.305	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 92.620%			
Target Compounds						Qvalue
3) Chloromethane	1.294	50	302	0.275	ug/l #	42
5) Bromomethane	1.617	94	136	0.262	ug/l	97
6) Chloroethane	1.526	64	4901	5.887	ug/l #	57
11) Tert butyl alcohol	2.959	59	85426	322.568	ug/l	99
13) Acrolein	2.215	56	112	2.265	ug/l #	1
15) Acrylonitrile	3.123	53	364	0.628	ug/l #	33
16) Acetone	2.386	43	1455	2.426	ug/l #	87
18) Methyl Acetate	2.788	43	506	0.264	ug/l #	52
19) Methyl tert-butyl Ether	3.117	73	34527	10.441	ug/l	98
22) Diisopropyl ether	3.763	45	22992	7.029	ug/l #	84
23) Vinyl Acetate	3.763	43	11847	4.509	ug/l #	72
29) Tetrahydrofuran	5.013	42	310	0.577	ug/l #	53
31) Cyclohexane	5.476	56	1340	0.803	ug/l	98
36) 1,1-Dichloropropene	5.562	75	6903	4.543	ug/l #	49
38) Carbon Tetrachloride	5.556	117	9776	5.841	ug/l #	17
39) Methylcyclohexane	7.385	83	736	0.378	ug/l #	92
40) Benzene	6.043	78	350668	76.178	ug/l	99
42) 1,2-Dichloroethane	6.037	62	3121	2.084	ug/l #	77
48) Methyl methacrylate	7.903	41	475	0.352	ug/l #	36
51) 4-Methyl-2-Pentanone	8.573	43	508	0.282	ug/l	93
52) Toluene	8.726	92	1323	0.440	ug/l	97
59) 2-Hexanone	9.457	43	3456	2.430	ug/l	87
67) Ethyl Benzene	10.195	91	3751	0.676	ug/l	97
68) m/p-Xylenes	10.305	106	1208	0.533	ug/l	87
69) o-Xylene	10.646	106	1397	0.630	ug/l	90
73) Isopropylbenzene	10.963	105	3648	0.727	ug/l	98
74) N-amyl acetate	10.890	43	1142	0.526	ug/l #	53
76) 1,2,3-Trichloropropane	11.085	75	34423	23.870	ug/l #	37
80) 1,3,5-Trimethylbenzene	11.457	105	1839	0.436	ug/l	94
81) trans-1,4-Dichloro-2-b...	11.085	75	34423	60.134	ug/l #	9
84) 1,2,4-Trimethylbenzene	11.756	105	2820	0.676	ug/l	95
90) Hexachloroethane	12.646	117	349	0.423	ug/l #	11
95) Naphthalene	13.780	128	567	Below Cal	#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
MW-40

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120321\
Data File : VX025486.D
Acq On : 03 Dec 2021 16:42
Operator : JC/MD
Sample : M4918-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-40

Quant Time: Dec 04 06:51:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 17 15:36:16 2021
Response via : Initial Calibration




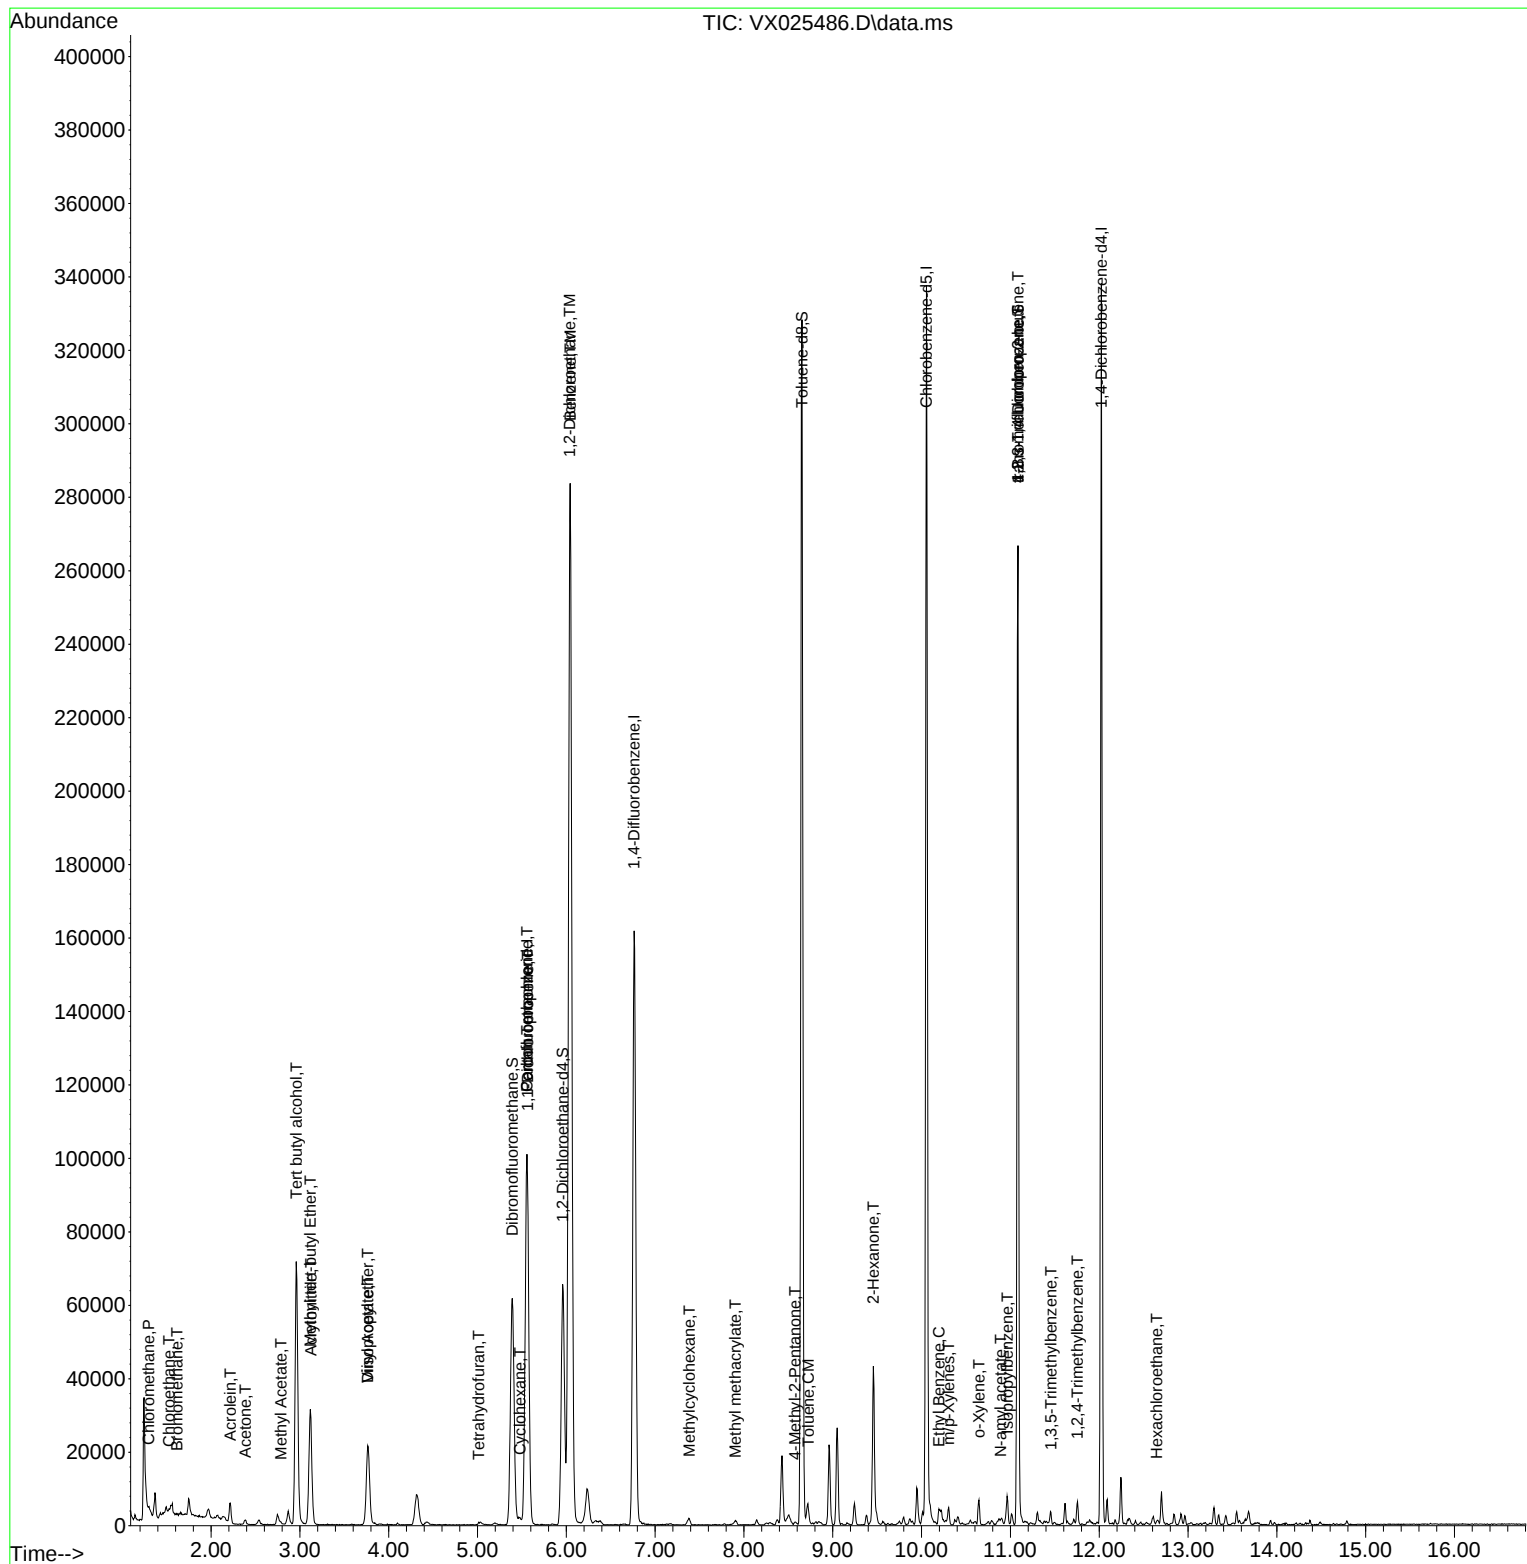


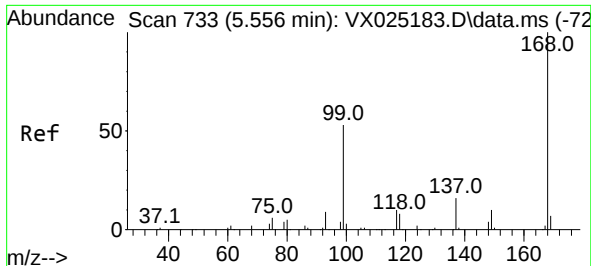

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:168 Resp: 102394
Ion Ratio Lower Upper
168 100
99 55.5 46.4 69.6

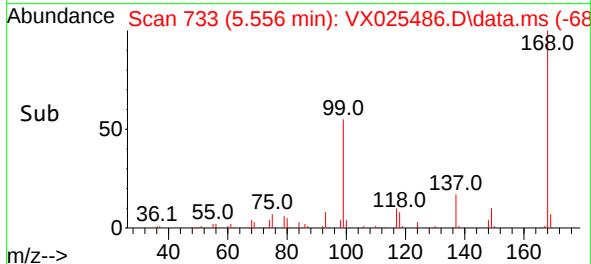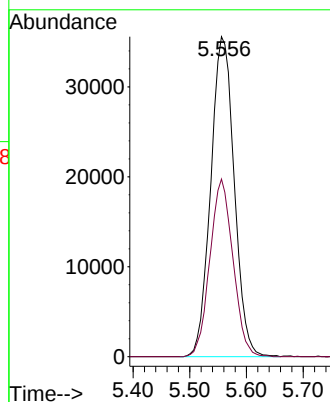

#3
Chloromethane
Concen: 0.275 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.006 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42

Tgt Ion: 50 Resp: 302
Ion Ratio Lower Upper
50 100
52 0.0 25.9 38.9#


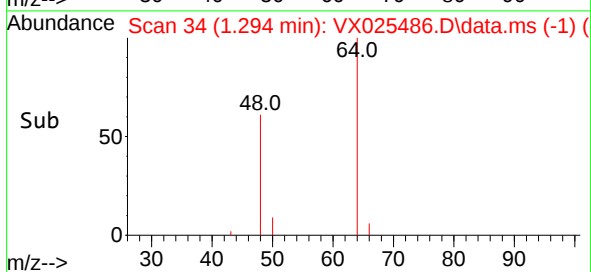
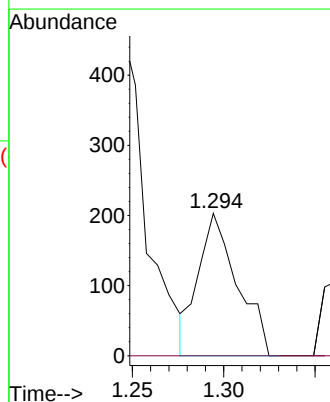
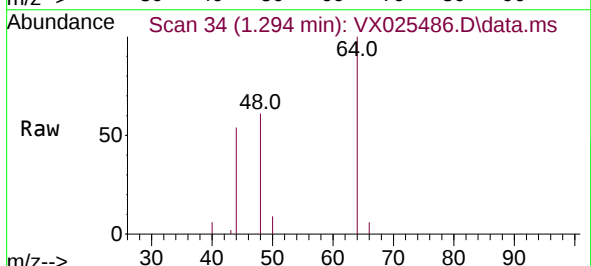


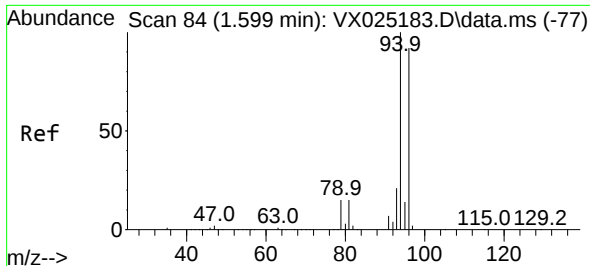

#5
Bromomethane
Concen: 0.262 ug/l
RT: 1.617 min Scan# 81
Delta R.T. 0.018 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 94 Resp: 136
Ion Ratio Lower Upper
94 100
96 90.9 74.8 112.2

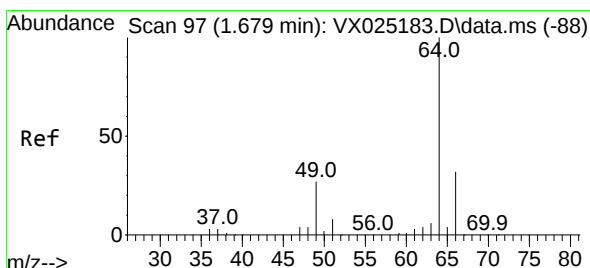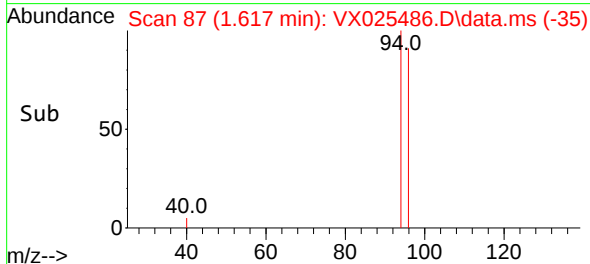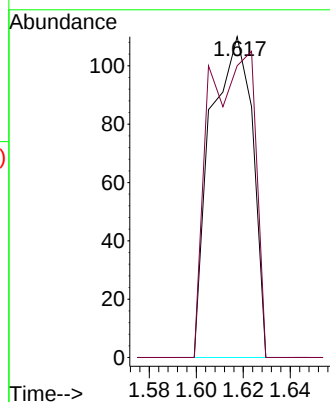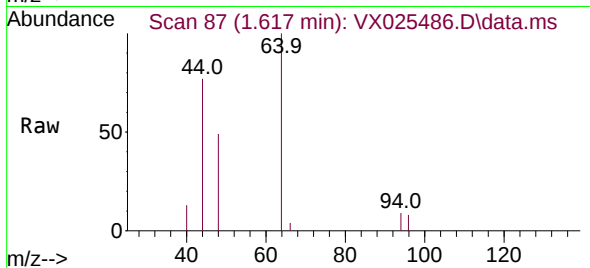

#6
Chloroethane
Concen: 5.887 ug/l
RT: 1.526 min Scan# 72
Delta R.T. -0.153 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42

Tgt Ion: 64 Resp: 4901
Ion Ratio Lower Upper
64 100
66 8.2 25.6 38.4#


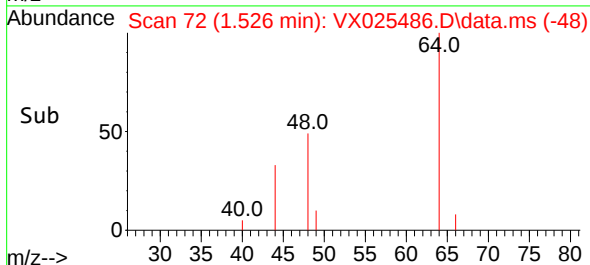

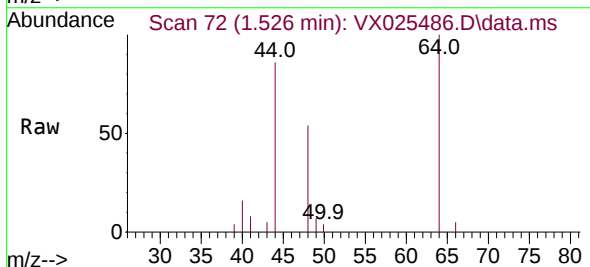




#11
Tert butyl alcohol
Concen: 322.568 ug/l
RT: 2.959 min Scan# 308
Delta R.T. -0.006 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 59 Resp: 85426
Ion Ratio Lower Upper
59 100
57 10.2 8.5 12.7

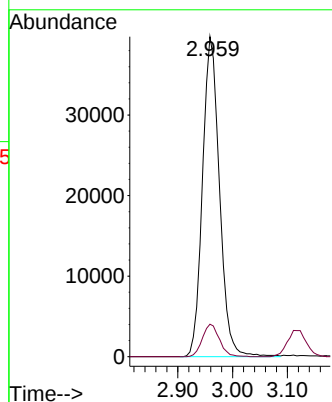

#13
Acrolein
Concen: 2.265 ug/l
RT: 2.215 min Scan# 185
Delta R.T. -0.018 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42

Tgt Ion: 56 Resp: 112
Ion Ratio Lower Upper
56 100
55 2499.1 58.6 87.8#

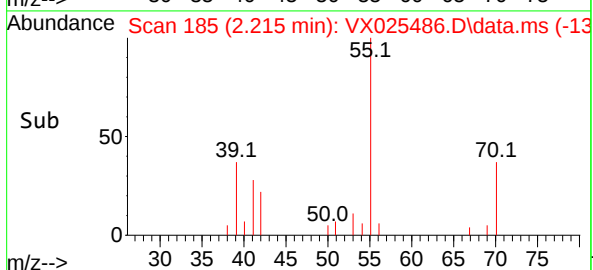

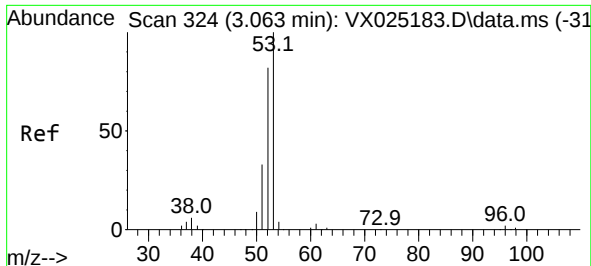

#15

Acrylonitrile

Concen: 0.628 ug/l

RT: 3.123 min Scan# 31

Delta R.T. 0.060 min

Lab File: VX025486.D

Acq: 03 Dec 2021 16:42

Instrument :

MSVOA_X

ClientSampleId :

MW-40





Tgt Ion: 53 Resp: 364

Ion Ratio Lower Upper

53 100

52 0.0 66.2 99.4#

51 43.4 29.8 44.8

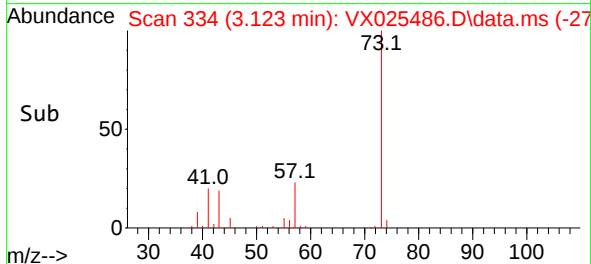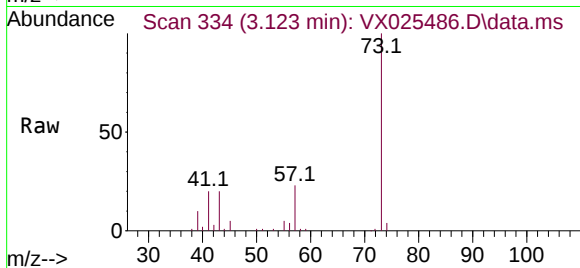

#16

Acetone

Concen: 2.426 ug/l

RT: 2.386 min Scan# 213

Delta R.T. 0.006 min

Lab File: VX025486.D




Acq: 03 Dec 2021 16:42


Tgt Ion: 43 Resp: 1455

Ion Ratio Lower Upper

43 100

58 22.9 24.0 36.0#

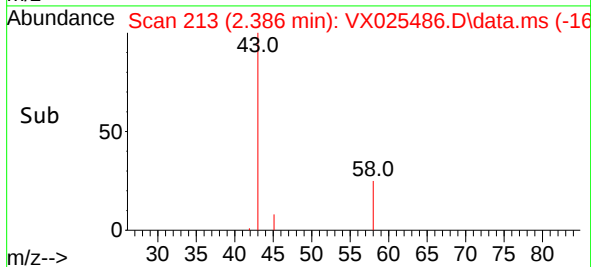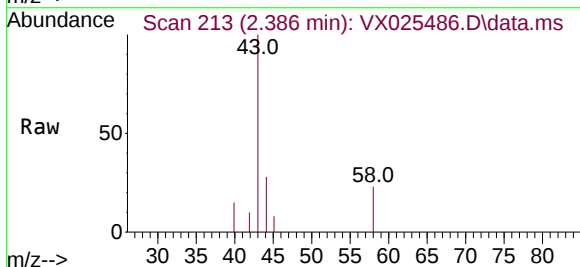



#18

Methyl Acetate

Concen: 0.264 ug/l

RT: 2.788 min Scan# 21

Delta R.T. 0.085 min

Lab File: VX025486.D

Acq: 03 Dec 2021 16:42

Instrument :

MSVOA_X

ClientSampleId :





MW-40

Tgt Ion: 43 Resp: 506

Ion Ratio Lower Upper

43 100

74 0.0 19.0 28.6#

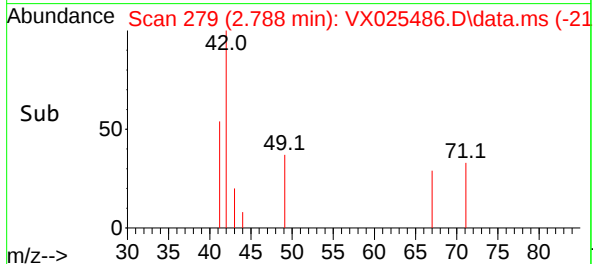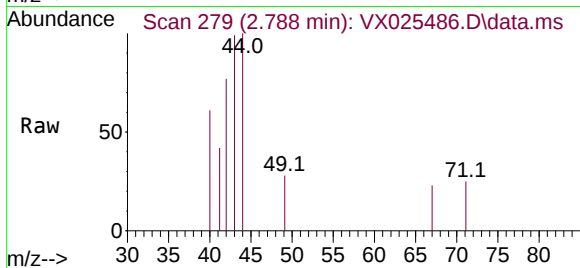

#19

Methyl tert-butyl Ether

Concen: 10.441 ug/l

RT: 3.117 min Scan# 333

Delta R.T. 0.000 min

Lab File: VX025486.D




Acq: 03 Dec 2021 16:42


Tgt Ion: 73 Resp: 34527

Ion Ratio Lower Upper

73 100

57 21.0 17.5 26.3


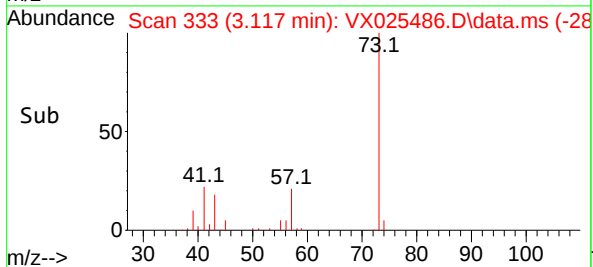

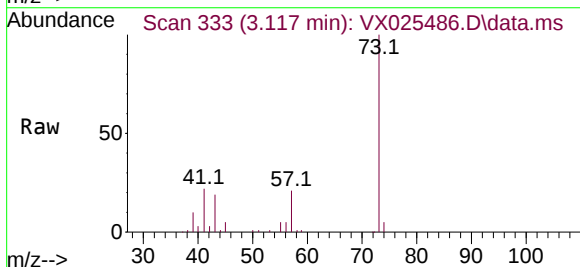


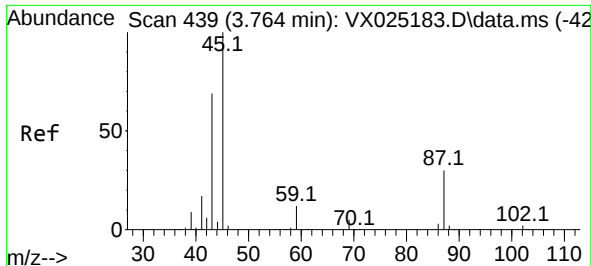

#22
Diisopropyl ether
Concen: 7.029 ug/l
RT: 3.763 min Scan# 41
Delta R.T. -0.001 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:	45	Resp:	22992
Ion	Ratio	Lower	Upper
45	100		
43	52.5	58.3	87.5#
87	30.5	23.7	35.5
59	11.3	9.4	14.0

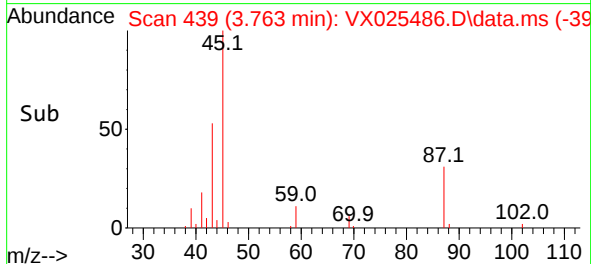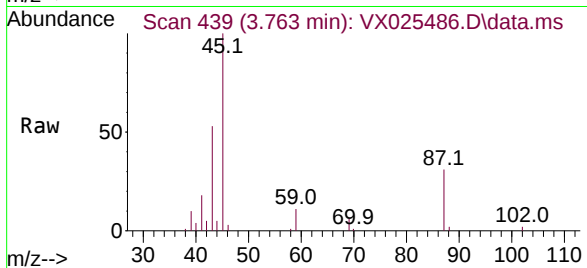

#23
Vinyl Acetate
Concen: 4.509 ug/l
RT: 3.763 min Scan# 439
Delta R.T. 0.042 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42

Tgt Ion:	43	Resp:	11847
Ion	Ratio	Lower	Upper
43	100		
86	0.0	8.2	12.4#

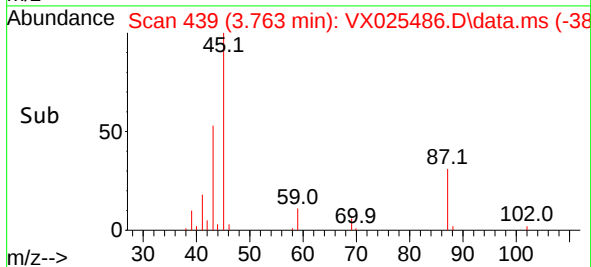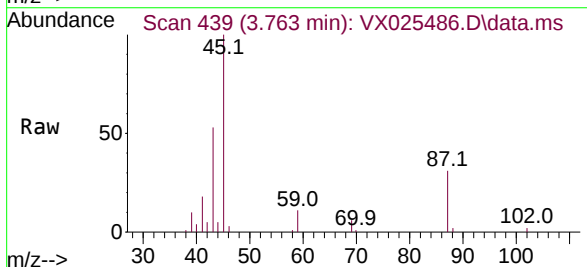



#29

Tetrahydrofuran

Concen: 0.577 ug/l

RT: 5.013 min Scan# 64

Delta R.T. 0.006 min

Lab File: VX025486.D

Acq: 03 Dec 2021 16:42

Instrument :

MSVOA_X

ClientSampleId :

MW-40





Tgt Ion: 42 Resp: 310

Ion Ratio Lower Upper

42 100

72 0.0 36.1 54.1#

71 57.1 33.7 50.5#

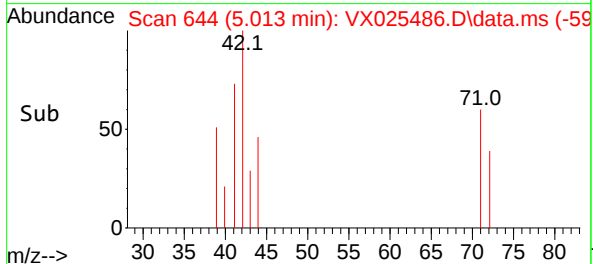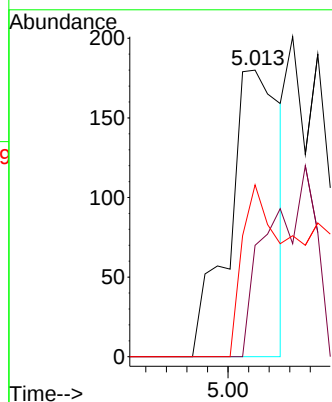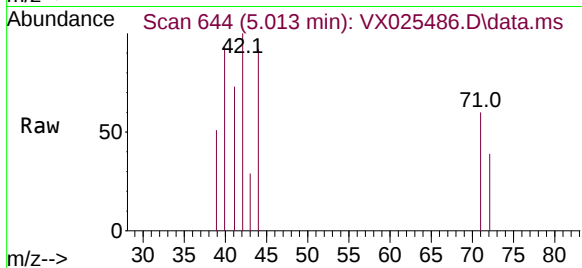

#31

Cyclohexane

Concen: 0.803 ug/l

RT: 5.476 min Scan# 720

Delta R.T. 0.005 min

Lab File: VX025486.D

Acq: 03 Dec 2021 16:42




Tgt Ion: 56 Resp: 1340


Ion Ratio Lower Upper

56 100

69 28.9 24.2 36.2

84 87.9 71.5 107.3

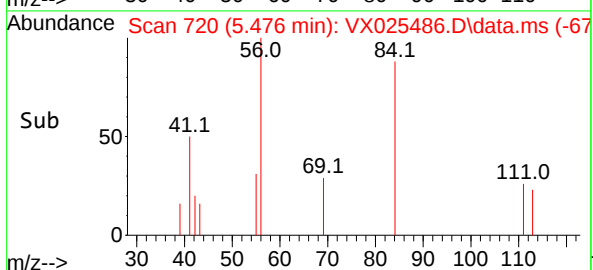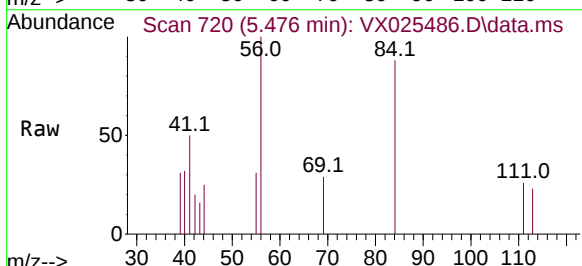

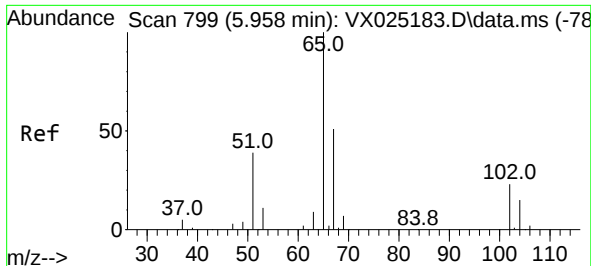

#33

1,2-Dichloroethane-d4

Concen: 56.632 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX025486.D

Acq: 03 Dec 2021 16:42

Instrument :

MSVOA_X

ClientSampleId :





MW-40

Tgt Ion: 65 Resp: 61123

Ion Ratio Lower Upper

65 100

67 52.2 0.0 101.0

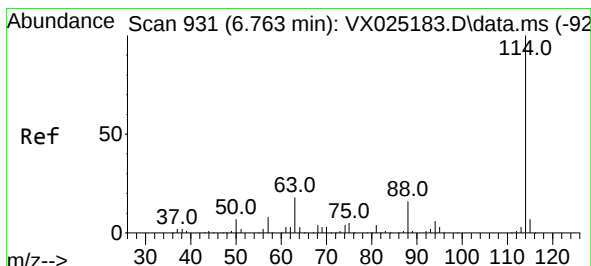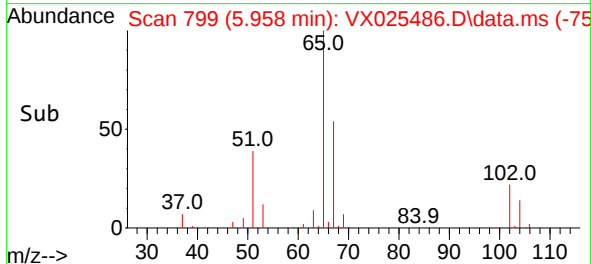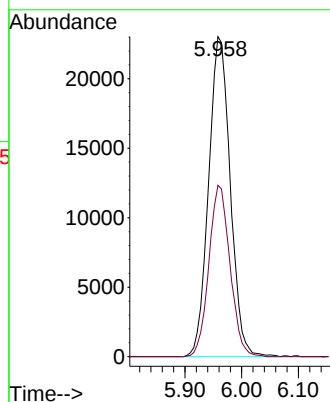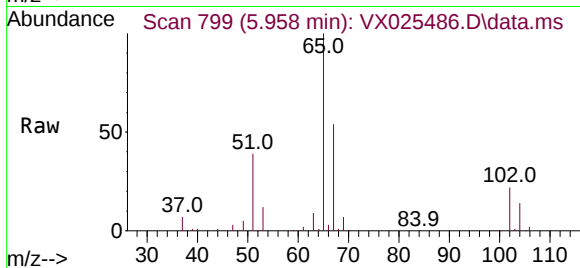

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX025486.D

Acq: 03 Dec 2021 16:42




Tgt Ion: 114 Resp: 174173


Ion Ratio Lower Upper

114 100

63 18.7 0.0 41.0

88 14.8 0.0 34.8


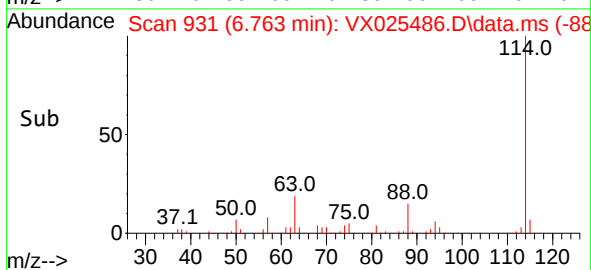

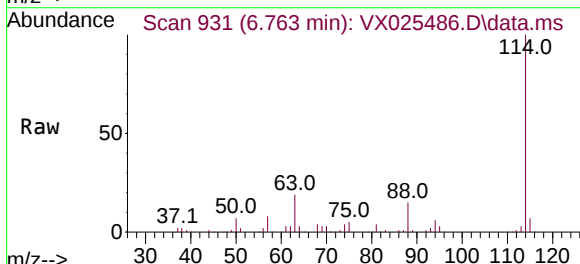




#35
Dibromofluoromethane
Concen: 50.271 ug/l
RT: 5.391 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:113 Resp: 53723
Ion Ratio Lower Upper
113 100
111 102.9 82.1 123.1
192 21.0 15.6 23.4

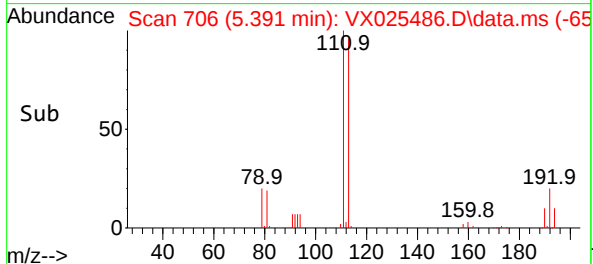

#36
1,1-Dichloropropene
Concen: 4.543 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.134 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42

Tgt Ion: 75 Resp: 6903
Ion Ratio Lower Upper
75 100
110 8.6 18.1 54.3#
77 0.0 24.4 36.6#

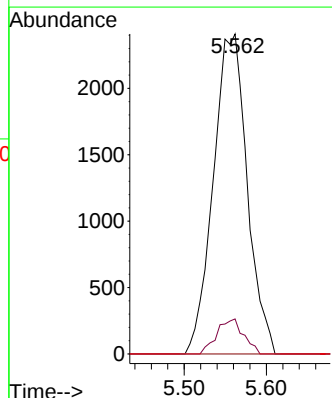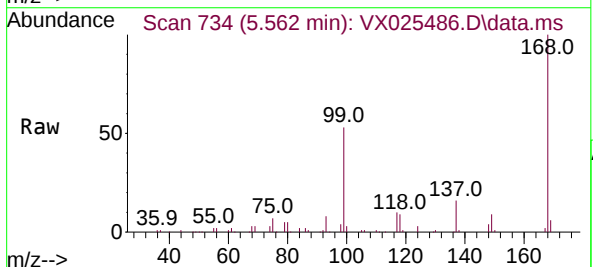



#38

Carbon Tetrachloride

Concen: 5.841 ug/l

RT: 5.556 min Scan# 71

Delta R.T. -0.122 min

Lab File: VX025486.D

Acq: 03 Dec 2021 16:42

Instrument :

MSVOA_X

ClientSampleId :

MW-40





Tgt Ion:117 Resp: 9776

Ion Ratio Lower Upper

117 100

119 5.3 75.6 113.4#

121 0.0 23.7 35.5#

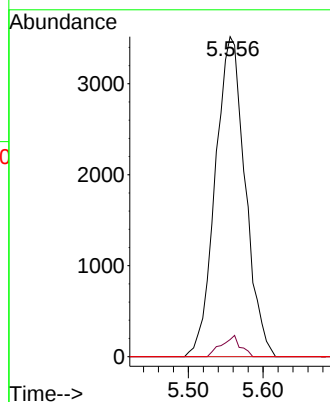

#39

Methylcyclohexane

Concen: 0.378 ug/l

RT: 7.385 min Scan# 1033

Delta R.T. -0.000 min

Lab File: VX025486.D

Acq: 03 Dec 2021 16:42




Tgt Ion: 83 Resp: 736


Ion Ratio Lower Upper

83 100

55 75.3 60.8 91.2

98 33.4 37.0 55.4#


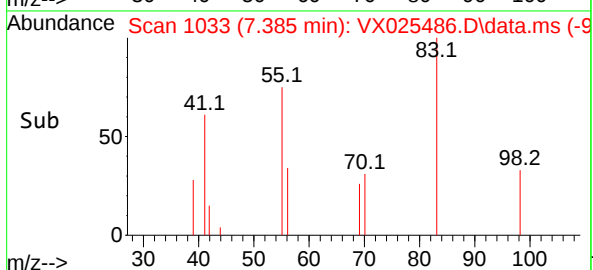






#40
Benzene
Concen: 76.178 ug/l
RT: 6.043 min Scan# 81
Delta R.T. -0.001 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 78 Resp: 350668
Ion Ratio Lower Upper
78 100
77 23.5 18.3 27.5

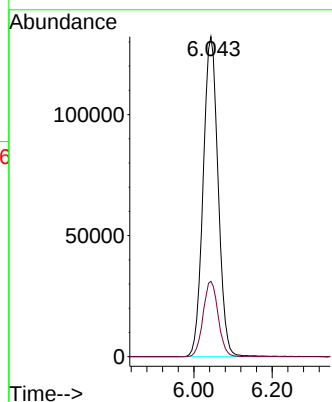

#42
1,2-Dichloroethane
Concen: 2.084 ug/l
RT: 6.037 min Scan# 812
Delta R.T. -0.049 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42

Tgt Ion: 62 Resp: 3121
Ion Ratio Lower Upper
62 100
98 0.0 0.0 16.0

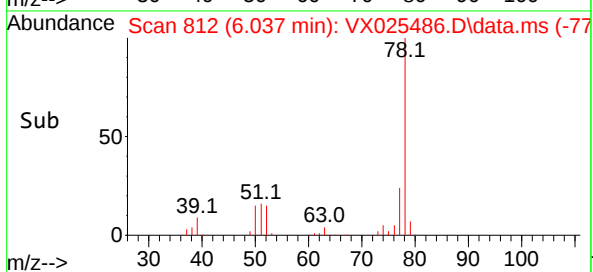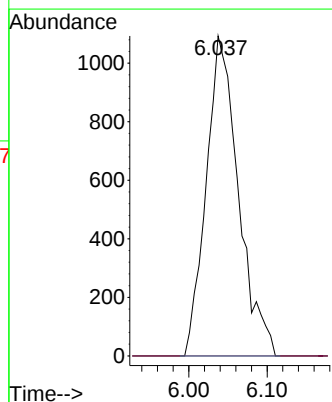



#48

Methyl methacrylate

Concen: 0.352 ug/l

RT: 7.903 min Scan# 1118

Delta R.T. 0.207 min

Lab File: VX025486.D

Acq: 03 Dec 2021 16:42

Instrument :

MSVOA_X

ClientSampleId :

MW-40





Tgt Ion: 41 Resp: 475

Ion Ratio Lower Upper

41 100

69 0.0 64.5 96.7#

39 38.9 46.9 70.3#

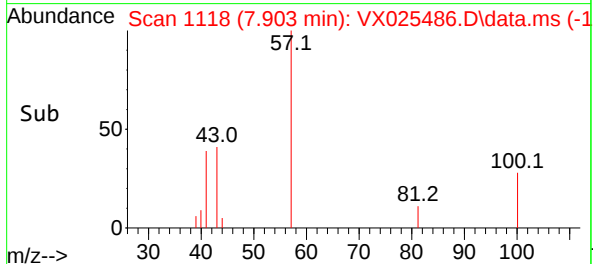

#50

Toluene-d8

Concen: 49.749 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX025486.D




Acq: 03 Dec 2021 16:42


Tgt Ion: 98 Resp: 199895

Ion Ratio Lower Upper

98 100

100 66.4 51.4 77.0


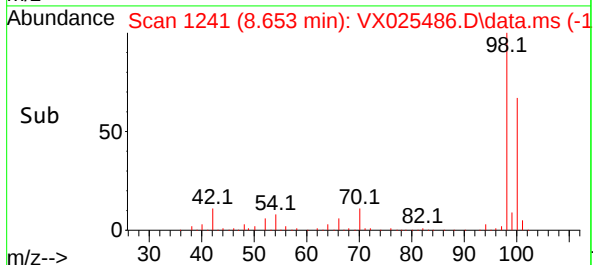

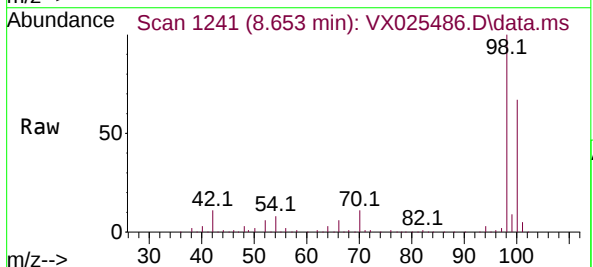




#51
4-Methyl-2-Pentanone
Concen: 0.282 ug/l
RT: 8.573 min Scan# 11
Delta R.T. -0.001 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 43 Resp: 508
Ion Ratio Lower Upper
43 100
58 34.6 30.9 46.3

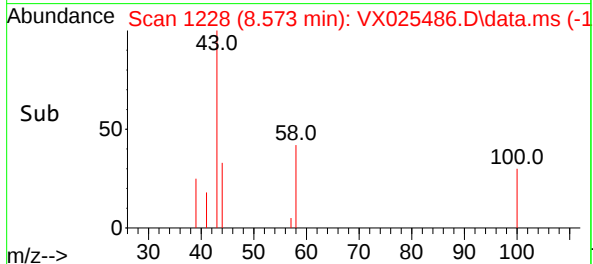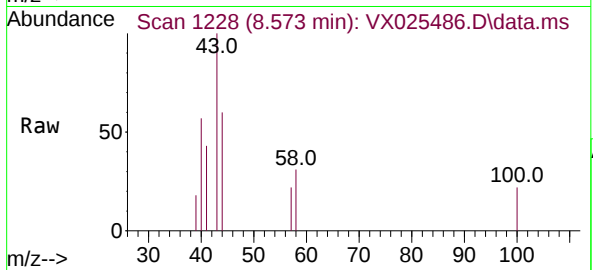

#52
Toluene
Concen: 0.440 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. 0.006 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42

Tgt Ion: 92 Resp: 1323
Ion Ratio Lower Upper
92 100
91 169.4 138.6 208.0

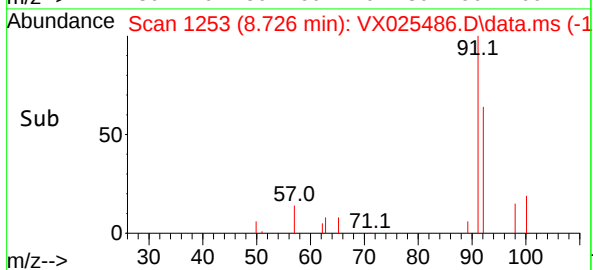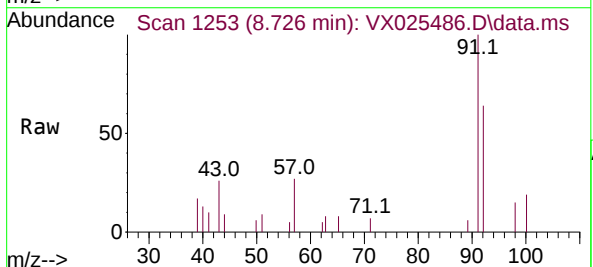



#59

2-Hexanone

Concen: 2.430 ug/l

RT: 9.457 min Scan# 1

Delta R.T. 0.024 min

Lab File: VX025486.D

Acq: 03 Dec 2021 16:42

Instrument :

MSVOA_X

ClientSampleId :





MW-40

Tgt Ion: 43 Resp: 3456

Ion Ratio Lower Upper

43 100

58 44.2 26.6 79.7

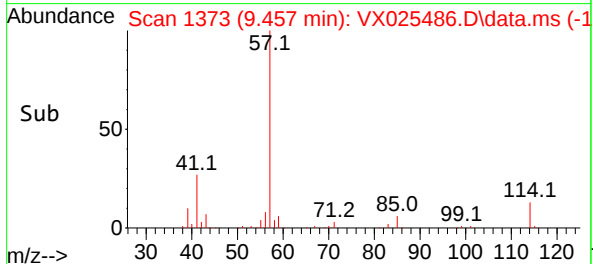

#62

4-Bromofluorobenzene

Concen: 46.305 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. 0.006 min

Lab File: VX025486.D

Acq: 03 Dec 2021 16:42




Tgt Ion: 95 Resp: 70387


Ion Ratio Lower Upper

95 100

174 83.8 0.0 158.0

176 81.4 0.0 153.6


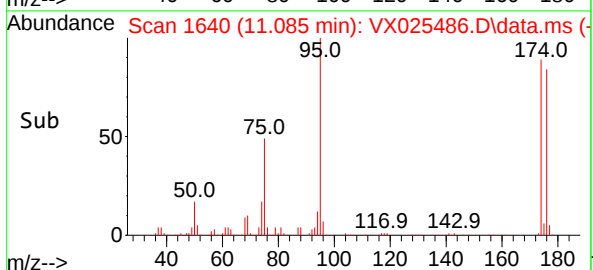
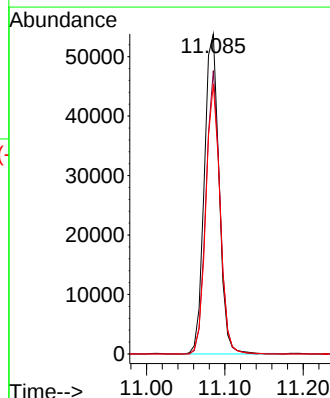





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:117 Resp: 157508
Ion Ratio Lower Upper
117 100
82 50.4 44.6 67.0
119 31.9 24.8 37.2

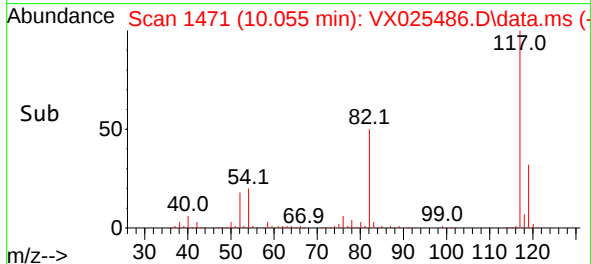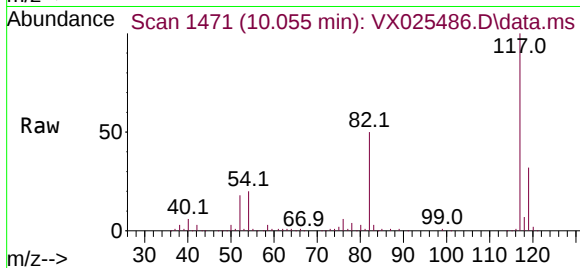

#67
Ethyl Benzene
Concen: 0.676 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42

Tgt Ion: 91 Resp: 3751
Ion Ratio Lower Upper
91 100
106 29.1 24.7 37.1


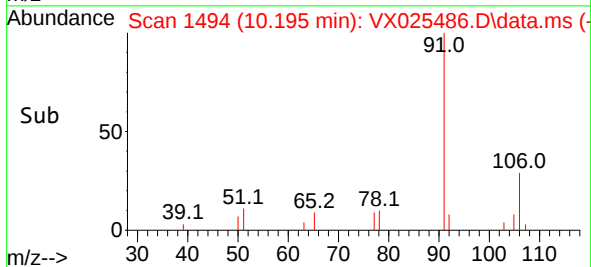

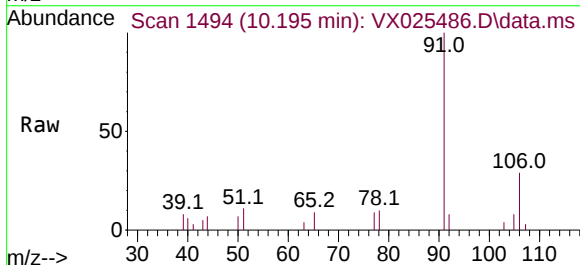




#68
m/p-Xylenes
Concen: 0.533 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:106 Resp: 1208
Ion Ratio Lower Upper
106 100
91 185.0 163.4 245.0

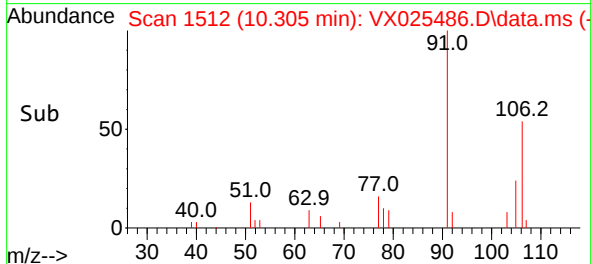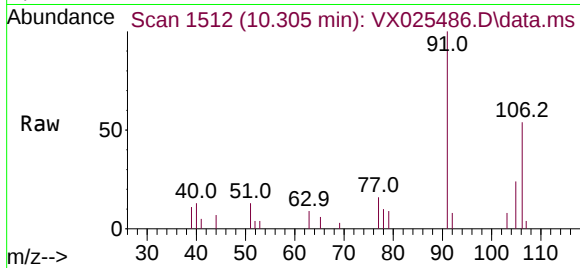

#69
o-Xylene
Concen: 0.630 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.001 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42

Tgt Ion:106 Resp: 1397
Ion Ratio Lower Upper
106 100
91 234.6 109.5 328.4


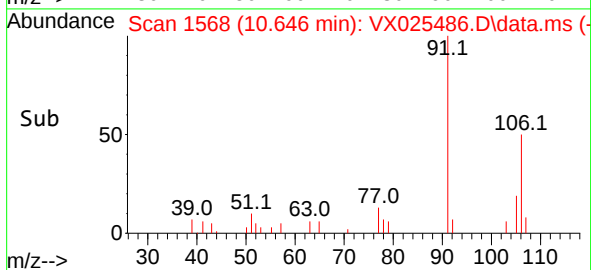

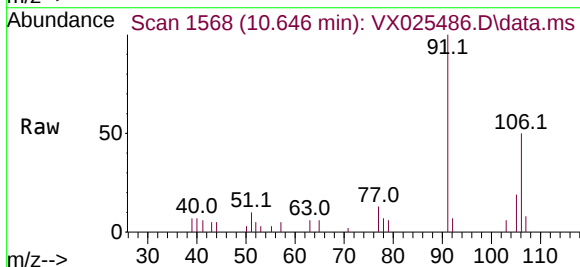




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:152 Resp: 70421
Ion Ratio Lower Upper
152 100
115 56.9 43.3 129.8
150 157.9 0.0 351.2

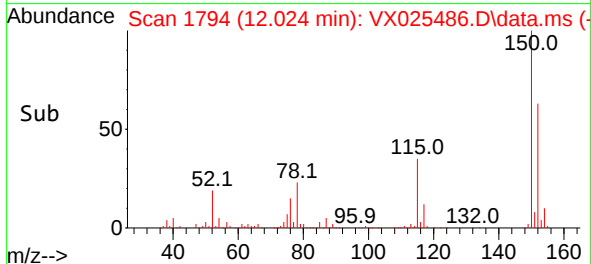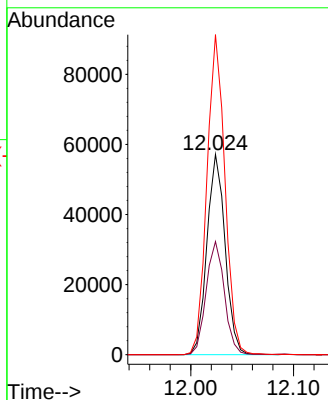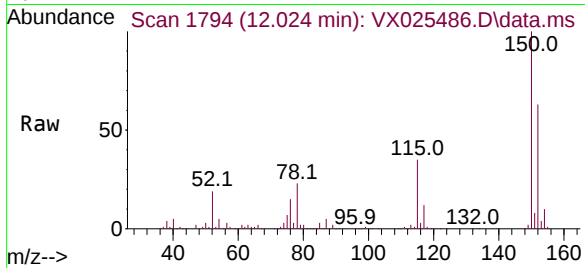

#73
Isopropylbenzene
Concen: 0.727 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.001 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42

Tgt Ion:105 Resp: 3648
Ion Ratio Lower Upper
105 100
120 27.6 13.3 39.8


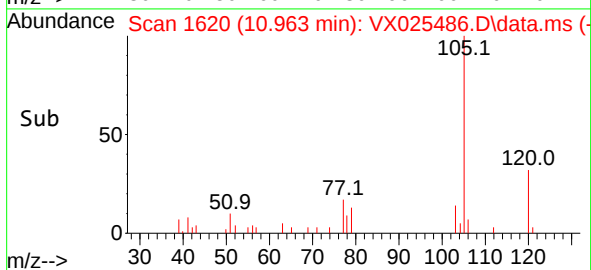
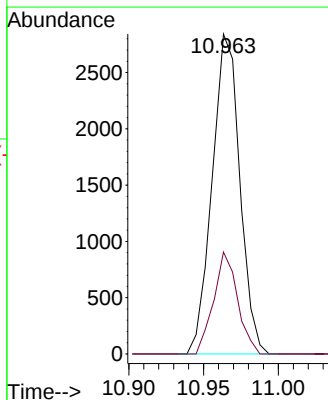
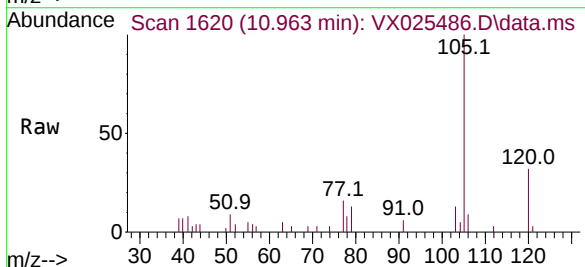




#74
N-amy1 acetate
Concen: 0.526 ug/l
RT: 10.890 min Scan# 1
Delta R.T. 0.048 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion: 43	Resp:	1142
Ion	Ratio	Lower Upper
43	100	
70	6.2	33.7 50.5#
55	10.3	19.7 29.5#
61	0.0	19.0 28.4#

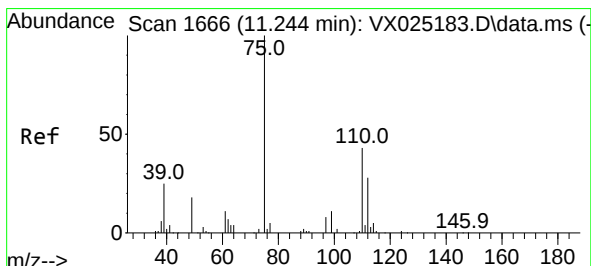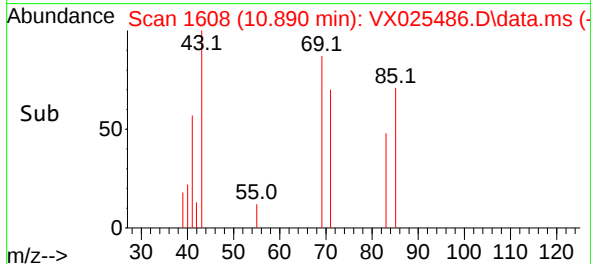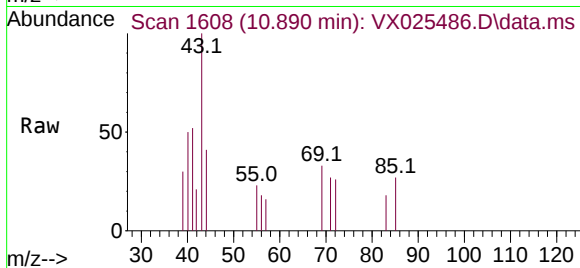

#76
1,2,3-Trichloropropane
Concen: 23.870 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42

Tgt Ion: 75	Resp:	34423
Ion	Ratio	Lower Upper
75	100	
77	1.0	20.0 59.9#


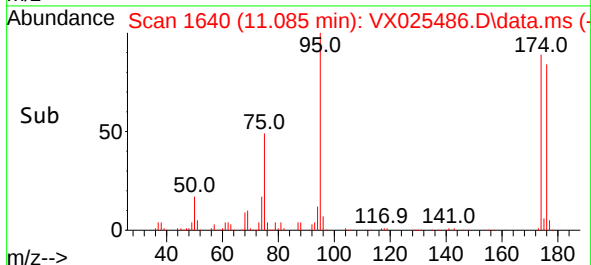

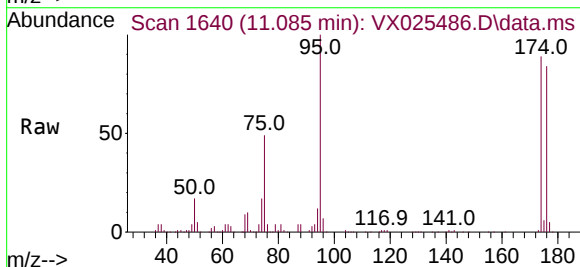


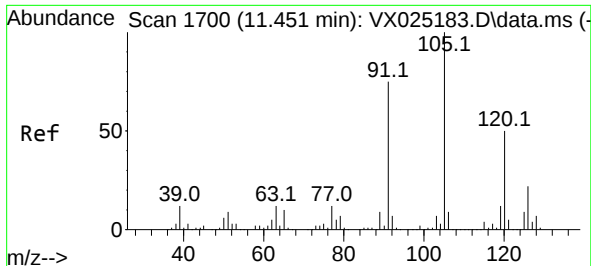

#80
1,3,5-Trimethylbenzene
Concen: 0.436 ug/l
RT: 11.457 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42




Instrument :
MSVOA_X
ClientSampleId :
MW-40


Tgt Ion:105 Resp: 1839
Ion Ratio Lower Upper
105 100
120 43.7 23.8 71.5

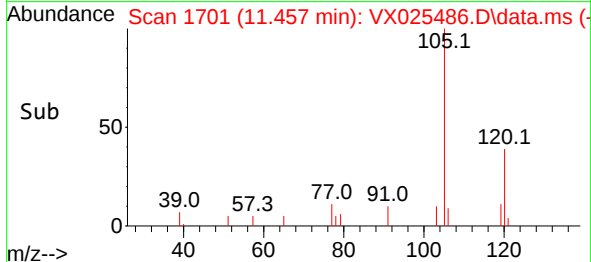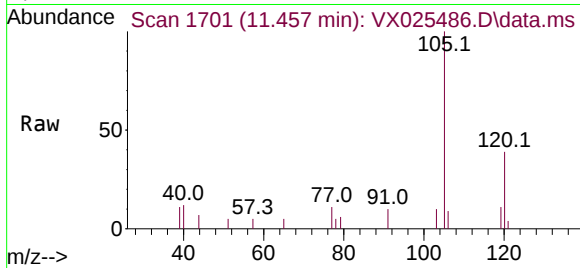

#81
trans-1,4-Dichloro-2-butene
Concen: 60.134 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.067 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42

Tgt Ion: 75 Resp: 34423
Ion Ratio Lower Upper
75 100
53 0.0 81.9 122.9#
89 0.0 38.2 57.2#


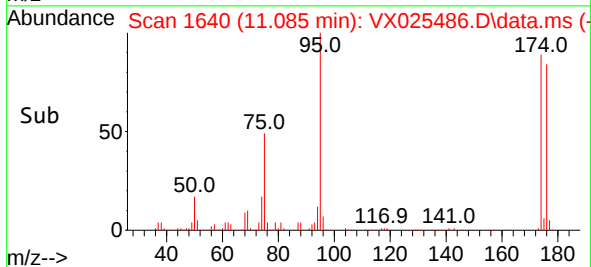

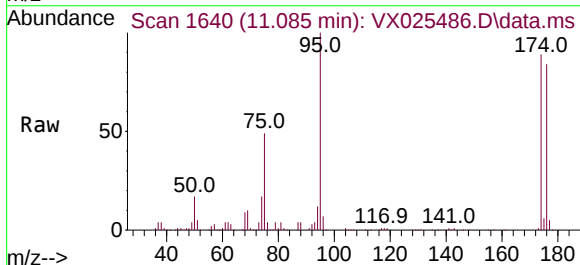


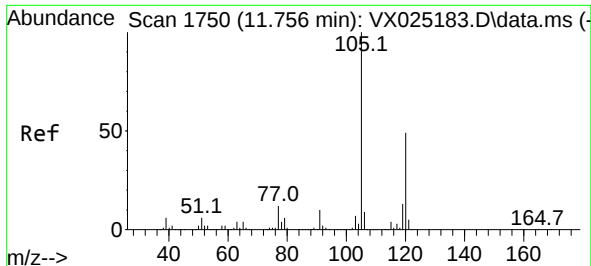

#84
 1,2,4-Trimethylbenzene
 Concen: 0.676 ug/l
 RT: 11.756 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX025486.D
 Acq: 03 Dec 2021 16:42




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-40


Tgt Ion:105 Resp: 2820
 Ion Ratio Lower Upper
 105 100
 120 47.7 22.1 66.3

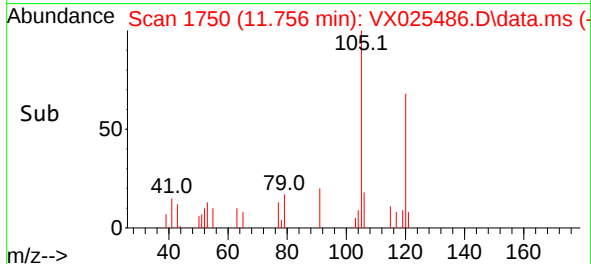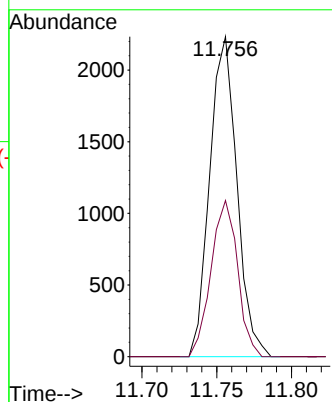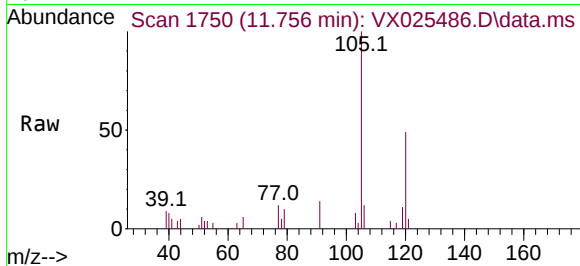

#90
 Hexachloroethane
 Concen: 0.423 ug/l
 RT: 12.646 min Scan# 1896
 Delta R.T. 0.103 min
 Lab File: VX025486.D
 Acq: 03 Dec 2021 16:42


Tgt Ion:117 Resp: 349
 Ion Ratio Lower Upper
 117 100
 201 0.0 38.9 116.6#

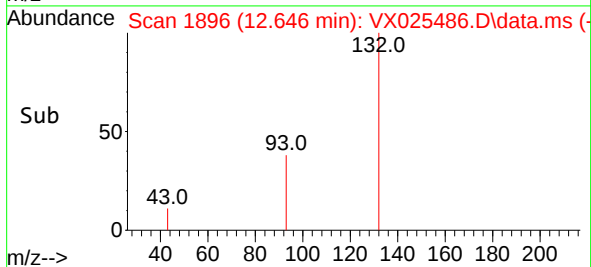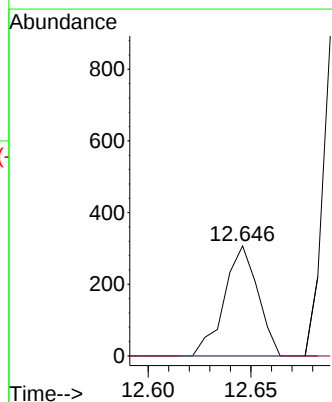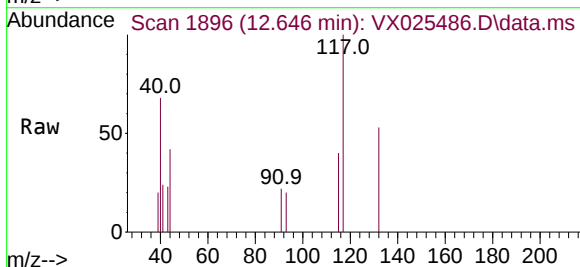



#95
Naphthalene
Concen: Below Cal
RT: 13.780 min Scan# 20
Delta R.T. -0.000 min
Lab File: VX025486.D
Acq: 03 Dec 2021 16:42

Instrument :
MSVOA_X
ClientSampleId :
MW-40

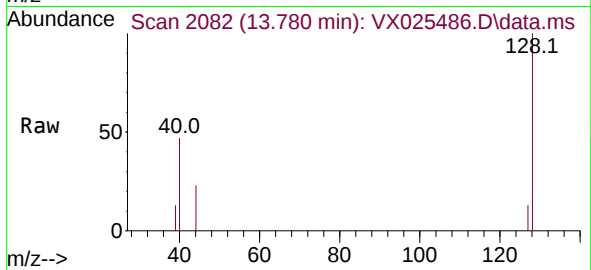

Tgt Ion:128 Resp: 567
Ion Ratio Lower Upper
128 100
127 8.1 10.3 15.5#
129 0.0 8.8 13.2#

