


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120321\
Data File : VX025498.D
Acq On : 03 Dec 2021 21:47
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Title : SW846 8260
Last Update : Wed Nov 17 15:36:16 2021

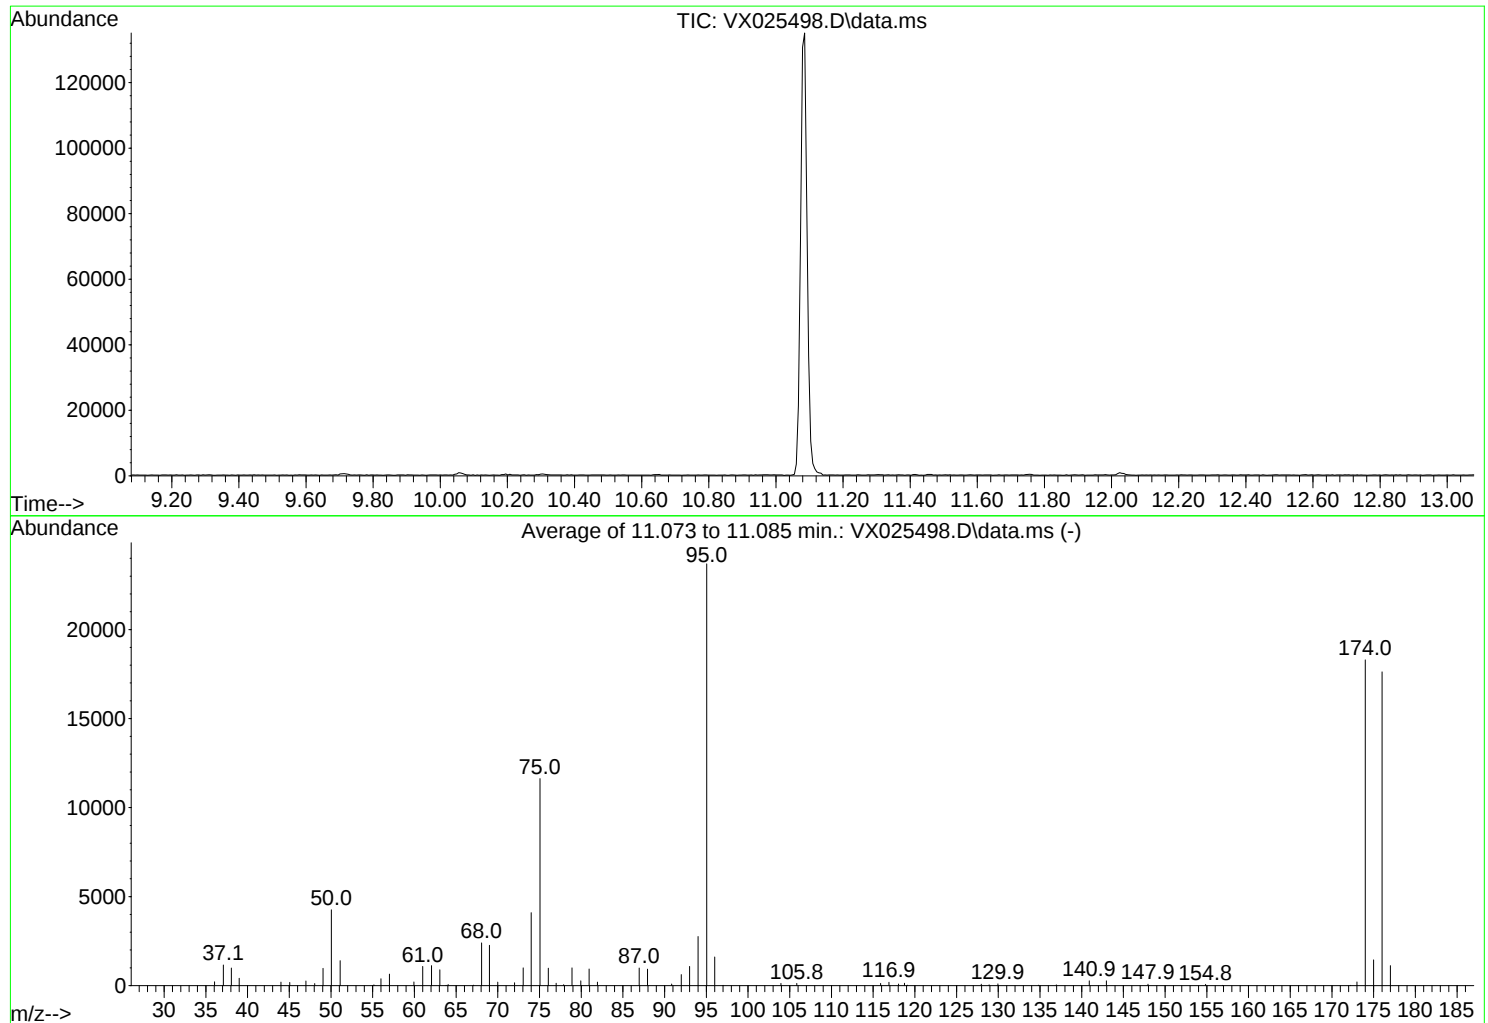

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.0	4263	PASS
75	95	30	60	49.1	11627	PASS
95	95	100	100	100.0	23690	PASS
96	95	5	9	6.8	1611	PASS
173	174	0.00	2	1.1	205	PASS
174	95	50	100	77.2	18295	PASS
175	174	5	9	7.9	1450	PASS
176	174	95	101	96.3	17623	PASS
177	176	5	9	6.4	1127	PASS