

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120325\
 Data File : VX048702.D
 Acq On : 03 Dec 2025 13:47
 Operator : JC/MD
 Sample : VX1203MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1203MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120325W.M
 Title : SW846 8260

Signal : TIC: VX048702.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.532	554	565	578	rBV3	4306	16750	1.91%	0.354%
2	5.373	692	703	721	rBV	90313	303714	34.65%	6.422%
3	5.538	721	730	749	rVB3	141383	445873	50.87%	9.428%
4	5.940	787	796	810	rBV2	92180	271521	30.98%	5.741%
5	6.745	917	928	952	rBV	218874	576541	65.77%	12.191%
6	8.635	1231	1238	1256	rBV	422937	720974	82.25%	15.245%
7	10.037	1462	1468	1483	rBV	559255	805016	91.84%	17.022%
8	11.061	1631	1636	1649	rBV	430554	597953	68.22%	12.643%
9	11.439	1694	1698	1707	rVB2	8945	12735	1.45%	0.269%
10	11.695	1736	1740	1744	rBV	7205	9352	1.07%	0.198%
11	11.872	1764	1769	1774	rVB2	8489	10914	1.25%	0.231%
12	12.000	1785	1790	1804	rVB	628609	876558	100.00%	18.534%
13	12.317	1837	1842	1850	rBV2	14227	18452	2.11%	0.390%
14	13.268	1991	1998	2004	rBV	9010	12373	1.41%	0.262%
15	13.573	2044	2048	2055	rVB	9101	12934	1.48%	0.273%
16	13.707	2066	2070	2074	rBV2	11887	15454	1.76%	0.327%
17	13.762	2074	2079	2084	rBV	7012	9458	1.08%	0.200%
18	13.945	2104	2109	2117	rVB	9311	12778	1.46%	0.270%




Sum of corrected areas: 4729350

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120325\
Data File : VX048702.D
Acq On : 03 Dec 2025 13:47
Operator : JC/MD
Sample : VX1203MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1203MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120325W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

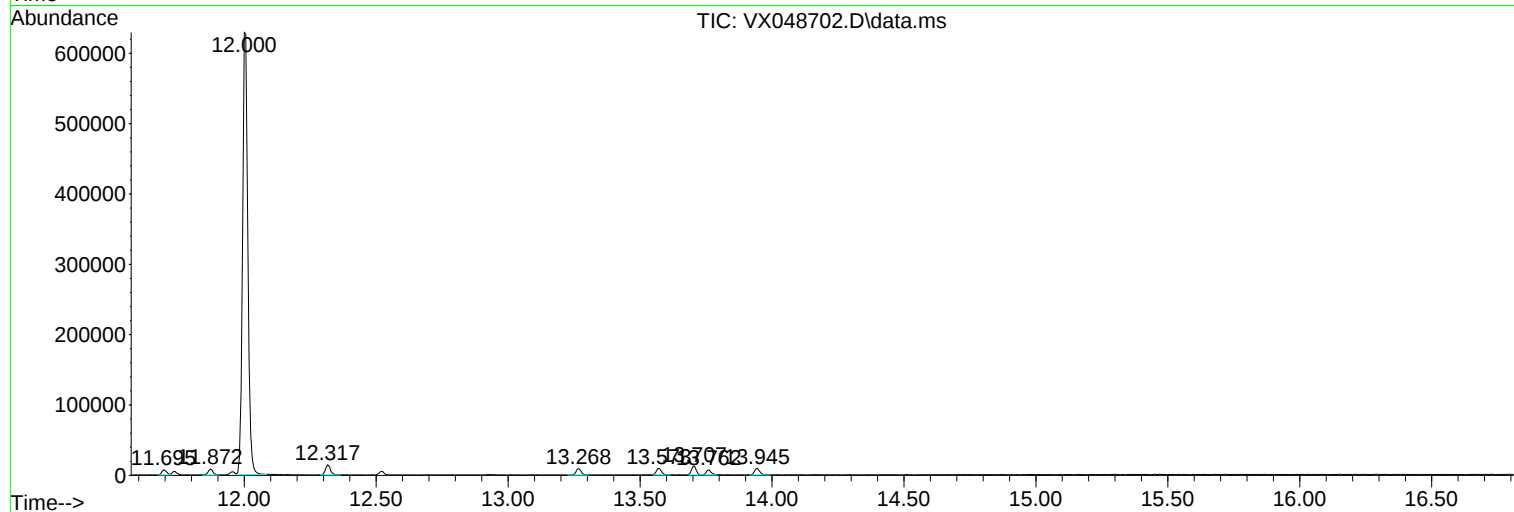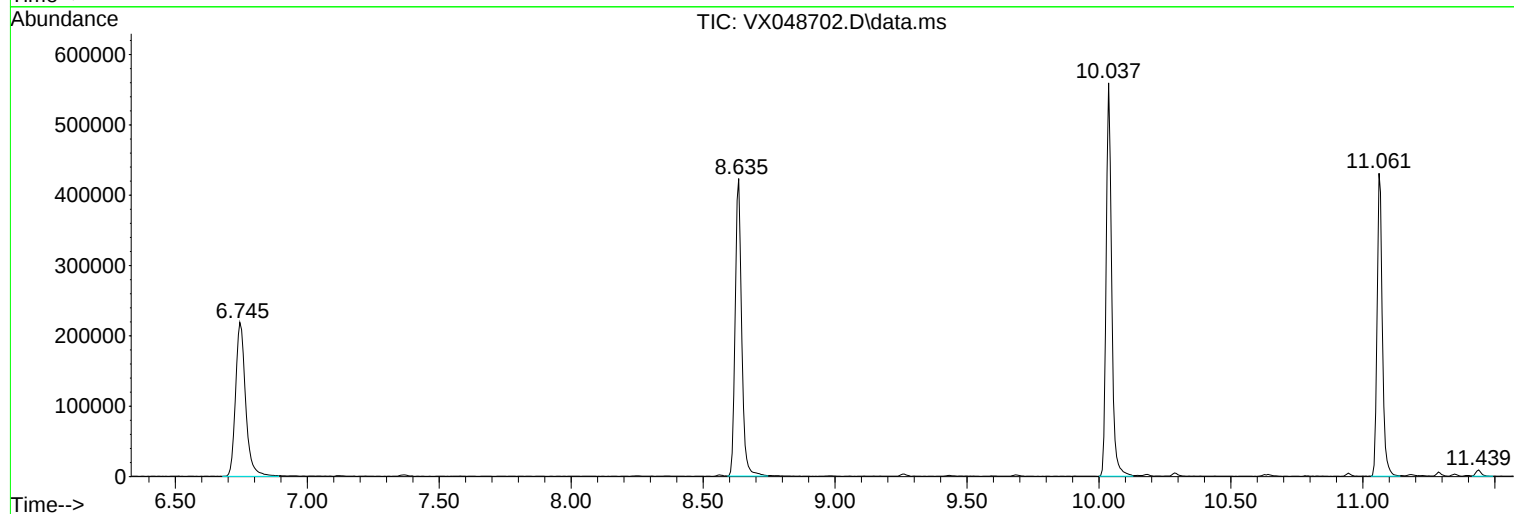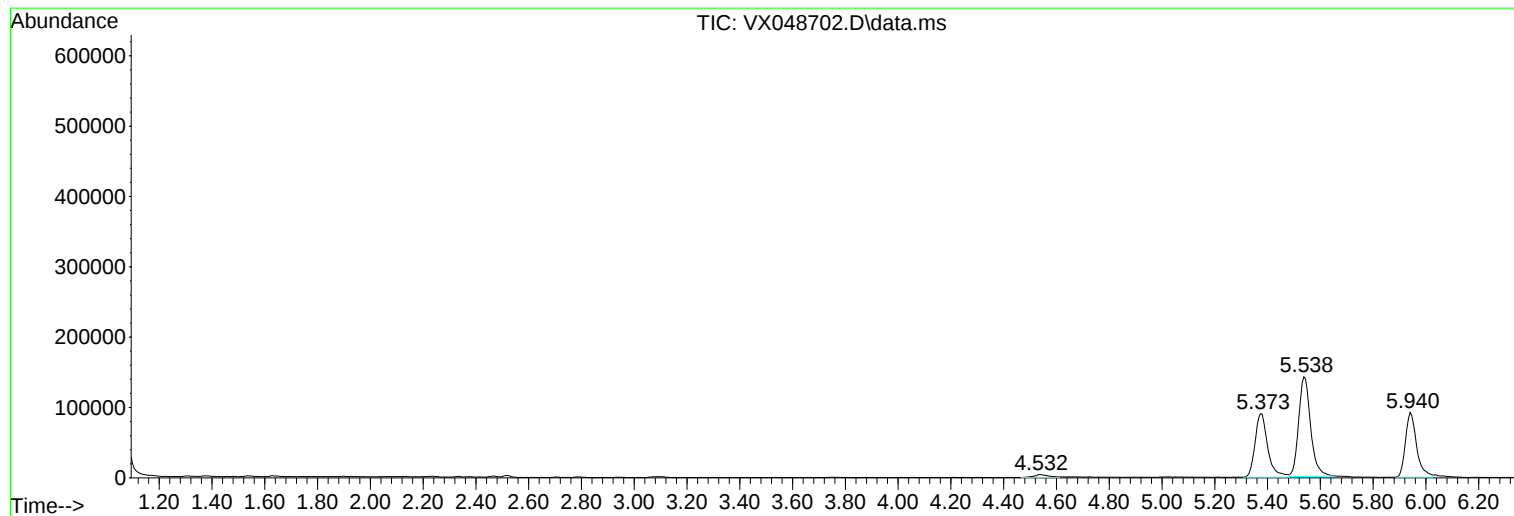

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120325\
Data File : VX048702.D
Acq On : 03 Dec 2025 13:47
Operator : JC/MD
Sample : VX1203MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1203MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120325W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120325\
Data File : VX048702.D
Acq On : 03 Dec 2025 13:47
Operator : JC/MD
Sample : VX1203MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1203MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120325W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc