
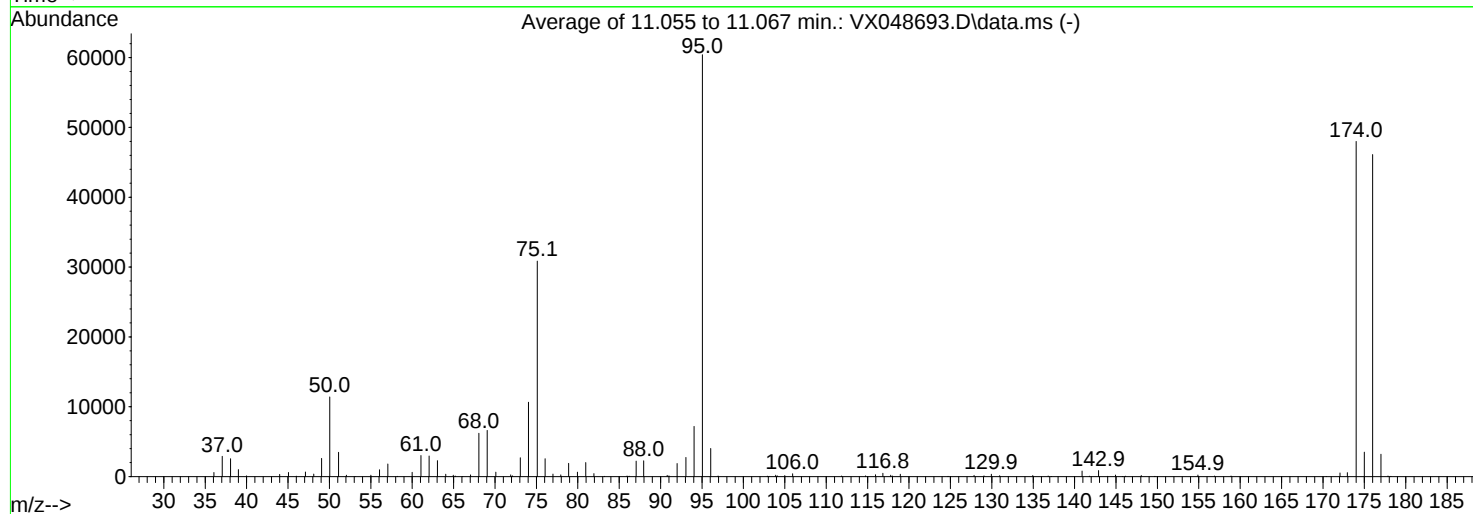


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120325\
Data File : VX048693.D
Acq On : 03 Dec 2025 08:16
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120325W.M
Title : SW846 8260
Last Update : Thu Dec 04 02:13:49 2025

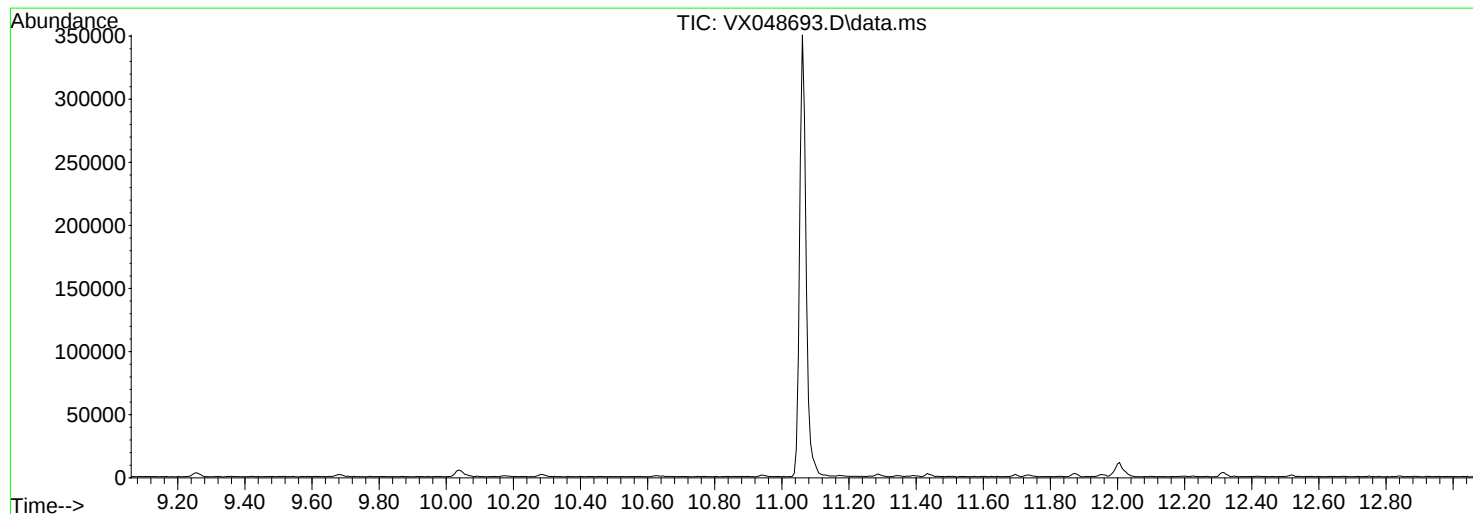

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	11390	PASS
75	95	30	60	51.1	30856	PASS
95	95	100	100	100.0	60400	PASS
96	95	5	9	6.7	4031	PASS
173	174	0.00	2	1.2	569	PASS
174	95	50	100	79.5	47997	PASS
175	174	5	9	7.3	3498	PASS
176	174	95	101	96.1	46123	PASS
177	176	5	9	6.9	3186	PASS