

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX120418\
 Data File : VX006277.D
 Acq On : 04 Dec 2018 14:42
 Operator : JC/MD
 Sample : J6215-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DSN001

Quant Time: Dec 05 00:47:06 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 30 03:55:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	842639	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	1256321	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	1134386	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	557382	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	411629	47.85	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.70%	
35) Dibromofluoromethane	5.51	113	400071	49.18	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.36%	
50) Toluene-d8	8.71	98	1465336	49.53	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.06%	
62) 4-Bromofluorobenzene	11.13	95	543209	48.72	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.44%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX120418\
Data File : VX006277.D
Acq On : 04 Dec 2018 14:42
Operator : JC/MD
Sample : J6215-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN001

Quant Time: Dec 05 00:47:06 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 30 03:55:33 2018
Response via : Initial Calibration

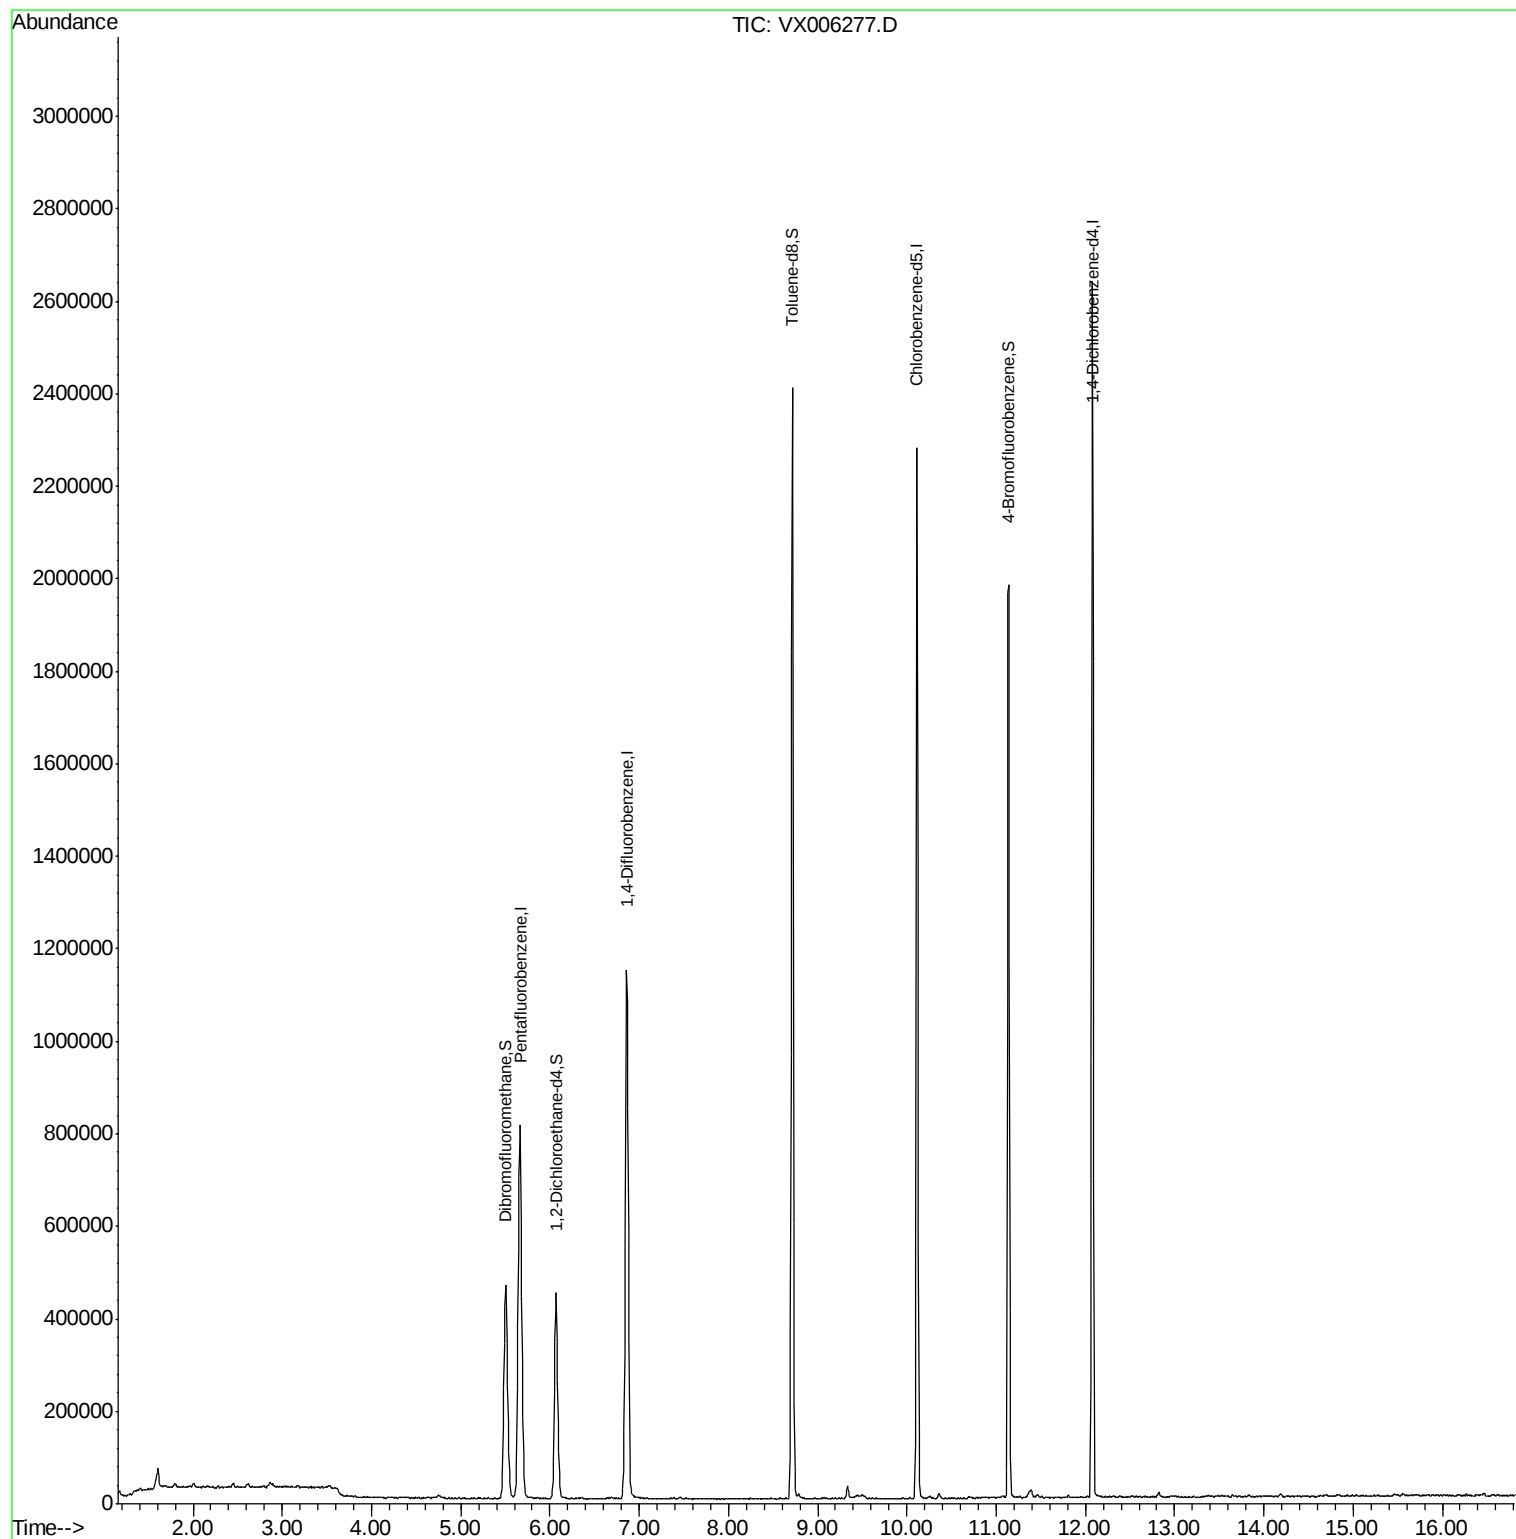

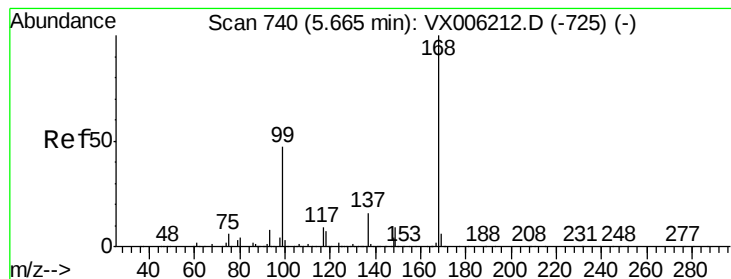

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX006277.D

Acq: 04 Dec 2018 14:42

Instrument :

MSVOA_X

ClientSampleId :


DSN001

Tgt Ion:168 Resp: 842639

Ion Ratio Lower Upper

168 100

99 50.4 37.8 56.8

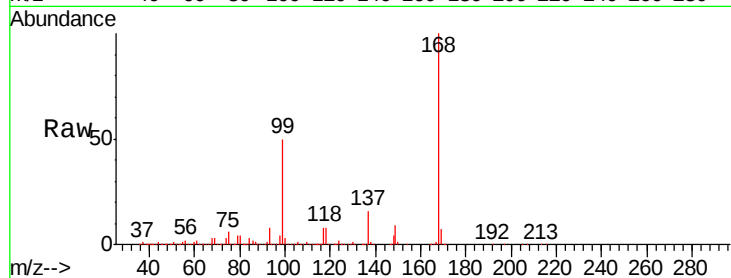

Abundance Ion 167.90 (167.60 to 168.60): VX006277.D (-691) (-)

Ion 98.90 (98.60 to 99.60): VX006277.D (-691) (-)

5.67

300000



200000

100000

0

Time-->

5.50 5.60 5.70 5.80

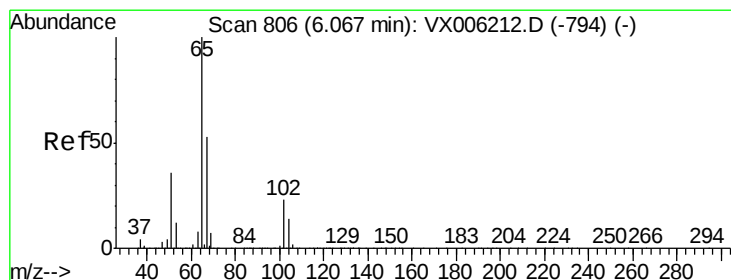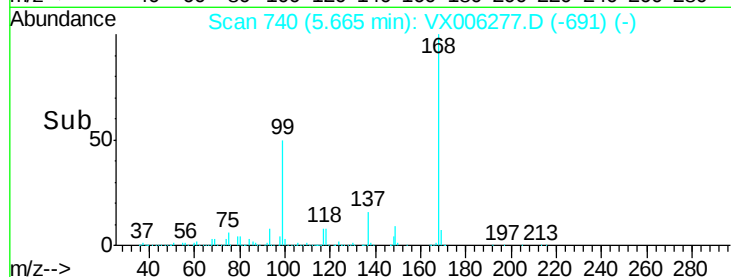

#33

1,2-Dichloroethane-d4

Concen: 47.853 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.00 min

Lab File: VX006277.D


Acq: 04 Dec 2018 14:42

Tgt Ion: 65 Resp: 411629

Ion Ratio Lower Upper

65 100

67 52.7 0.0 107.2

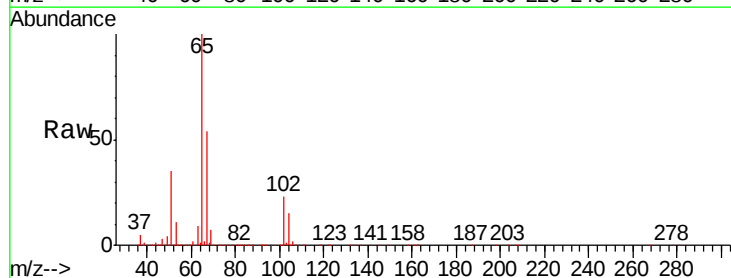

Abundance Ion 64.90 (64.60 to 65.60): VX006277.D (-757) (-)

Ion 66.90 (66.60 to 67.60): VX006277.D (-757) (-)

6.07

150000


100000


50000

0

Time-->

5.90 6.00 6.10 6.20

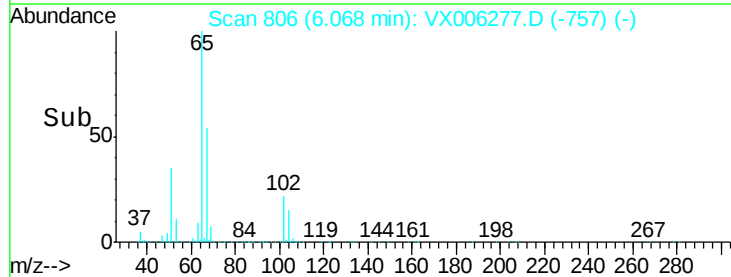

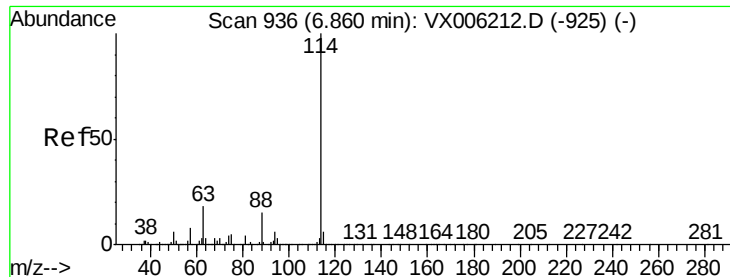

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX006277.D

Acq: 04 Dec 2018 14:42

Instrument :

MSVOA_X

ClientSampleId :

DSN001


Tgt Ion:114 Resp: 1256321

Ion Ratio Lower Upper

114 100

63 17.8 0.0 36.6




88 15.4 0.0 29.0

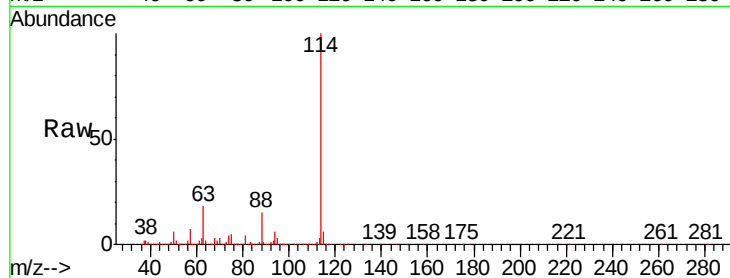

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

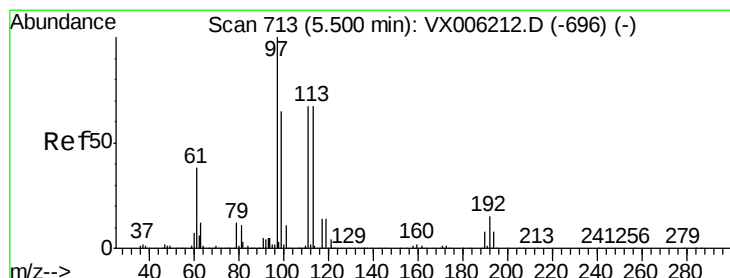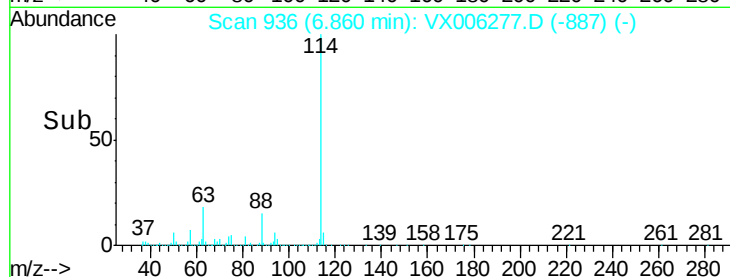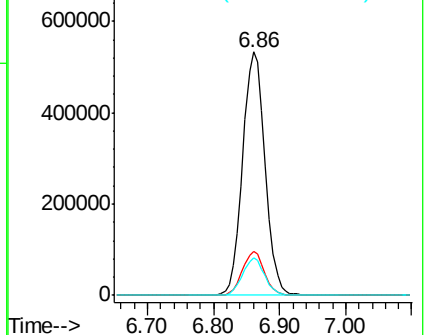

#35

Dibromofluoromethane

Concen: 49.184 ug/l

RT: 5.51 min Scan# 714

Delta R.T. 0.01 min

Lab File: VX006277.D

Acq: 04 Dec 2018 14:42


Tgt Ion:113 Resp: 400071

Ion Ratio Lower Upper

113 100

111 101.5 81.1 121.7



192 22.1 18.2 27.2

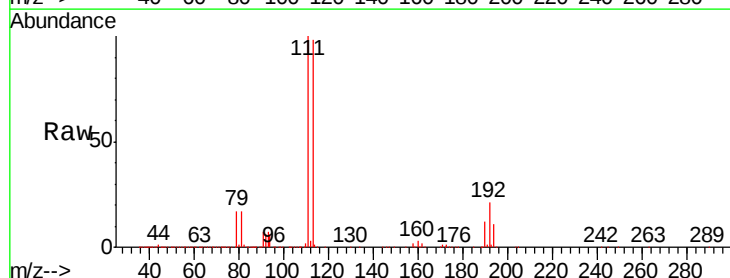


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

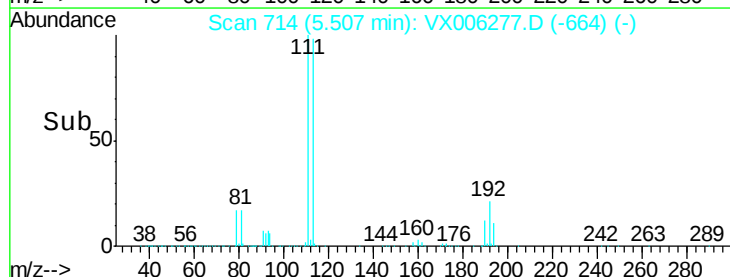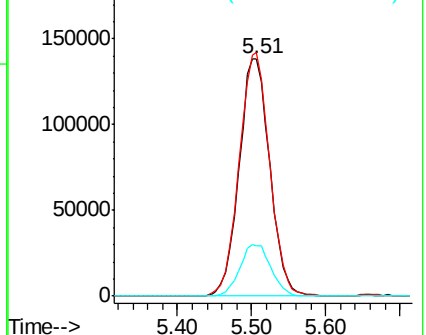

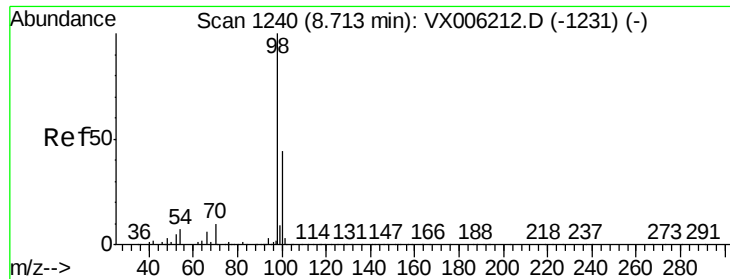

#50

Toluene-d8

Concen: 49.526 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX006277.D

Acq: 04 Dec 2018 14:42

Instrument :

MSVOA_X

ClientSampleId :


DSN001

Tgt Ion: 98 Resp: 1465336

Ion Ratio Lower Upper




98 100

100 64.9 52.2 78.2

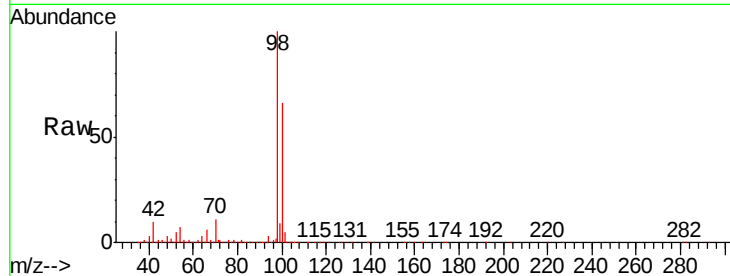

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

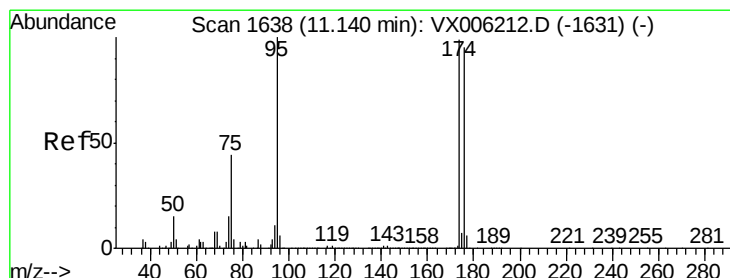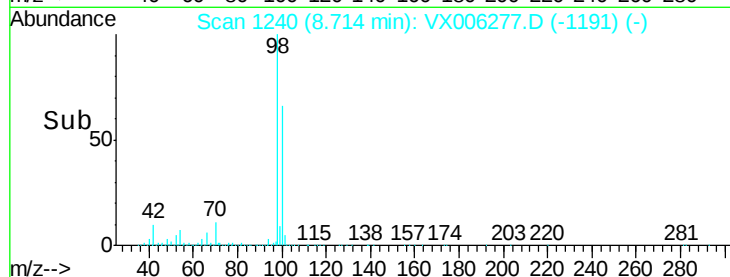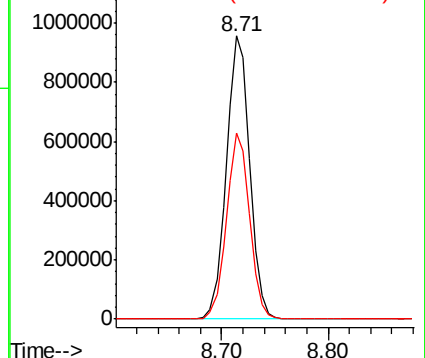

#62

4-Bromofluorobenzene

Concen: 48.721 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.01 min

Lab File: VX006277.D

Acq: 04 Dec 2018 14:42


Tgt Ion: 95 Resp: 543209

Ion Ratio Lower Upper

95 100

174 90.0 0.0 187.0



176 87.6 0.0 181.8

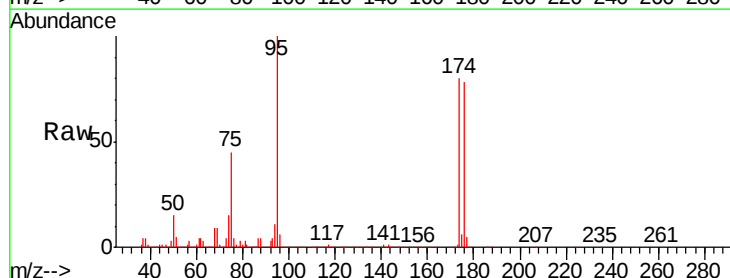


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

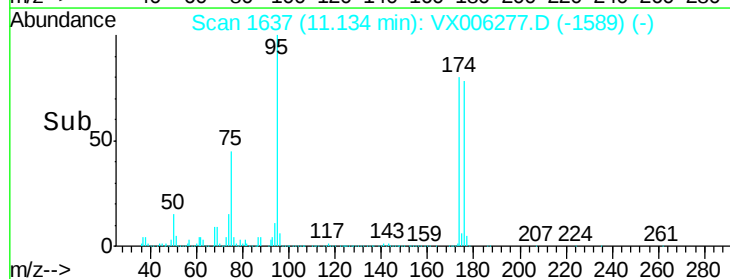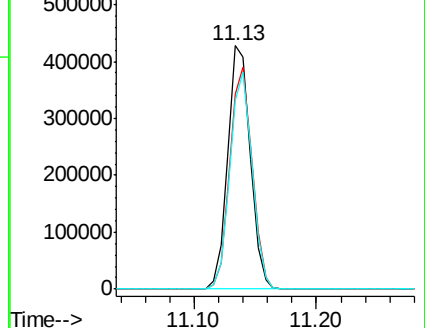

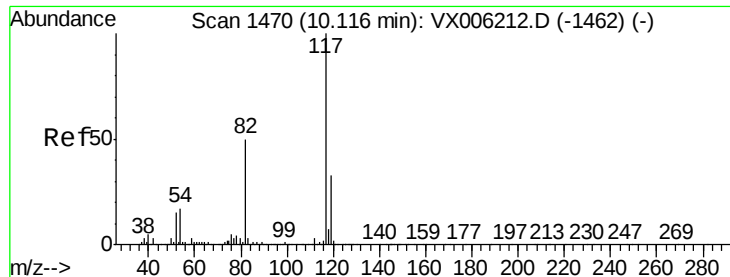

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.12 min Scan# 1470

Delta R.T. 0.00 min

Lab File: VX006277.D

Acq: 04 Dec 2018 14:42

Instrument :

MSVOA_X

ClientSampleId :

DSN001


Tgt Ion:117 Resp: 1134386

Ion Ratio Lower Upper

117 100

82 49.0 39.6 59.4




119 32.5 26.3 39.5

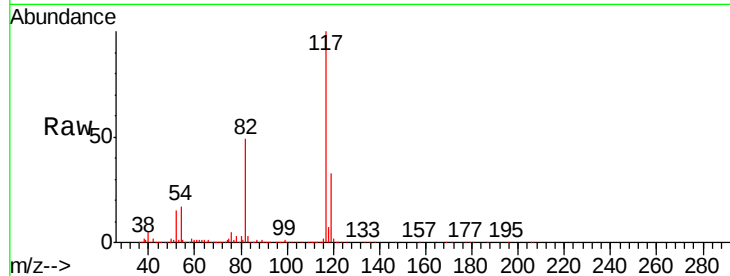

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

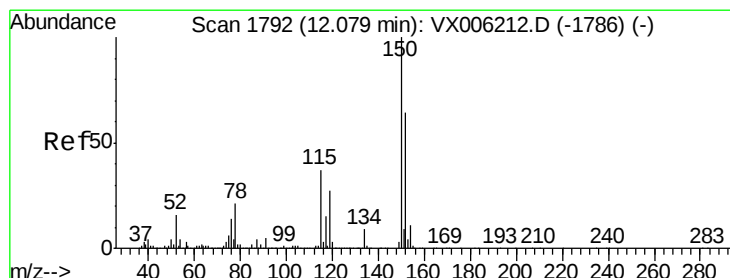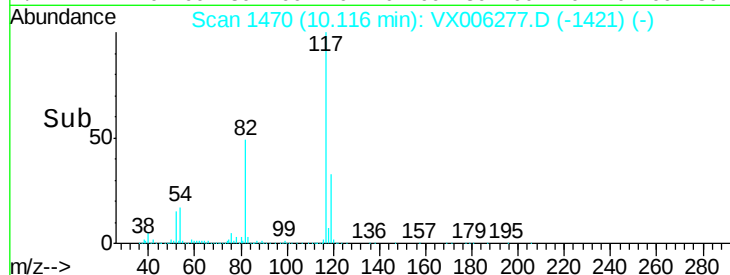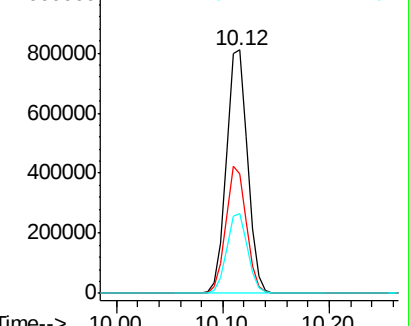

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX006277.D

Acq: 04 Dec 2018 14:42


Tgt Ion:152 Resp: 557382

Ion Ratio Lower Upper

152 100

115 56.0 39.0 116.9

150 156.9 0.0 345.8

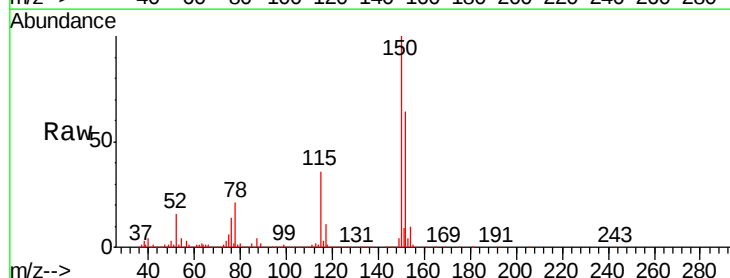

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

