


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120418\
 Data File : VX006267.D
 Acq On : 04 Dec 2018 09:38
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
 Title : SW846 8260
 Last Update : Fri Nov 30 03:55:33 2018

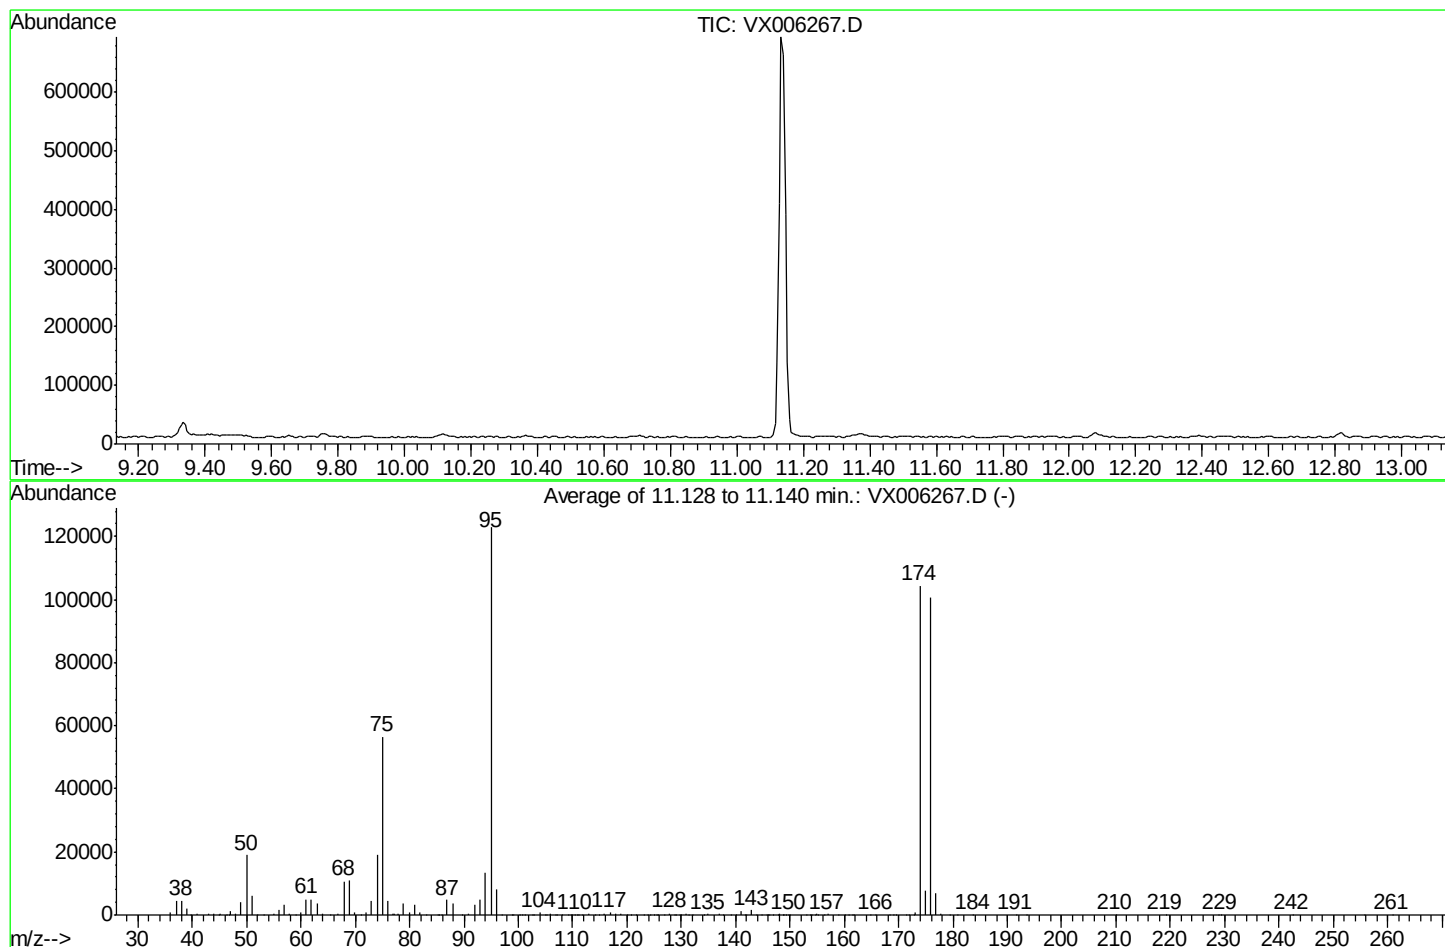

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	18941	PASS
75	95	30	60	46.1	56586	PASS
95	95	100	100	100.0	122863	PASS
96	95	5	9	6.5	8020	PASS
173	174	0.00	2	0.8	846	PASS
174	95	50	100	85.0	104474	PASS
175	174	5	9	7.5	7788	PASS
176	174	95	101	96.4	100672	PASS
177	176	5	9	6.9	6917	PASS