

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX120419\
 Data File : VX013747.D
 Acq On : 04 Dec 2019 14:20
 Operator : JC/SP
 Sample : K6095-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6

Quant Time: Dec 05 01:26:32 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 26 15:53:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	683835	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	1034083	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	910289	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	403734	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	365683	46.07	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.14%	
35) Dibromofluoromethane	5.49	113	307770	48.14	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.28%	
50) Toluene-d8	8.71	98	1205243	48.39	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.78%	
62) 4-Bromofluorobenzene	11.14	95	408986	45.54	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.08%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX120419\
Data File : VX013747.D
Acq On : 04 Dec 2019 14:20
Operator : JC/SP
Sample : K6095-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Quant Time: Dec 05 01:26:32 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 26 15:53:00 2019
Response via : Initial Calibration

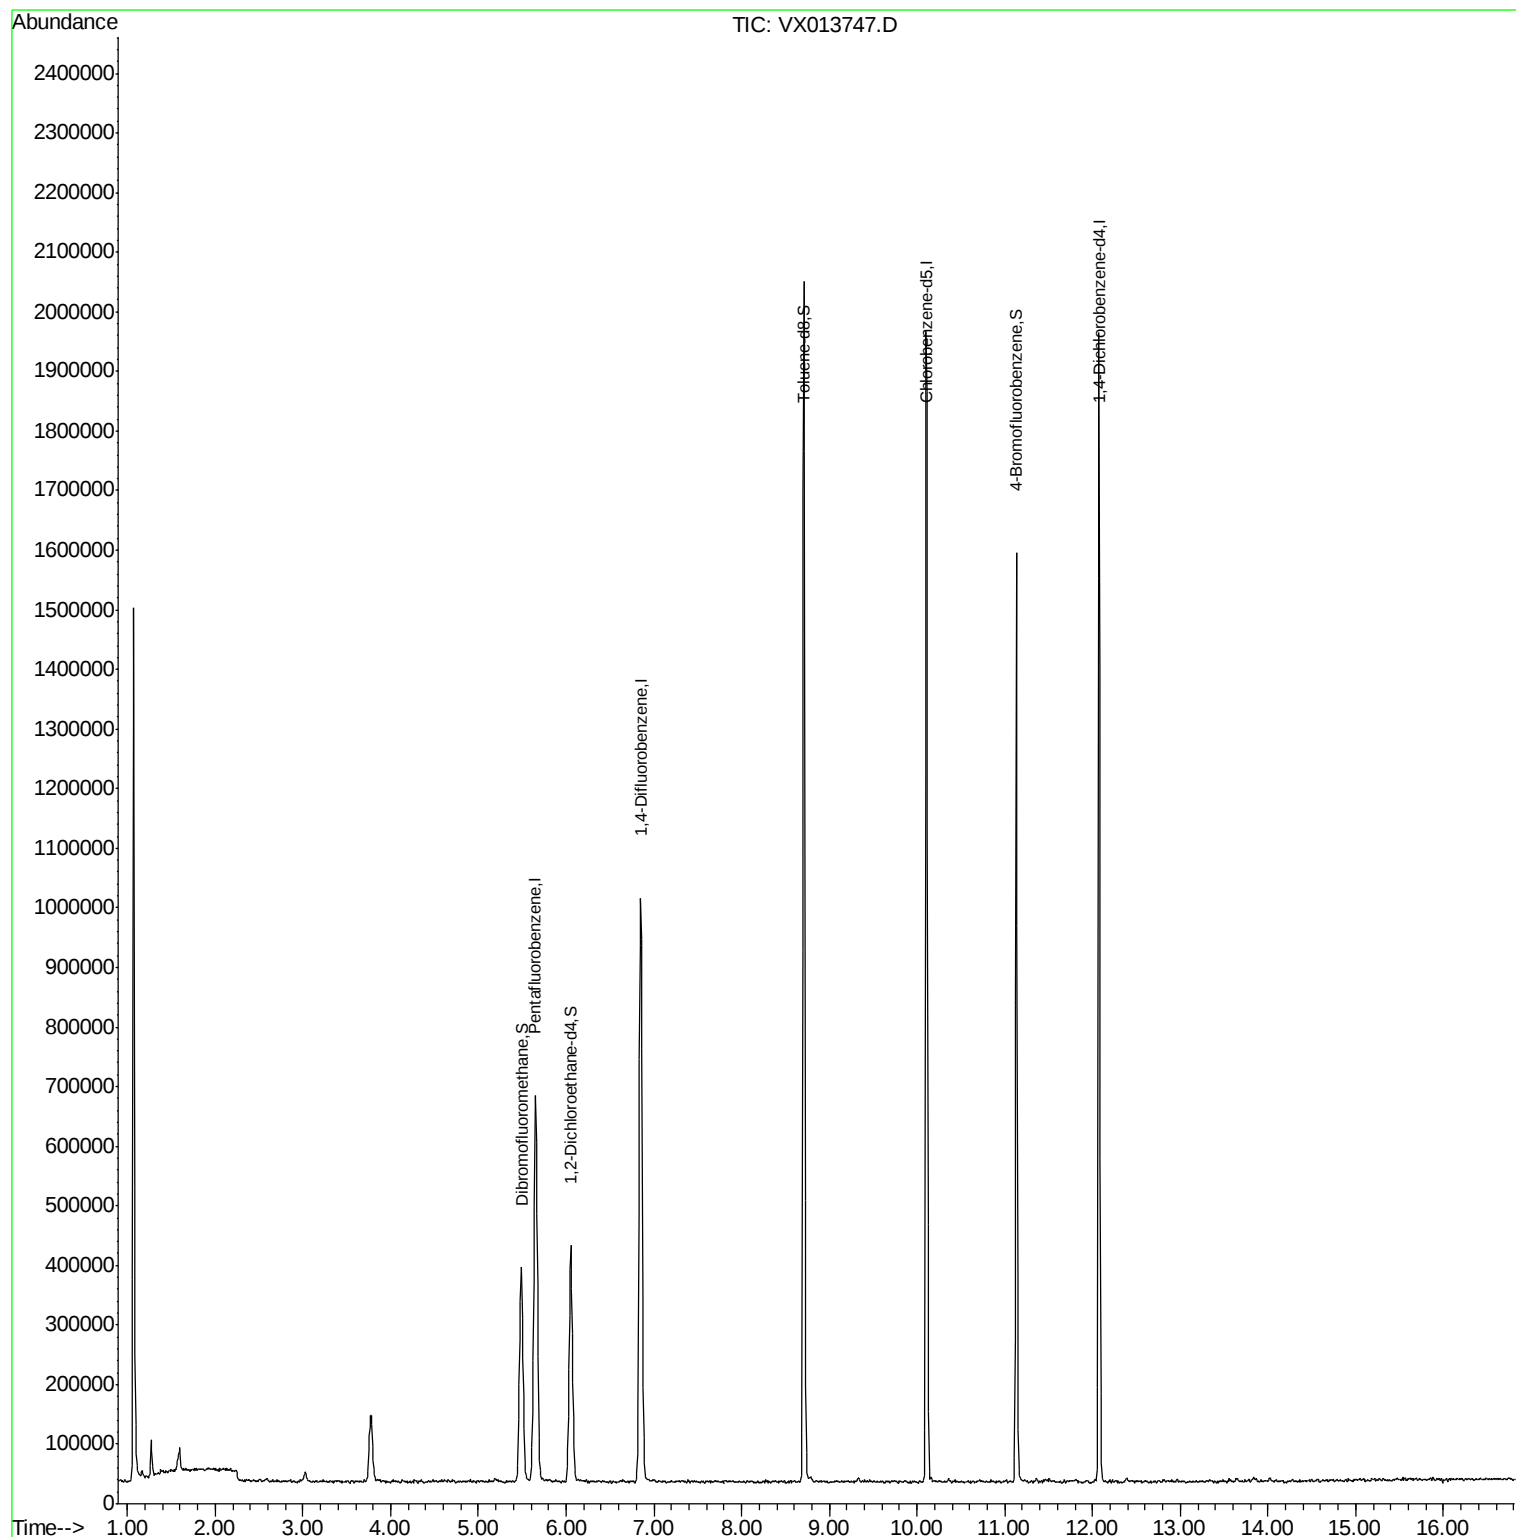

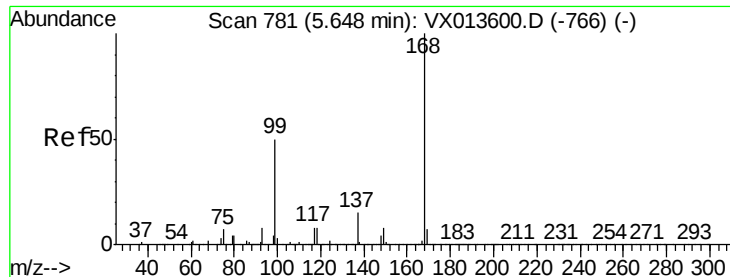

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 781

Delta R.T. 0.00 min

Lab File: VX013747.D

Acq: 04 Dec 2019 14:20

Instrument :

MSVOA_X

ClientSampleId :


STORAGE-BLANK-SOIL-REF-6

Tot Ion:168 Resp: 683835

Ion Ratio Lower Upper

168 100

99 49.3 39.8 59.8

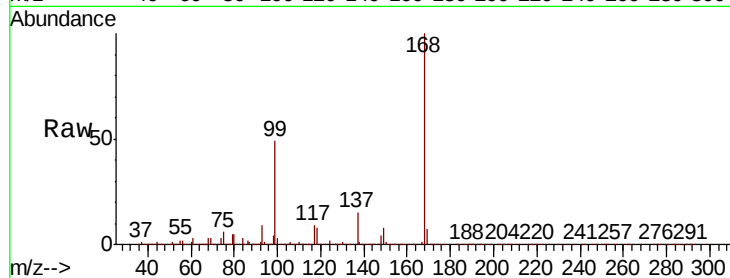

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

250000

200000

150000



100000

50000

0

5.50 5.60 5.70 5.80

Time-->

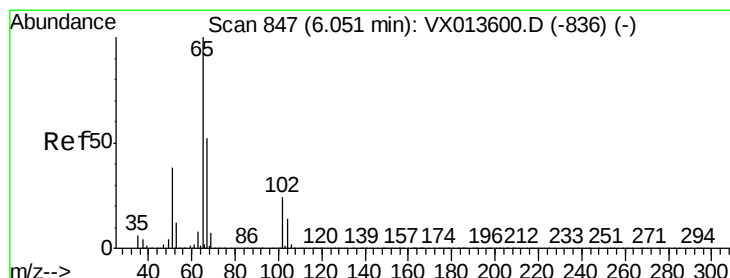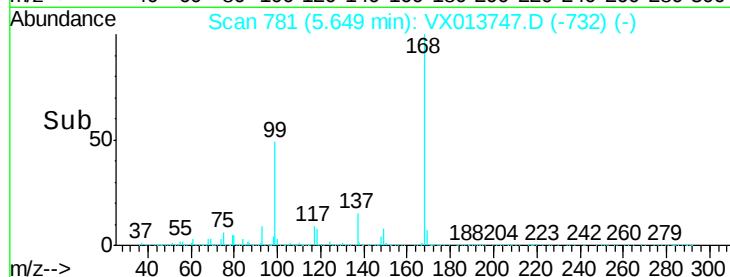

#33

1,2-Dichloroethane-d4

Concen: 46.069 ug/l

RT: 6.05 min Scan# 847

Delta R.T. 0.00 min

Lab File: VX013747.D


Acq: 04 Dec 2019 14:20

Tgt Ion: 65 Resp: 365683

Ion Ratio Lower Upper

65 100

67 53.5 0.0 104.4

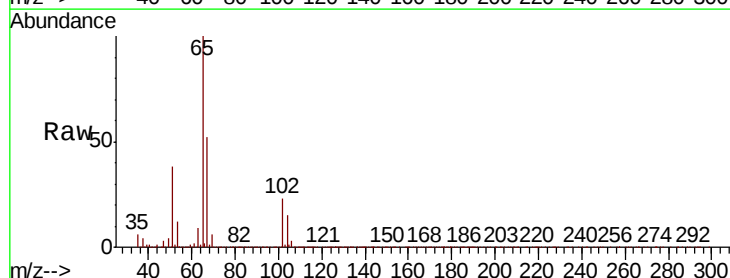

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

150000


100000


50000

0

5.90 6.00 6.10 6.20

Time-->

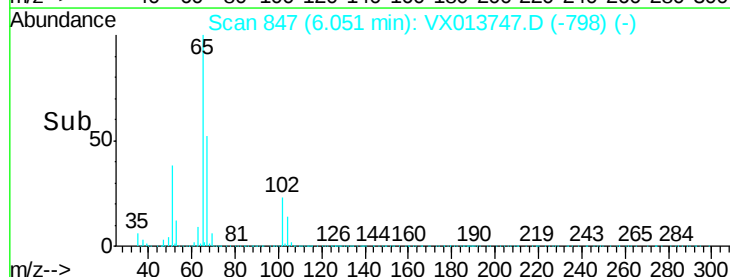

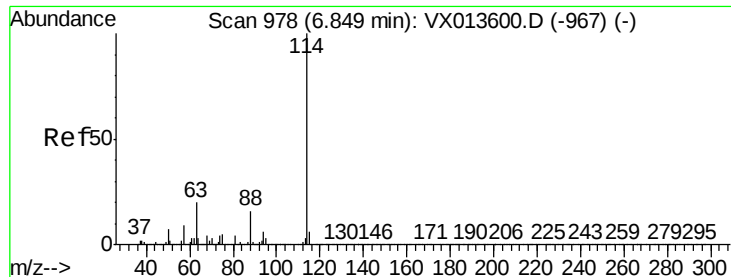

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. 0.00 min

Lab File: VX013747.D

Acq: 04 Dec 2019 14:20

Instrument :

MSVOA_X

ClientSampleId :

STORAGE-BLANK-SOIL-REF-6


Tot Ion:114 Resp: 1034083

Ion Ratio Lower Upper

114 100

63 19.4 0.0 39.6




88 15.3 0.0 31.4

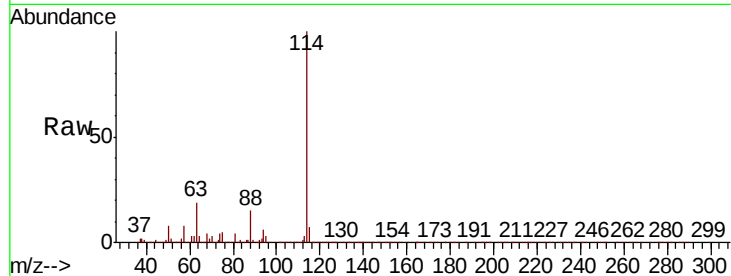

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

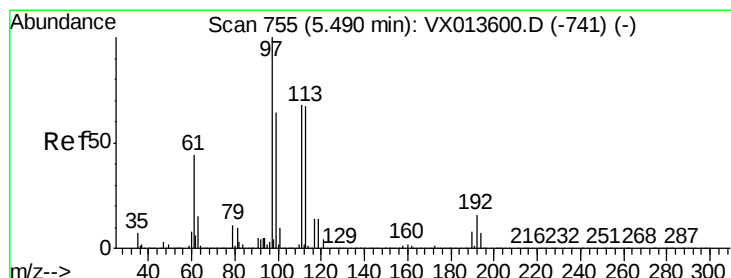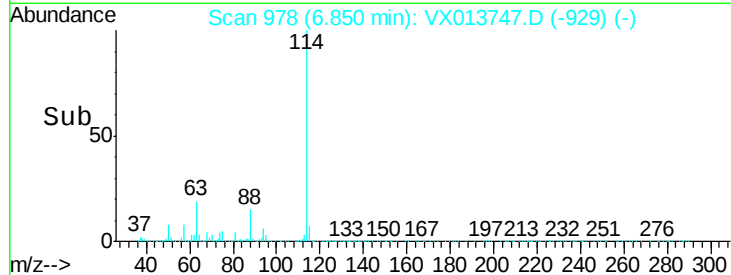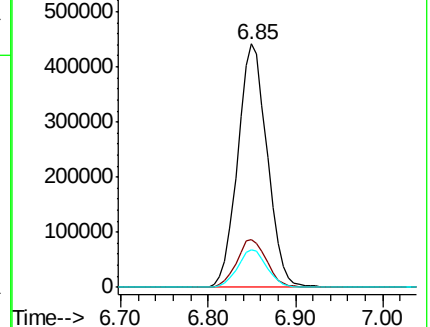

#35

Dibromofluoromethane

Concen: 48.143 ug/l

RT: 5.49 min Scan# 755

Delta R.T. 0.00 min

Lab File: VX013747.D

Acq: 04 Dec 2019 14:20


Tgt Ion:113 Resp: 307770

Ion Ratio Lower Upper

113 100

111 103.5 83.6 125.4



192 24.4 19.2 28.8

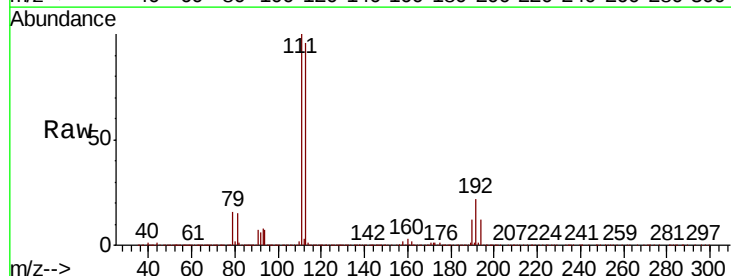


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

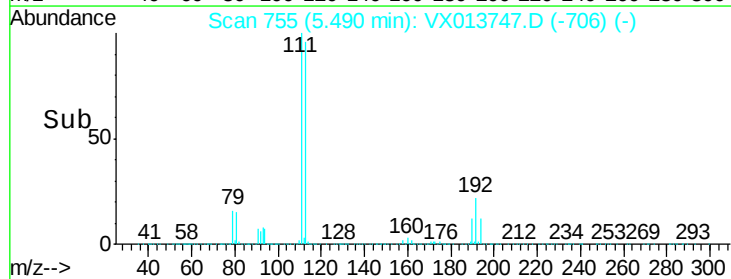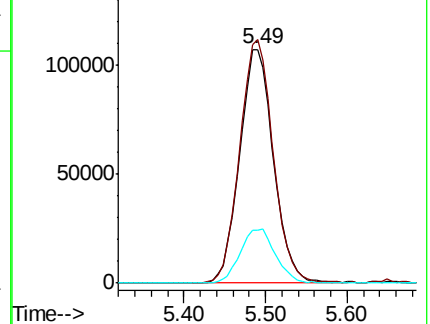

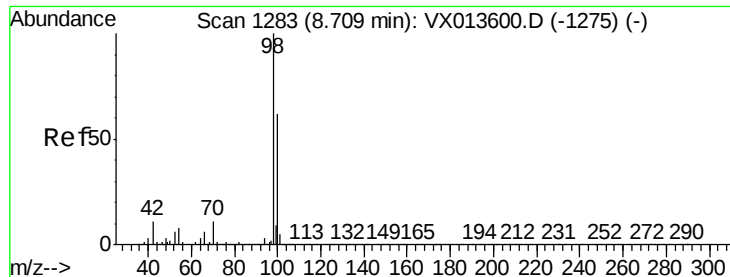

#50

Toluene-d8

Concen: 48.389 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. 0.00 min

Lab File: VX013747.D

Acq: 04 Dec 2019 14:20

Instrument :

MSVOA_X

ClientSampleId :





STORAGE-BLANK-SOIL-REF-6

Tot Ion: 98 Resp: 1205243

Ion Ratio Lower Upper

98 100

100 65.6 53.1 79.7

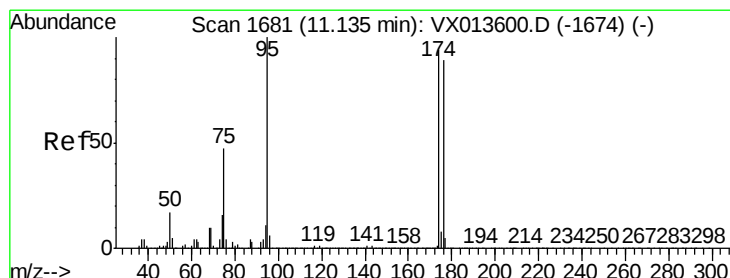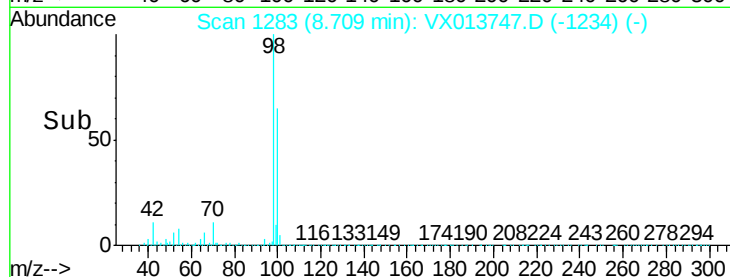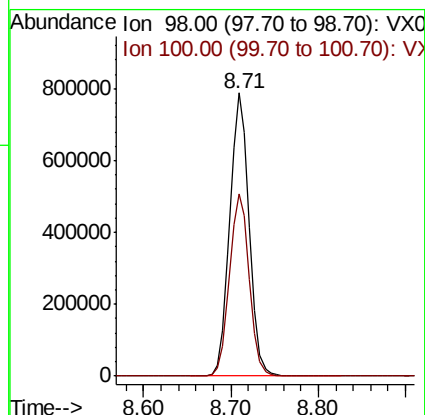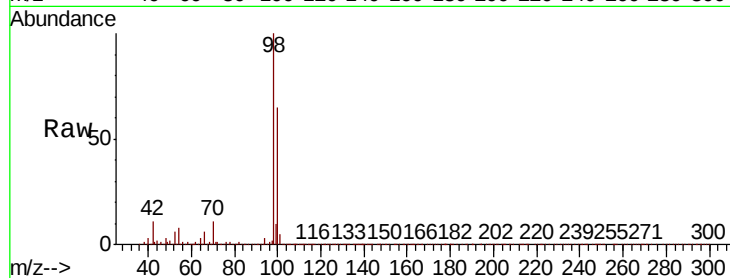

#62

4-Bromofluorobenzene

Concen: 45.536 ug/l

RT: 11.14 min Scan# 1681

Delta R.T. 0.00 min

Lab File: VX013747.D

Acq: 04 Dec 2019 14:20




Tgt Ion: 95 Resp: 408986


Ion Ratio Lower Upper

95 100

174 90.1 0.0 180.0

176 88.5 0.0 173.6


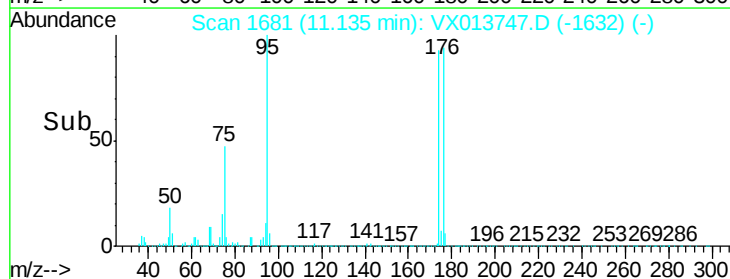
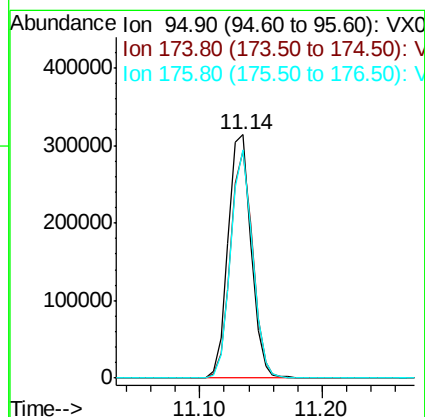
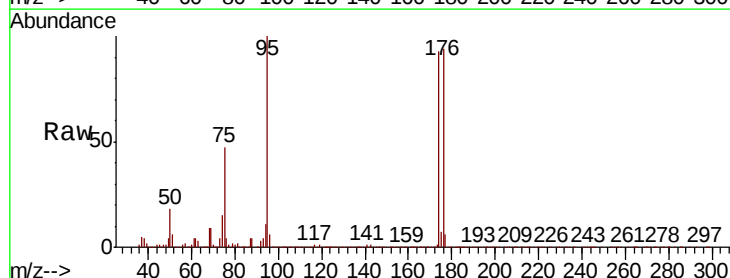


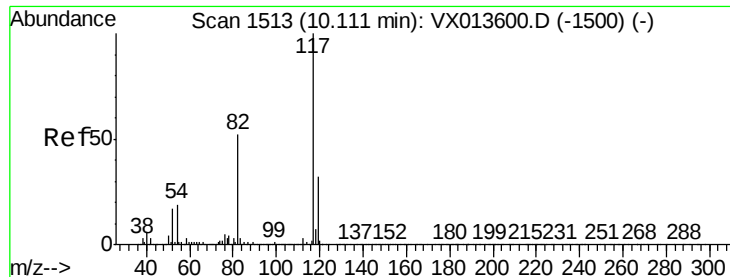

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1512
Delta R.T. -0.01 min
Lab File: VX013747.D
Acq: 04 Dec 2019 14:20

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tot Ion	Ratio	Lower	Upper
117	100		
82	54.9	41.8	62.8
119	32.4	25.8	38.8

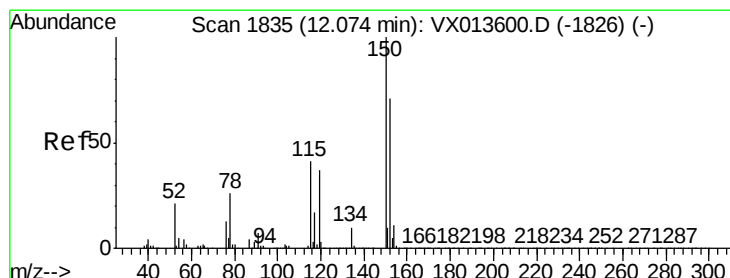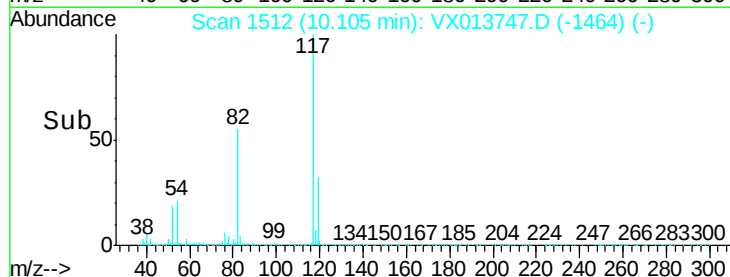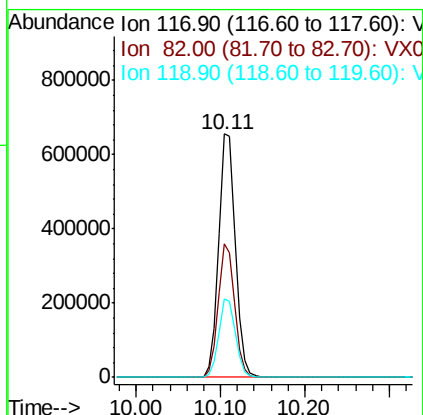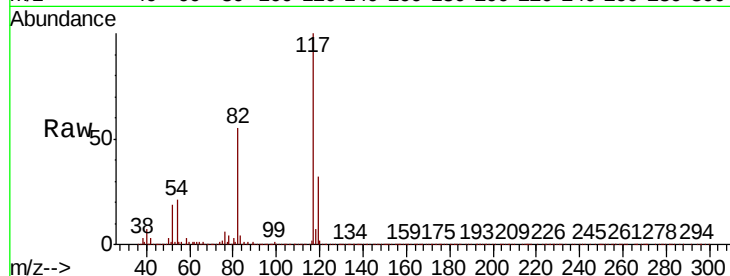

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. 0.00 min
Lab File: VX013747.D
Acq: 04 Dec 2019 14:20

Tgt Ion	Ratio	Lower	Upper
152	100		
115	55.0	38.4	115.1
150	155.8	0.0	346.8

